

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2021 01:19
 Operator : AR\AJ
 Sample : M3407-27
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:12:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.568	9724962	26117755	23.511	25.723
28)	SA Decachlor...	10.403	11.487	10048694	17609298	17.485	18.149
Target Compounds							
4)	MA Heptachlor	0.000	7.197	0	337392	N.D.	0.251 #
7)	B delta-BHC	0.000	7.042f	0	187978	N.D.	0.149 #
10)	B gamma-Chl...	0.000	8.292	0	274255	N.D.	0.239 #
15)	B Endosulfa...	0.000	9.214	0	317087	N.D.	0.346 #
22)	Mirex	0.000	10.557f	0	102924	N.D.	0.130 #
25)	Chlordane-3	0.000	8.292	0	274255	N.D.	1.679 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2021 01:19
Operator : AR\AJ
Sample : M3407-27
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:12:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

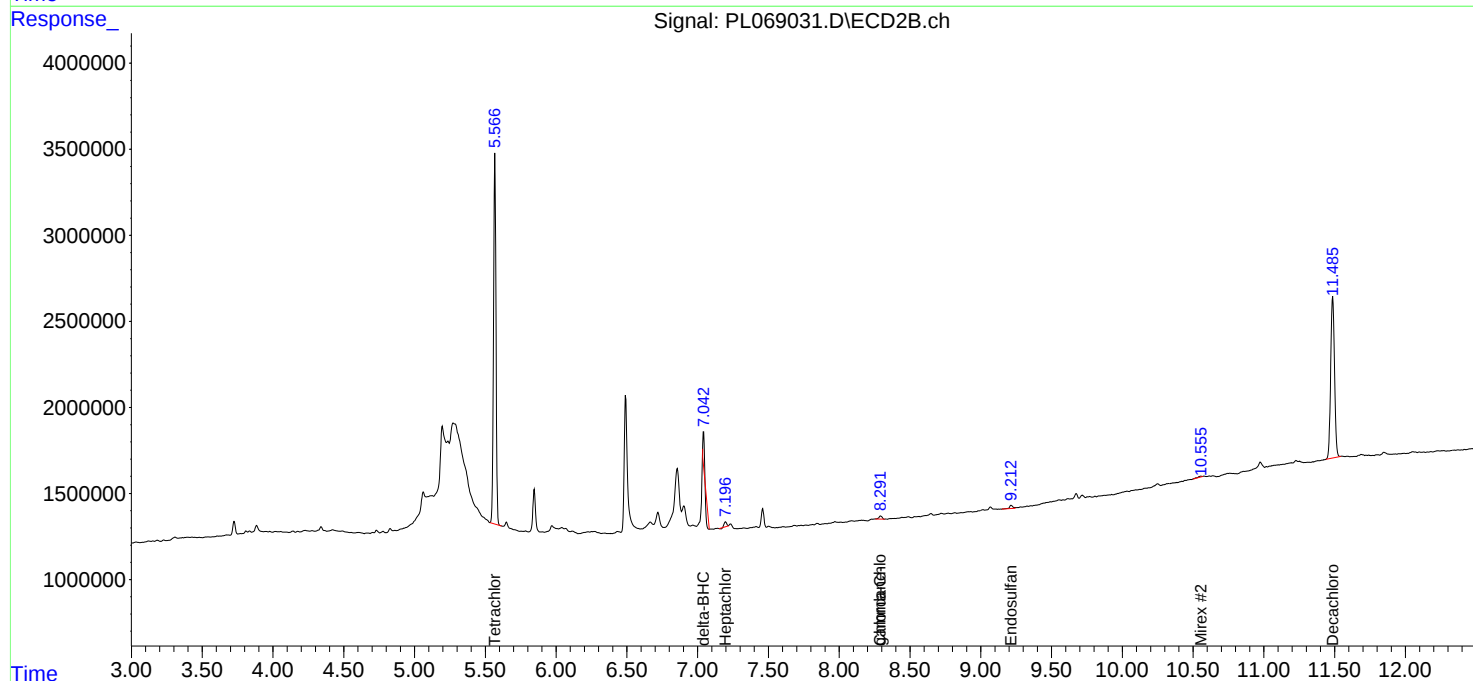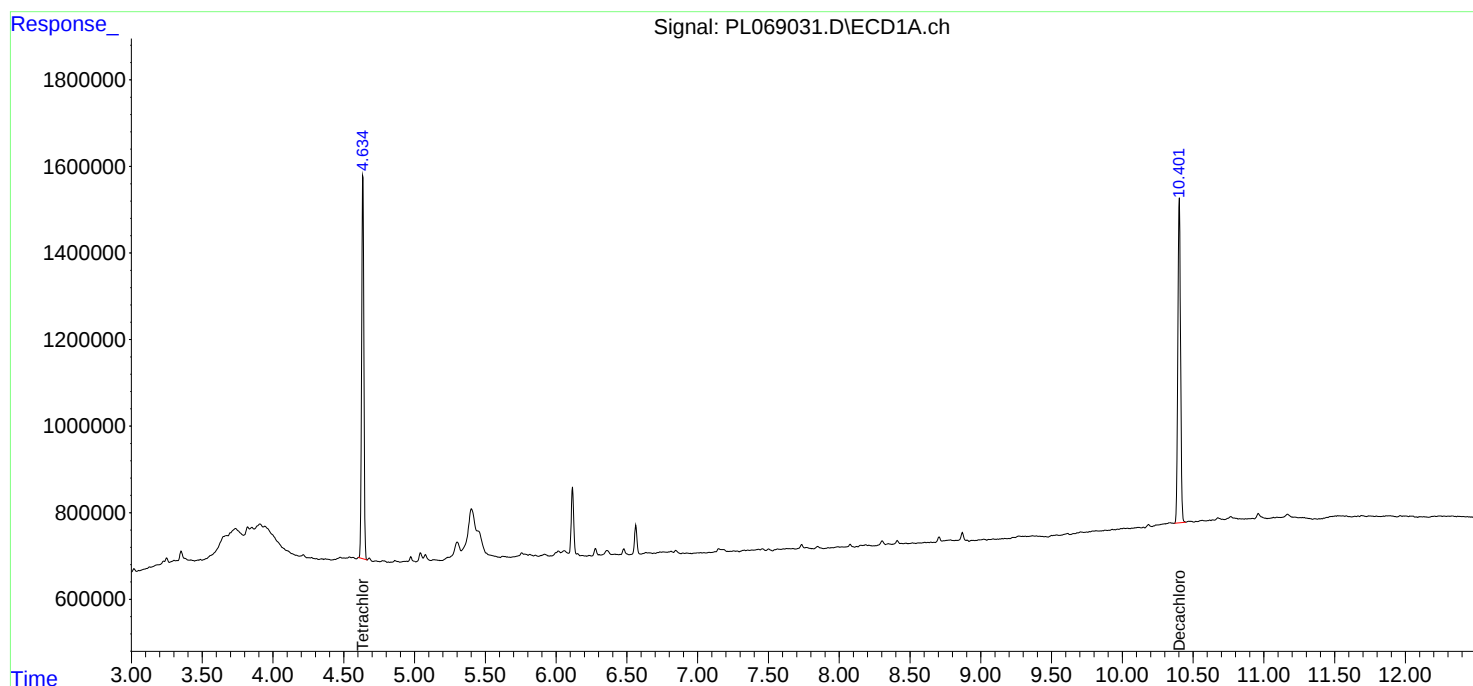


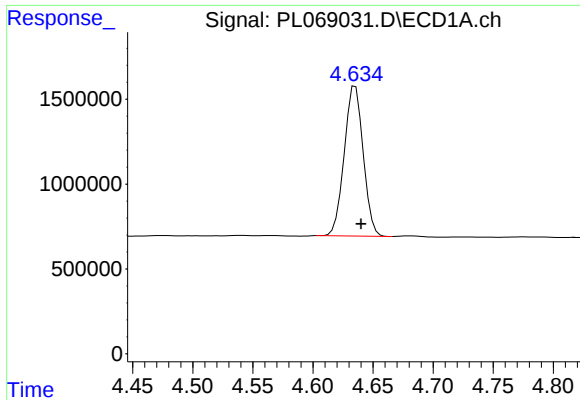

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.005 min
Response: 9724962
Conc: 23.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

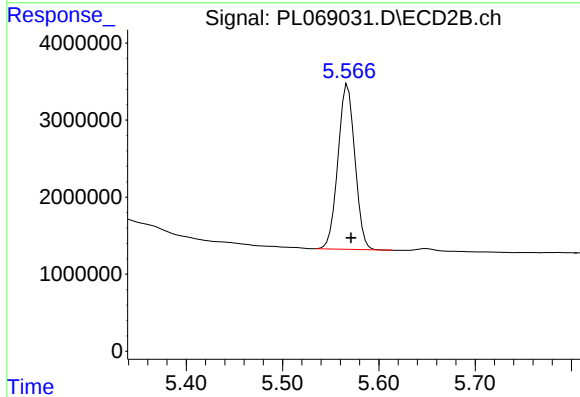


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 26117755
Conc: 25.72 ng/ml

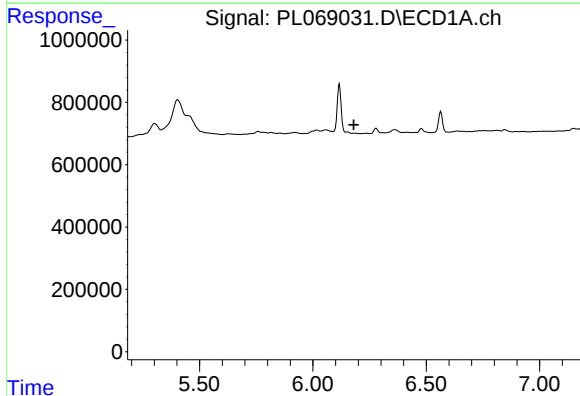


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.180 min
Response: 0
Conc: N.D.

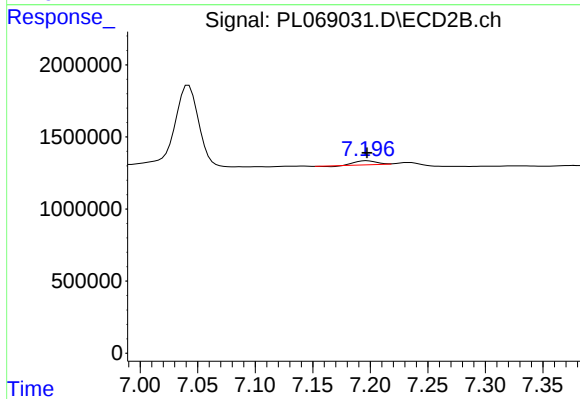

#4 Heptachlor


R.T.: 7.197 min
Delta R.T.: 0.000 min
Response: 337392
Conc: 0.25 ng/ml

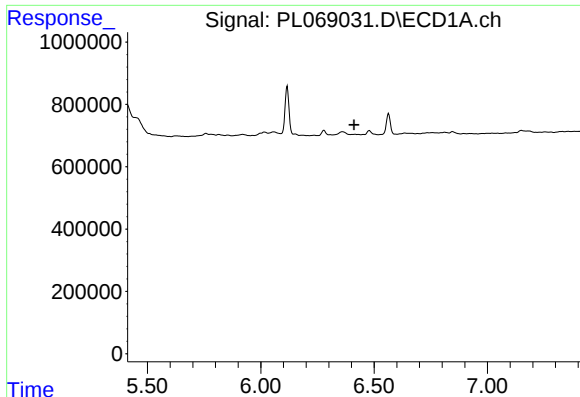

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

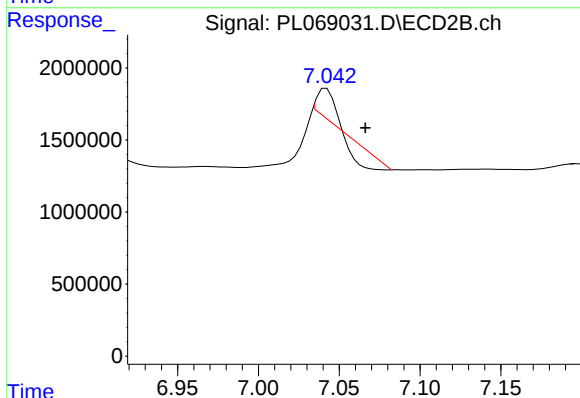


#7 delta-BHC

R.T.: 7.042 min
Delta R.T.: -0.024 min
Response: 187978
Conc: 0.15 ng/ml

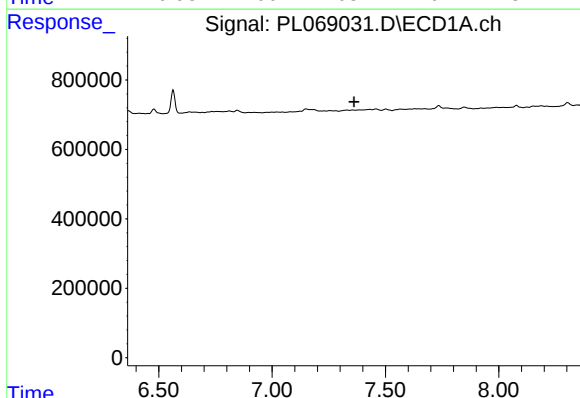


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.361 min
Response: 0
Conc: N.D.

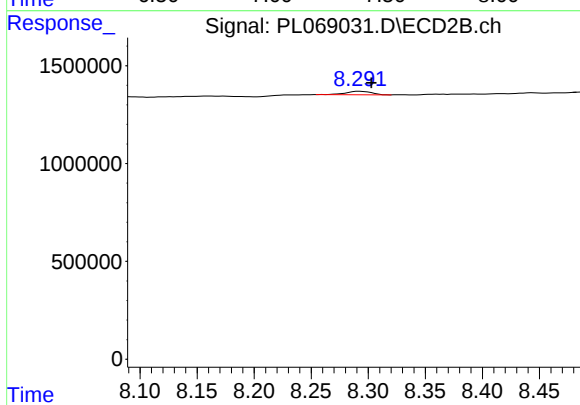

#10 gamma-Chlordane


R.T.: 8.292 min
Delta R.T.: -0.010 min
Response: 274255
Conc: 0.24 ng/ml

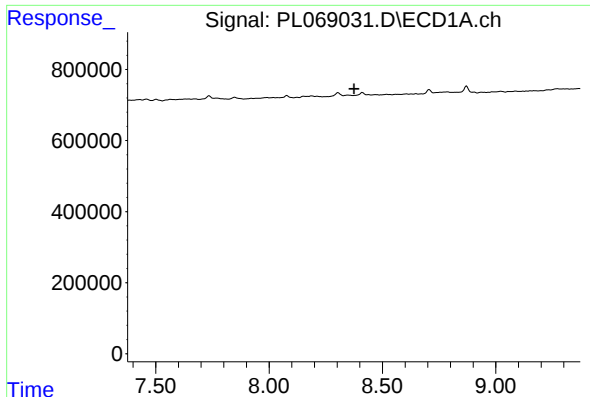

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

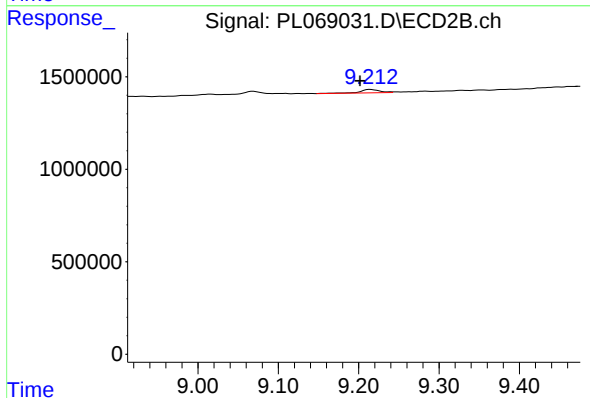


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.013 min
Response: 317087
Conc: 0.35 ng/ml

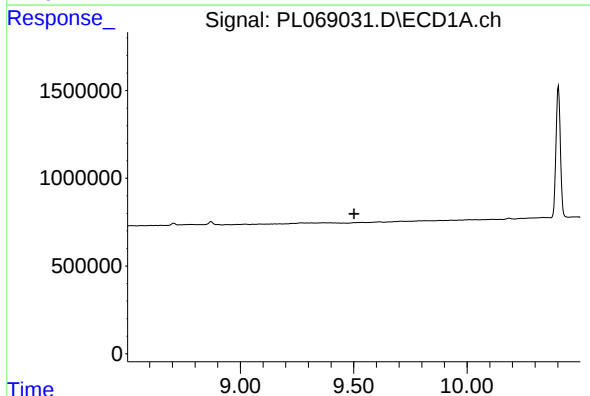


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

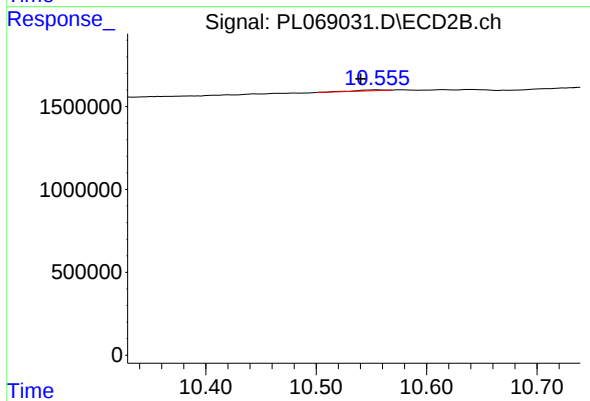

#22 Mirex


R.T.: 10.557 min
Delta R.T.: 0.017 min
Response: 102924
Conc: 0.13 ng/ml

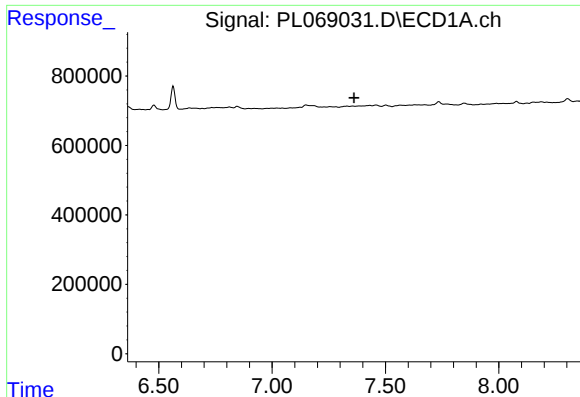

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

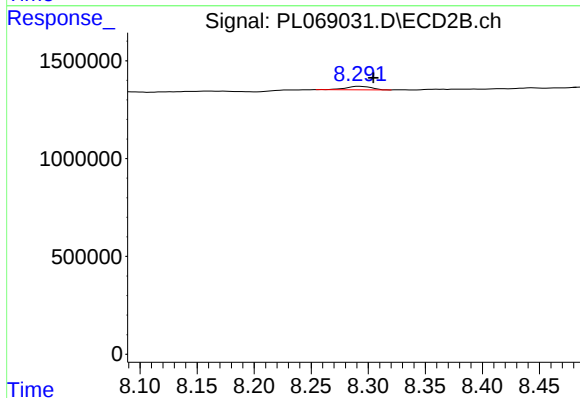


#25 Chlordane-3

R.T.: 8.292 min
Delta R.T.: -0.012 min
Response: 274255
Conc: 1.68 ng/ml

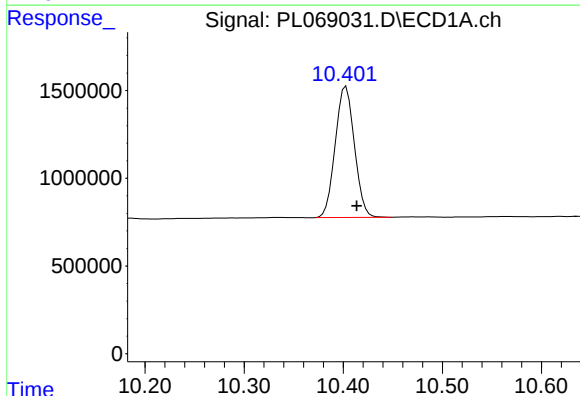

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.011 min
Response: 10048694
Conc: 17.49 ng/ml

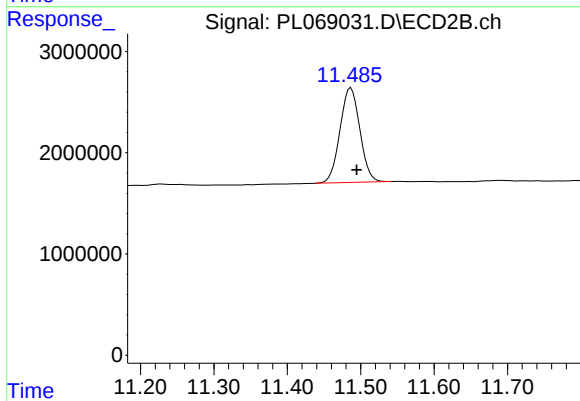

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 17609298
Conc: 18.15 ng/ml