

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
 Data File : PL069034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2021 02:09
 Operator : AR\AJ
 Sample : M3408-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:12:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	9143281	24291315	22.104	23.924
28)	SA Decachlor...	10.403	11.487	11902946	20765693	20.712	21.403
Target Compounds							
9)	A Endosulfan I	0.000	8.446	0	41839	N.D.	0.040 #
11)	B alpha-Chl...	0.000	8.389	0	158904	N.D.	0.138 #
13)	MA Dieldrin	0.000	8.723	0	216570	N.D.	0.200 #
14)	MA Endrin	0.000	8.978	0	100276	N.D.	0.110 #
15)	B Endosulfa...	0.000	9.213	0	185690	N.D.	0.202 #
26)	Chlordane-4	0.000	8.389	0	158904	N.D.	0.801 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081521\
Data File : PL069034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2021 02:09
Operator : AR\AJ
Sample : M3408-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:12:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

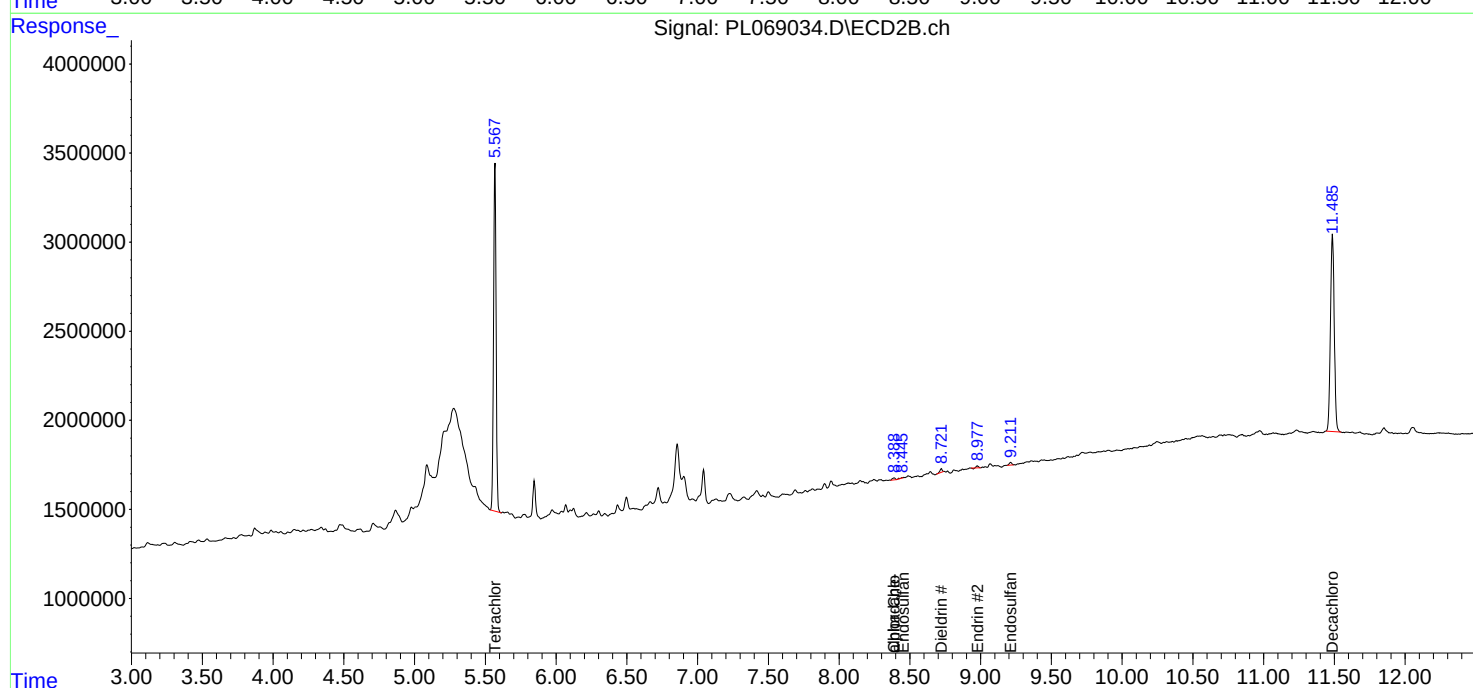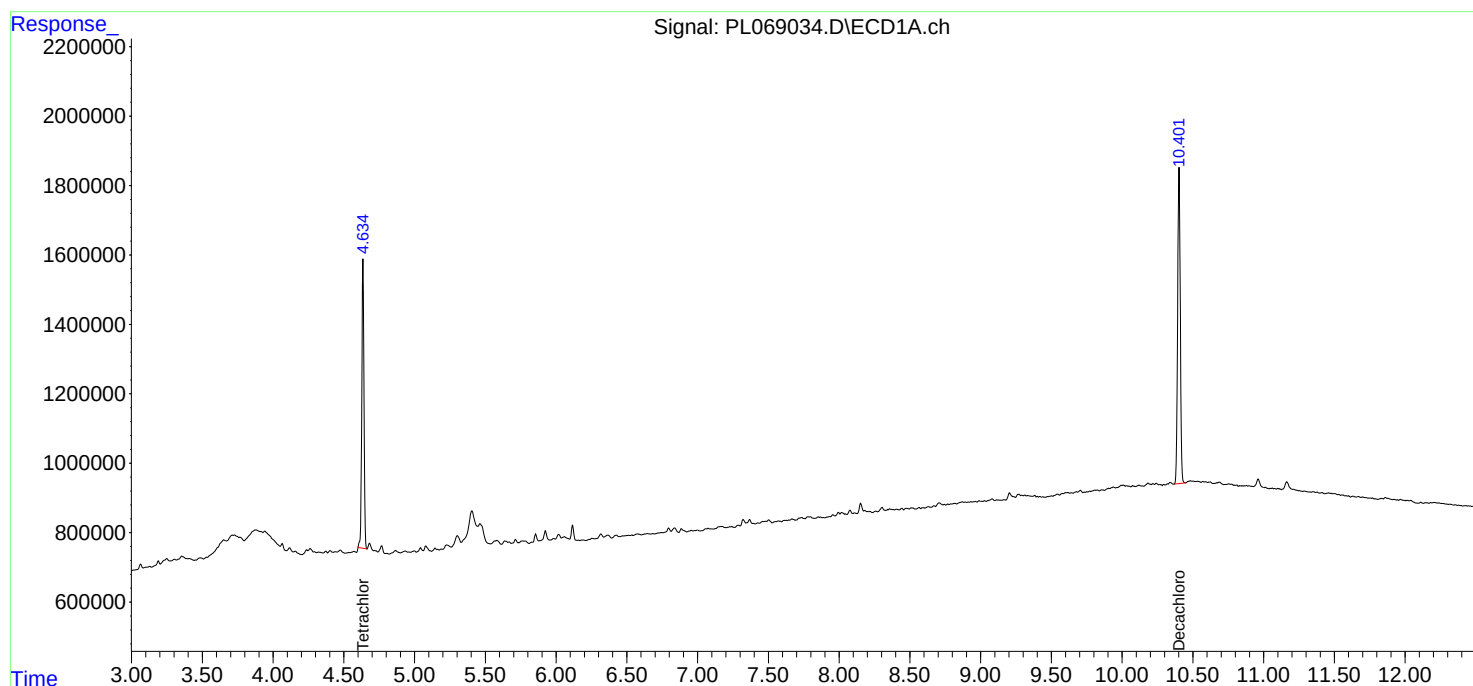


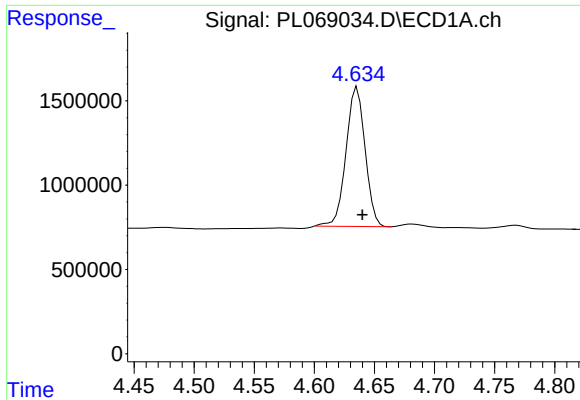

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 9143281
Conc: 22.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

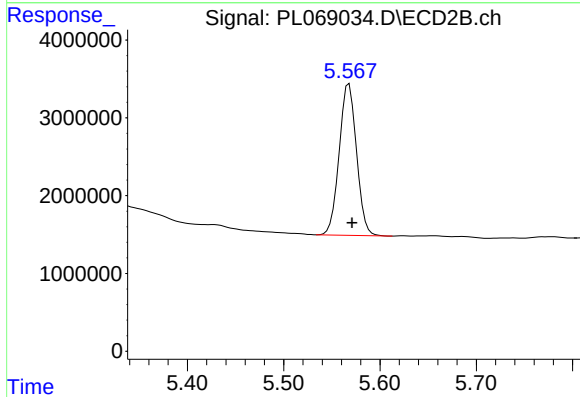


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 24291315
Conc: 23.92 ng/ml

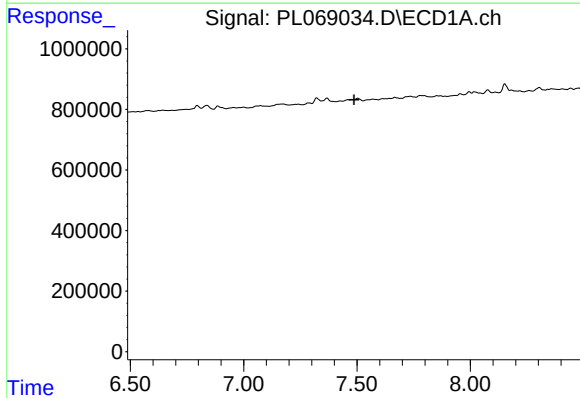


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

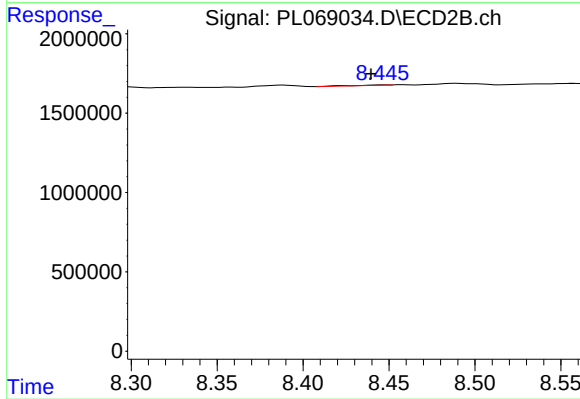

#9 Endosulfan I


R.T.: 8.446 min
Delta R.T.: 0.007 min
Response: 41839
Conc: 0.04 ng/ml

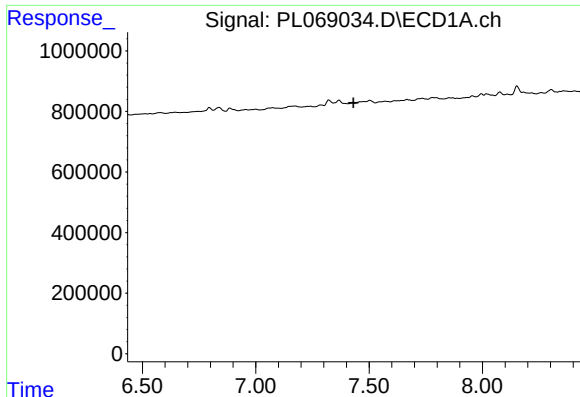

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

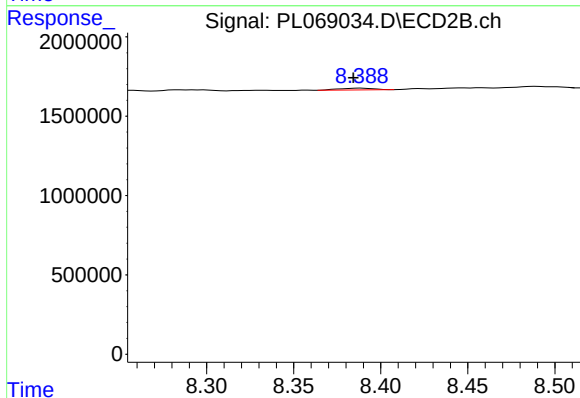


#11 alpha-Chlordane

R.T.: 8.389 min
Delta R.T.: 0.005 min
Response: 158904
Conc: 0.14 ng/ml

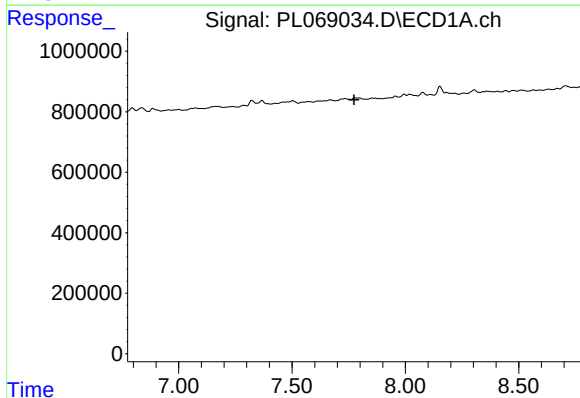


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

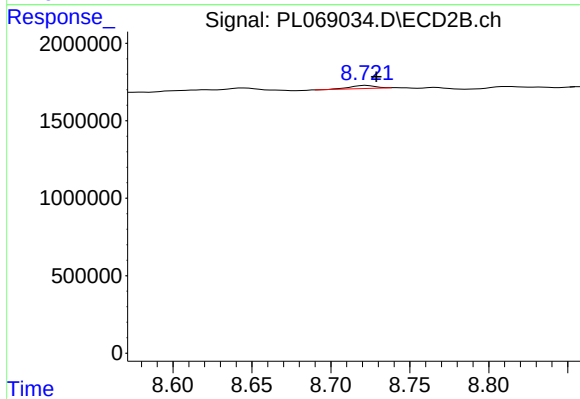

#13 Dieldrin


R.T.: 8.723 min
Delta R.T.: -0.006 min
Response: 216570
Conc: 0.20 ng/ml

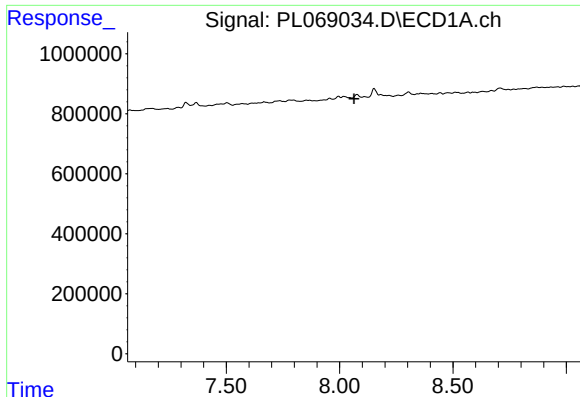

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

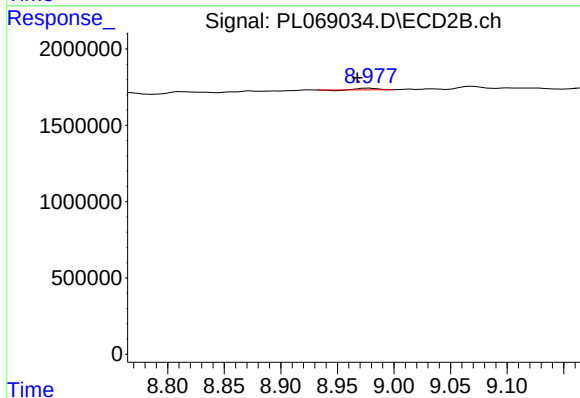


#14 Endrin

R.T.: 8.978 min
Delta R.T.: 0.010 min
Response: 100276
Conc: 0.11 ng/ml

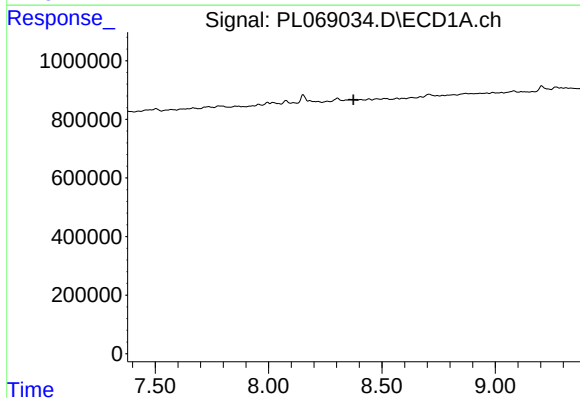


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

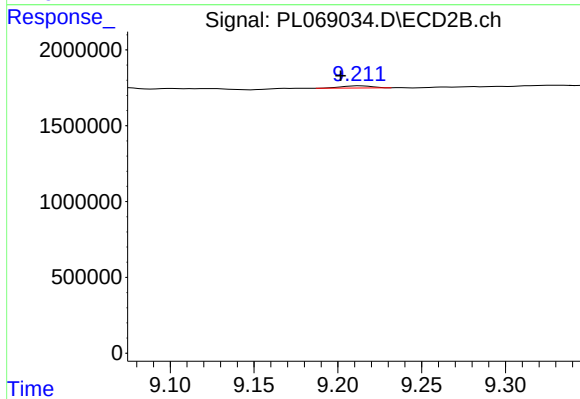

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.011 min
Response: 185690
Conc: 0.20 ng/ml

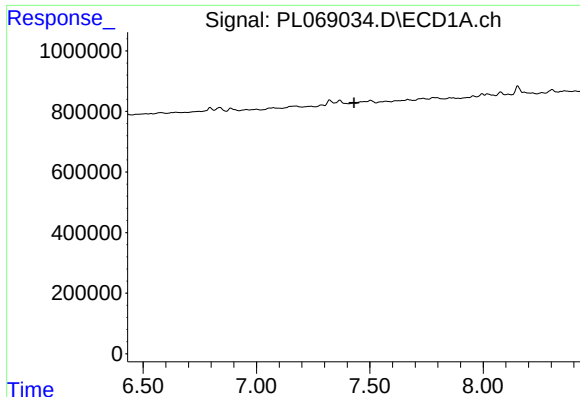

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

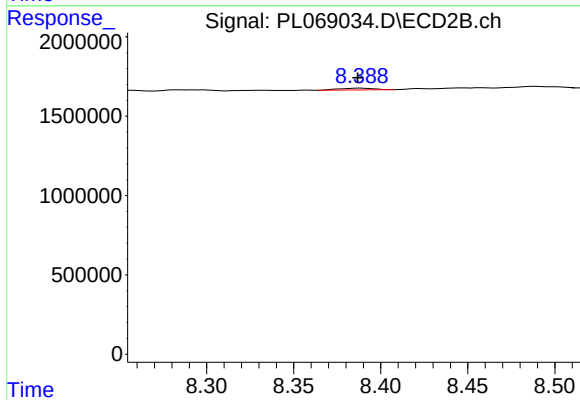


#26 Chlordane-4

R.T.: 8.389 min
Delta R.T.: 0.002 min
Response: 158904
Conc: 0.80 ng/ml

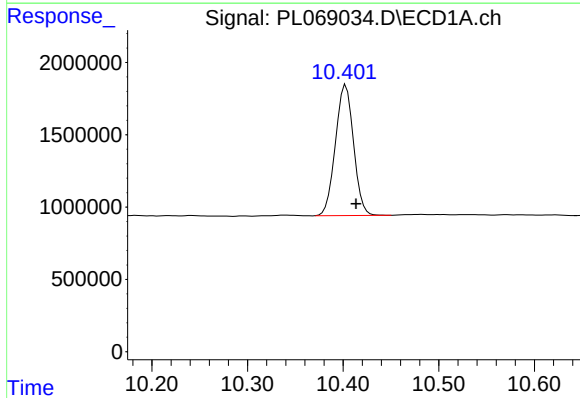

#28 Decachlorobiphenyl

R.T.: 10.403 min
Delta R.T.: -0.011 min
Response: 11902946
Conc: 20.71 ng/ml

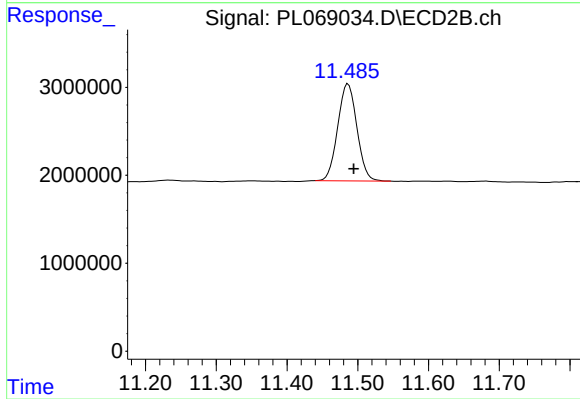

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 20765693
Conc: 21.40 ng/ml