

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
 Data File : PL077122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 19:49
 Operator : AR\AJ
 Sample : N4208-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:58:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.635	16759450	46291835	17.092	16.171
28)	SA Decachlor...	8.906	7.737	14278783	39976069	18.914	17.758
Target Compounds							
9)	A Endosulfan I	0.000	4.941	0	634868	N.D.	0.232 #
10)	B gamma-Chl...	0.000	4.831f	0	7530128	N.D.	2.472 #
11)	B alpha-Chl...	5.901	0.000	362264	0	0.363	N.D. #
12)	B 4,4'-DDE	6.077	5.064	102551	1313391	0.118	0.455 #
14)	MA Endrin	0.000	5.482f	0	579855	N.D.	0.228 #
15)	B Endosulfa...	6.709f	0.000	232906	0	0.272	N.D. #
17)	MA 4,4'-DDT	0.000	5.859	0	337056	N.D.	0.149 #
25)	Chlordane-3	0.000	4.831f	0	7530128	N.D.	23.784 #
26)	Chlordane-4	5.901	0.000	362264	0	2.052	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
Data File : PL077122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 19:49
Operator : AR\AJ
Sample : N4208-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:58:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

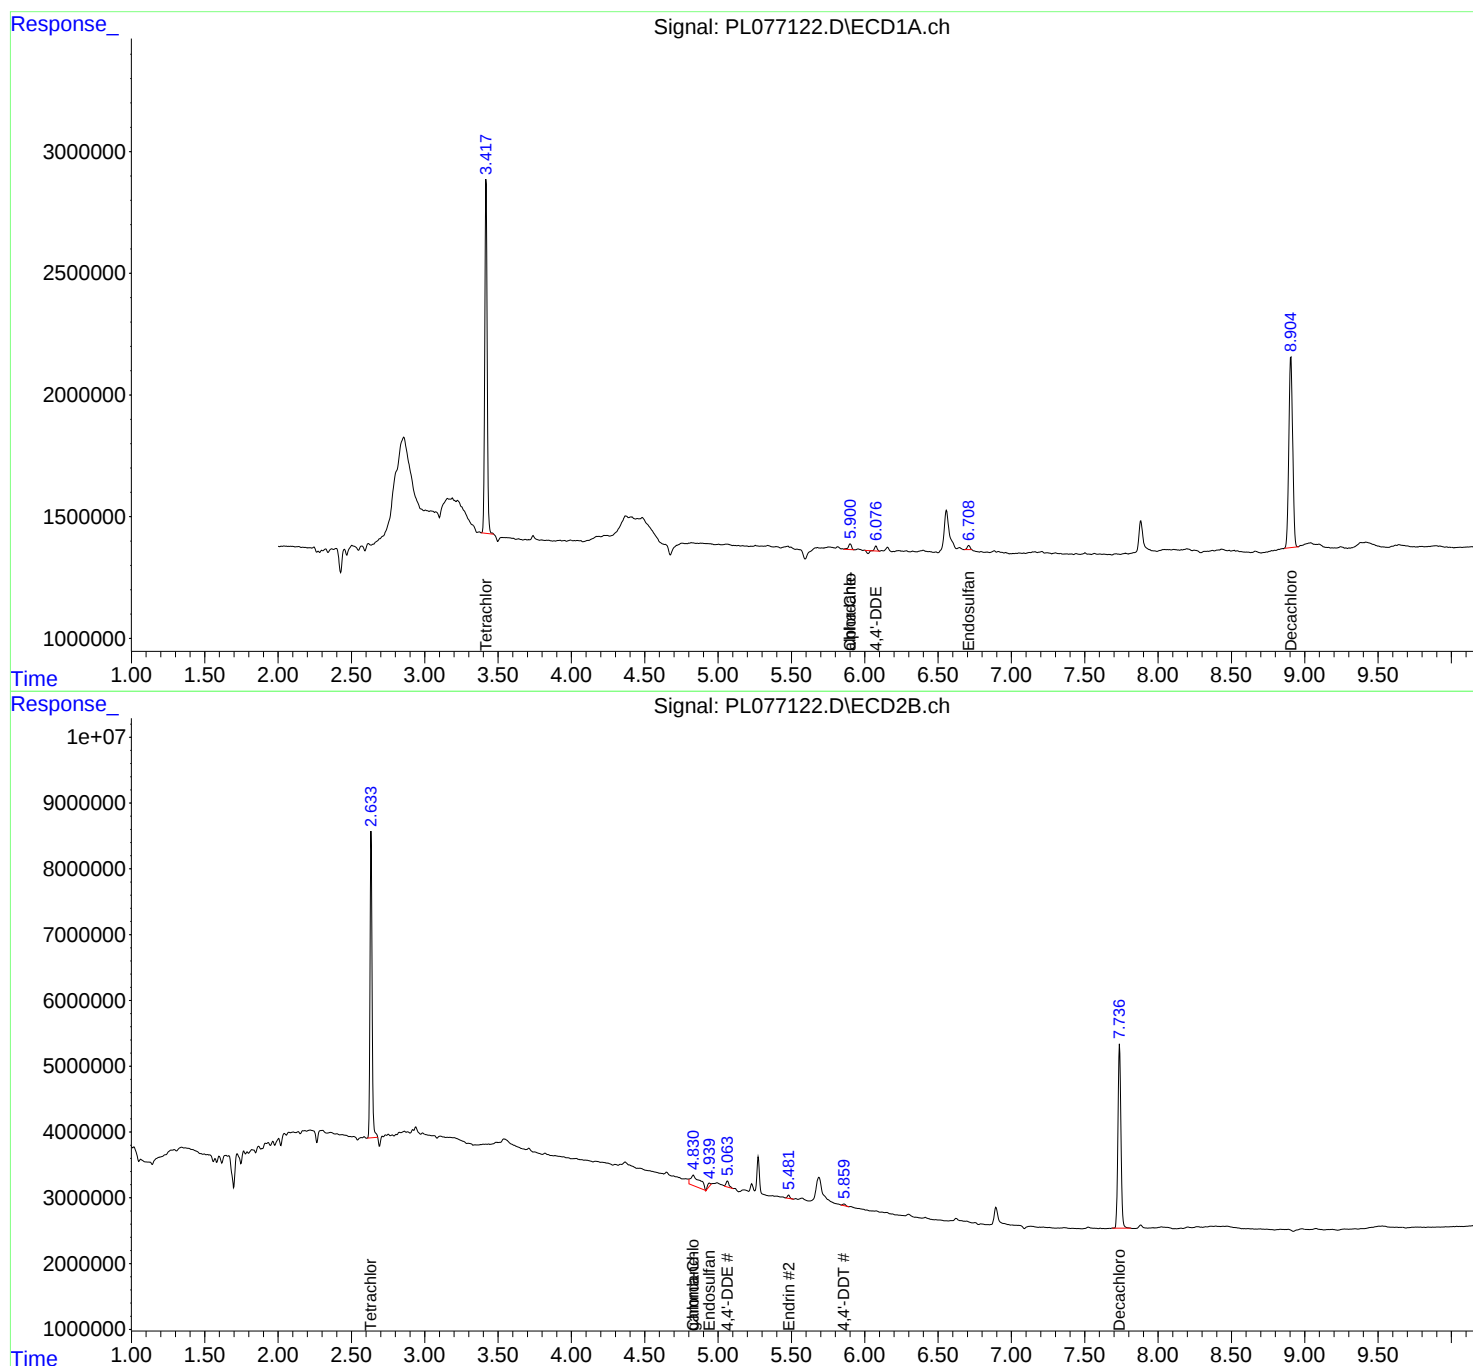


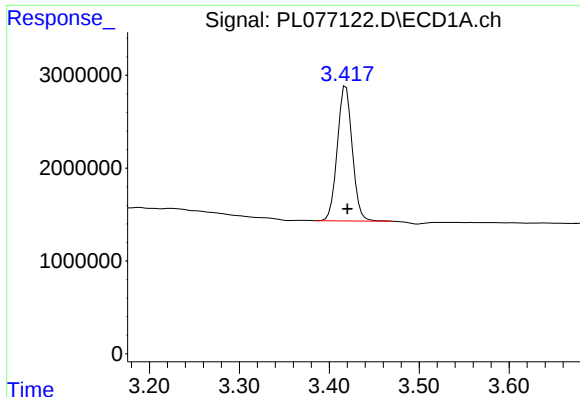

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 16759450
Conc: 17.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

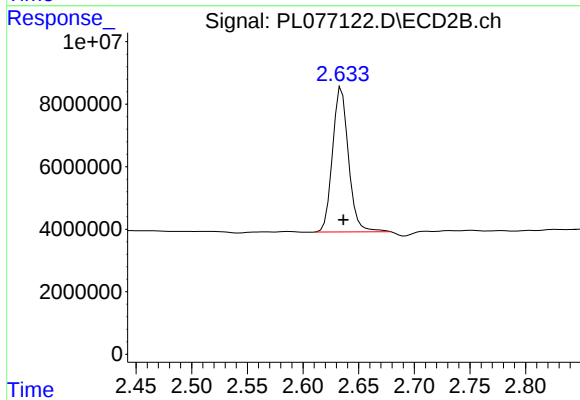


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.002 min
Response: 46291835
Conc: 16.17 ng/ml

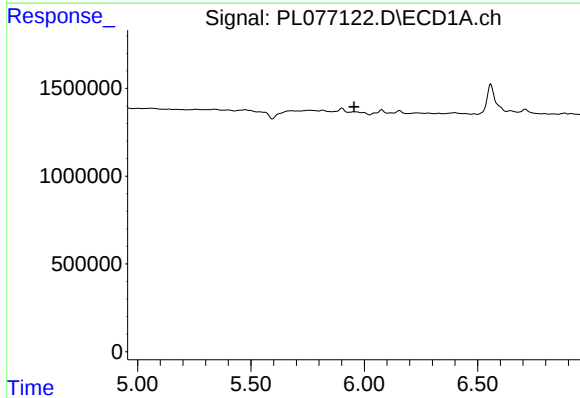


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

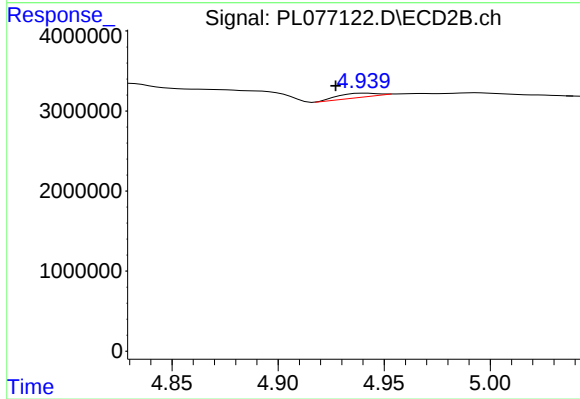

#9 Endosulfan I


R.T.: 4.941 min
Delta R.T.: 0.014 min
Response: 634868
Conc: 0.23 ng/ml

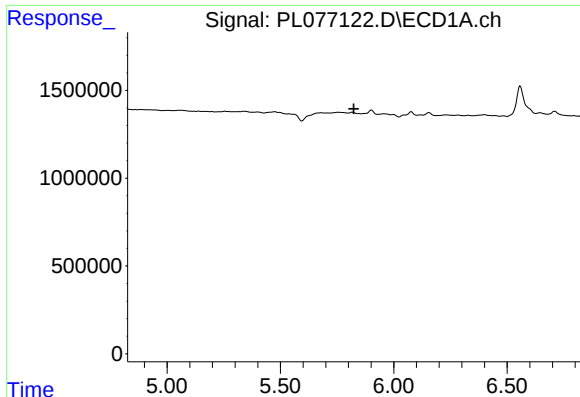

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

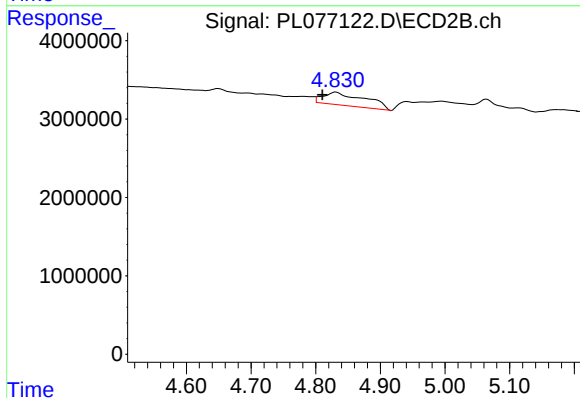


#10 gamma-Chlordane

R.T.: 4.831 min
Delta R.T.: 0.021 min
Response: 7530128
Conc: 2.47 ng/ml

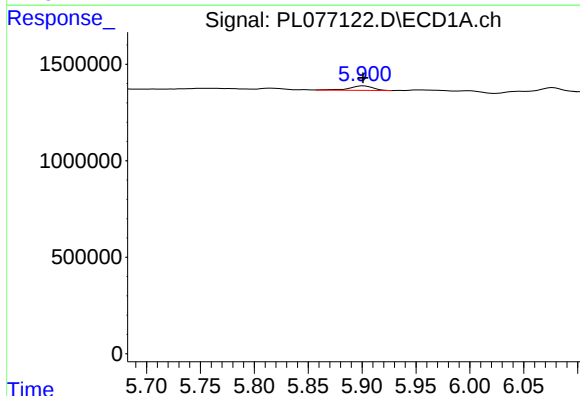


#11 alpha-Chlordane

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 362264
Conc: 0.36 ng/ml

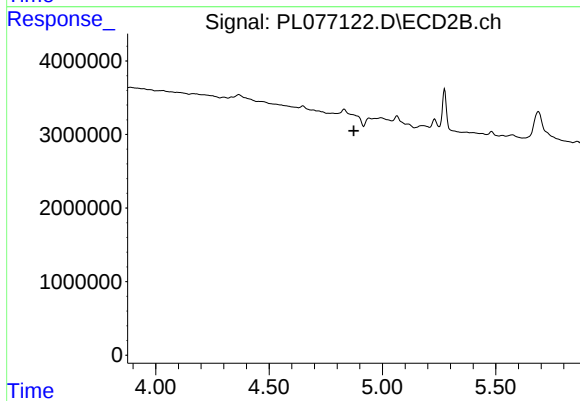

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.873 min
Response: 0
Conc: N.D.

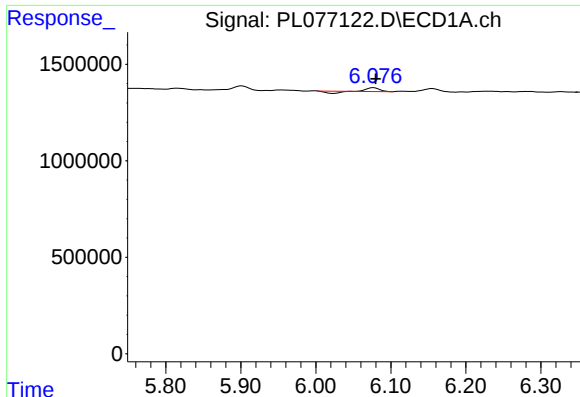

#12 4,4'-DDE


R.T.: 6.077 min
Delta R.T.: -0.003 min
Response: 102551
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

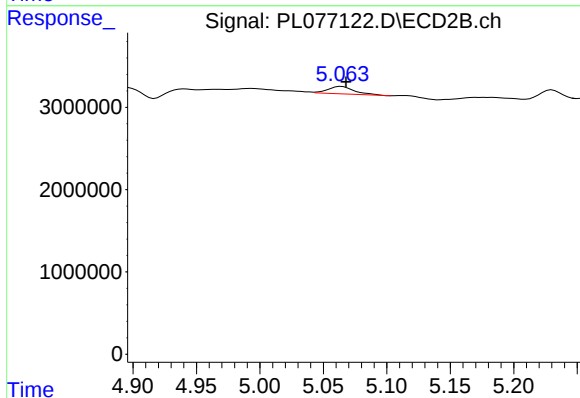


#12 4,4'-DDE

R.T.: 5.064 min
Delta R.T.: -0.004 min
Response: 1313391
Conc: 0.46 ng/ml

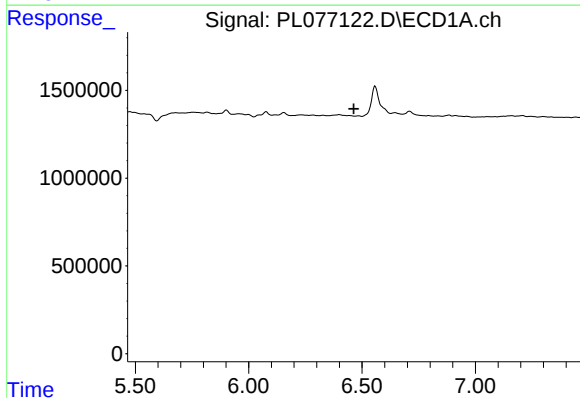


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

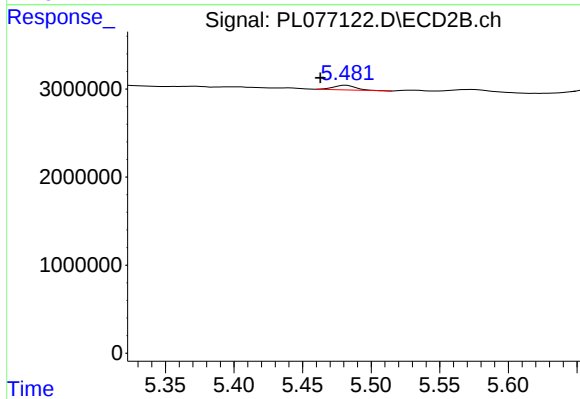

#14 Endrin


R.T.: 5.482 min
Delta R.T.: 0.019 min
Response: 579855
Conc: 0.23 ng/ml

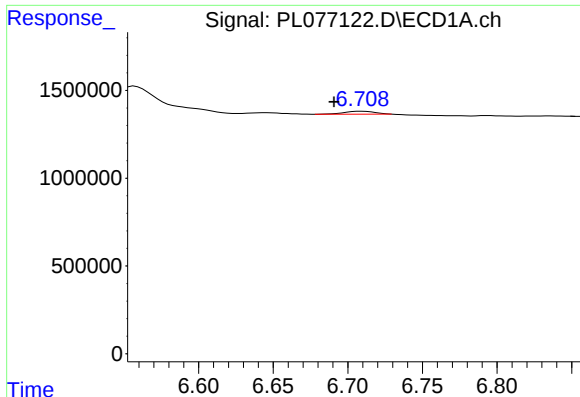

#15 Endosulfan II


R.T.: 6.709 min
Delta R.T.: 0.019 min
Response: 232906
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

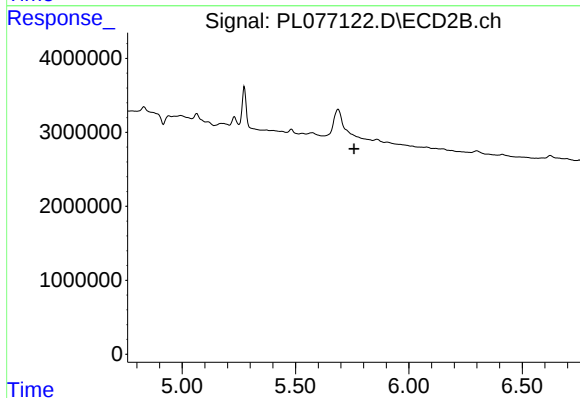


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.759 min
Response: 0
Conc: N.D.

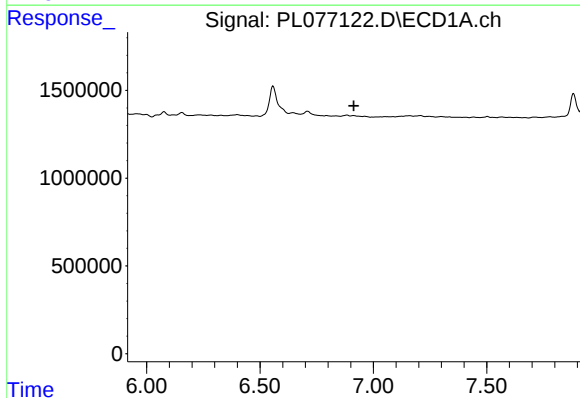


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

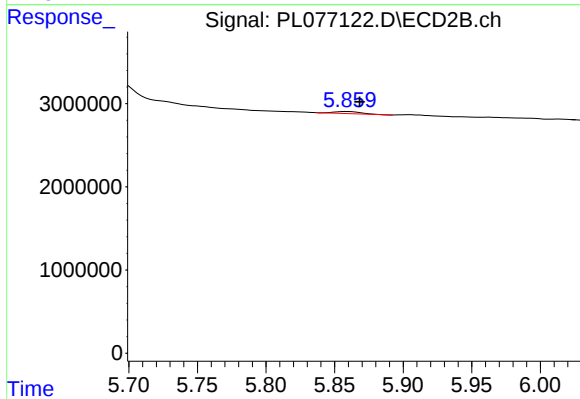

#17 4,4'-DDT


R.T.: 5.859 min
Delta R.T.: -0.010 min
Response: 337056
Conc: 0.15 ng/ml

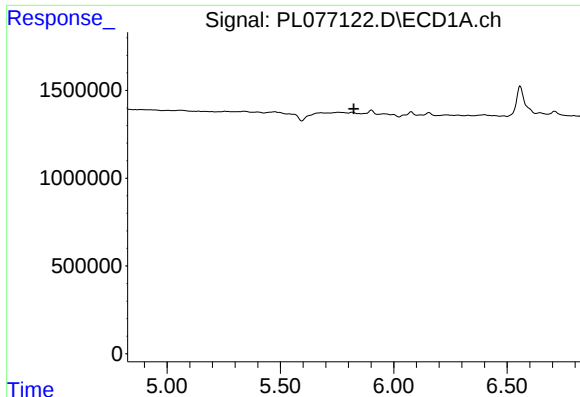

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

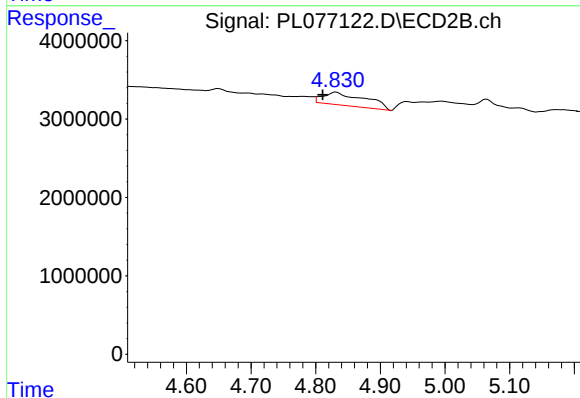


#25 Chlordane-3

R.T.: 4.831 min
Delta R.T.: 0.020 min
Response: 7530128
Conc: 23.78 ng/ml

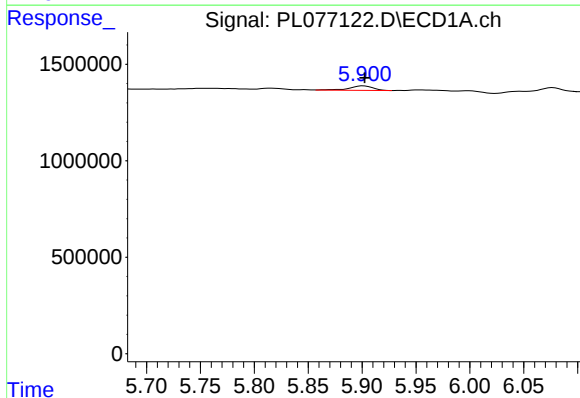


#26 Chlordane-4

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 362264
Conc: 2.05 ng/ml

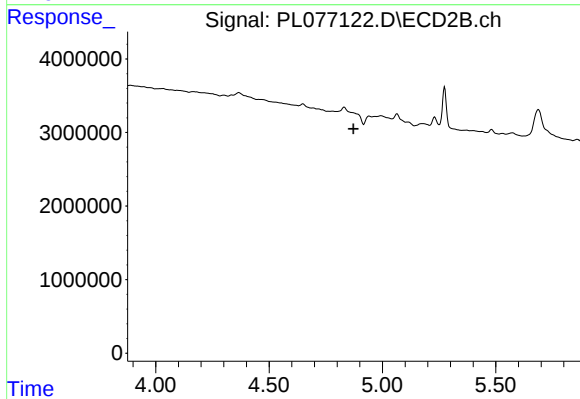

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 4.873 min
Response: 0
Conc: N.D.

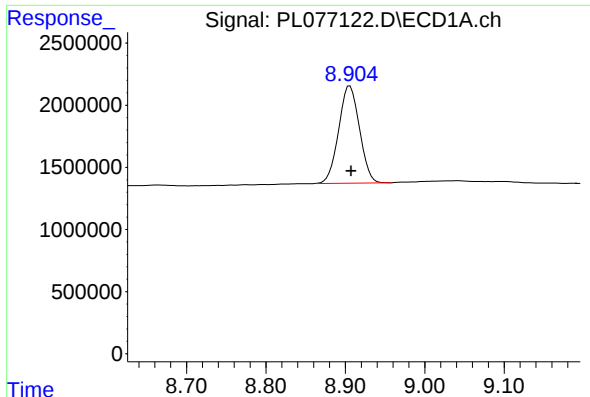

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.001 min
Response: 14278783
Conc: 18.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

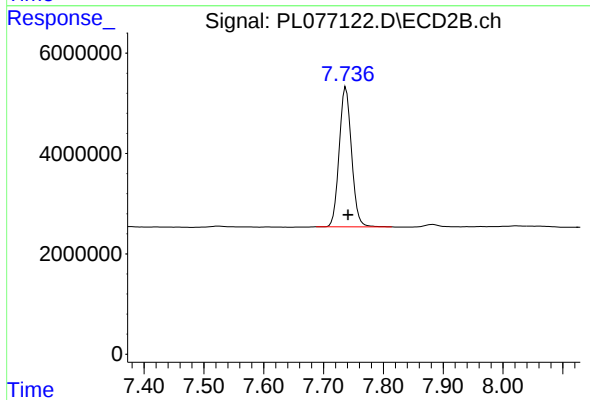

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 39976069
Conc: 17.76 ng/ml