

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
 Data File : PL077123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 20:03
 Operator : AR\AJ
 Sample : N4208-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:58:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.635	15793928	42682898	16.107	14.910
28)	SA Decachlor...	8.905	7.737	13643827	37397467	18.073	16.612
Target Compounds							
3)	MA gamma-BHC...	0.000	3.436f	0	113414	N.D.	0.030 #
10)	B gamma-Chl...	5.821	4.832f	729754	6986464	0.728	2.293 #
11)	B alpha-Chl...	5.901	4.870	3128418	4304239	3.134	1.445 #
13)	MA Dieldrin	0.000	5.172f	0	201462	N.D.	0.067 #
14)	MA Endrin	0.000	5.481f	0	231960	N.D.	0.091 #
15)	B Endosulfa...	6.708f	5.754	207645	1348428	0.242	0.515 #
25)	Chlordane-3	5.821	4.832f	729754	6986464	5.020	22.067 #
26)	Chlordane-4	5.901	4.870	3128418	4304239	17.720	13.068 #
27)	Chlordane-5	0.000	5.532	0	809234	N.D.	8.875 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
Data File : PL077123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 20:03
Operator : AR\AJ
Sample : N4208-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:58:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

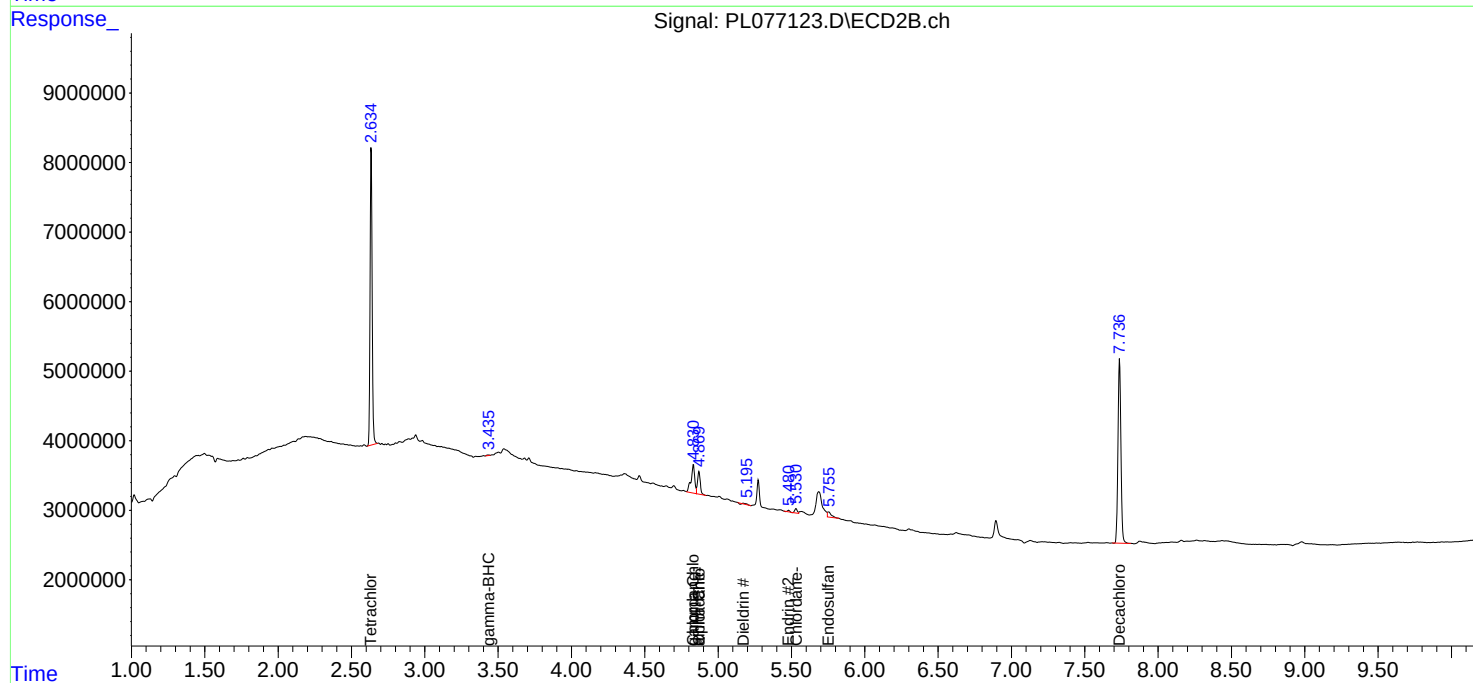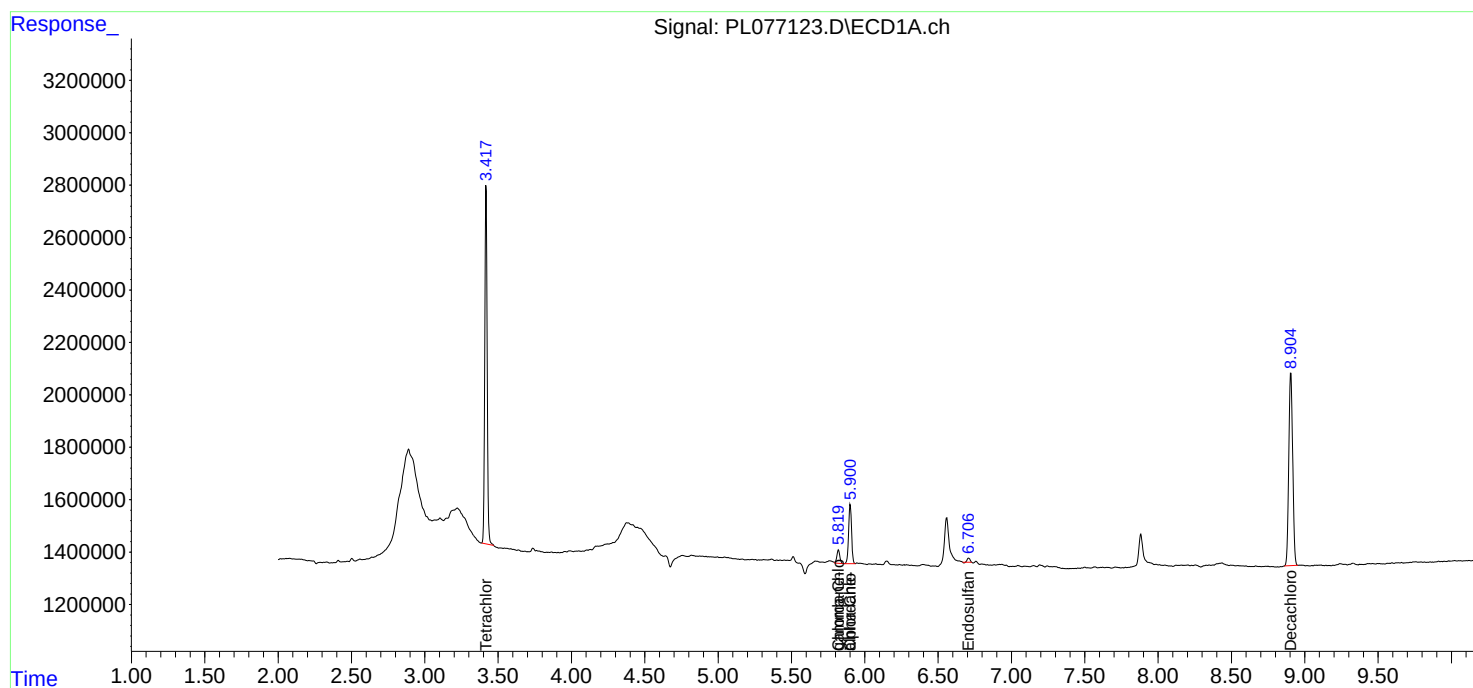


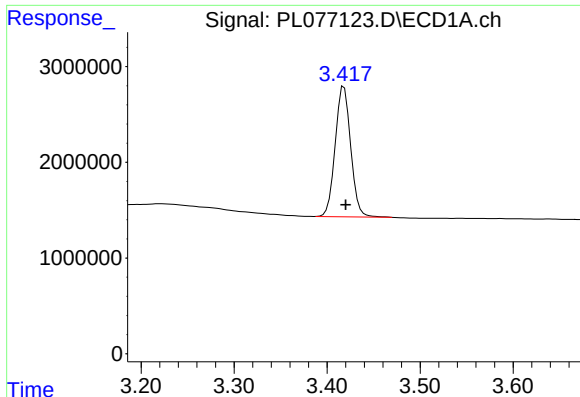

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: -0.002 min
Response: 15793928
Conc: 16.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

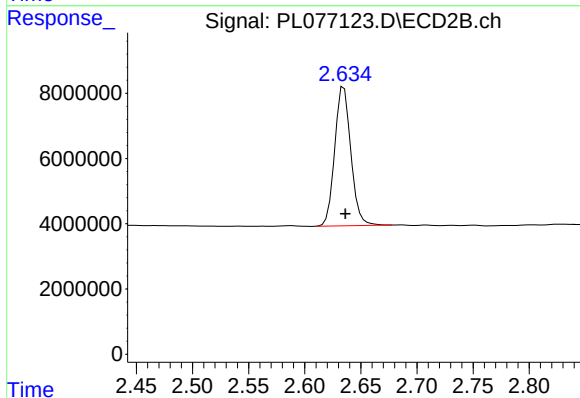


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.001 min
Response: 42682898
Conc: 14.91 ng/ml

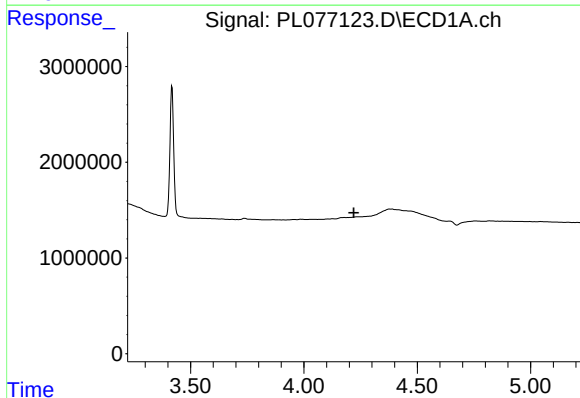


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.220 min
Response: 0
Conc: N.D.

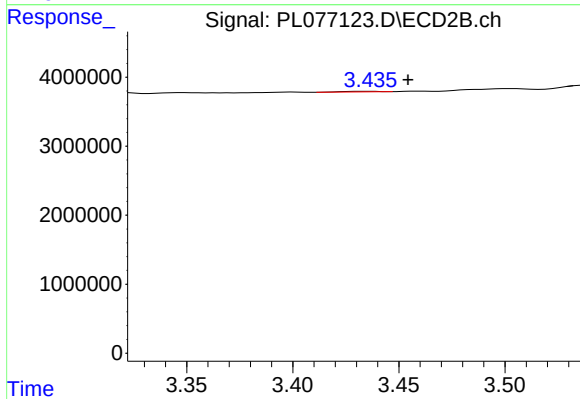

#3 gamma-BHC (Lindane)


R.T.: 3.436 min
Delta R.T.: -0.018 min
Response: 113414
Conc: 0.03 ng/ml

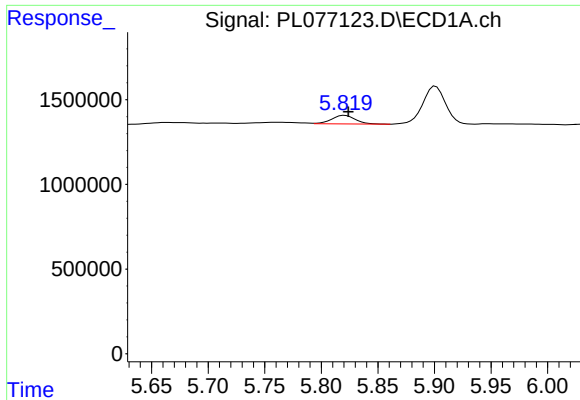

#10 gamma-Chlordane


R.T.: 5.821 min
Delta R.T.: -0.003 min
Response: 729754
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

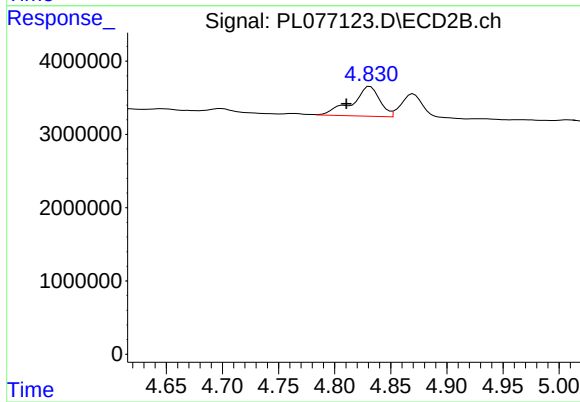


#10 gamma-Chlordane

R.T.: 4.832 min
Delta R.T.: 0.021 min
Response: 6986464
Conc: 2.29 ng/ml

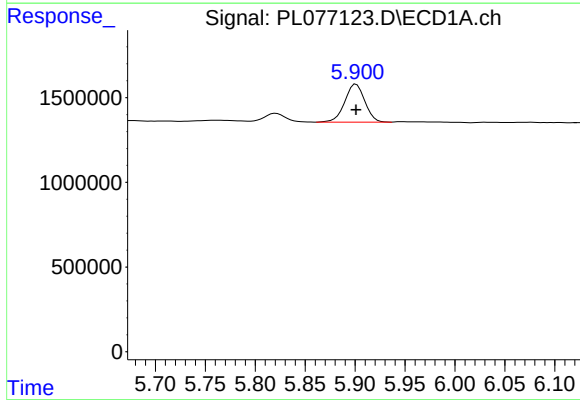


#11 alpha-Chlordane

R.T.: 5.901 min
Delta R.T.: 0.000 min
Response: 3128418
Conc: 3.13 ng/ml

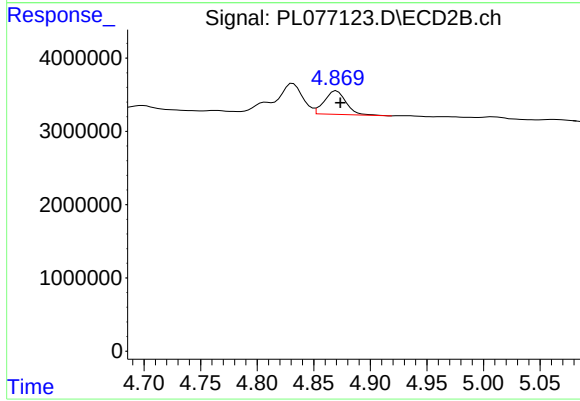

#11 alpha-Chlordane


R.T.: 4.870 min
Delta R.T.: -0.003 min
Response: 4304239
Conc: 1.45 ng/ml

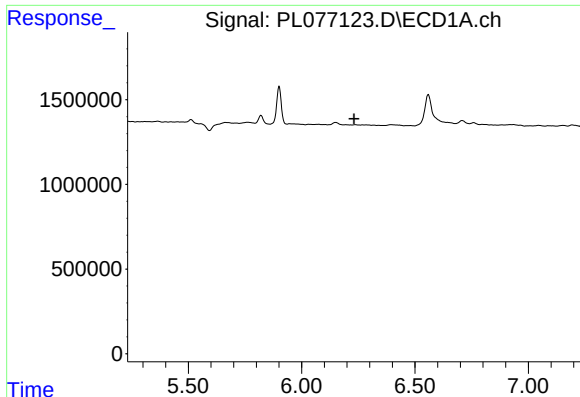

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.232 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

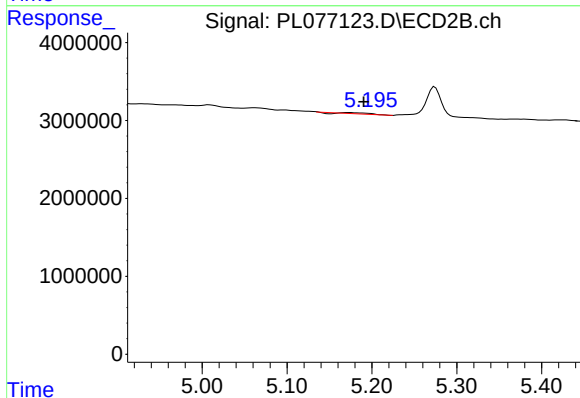


#13 Dieldrin

R.T.: 5.172 min
Delta R.T.: -0.018 min
Response: 201462
Conc: 0.07 ng/ml

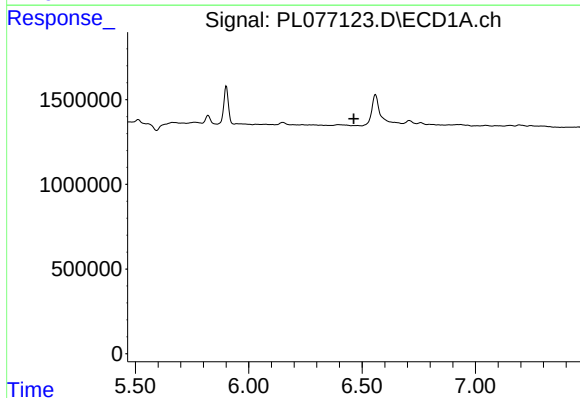


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

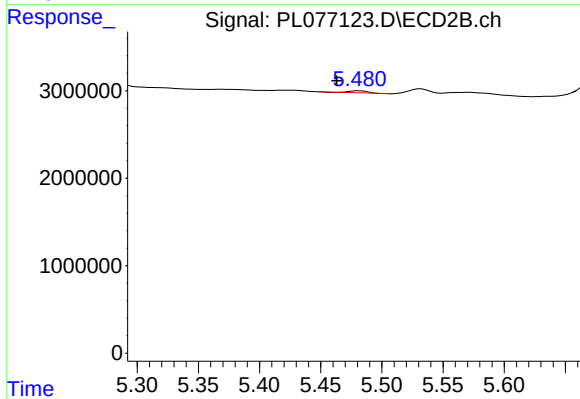

#14 Endrin


R.T.: 5.481 min
Delta R.T.: 0.018 min
Response: 231960
Conc: 0.09 ng/ml

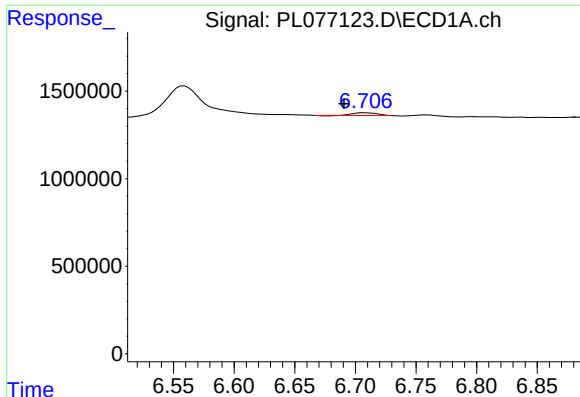

#15 Endosulfan II


R.T.: 6.708 min
Delta R.T.: 0.017 min
Response: 207645
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

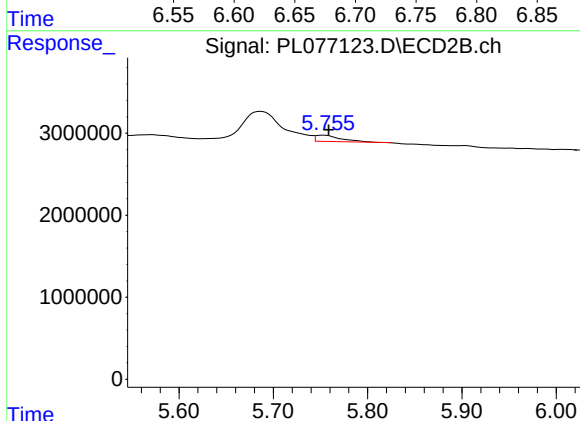


#15 Endosulfan II

R.T.: 5.754 min
Delta R.T.: -0.004 min
Response: 1348428
Conc: 0.51 ng/ml

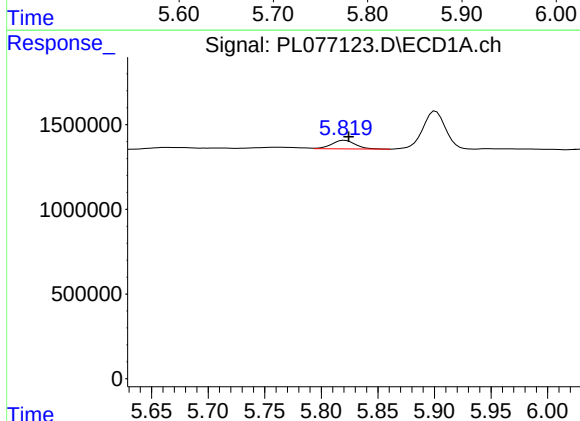


#25 Chlordane-3

R.T.: 5.821 min
Delta R.T.: -0.003 min
Response: 729754
Conc: 5.02 ng/ml

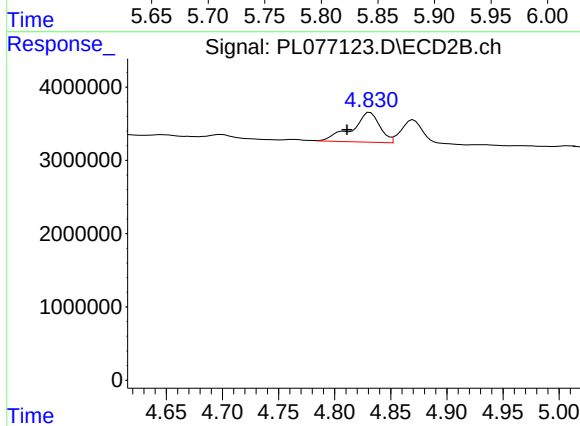

#25 Chlordane-3


R.T.: 4.832 min
Delta R.T.: 0.021 min
Response: 6986464
Conc: 22.07 ng/ml

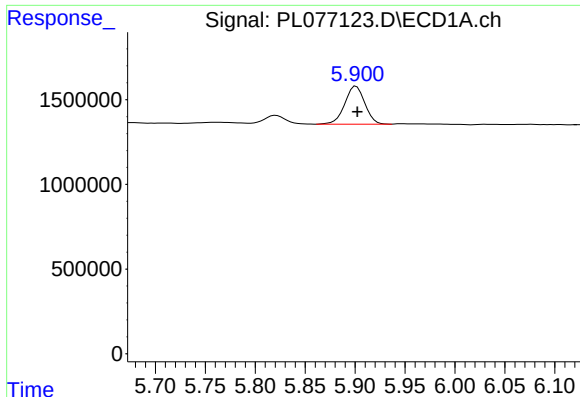

#26 Chlordane-4


R.T.: 5.901 min
Delta R.T.: -0.001 min
Response: 3128418
Conc: 17.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

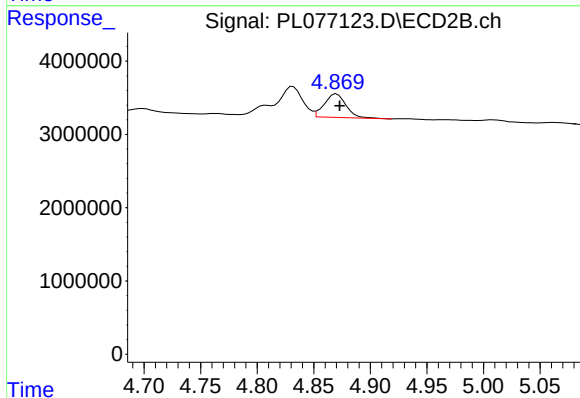


#26 Chlordane-4

R.T.: 4.870 min
Delta R.T.: -0.003 min
Response: 4304239
Conc: 13.07 ng/ml

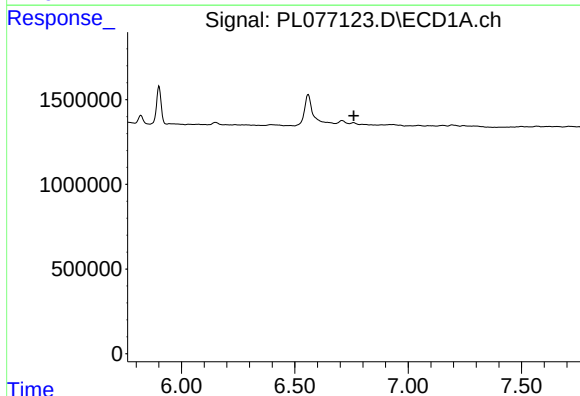


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.760 min
Response: 0
Conc: N.D.

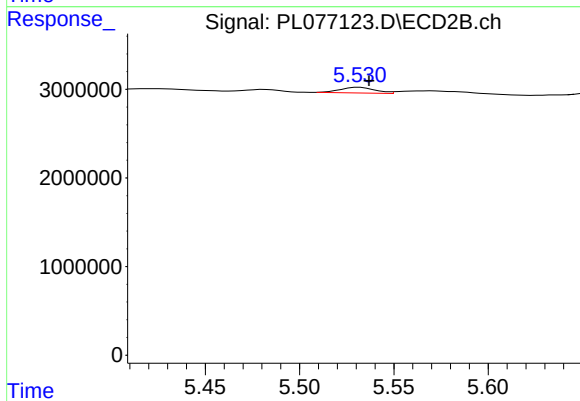

#27 Chlordane-5


R.T.: 5.532 min
Delta R.T.: -0.005 min
Response: 809234
Conc: 8.87 ng/ml

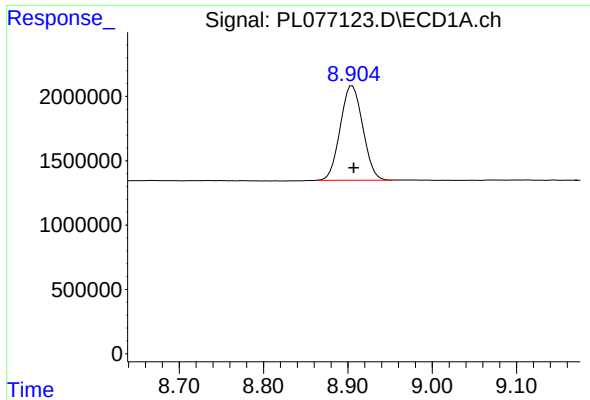

#28 Decachlorobiphenyl

R.T.: 8.905 min
Delta R.T.: -0.002 min
Response: 13643827
Conc: 18.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

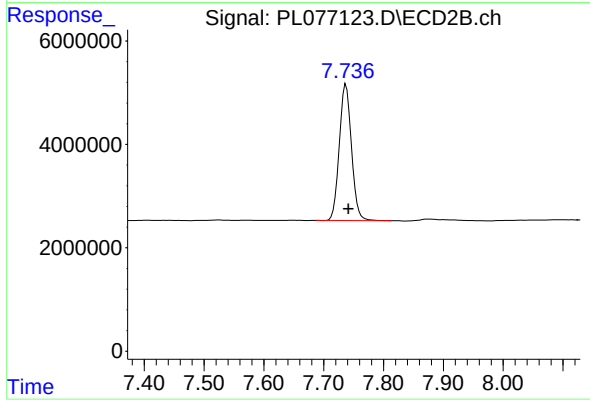

#28 Decachlorobiphenyl

R.T.: 7.737 min
Delta R.T.: -0.004 min
Response: 37397467
Conc: 16.61 ng/ml