

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
 Data File : PL077134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 22:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 07:01:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.635	17305211	46337853	17.648	16.187
28)	SA Decachlor...	8.906	7.738	15607646	40795298	20.674	18.121
Target Compounds							
2)	A alpha-BHC	0.000	3.115	0	252215	N.D.	0.059 #
5)	MB Aldrin	0.000	4.076	0	225184	N.D.	0.064 #
7)	B delta-BHC	0.000	3.988	0	391940	N.D.	0.103 #
8)	B Heptachlo...	5.569	0.000	643272	0	0.637	N.D. #
13)	MA Dieldrin	0.000	5.174f	0	555029	N.D.	0.185 #
14)	MA Endrin	0.000	5.483f	0	375781	N.D.	0.148 #
15)	B Endosulfa...	6.709f	0.000	225191	0	0.263	N.D. #
24)	Chlordane-2	0.000	4.171f	0	981392	N.D.	8.533 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
Data File : PL077134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 22:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 07:01:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

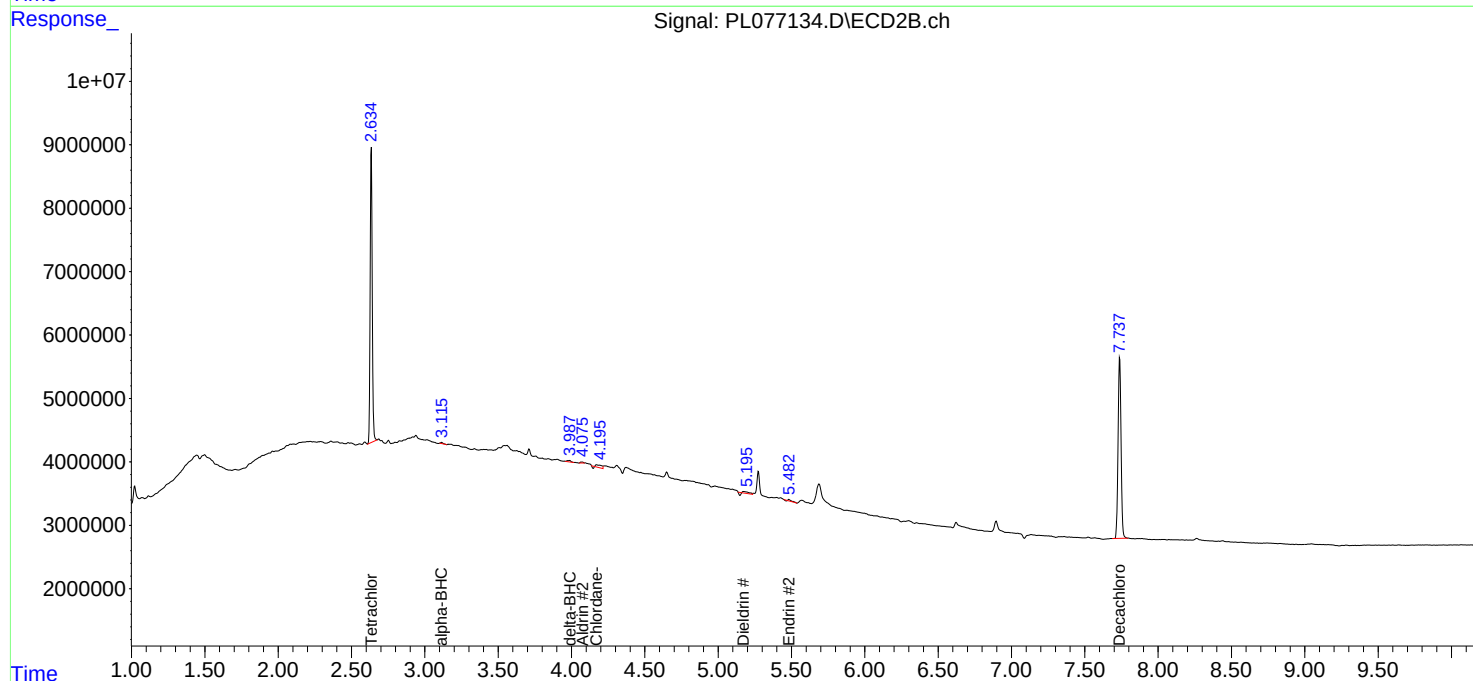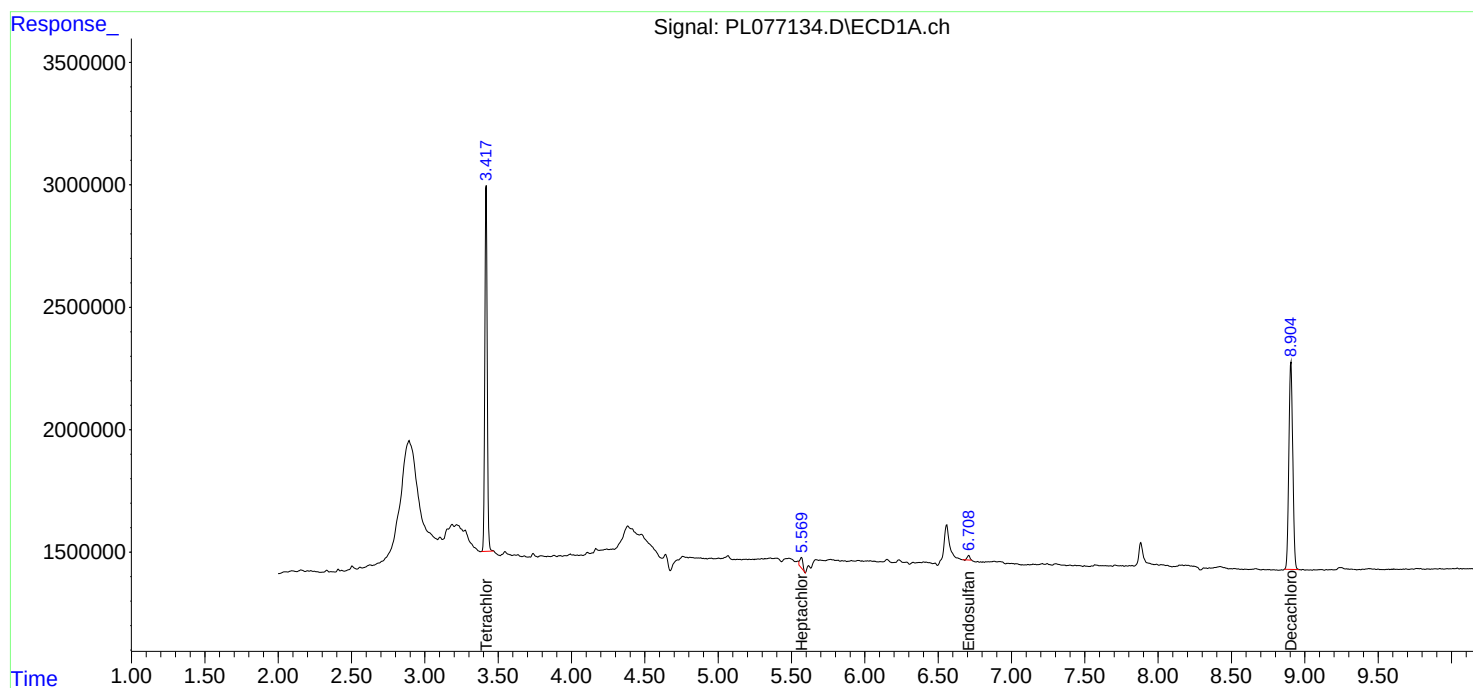


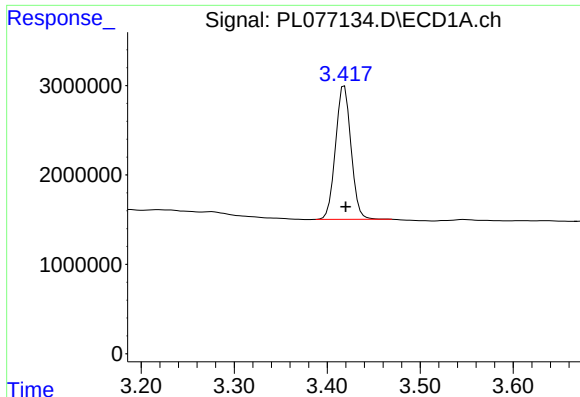

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 17305211
Conc: 17.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

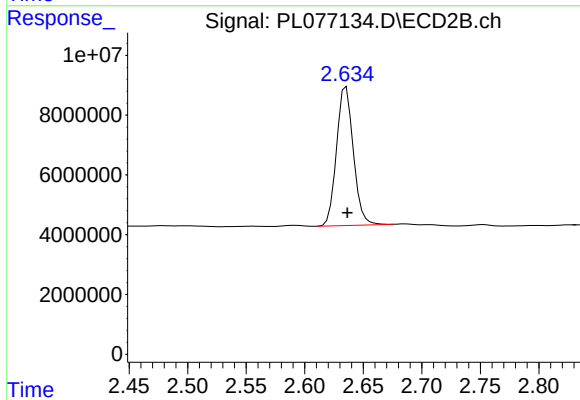


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.001 min
Response: 46337853
Conc: 16.19 ng/ml

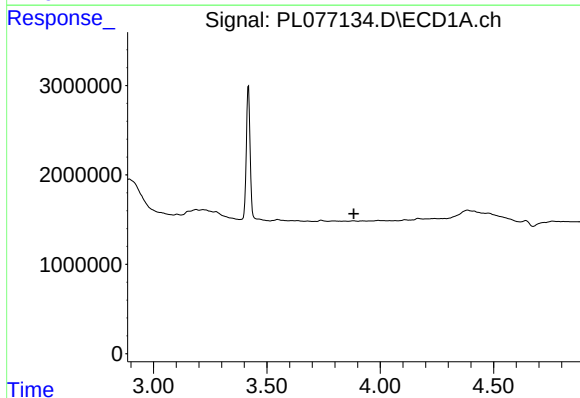


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.884 min
Response: 0
Conc: N.D.

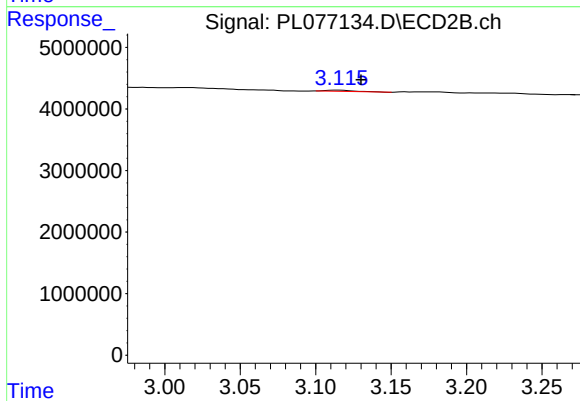

#2 alpha-BHC


R.T.: 3.115 min
Delta R.T.: -0.015 min
Response: 252215
Conc: 0.06 ng/ml

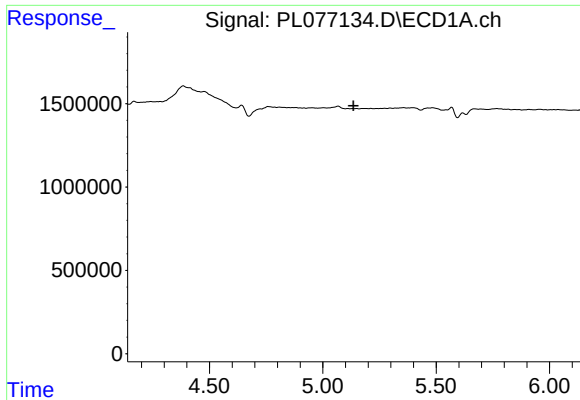

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.136 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

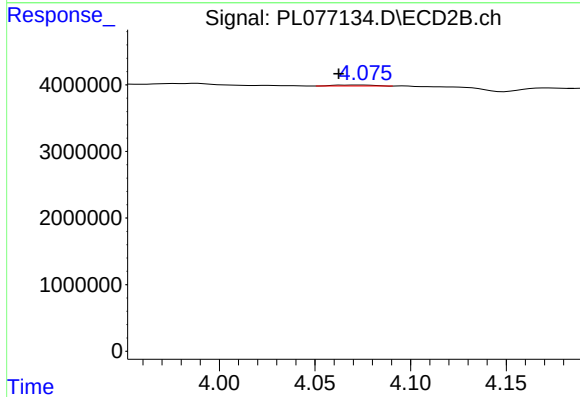


#5 Aldrin

R.T.: 4.076 min
Delta R.T.: 0.014 min
Response: 225184
Conc: 0.06 ng/ml

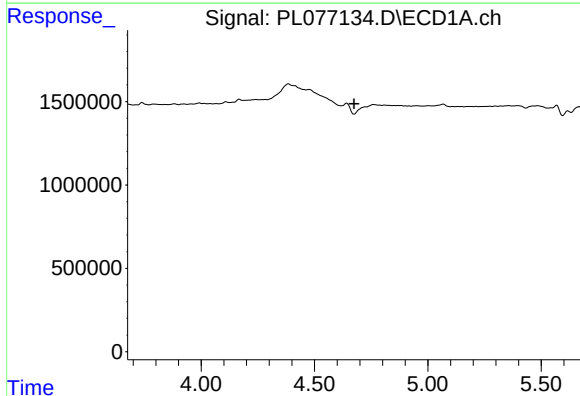


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.674 min
Response: 0
Conc: N.D.

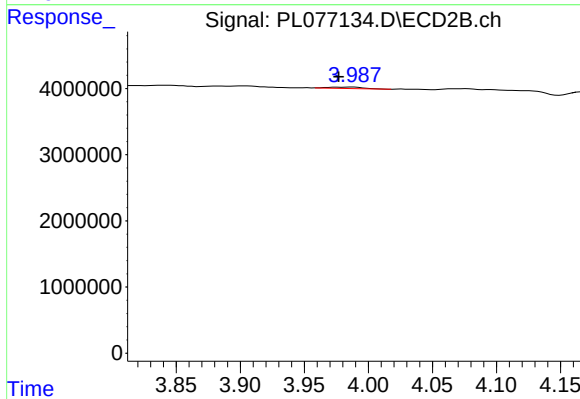

#7 delta-BHC


R.T.: 3.988 min
Delta R.T.: 0.011 min
Response: 391940
Conc: 0.10 ng/ml

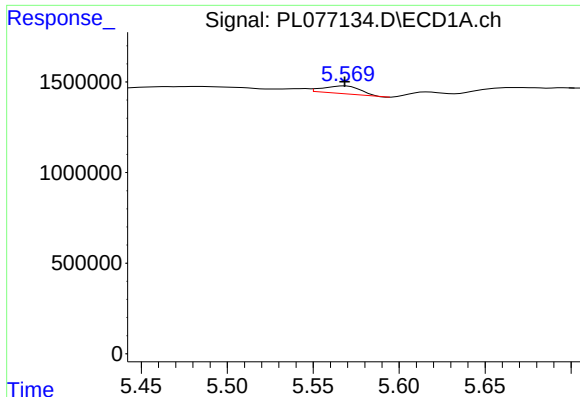

#8 Heptachlor epoxide


R.T.: 5.569 min
Delta R.T.: 0.000 min
Response: 643272
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

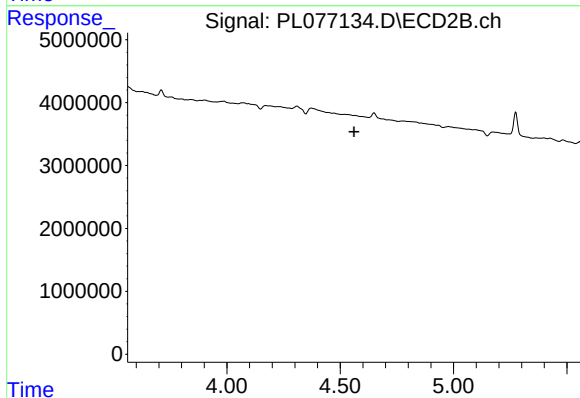


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.561 min
Response: 0
Conc: N.D.

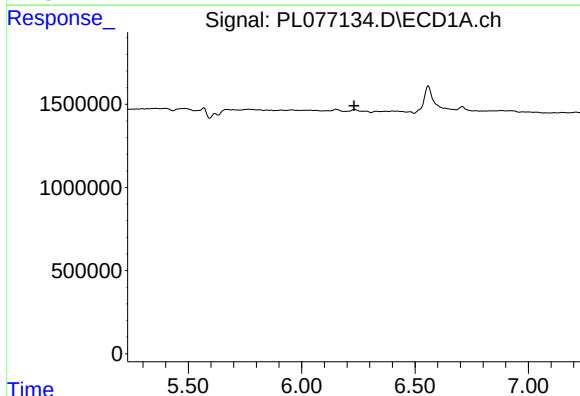


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

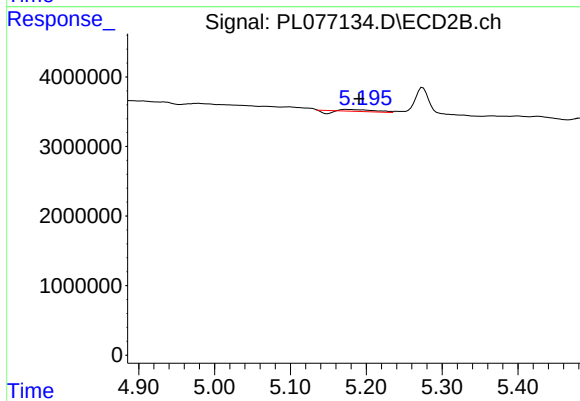

#13 Dieldrin


R.T.: 5.174 min
Delta R.T.: -0.016 min
Response: 555029
Conc: 0.19 ng/ml

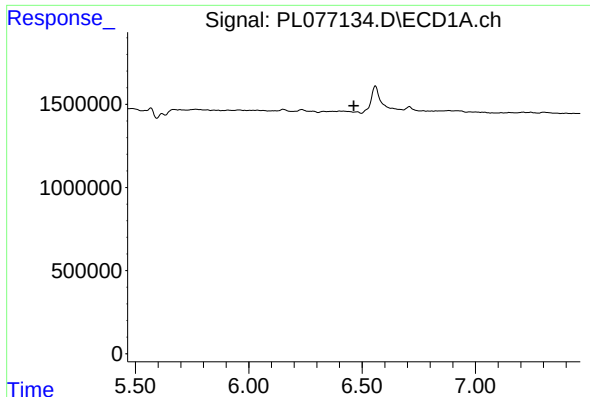

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

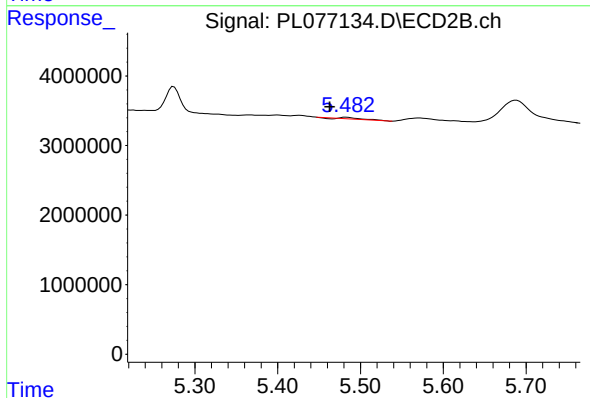


#14 Endrin

R.T.: 5.483 min
Delta R.T.: 0.020 min
Response: 375781
Conc: 0.15 ng/ml

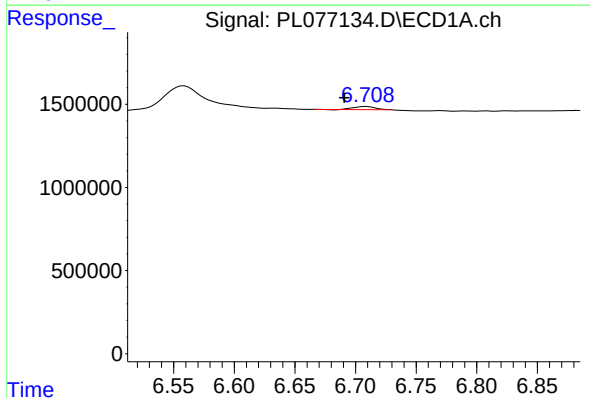


#15 Endosulfan II

R.T.: 6.709 min
Delta R.T.: 0.019 min
Response: 225191
Conc: 0.26 ng/ml

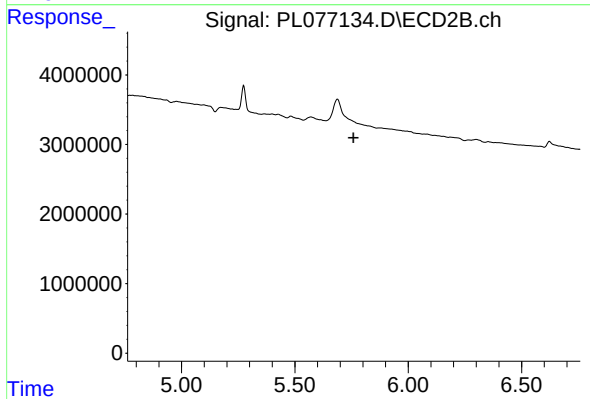

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.759 min
Response: 0
Conc: N.D.

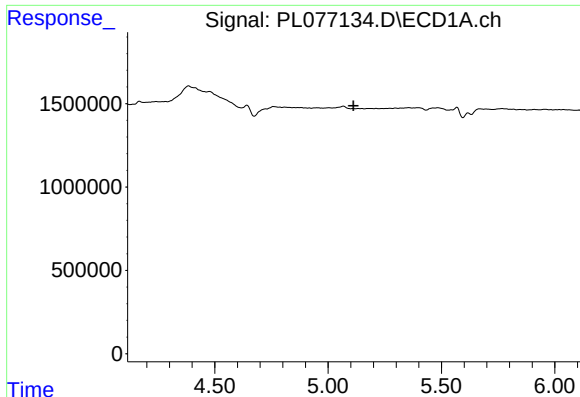

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

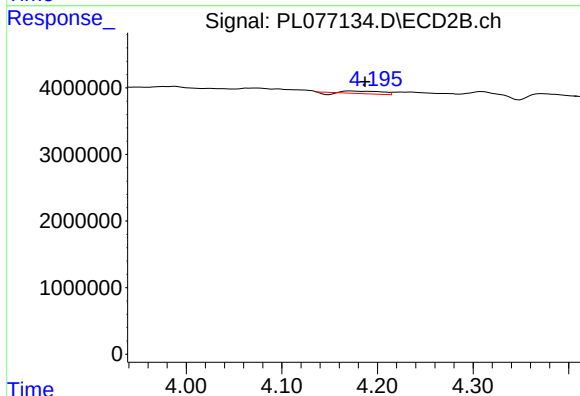


#24 Chlordane-2

R.T.: 4.171 min
Delta R.T.: -0.016 min
Response: 981392
Conc: 8.53 ng/ml

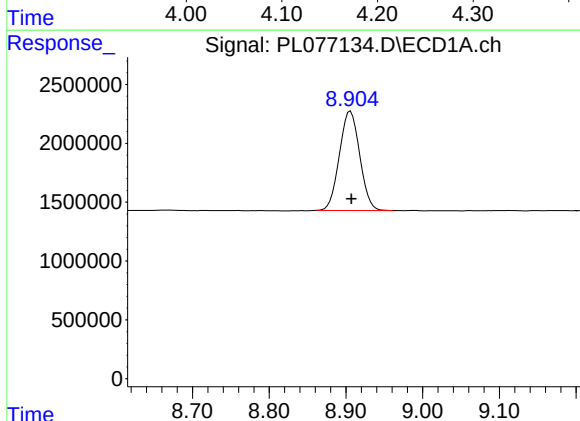

#28 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.001 min
Response: 15607646
Conc: 20.67 ng/ml

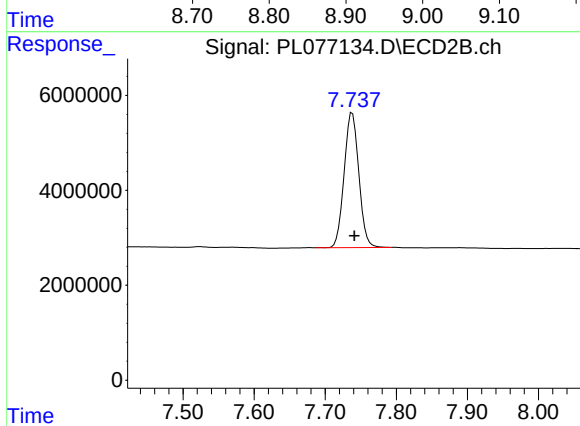

#28 Decachlorobiphenyl

R.T.: 7.738 min
Delta R.T.: -0.003 min
Response: 40795298
Conc: 18.12 ng/ml