

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
 Data File : PL077092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2022 12:10
 Operator : AR\AJ
 Sample : N4140-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 06:52:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	7119805	20144061	7.261	7.037
28)	SA Decachlor...	8.907	7.739	6773135	18237698	8.972	8.101
Target Compounds							
12)	B 4,4'-DDE	6.079	5.066	23057206	64220866	26.425	22.258
16)	A 4,4'-DDD	6.602	5.618	3949093	8526036	5.184	3.784 #
17)	MA 4,4'-DDT	6.914	5.865	1793009	5109422	2.333	2.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081522\
Data File : PL077092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2022 12:10
Operator : AR\AJ
Sample : N4140-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 06:52:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

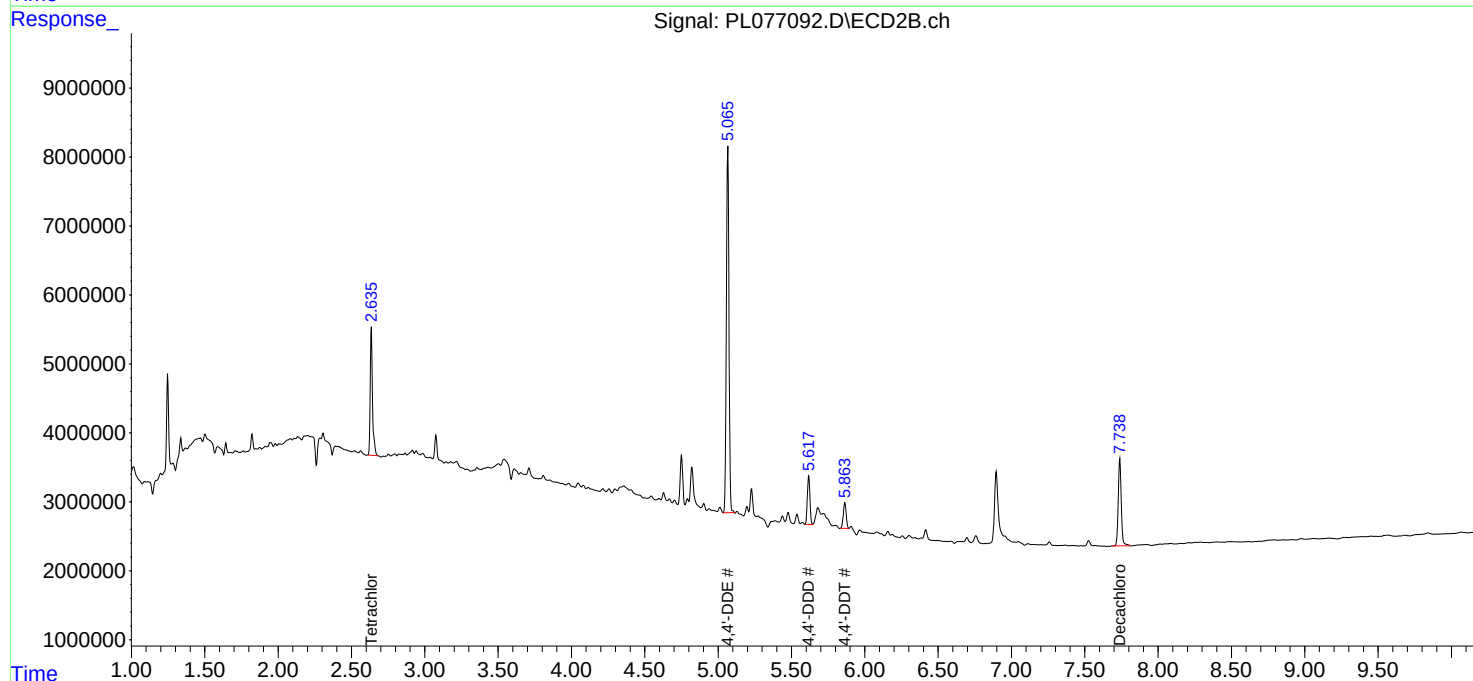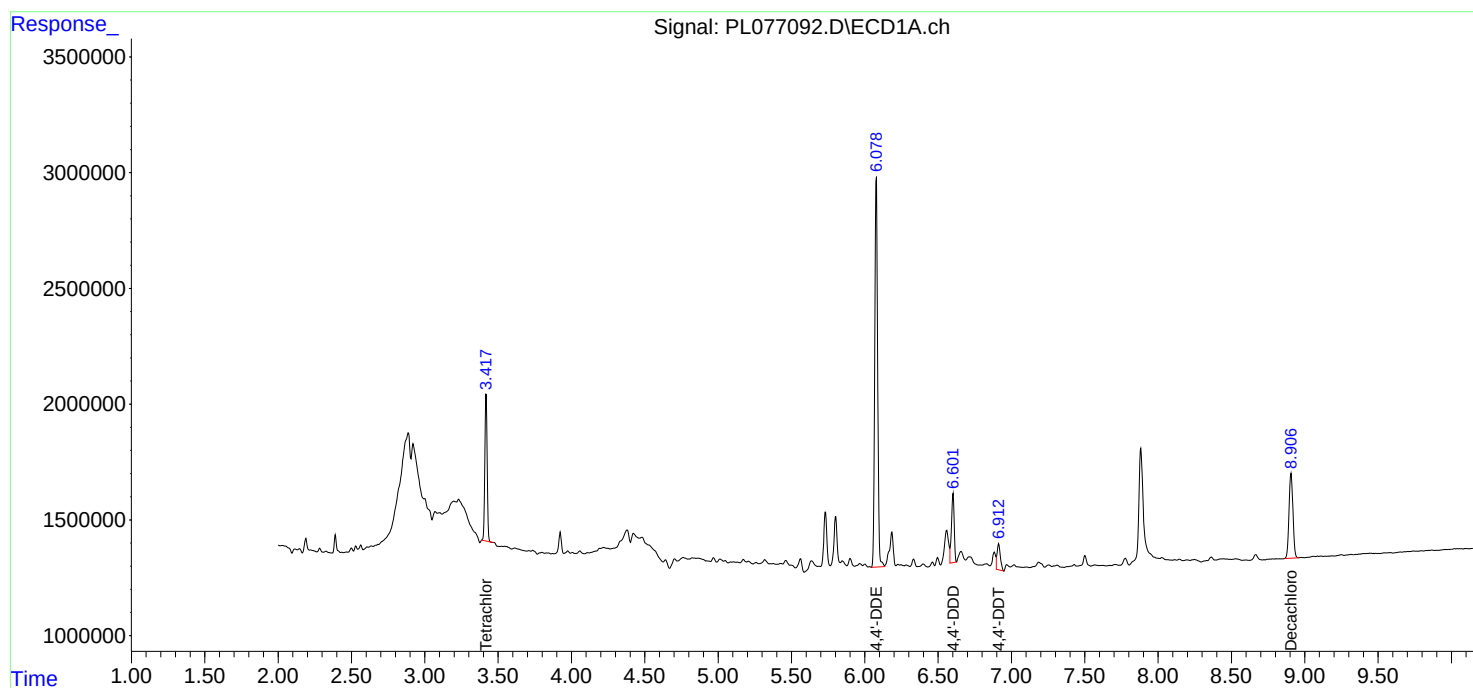


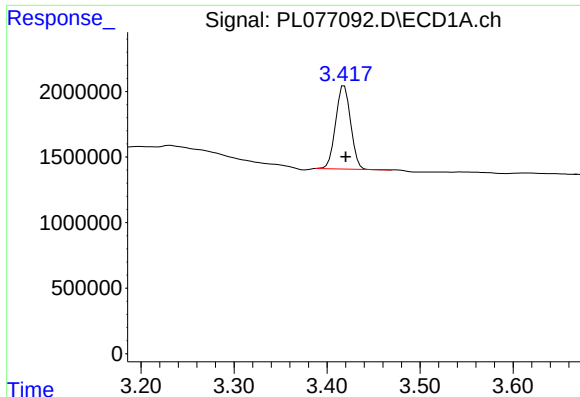

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 7119805
Conc: 7.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

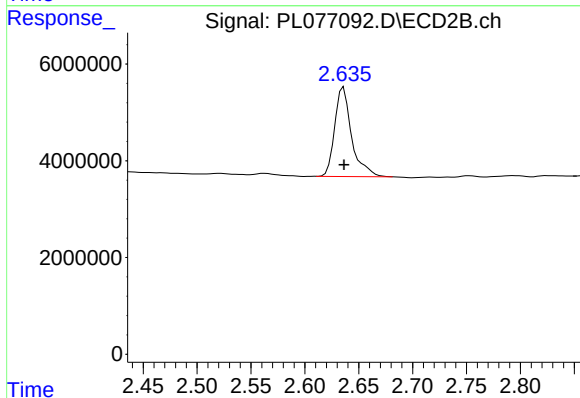


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 20144061
Conc: 7.04 ng/ml

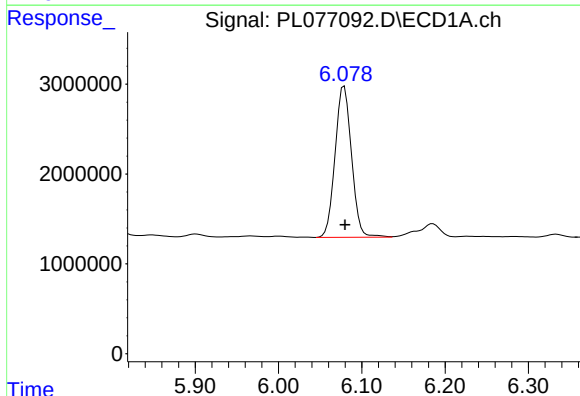


#12 4,4'-DDE

R.T.: 6.079 min
Delta R.T.: -0.001 min
Response: 23057206
Conc: 26.42 ng/ml

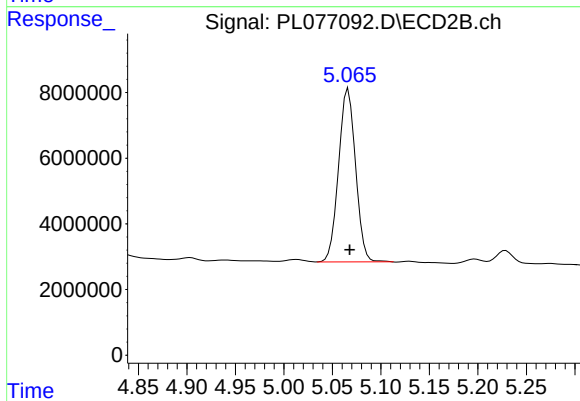

#12 4,4'-DDE


R.T.: 5.066 min
Delta R.T.: -0.001 min
Response: 64220866
Conc: 22.26 ng/ml

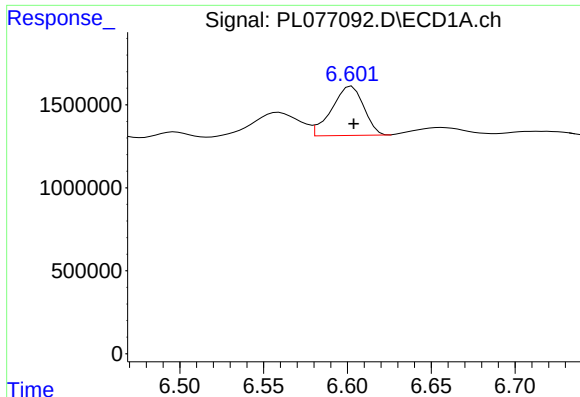

#16 4,4'-DDD


R.T.: 6.602 min
Delta R.T.: -0.001 min
Response: 3949093
Conc: 5.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

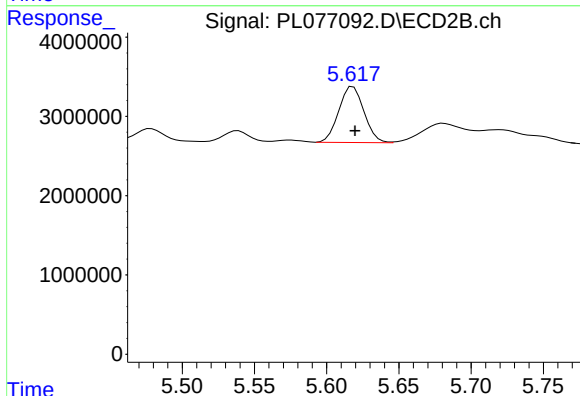


#16 4,4'-DDD

R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 8526036
Conc: 3.78 ng/ml

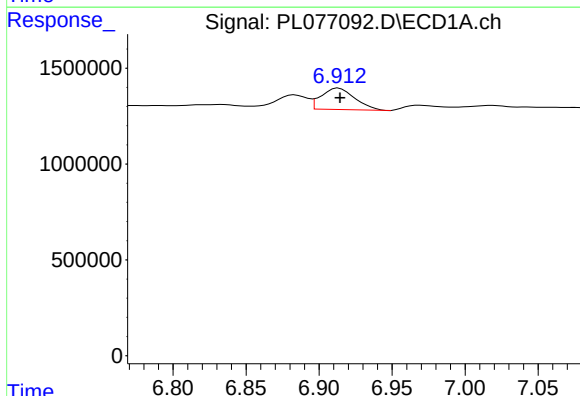


#17 4,4'-DDT

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 1793009
Conc: 2.33 ng/ml

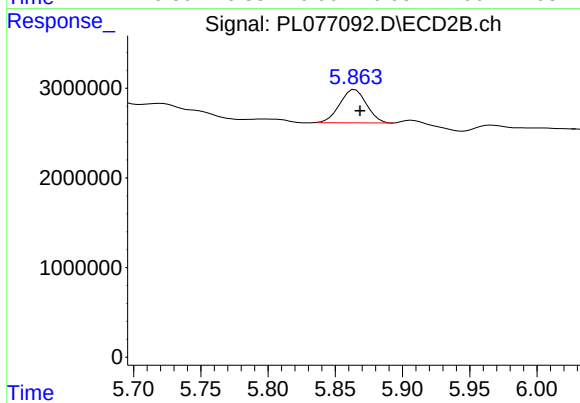

#17 4,4'-DDT


R.T.: 5.865 min
Delta R.T.: -0.004 min
Response: 5109422
Conc: 2.25 ng/ml

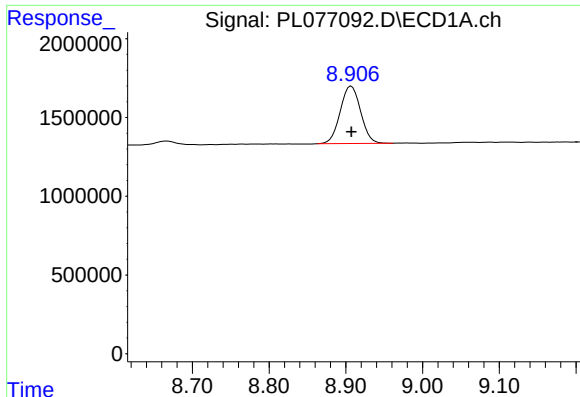

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 6773135
Conc: 8.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

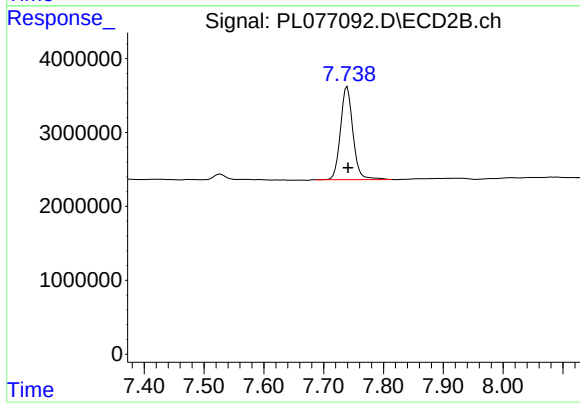

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: -0.002 min
Response: 18237698
Conc: 8.10 ng/ml