

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
 Data File : PL084737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2023 00:10
 Operator : AR\AJ
 Sample : TOXAPH301
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 04:05:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 04:04:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.686	58989955	28546261	20.000	20.000
27)	SA Decachlor...	9.028	7.867	78229039	69152604	40.000	40.000
Target Compounds							
22)	Toxaphene-1	6.192	5.254	40969827	15038111	2000.000	2000.000
23)	Toxaphene-2	7.016	5.615	129.7E6	17730548	2000.000	2000.000
24)	Toxaphene-3	7.106	6.660	92962684	96717940	2000.000	2000.000
25)	Toxaphene-4	7.204	6.976	53083932	63652994	2000.000	2000.000
26)	Toxaphene-5	7.892	7.110	65258830	38086562	2000.000	2000.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
Data File : PL084737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2023 00:10
Operator : AR\AJ
Sample : TOXAPH301
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 04:05:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 04:04:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

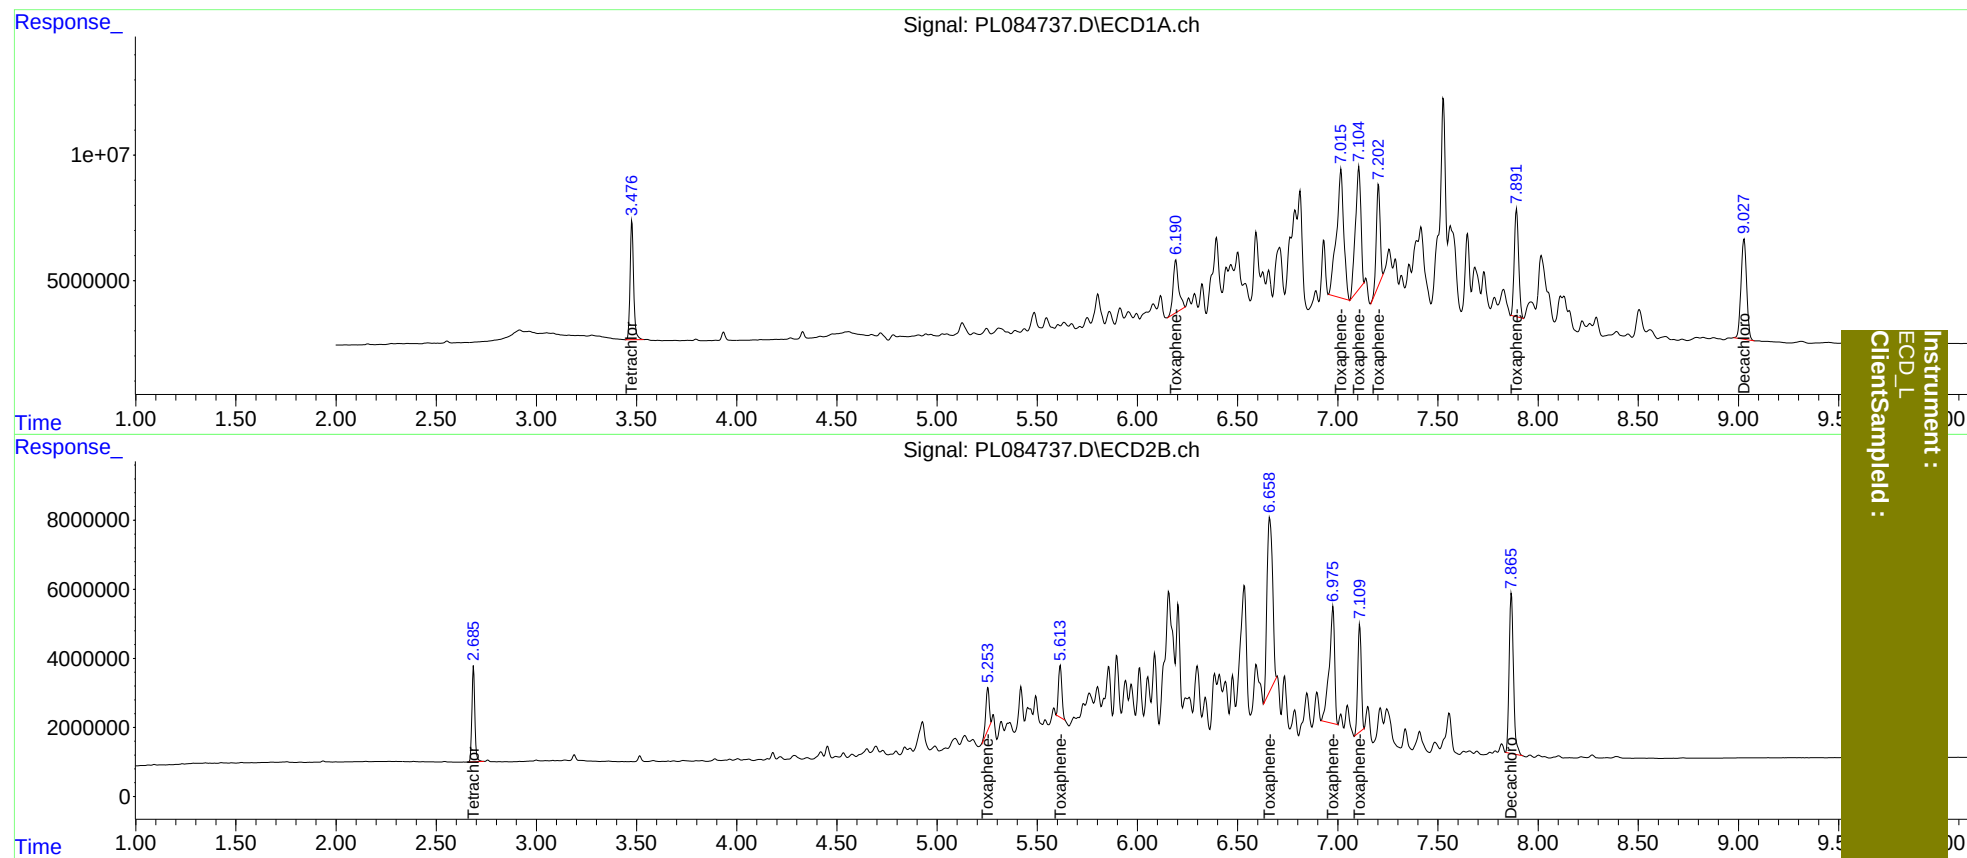

Instrument :
ECD_L
ClientSampled :
PL081523CLP.M Tue Aug 15 04:05:14 2023