

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
 Data File : PL084733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 23:14
 Operator : AR\AJ
 Sample : RESC353
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESC212

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 05:54:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 05:52:51 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.477	2.686	51348523	24551875	20.483	20.798
27)	SA Decachlor...	9.027	7.865	69411772	54744883	40.503	40.420
Target Compounds							
2)	A alpha-BHC	3.935	3.190	35299194	16509254	9.763	9.733
3)	MA gamma-BHC...	4.269	3.520	34330796	16026319	9.915	9.883
4)	MA Heptachlor	4.861	3.861	39301015	16453426	10.149	10.155
5)	MB Aldrin	5.203	4.141	36796298	15805925	10.184	10.077
6)	B beta-BHC	4.468	3.822	18176644	8312883	10.292	10.119
7)	B delta-BHC	4.715	4.050	35114800	16510258	9.623	9.518
8)	B Heptachlo...	5.633	4.647	34283441	15064046	10.270	9.961
9)	A Endosulfan I	6.019	5.017	29861650	13473792	10.479	9.993
10)	B trans-Chl...	5.891	4.900	31581789	14934399	10.013	9.912
11)	B cis-Chlor...	5.971	4.964	32005432	15070858	10.043	9.742
12)	B 4,4'-DDE	6.149	5.162	51381512	28128264	19.421	19.197
13)	MA Dieldrin	6.296	5.285	57461113	30900969	20.093	19.936
14)	MA Endrin	6.526	5.560	46099315	27971569	20.235	20.317
15)	B Endosulfa...	6.746	5.858	46775569	27410418	19.890	19.735
16)	A 4,4'-DDD	6.668	5.720	37865075	23695219	20.015	19.819
17)	MA 4,4'-DDT	6.984	5.973	40267724	25954703	20.889	20.025
18)	B Endrin al...	6.877	6.040	38132422	23387448	20.498	20.570
19)	B Endosulfa...	7.113	6.264	44876955	27311975	20.288	19.989
20)	A Methoxychlor	7.466	6.557	101.7E6	76068251	104.811	107.490
21)	B Endrin ke...	7.597	6.769	44447922	32820965	20.249	20.345

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
Data File : PL084733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 23:14
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 05:54:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

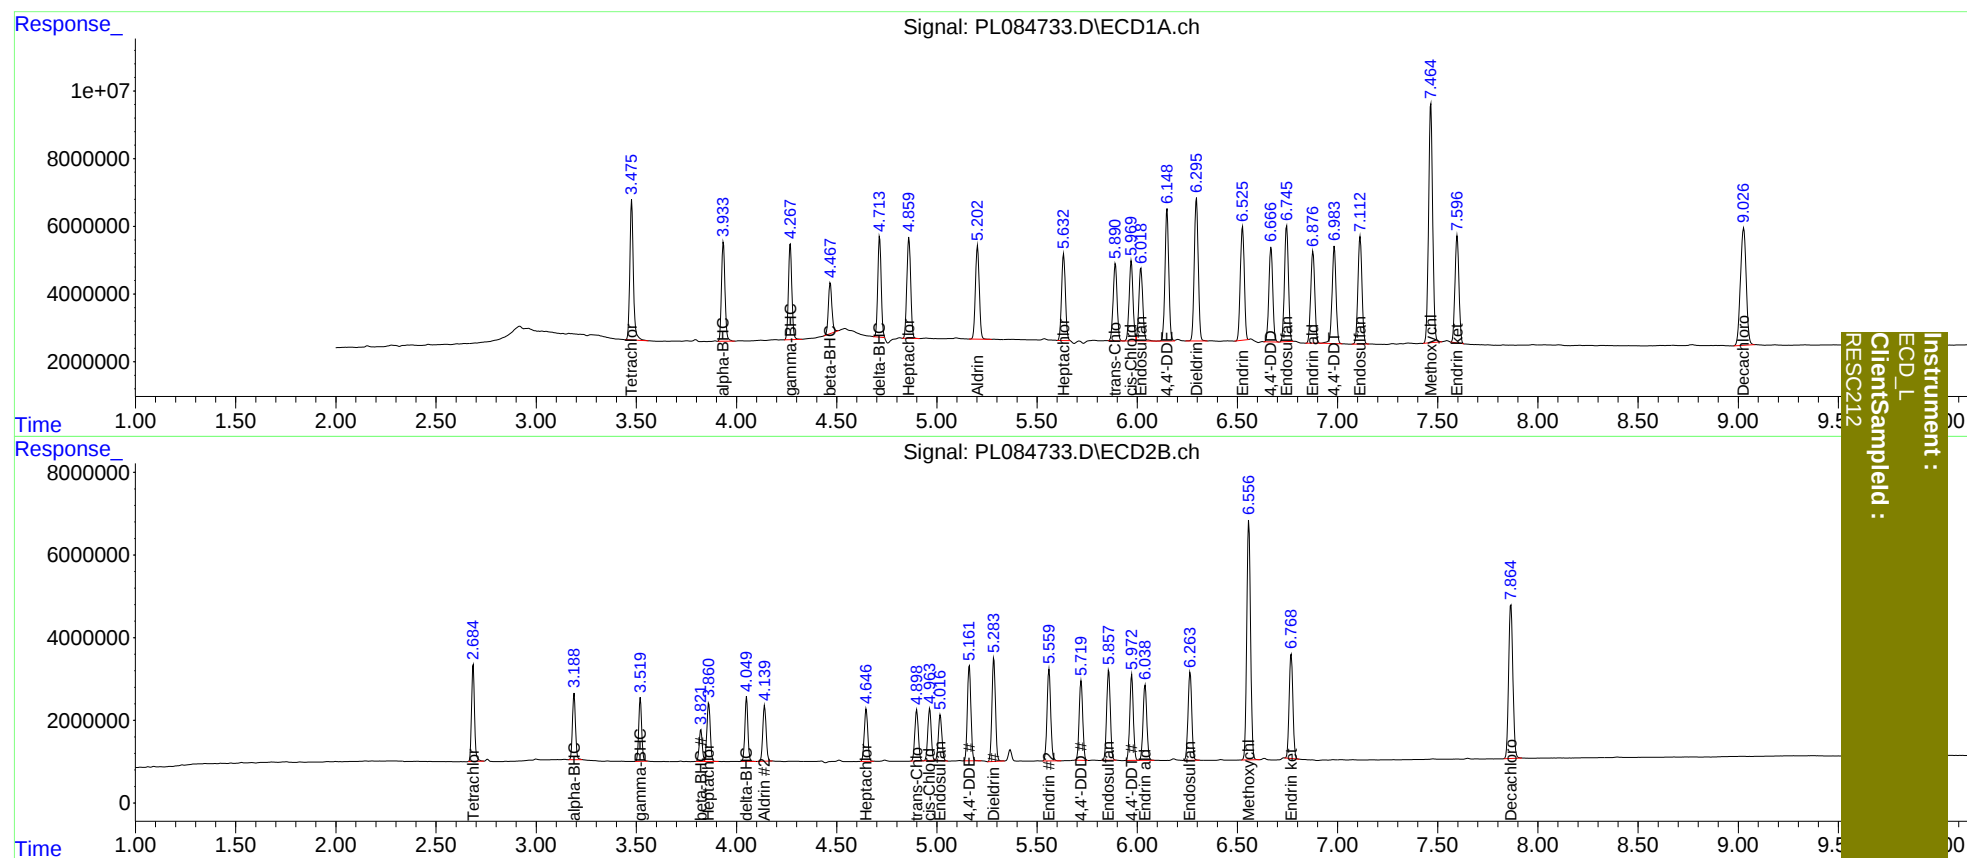

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
Data File : PL084733.D
Acq On : 14 Aug 2023 23:14
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC212

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Title : GC Extractables
Last Update : Tue Aug 15 05:52:51 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.477	3.935	100.00%
3.935	4.269	100.00%
4.269	4.468	100.00%
4.468	4.715	100.00%
4.715	4.861	100.00%
4.861	5.203	100.00%
5.203	5.633	100.00%
5.633	5.891	100.00%
5.891	5.971	100.00%
5.971	6.019	93.80%
6.019	6.149	100.00%
6.149	6.296	100.00%
6.296	6.526	100.00%
6.526	6.668	100.00%
6.668	6.746	100.00%
6.746	6.877	100.00%
6.877	6.984	100.00%
6.984	7.113	100.00%
7.113	7.466	100.00%
7.466	7.597	100.00%
7.597	9.027	100.00%

Signal #2


2.686	3.190	100.00%
3.190	3.520	100.00%
3.520	3.822	100.00%
3.822	3.861	91.38%
3.861	4.050	100.00%
4.050	4.141	100.00%
4.141	4.647	100.00%
4.647	4.900	100.00%
4.900	4.964	100.00%
4.964	5.017	100.00%
5.017	5.162	100.00%
5.162	5.285	100.00%
5.285	5.560	100.00%
5.560	5.720	100.00%
5.720	5.858	100.00%
5.858	5.973	100.00%
5.973	6.040	100.00%
6.040	6.264	100.00%
6.264	6.557	100.00%
6.557	6.769	100.00%
6.769	7.865	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
Data File : PL084733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 23:14
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC212

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 05:54:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

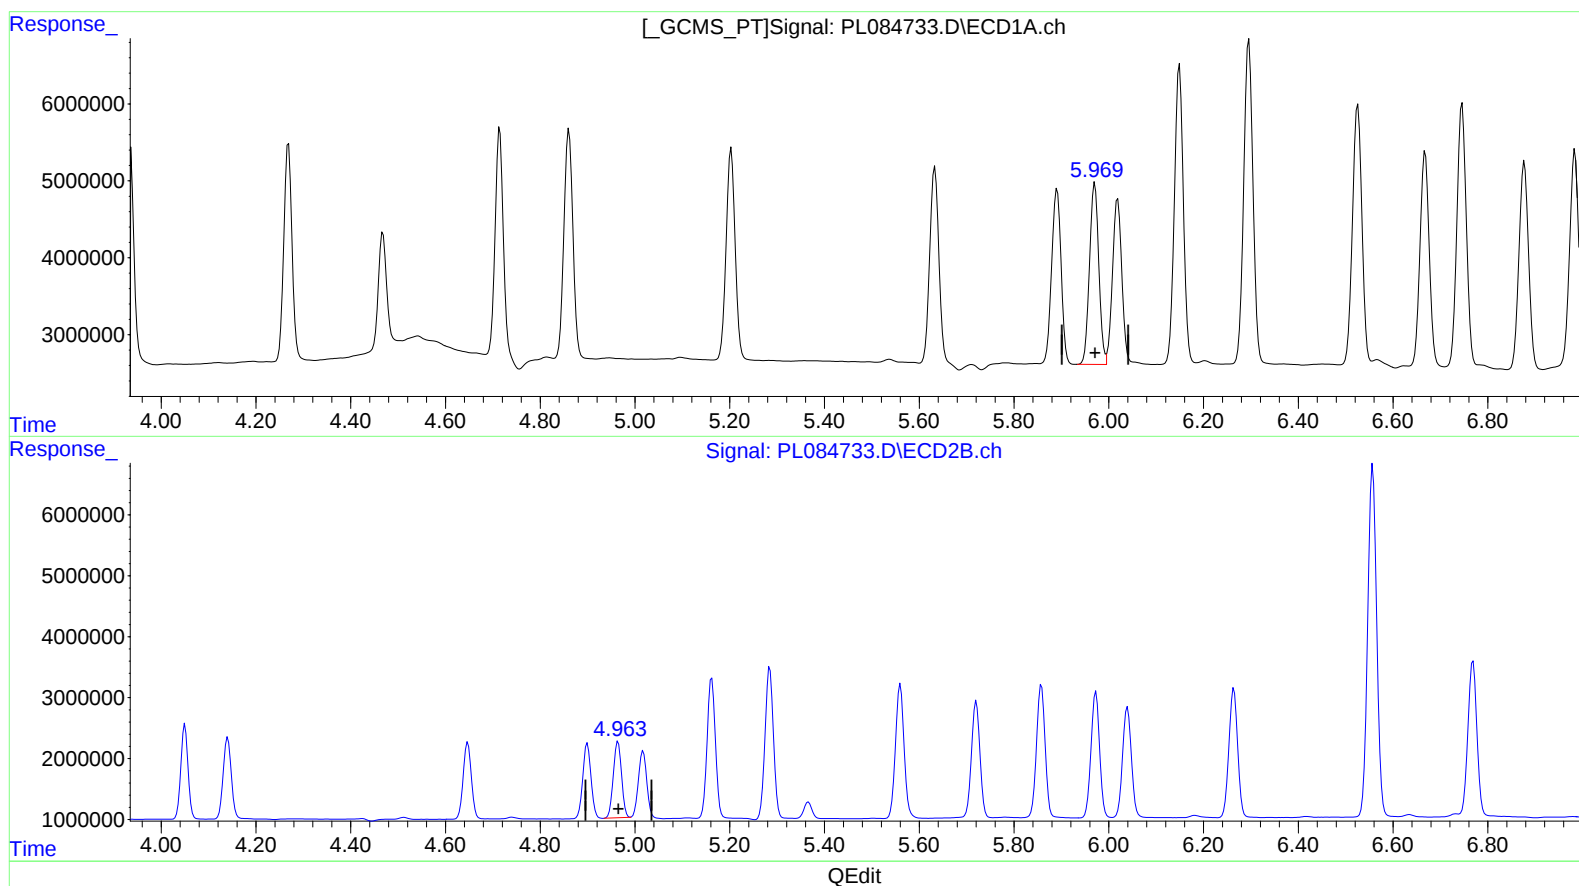

(11) cis-Chlordane (B)

5.971min 10.043 ng/ml

response 32005432

(11) cis-Chlordane #2 (B)

4.964min 9.742 ng/ml


response 15070858

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081523\
Data File : PL084733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 23:14
Operator : AR\AJ
Sample : RESC353
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESC212

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 05:54:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 05:52:51 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

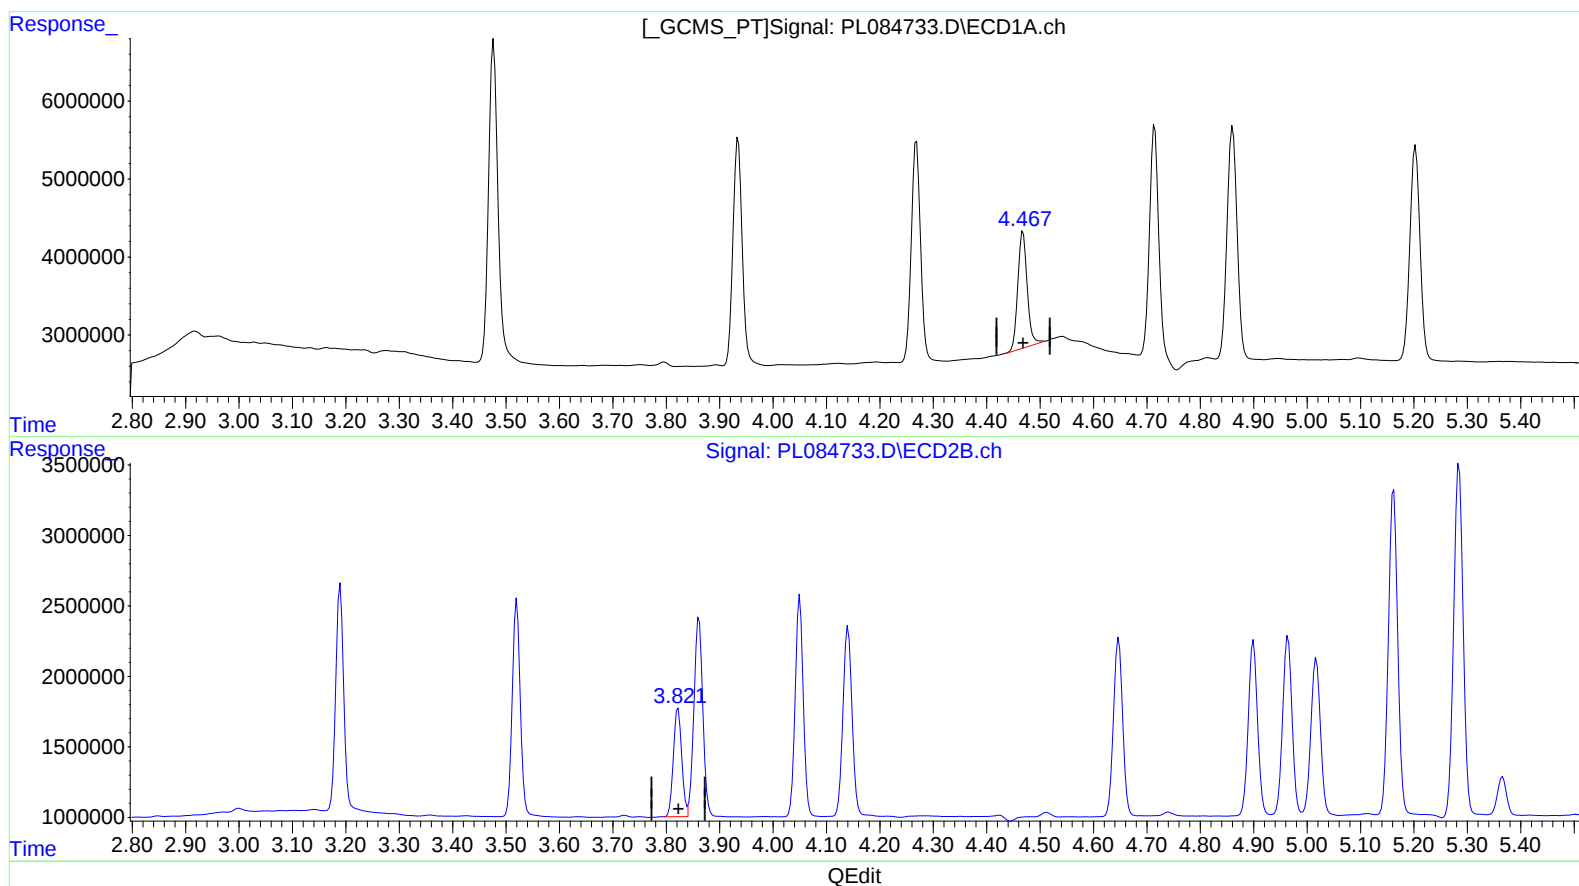

(6) beta-BHC (B)

4.468min 10.292 ng/ml

response 18176644

(6) beta-BHC #2 (B)

3.822min 10.119 ng/ml

response 8312883