

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081524\
 Data File : PL091124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2024 20:22
 Operator : AR\AJ
 Sample : P3598-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-081324-A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 07:26:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.785	28748164	26297031	13.389m	13.472
28) SA Decachlor...	9.055	7.925	22464561	24222990	14.735	12.789

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081524\
Data File : PL091124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2024 20:22
Operator : AR\AJ
Sample : P3598-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
JC-03-081324-A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/19/2024
Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 07:26:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

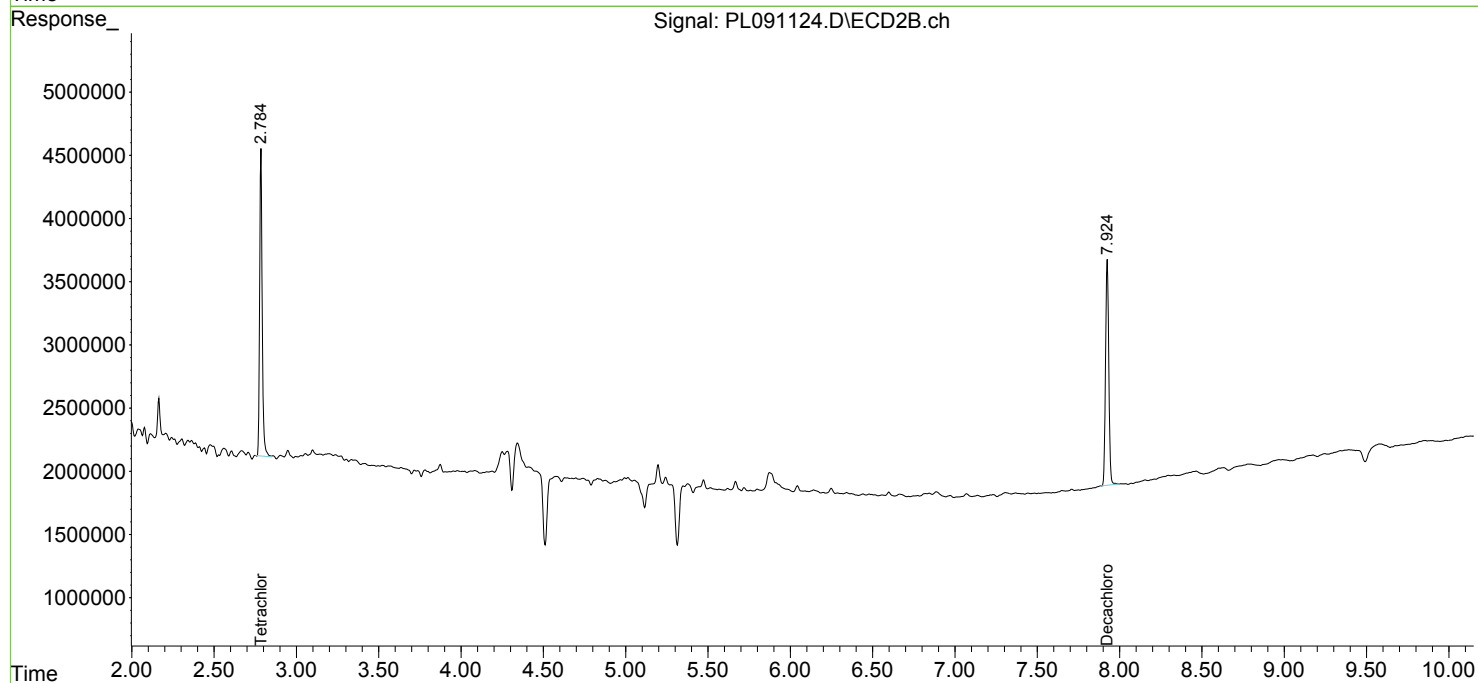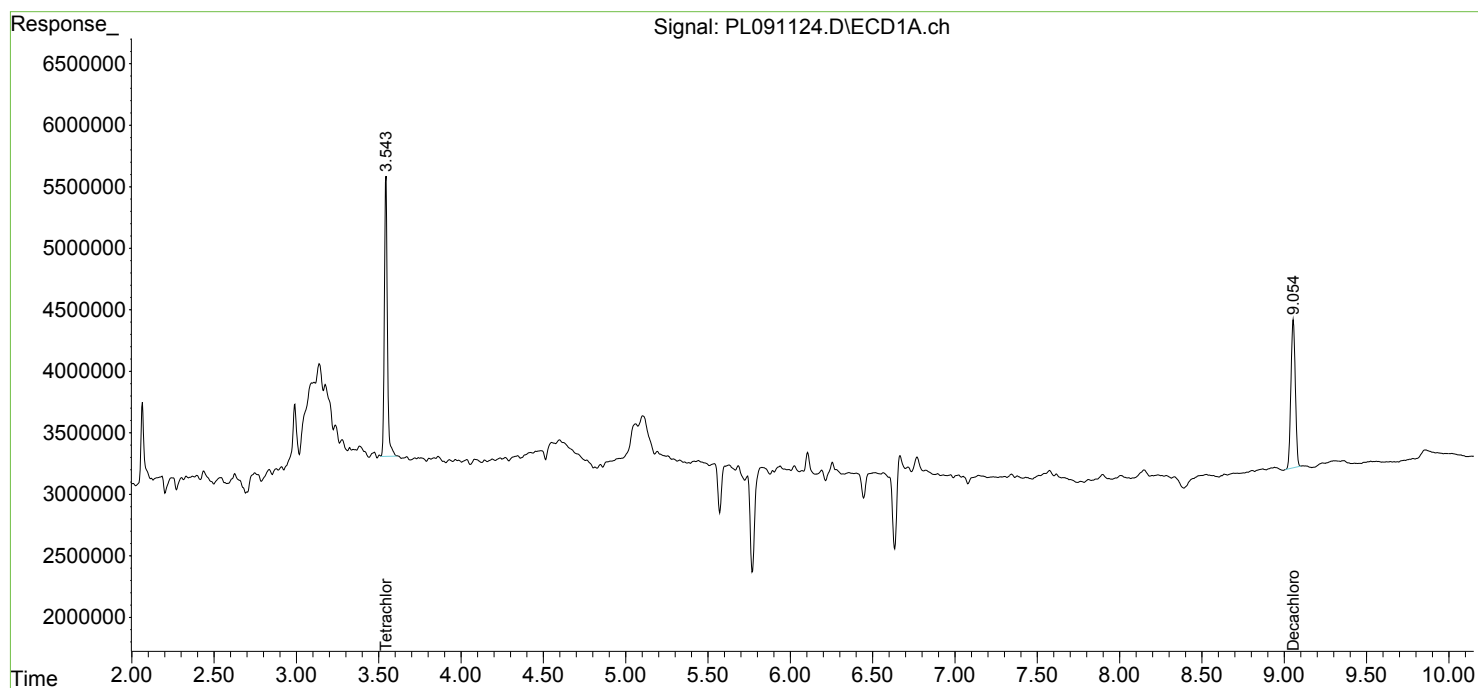

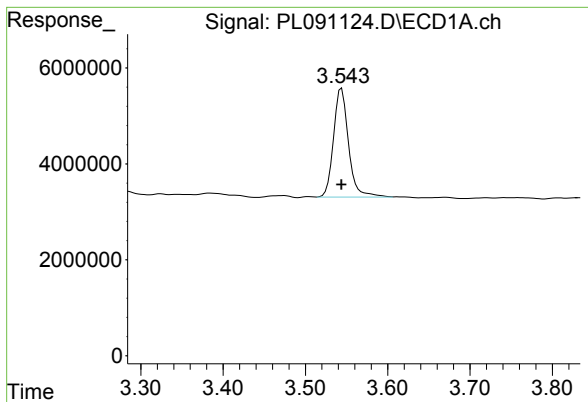


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 28748164
Conc: 13.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-081324-A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

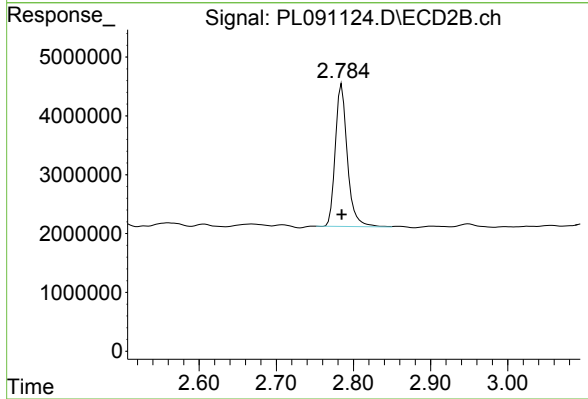


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 26297031
Conc: 13.47 ng/ml

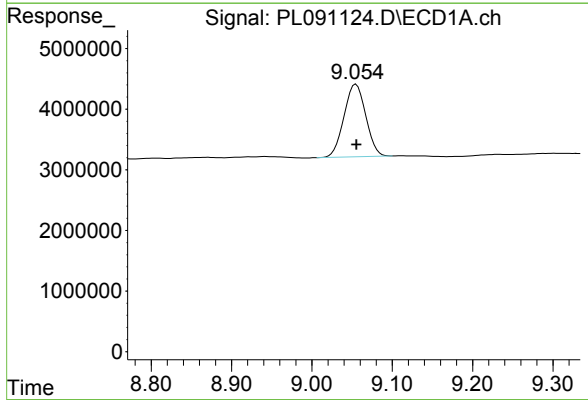

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 22464561
Conc: 14.74 ng/ml

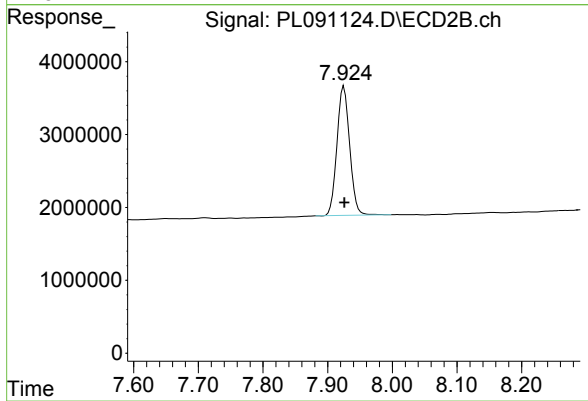

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 24222990
Conc: 12.79 ng/ml