

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
 Data File : PL096806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2025 19:43
 Operator : AR\AJ
 Sample : Q2844-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MOO-25-0226

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:17:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.825	26403265	40494416	8.301	8.476
28)	SA Decachlor...	9.006	7.989	26839680	36427171	11.255	8.397 #
Target Compounds							
8)	B Heptachlo...	5.649	0.000	16464174	0	4.269	N.D. #
10)	B gamma-Chl...	5.932f	5.075f	8824974	6528485	2.319	1.110 #
12)	B 4,4'-DDE	6.157	0.000	14186246	0	4.418	N.D. #
13)	MA Dieldrin	0.000	5.432	0	24667652	N.D.	4.176 #
14)	MA Endrin	6.536	0.000	9957241	0	3.290	N.D. #
15)	B Endosulfa...	0.000	5.987	0	7212390	N.D.	1.404 #
16)	A 4,4'-DDD	6.684	0.000	5055963	0	2.000	N.D. #
17)	MA 4,4'-DDT	0.000	6.101	0	9639372	N.D.	1.906 #
25)	Chlordane-3	5.932	5.075f	8824974	6528485	13.212	9.389 #
27)	Chlordane-5	0.000	5.987f	0	7212390	N.D.	28.271 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
Data File : PL096806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2025 19:43
Operator : AR\AJ
Sample : Q2844-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 05:17:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

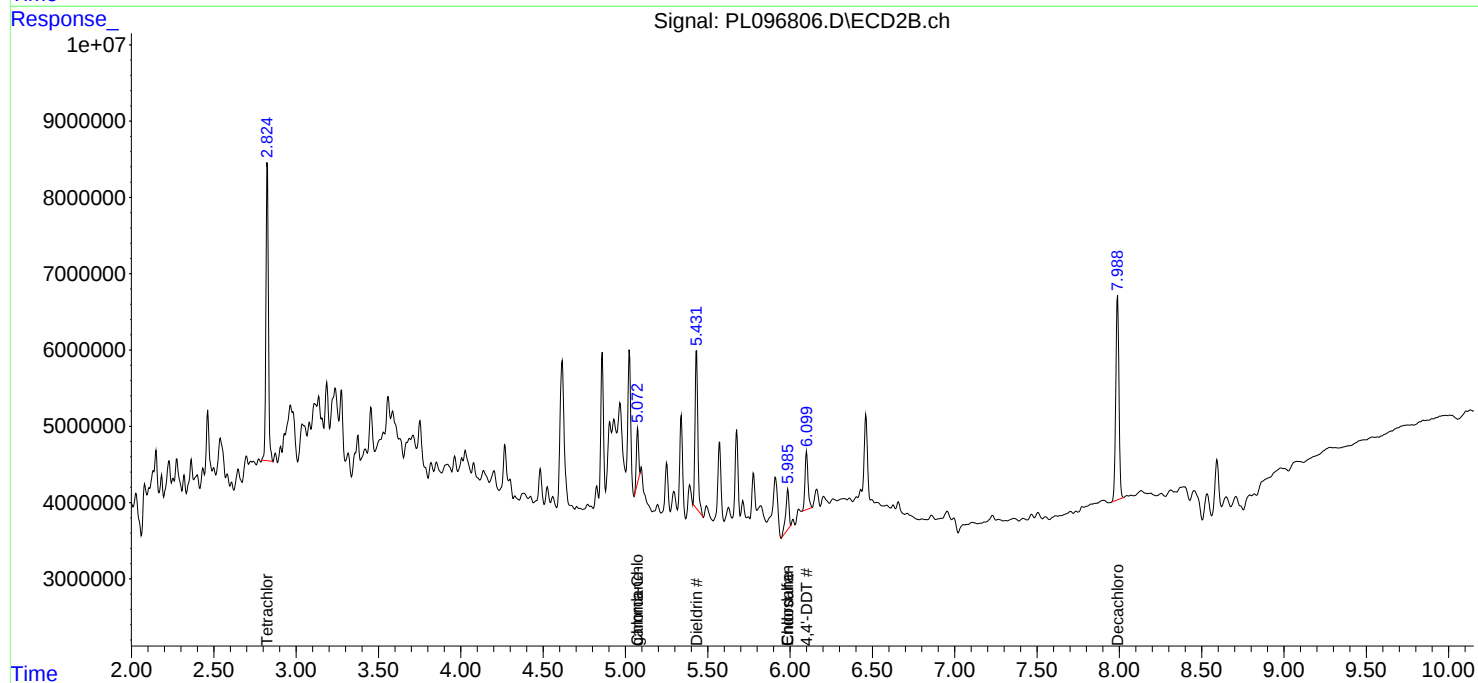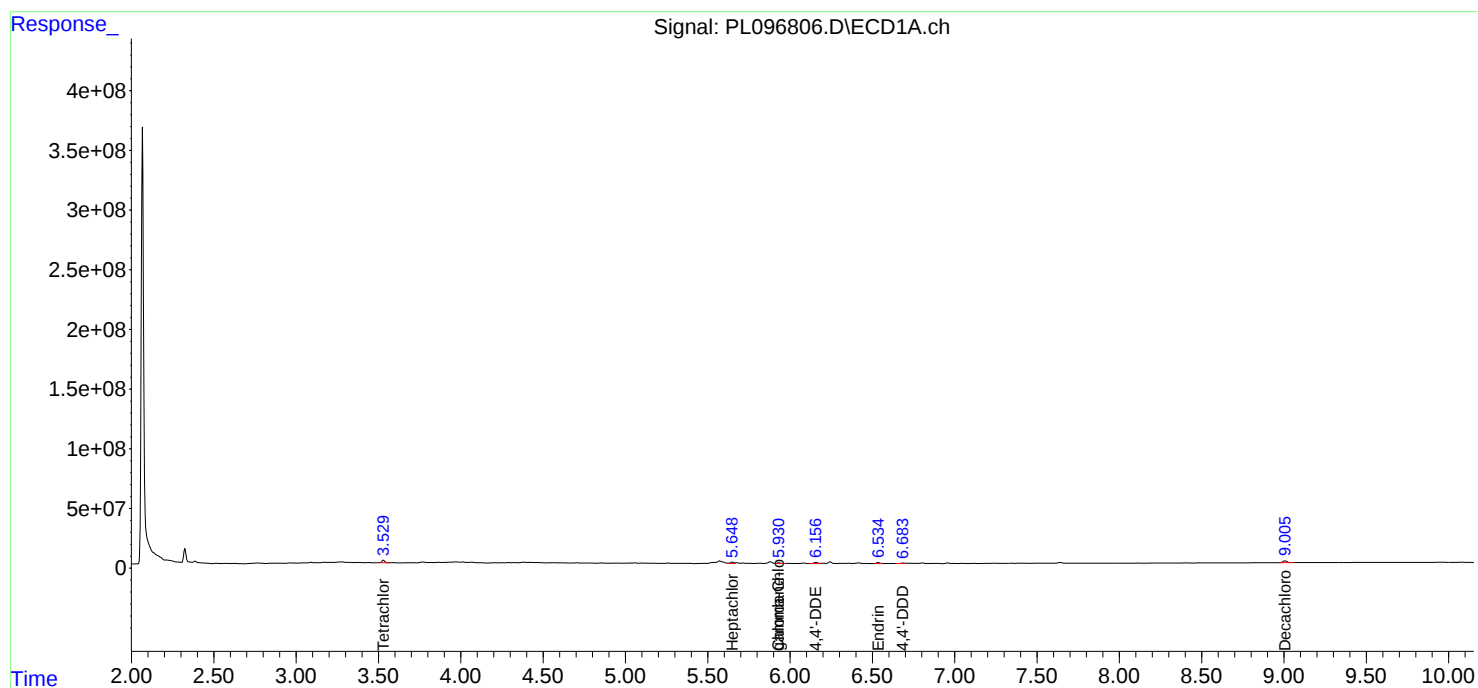


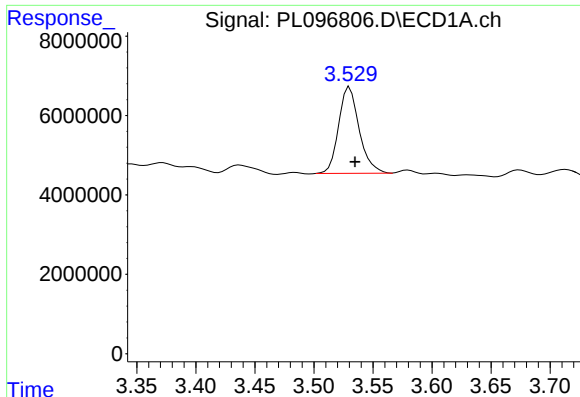

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 26403265
Conc: 8.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

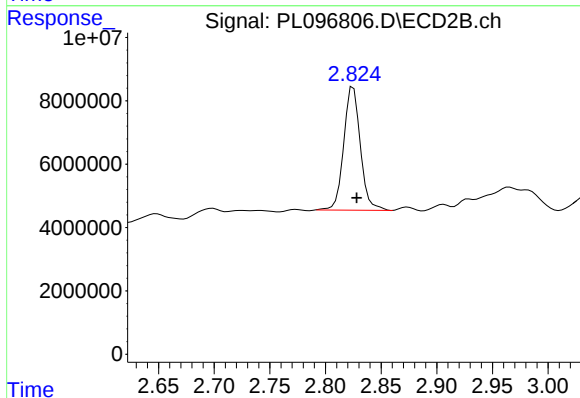


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 40494416
Conc: 8.48 ng/ml

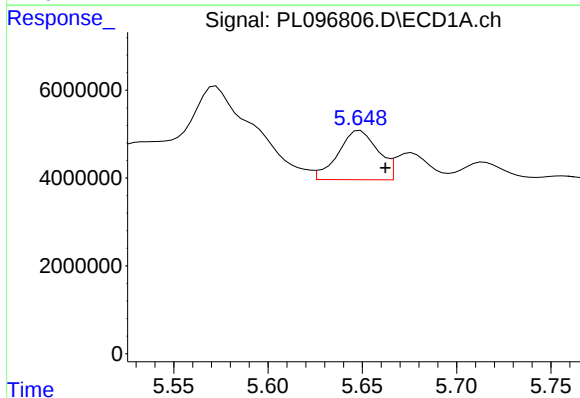


#8 Heptachlor epoxide

R.T.: 5.649 min
Delta R.T.: -0.013 min
Response: 16464174
Conc: 4.27 ng/ml

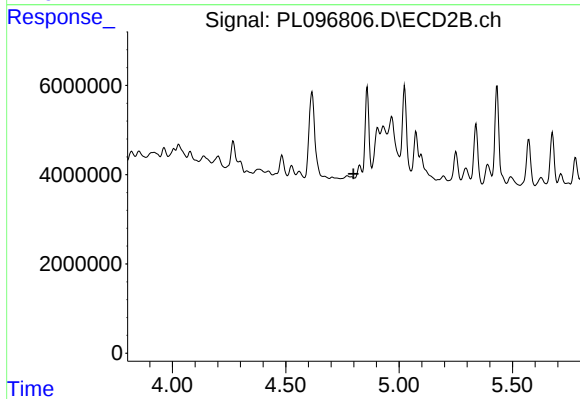

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

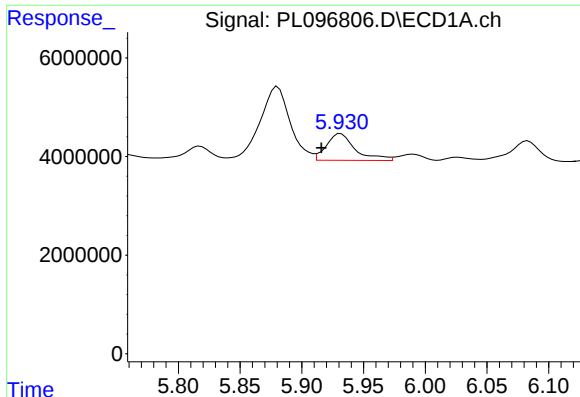

#10 gamma-Chlordane


R.T.: 5.932 min
Delta R.T.: 0.016 min
Response: 8824974
Conc: 2.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

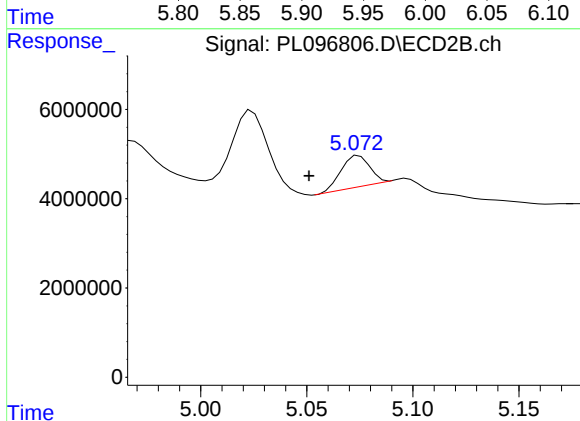


#10 gamma-Chlordane

R.T.: 5.075 min
Delta R.T.: 0.024 min
Response: 6528485
Conc: 1.11 ng/ml

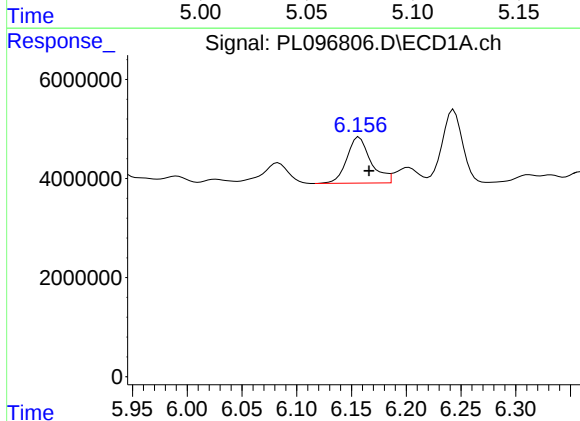


#12 4,4'-DDE

R.T.: 6.157 min
Delta R.T.: -0.009 min
Response: 14186246
Conc: 4.42 ng/ml

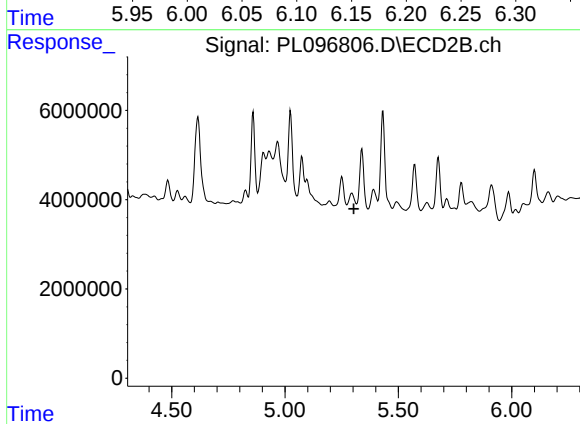

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

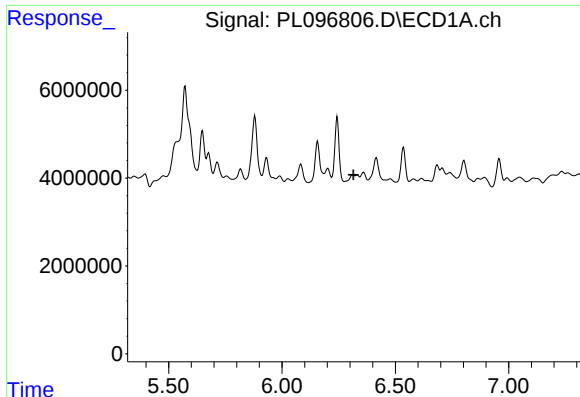

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

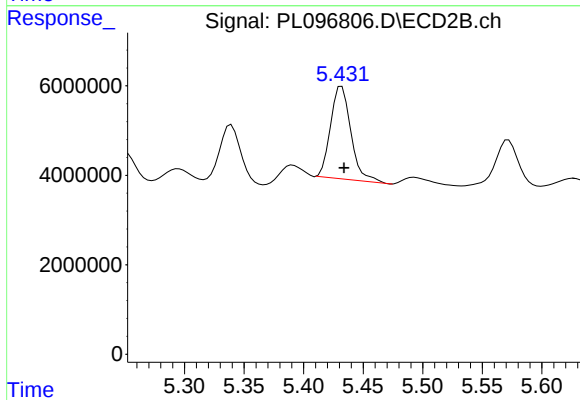


#13 Dieldrin

R.T.: 5.432 min
Delta R.T.: -0.002 min
Response: 24667652
Conc: 4.18 ng/ml

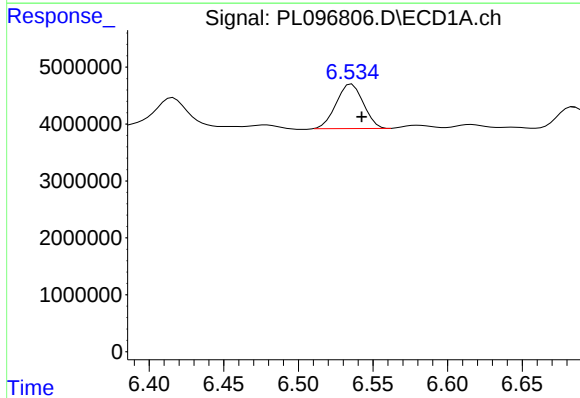


#14 Endrin

R.T.: 6.536 min
Delta R.T.: -0.007 min
Response: 9957241
Conc: 3.29 ng/ml

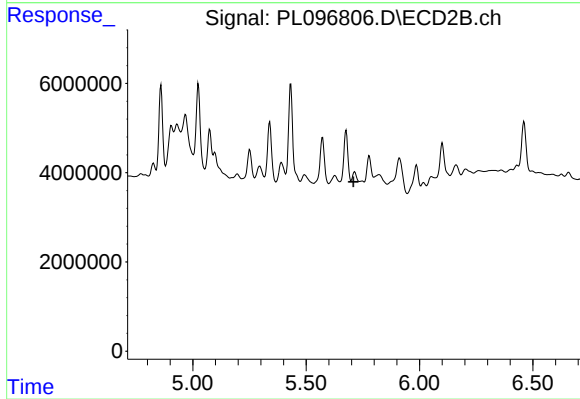

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.709 min
Response: 0
Conc: N.D.

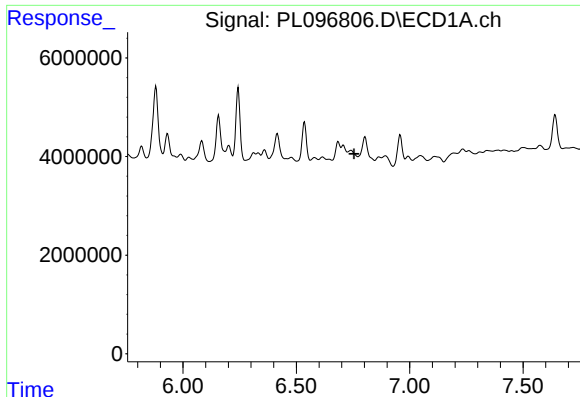

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

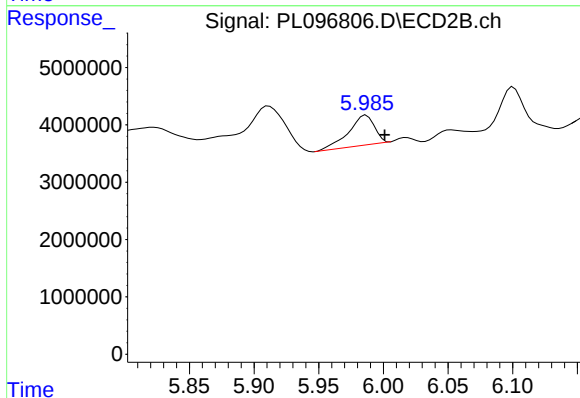


#15 Endosulfan II

R.T.: 5.987 min
Delta R.T.: -0.014 min
Response: 7212390
Conc: 1.40 ng/ml

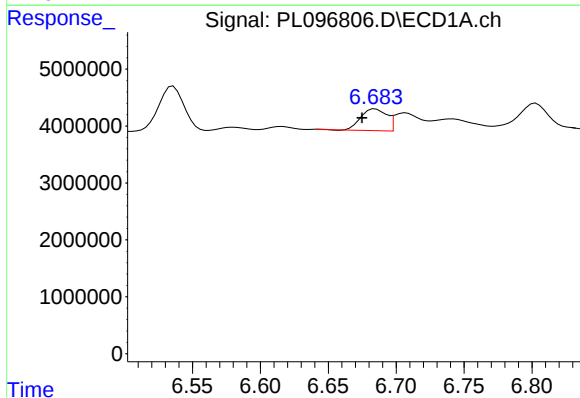


#16 4,4'-DDD

R.T.: 6.684 min
Delta R.T.: 0.009 min
Response: 5055963
Conc: 2.00 ng/ml

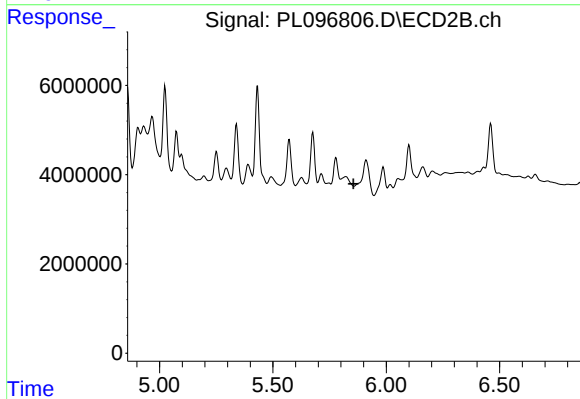

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.856 min
Response: 0
Conc: N.D.

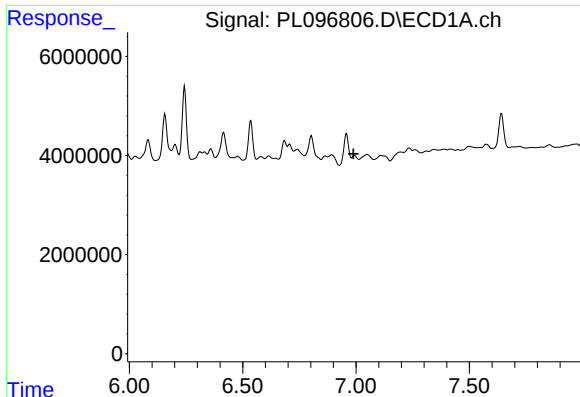

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

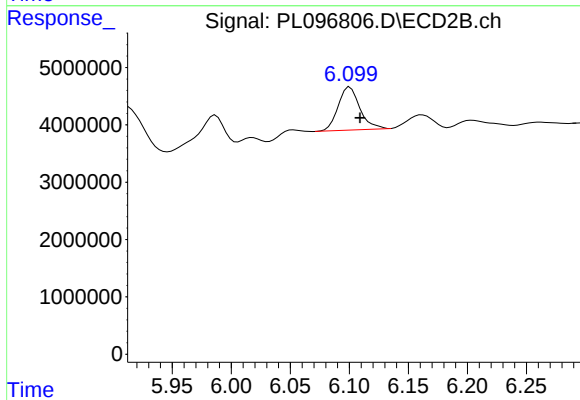


#17 4,4'-DDT

R.T.: 6.101 min
Delta R.T.: -0.008 min
Response: 9639372
Conc: 1.91 ng/ml

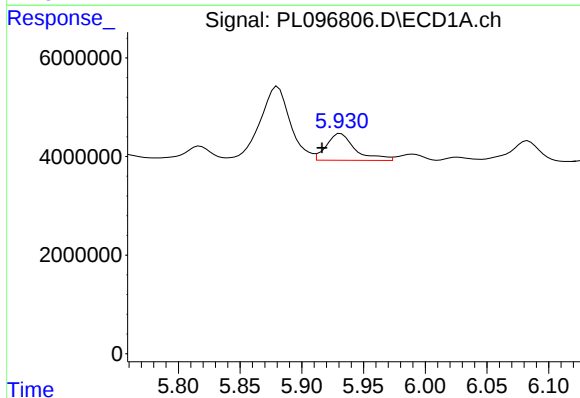


#25 Chlordane-3

R.T.: 5.932 min
Delta R.T.: 0.015 min
Response: 8824974
Conc: 13.21 ng/ml

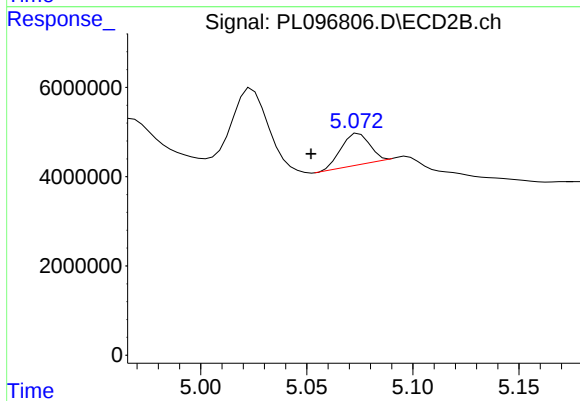

#25 Chlordane-3


R.T.: 5.075 min
Delta R.T.: 0.023 min
Response: 6528485
Conc: 9.39 ng/ml

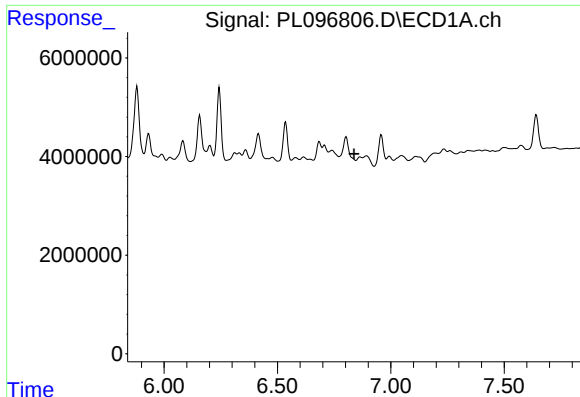

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MOO-25-0226

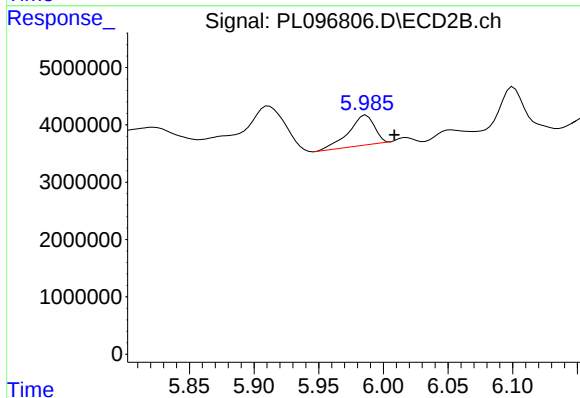


#27 Chlordane-5

R.T.: 5.987 min
Delta R.T.: -0.022 min
Response: 7212390
Conc: 28.27 ng/ml

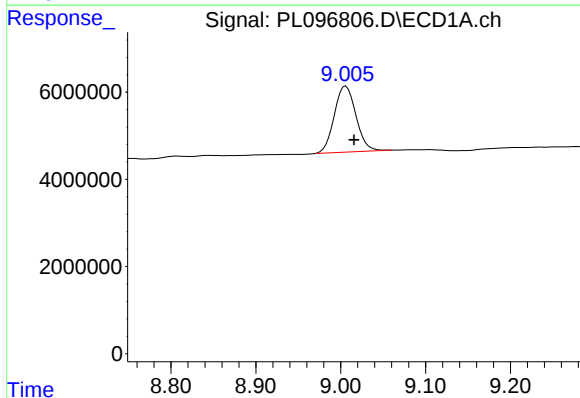

#28 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: -0.010 min
Response: 26839680
Conc: 11.26 ng/ml

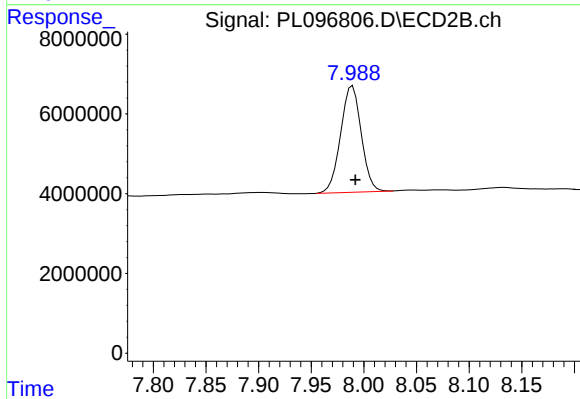

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.003 min
Response: 36427171
Conc: 8.40 ng/ml