

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
 Data File : PL096811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2025 20:51
 Operator : AR\AJ
 Sample : Q2855-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 #454

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:18:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.825	13851949	24416420	4.355	5.110
28)	SA Decachlor...	9.006	7.990	20849766	29287416	8.743	6.751
Target Compounds							
6)	B beta-BHC	0.000	3.963	0	6637844	N.D.	2.353 #
10)	B gamma-Chl...	5.927	0.000	6790197	0	1.784	N.D. #
11)	B alpha-Chl...	5.986	0.000	16960490	0	4.400	N.D. #
25)	Chlordane-3	5.927	0.000	6790197	0	10.166	N.D. #
26)	Chlordane-4	5.986	0.000	16960490	0	20.491	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
Data File : PL096811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2025 20:51
Operator : AR\AJ
Sample : Q2855-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
#454

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 05:18:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

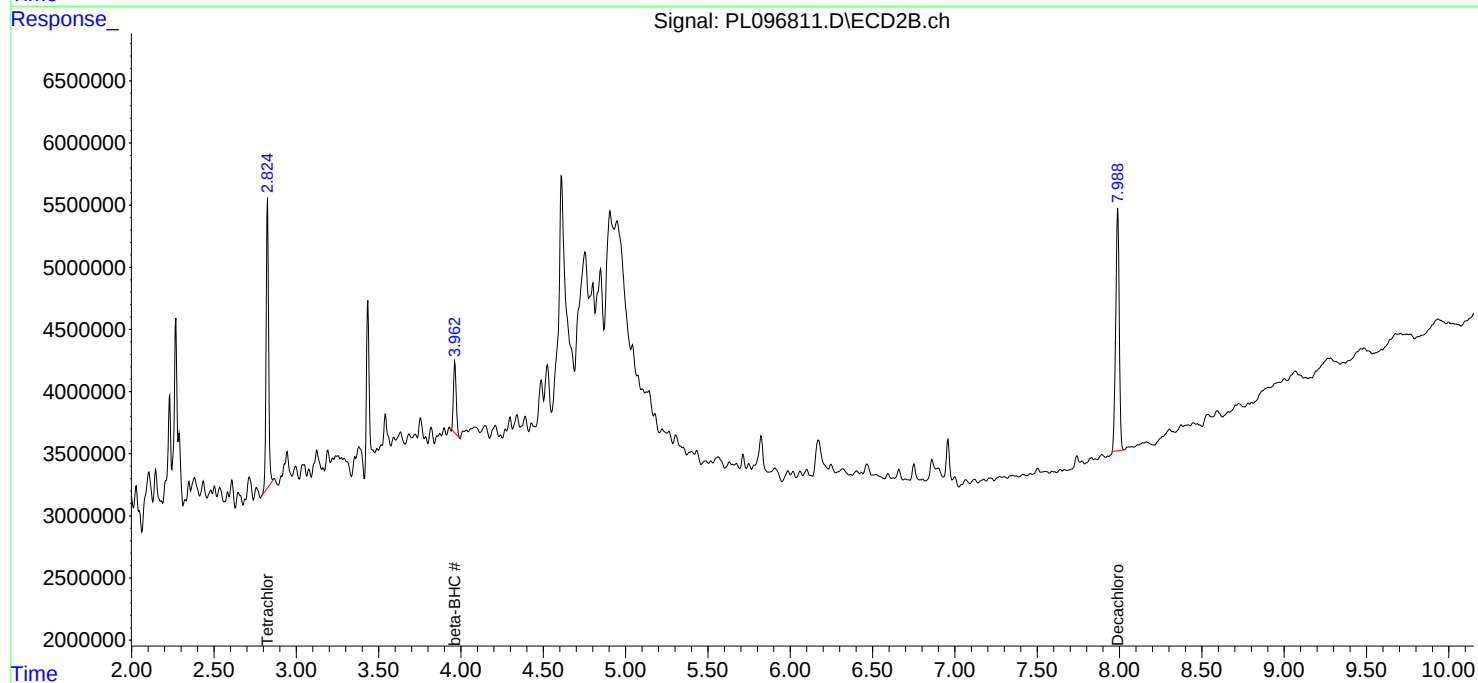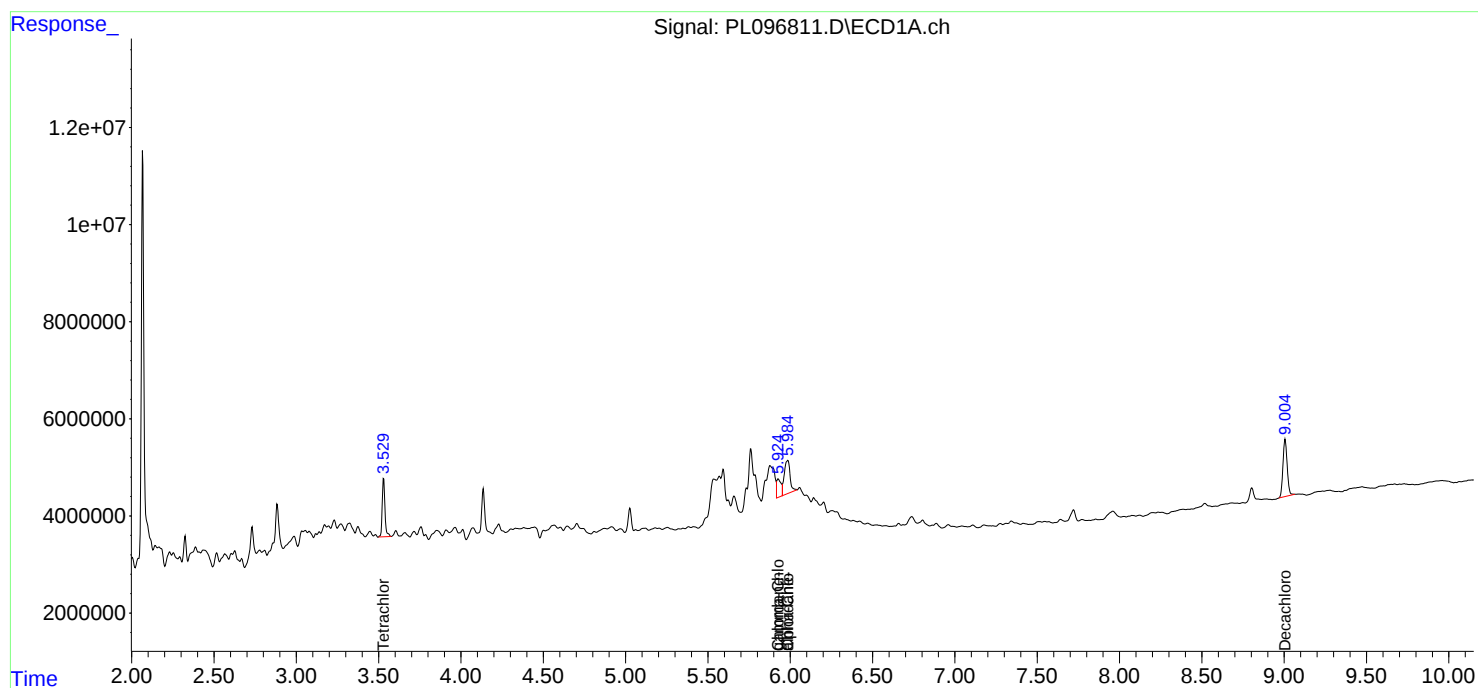


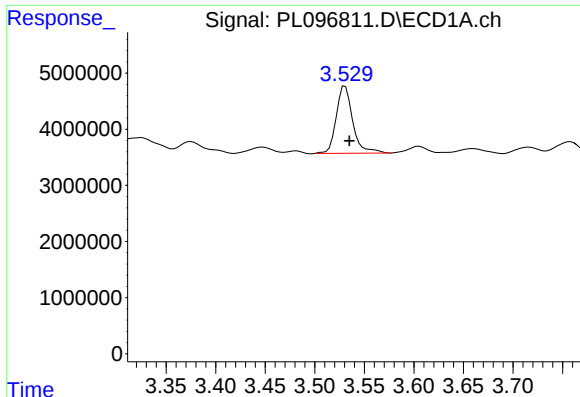

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.004 min
Response: 13851949
Conc: 4.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
#454

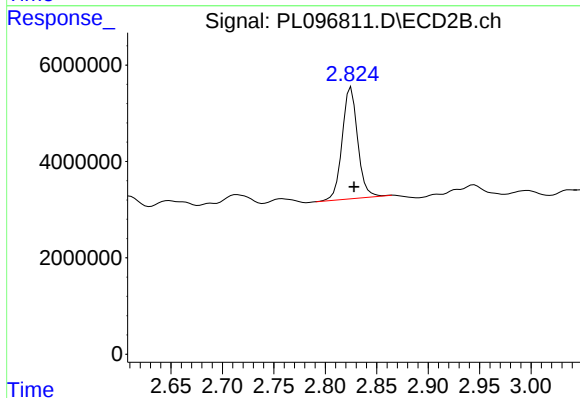


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: -0.003 min
Response: 24416420
Conc: 5.11 ng/ml

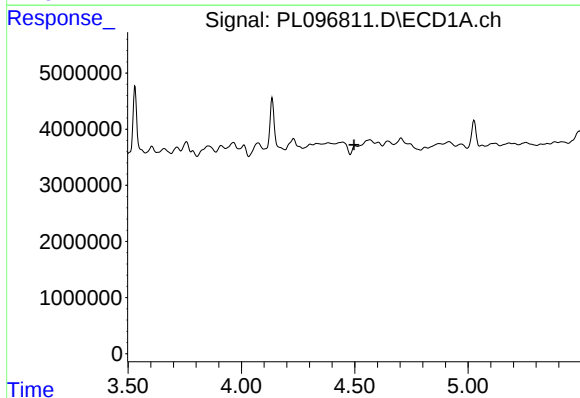


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.497 min
Response: 0
Conc: N.D.

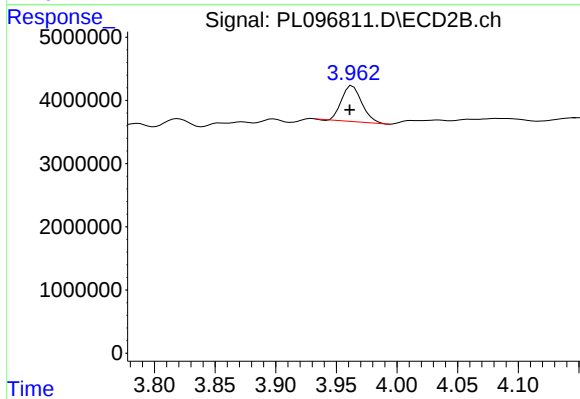

#6 beta-BHC


R.T.: 3.963 min
Delta R.T.: 0.002 min
Response: 6637844
Conc: 2.35 ng/ml

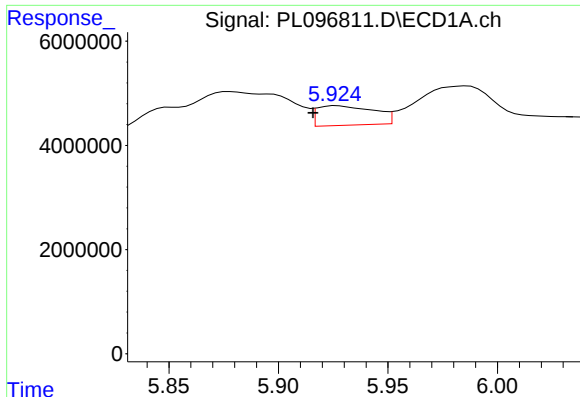

#10 gamma-Chlordane


R.T.: 5.927 min
Delta R.T.: 0.011 min
Response: 6790197
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
#454

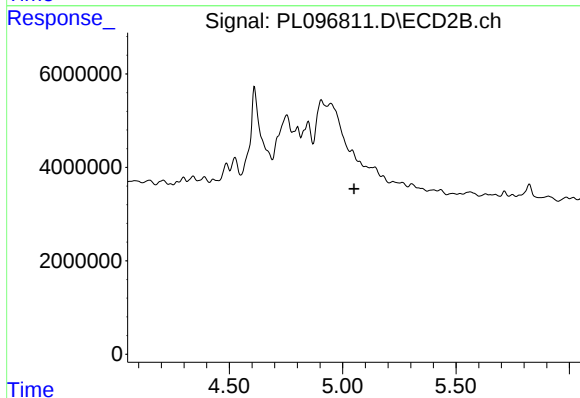


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.051 min
Response: 0
Conc: N.D.

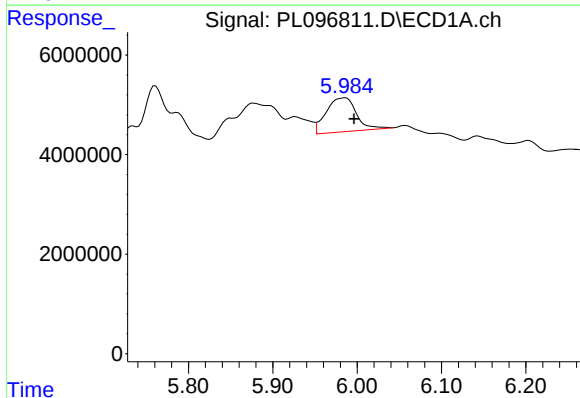


#11 alpha-Chlordane

R.T.: 5.986 min
Delta R.T.: -0.011 min
Response: 16960490
Conc: 4.40 ng/ml

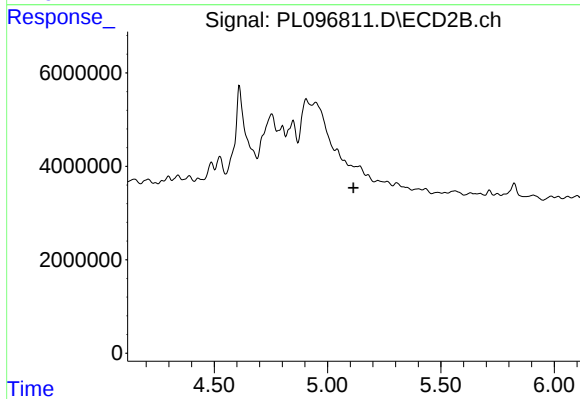

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

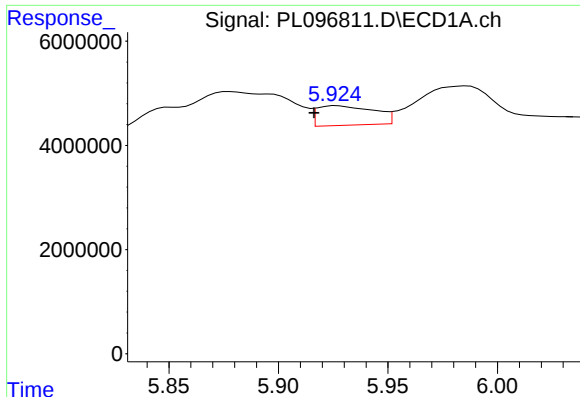

#25 Chlordane-3


R.T.: 5.927 min
Delta R.T.: 0.010 min
Response: 6790197
Conc: 10.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
#454

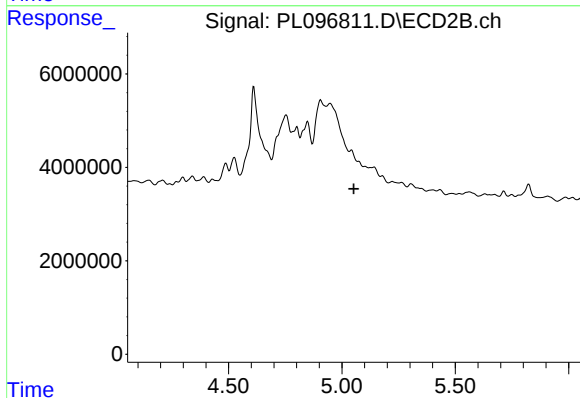


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.052 min
Response: 0
Conc: N.D.

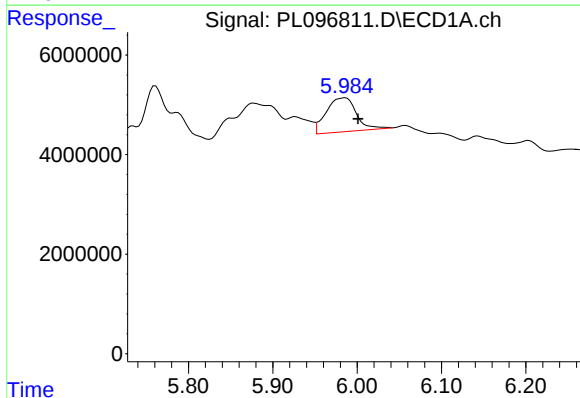


#26 Chlordane-4

R.T.: 5.986 min
Delta R.T.: -0.015 min
Response: 16960490
Conc: 20.49 ng/ml

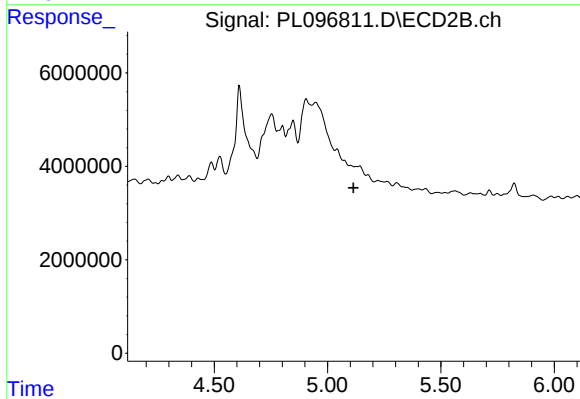

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

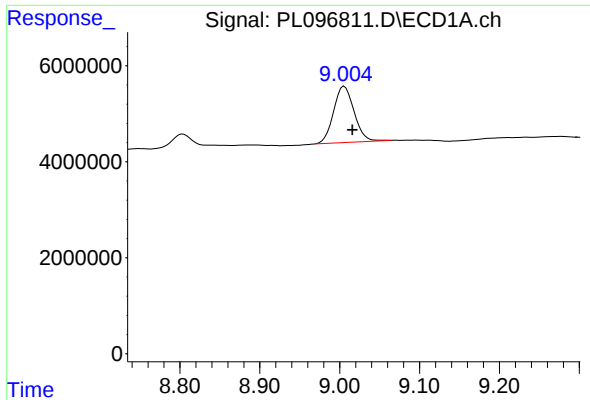

#28 Decachlorobiphenyl

R.T.: 9.006 min
Delta R.T.: -0.010 min
Response: 20849766
Conc: 8.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
#454

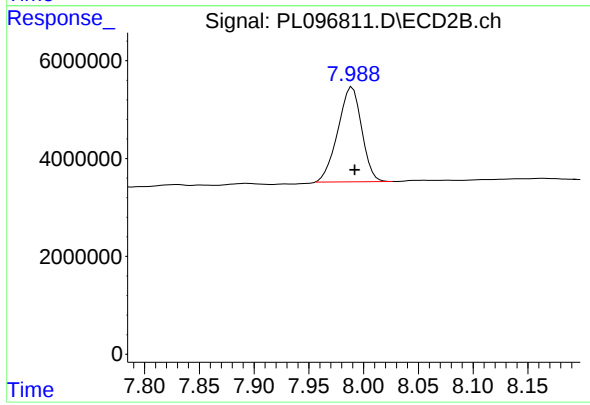

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 29287416
Conc: 6.75 ng/ml