

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
 Data File : PL096800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2025 18:22
 Operator : AR\AJ
 Sample : Q2838-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-11

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/20/2025
 Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:16:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.529	2.824	33527623	51500435	10.541	10.779
2) SA Decachlor...	9.004	7.988	42164621	80902325	17.682m	18.648

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081525\
Data File : PL096800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2025 18:22
Operator : AR\AJ
Sample : Q2838-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/20/2025
Supervised By : mohammad ahmed 08/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 05:16:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

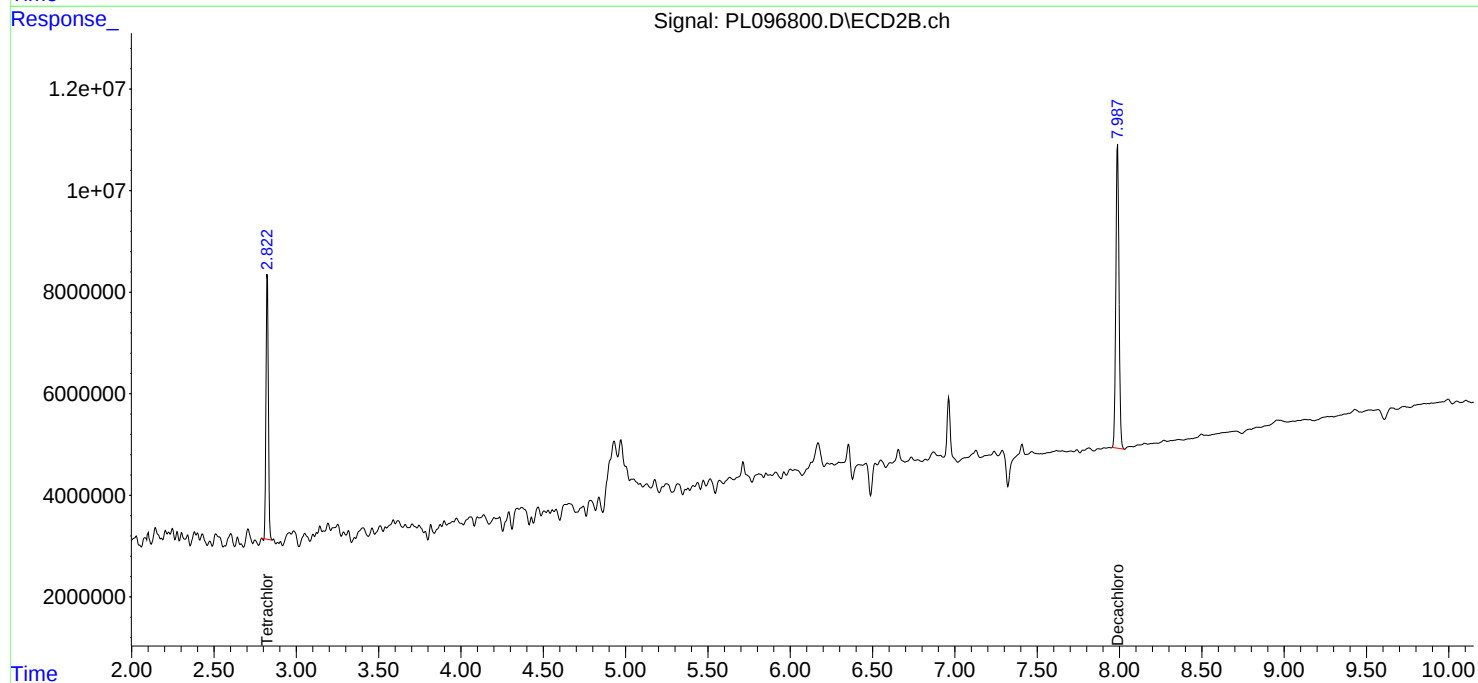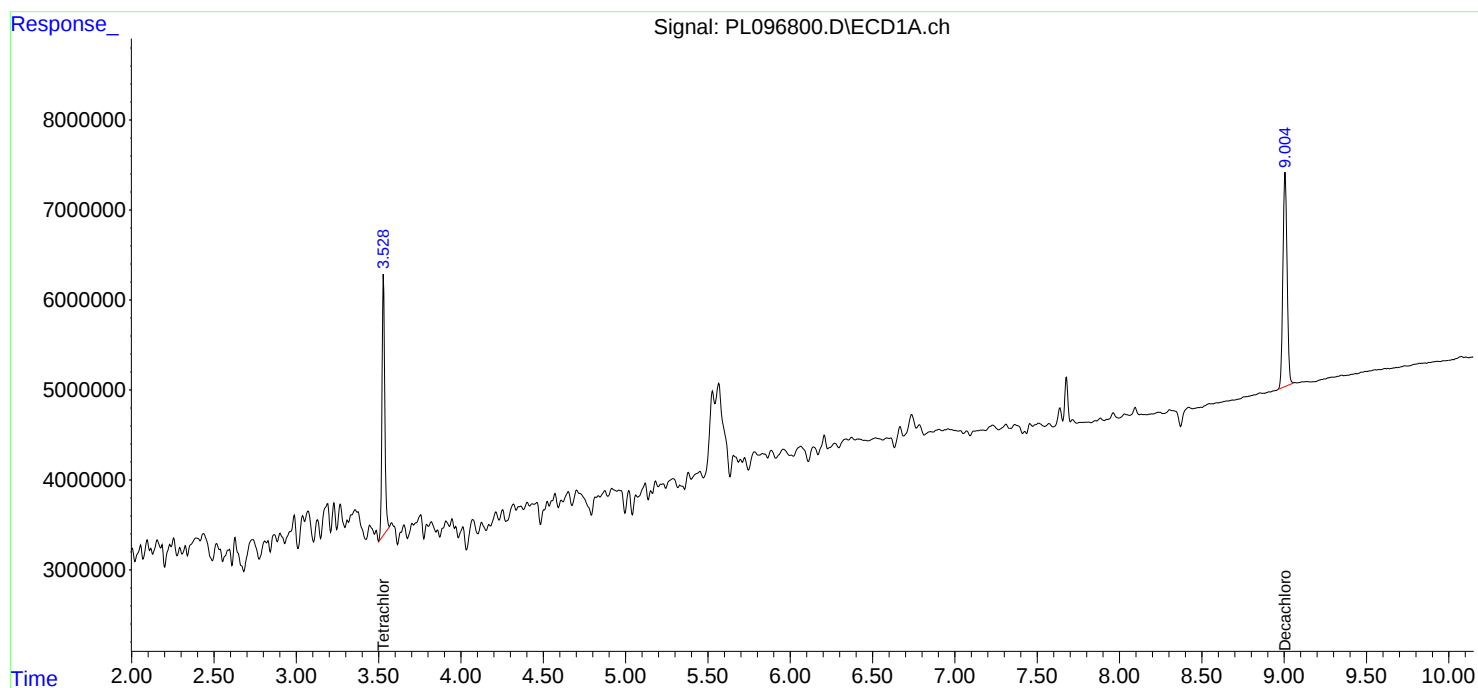

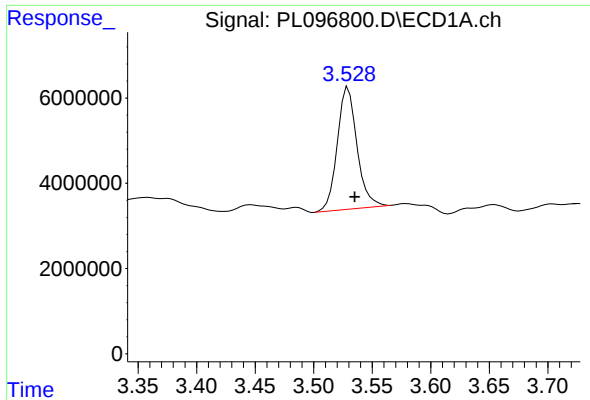


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.006 min
Response: 33527623
Conc: 10.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/20/2025
Supervised By :mohammad ahmed 08/21/2025

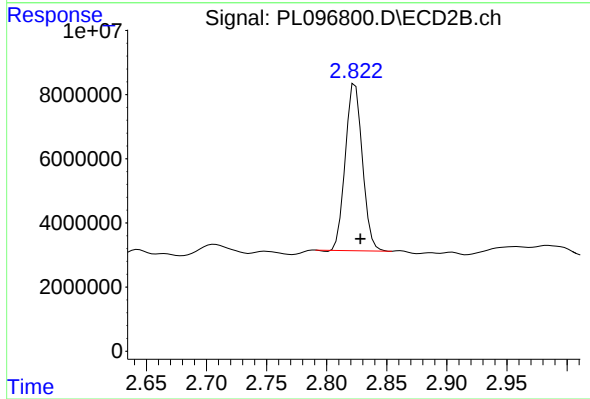


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: -0.004 min
Response: 51500435
Conc: 10.78 ng/ml

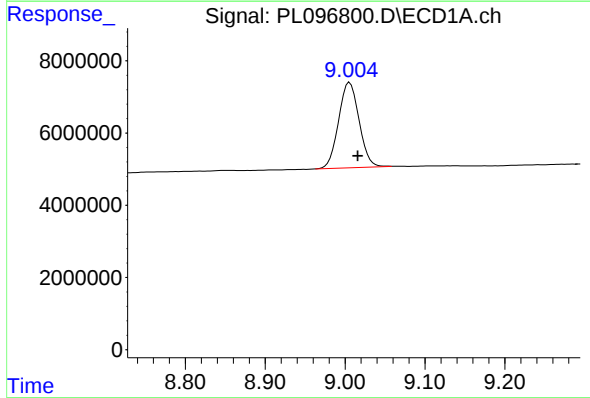

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: -0.011 min
Response: 42164621
Conc: 17.68 ng/ml m

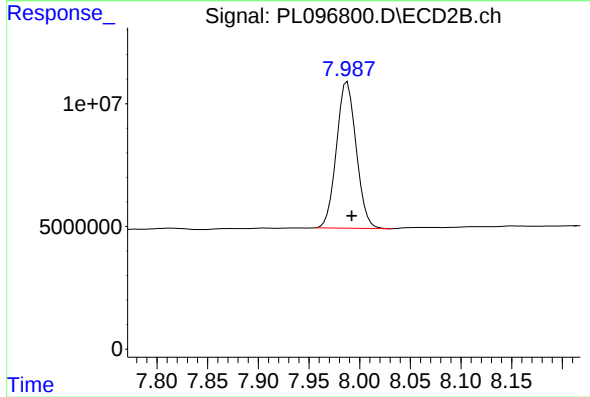

#28 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: -0.004 min
Response: 80902325
Conc: 18.65 ng/ml