

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
 Data File : PL039210.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 16:35
 Operator : AJ\SJ
 Sample : J4282-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 04:36:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	79847178	31013287	11.422	11.568
28)	SA Decachlor...	7.961	8.892	91664043	38334686	13.051	16.519 #
Target Compounds							
3)	MA gamma-BHC...	3.967f	0.000	2312850		0.218	N.D. #
6)	B beta-BHC	4.216f	0.000	17497925		3.767	N.D. #
9)	A Endosulfan I	5.240f	0.000	9205073		1.051	N.D. #
10)	B gamma-Chl...	5.204	0.000	14777816		1.496	N.D. #
11)	B alpha-Chl...	5.240	0.000	9205073		0.958	N.D. #
12)	B 4,4'-DDE	5.409	0.000	16389005		1.711	N.D. #
23)	Chlordane-1	4.118	0.000	6924999		21.874	N.D. #
24)	Chlordane-2	4.636	0.000	7387900		21.133	N.D. #
25)	Chlordane-3	5.204	0.000	14777816		13.530	N.D. #
26)	Chlordane-4	5.240	0.000	9205073		9.211	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
Data File : PL039210.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 16:35
Operator : AJ\SJ
Sample : J4282-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:36:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

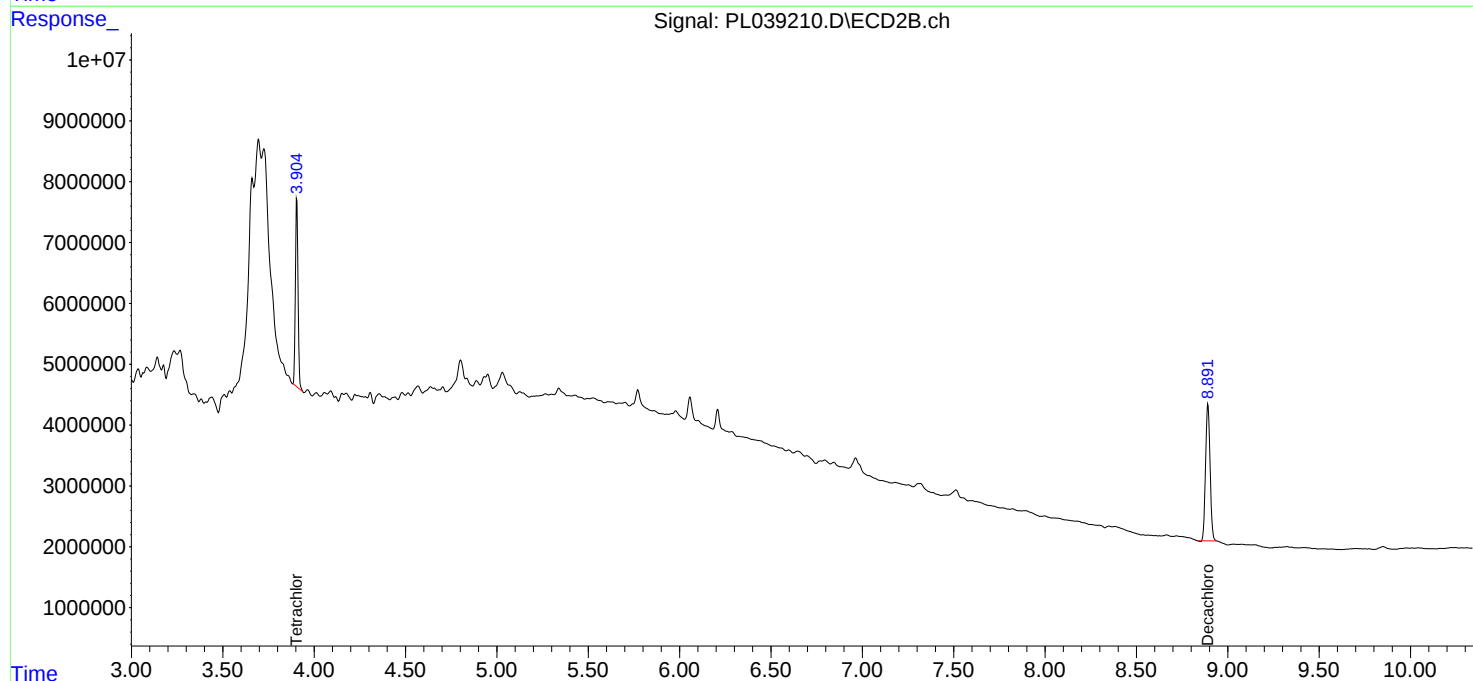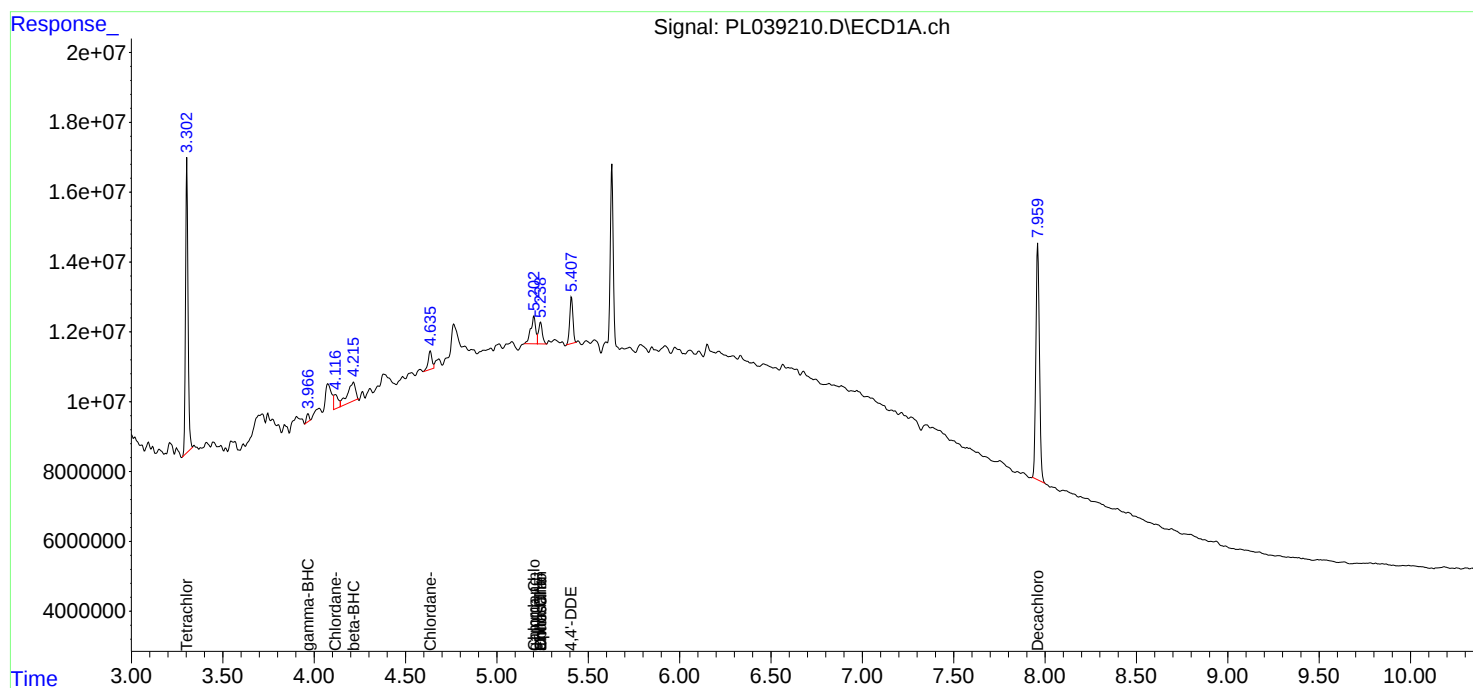


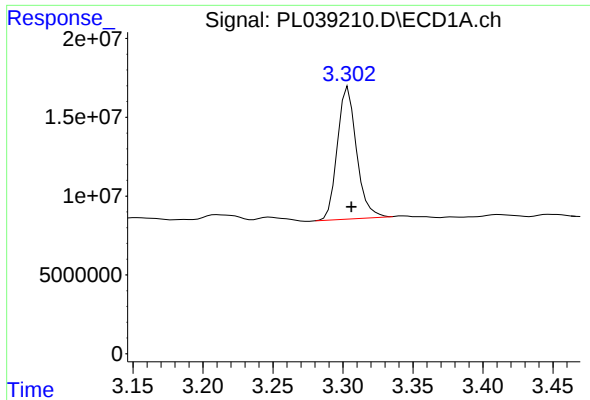

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 79847178
Conc: 11.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

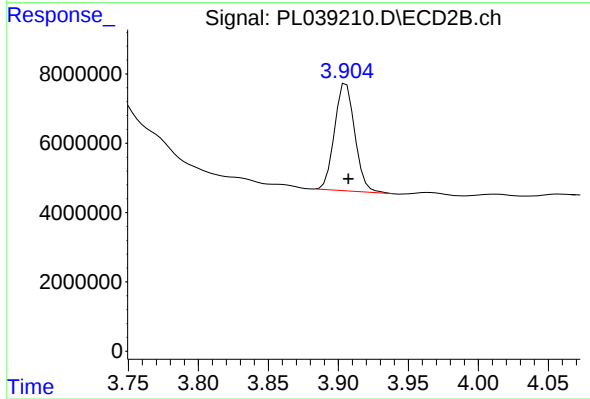


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: -0.002 min
Response: 31013287
Conc: 11.57 ng/ml

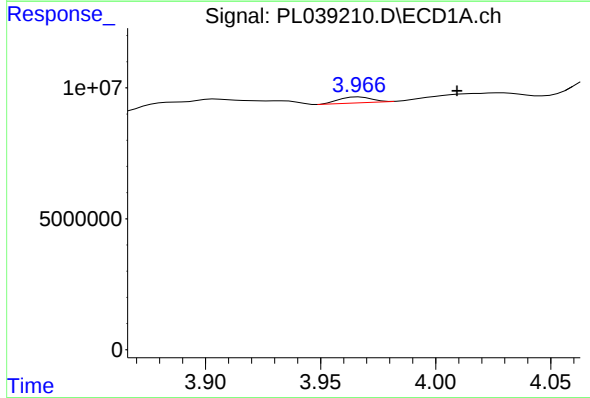


#3 gamma-BHC (Lindane)

R.T.: 3.967 min
Delta R.T.: -0.042 min
Response: 2312850
Conc: 0.22 ng/ml

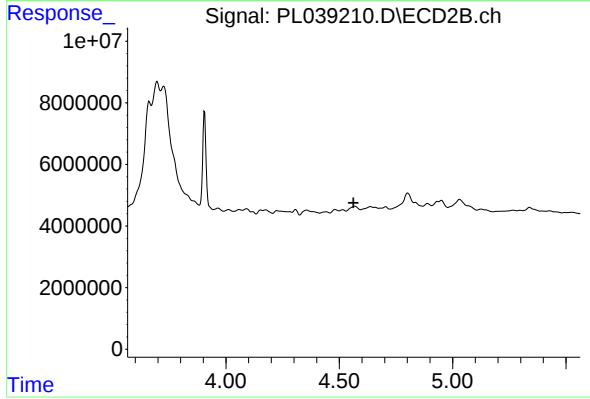

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

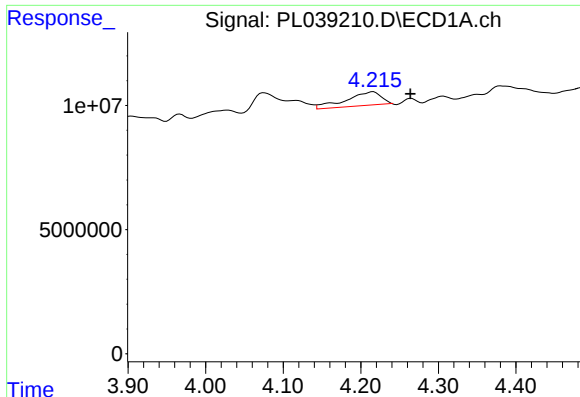

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 17497925
Conc: 3.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

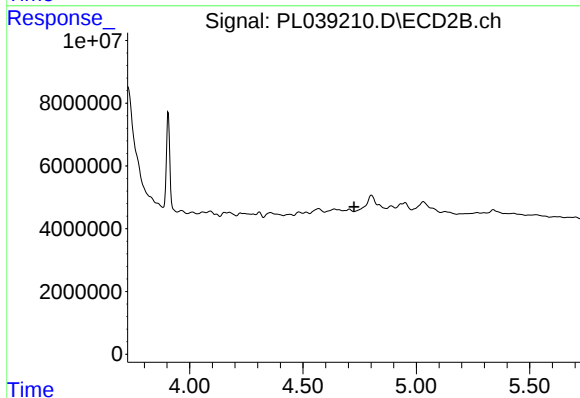


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

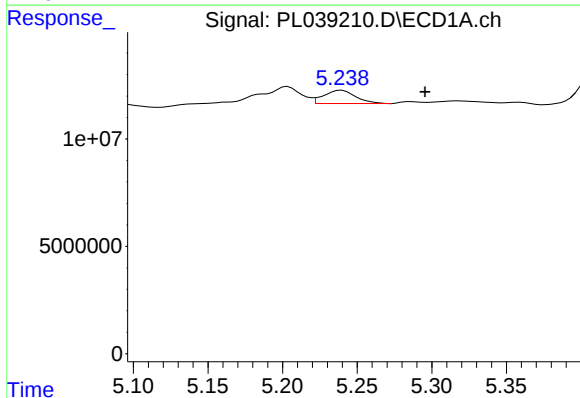


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: -0.056 min
Response: 9205073
Conc: 1.05 ng/ml

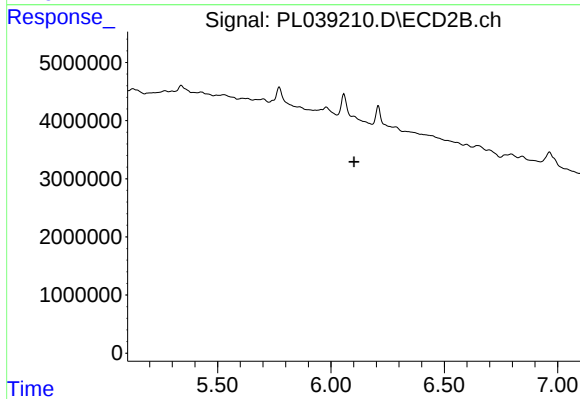

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

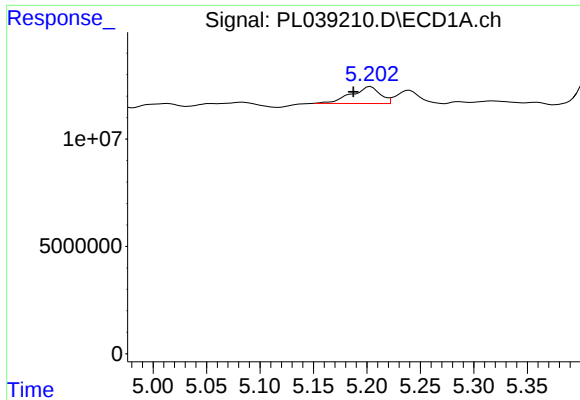

#10 gamma-Chlordane


R.T.: 5.204 min
Delta R.T.: 0.016 min
Response: 14777816
Conc: 1.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

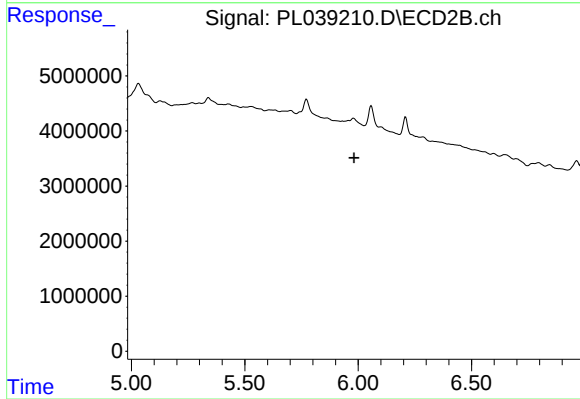


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

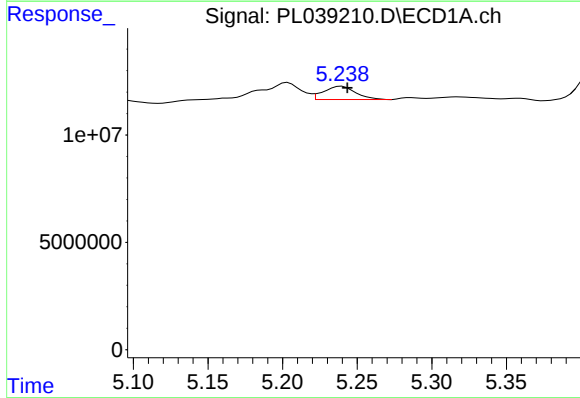


#11 alpha-Chlordane

R.T.: 5.240 min
Delta R.T.: -0.004 min
Response: 9205073
Conc: 0.96 ng/ml

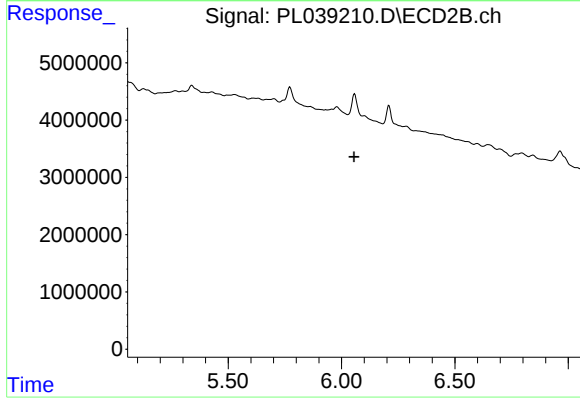

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

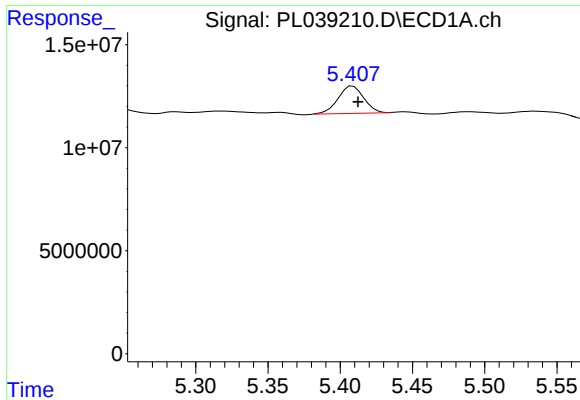

#12 4,4'-DDE


R.T.: 5.409 min
Delta R.T.: -0.004 min
Response: 16389005
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

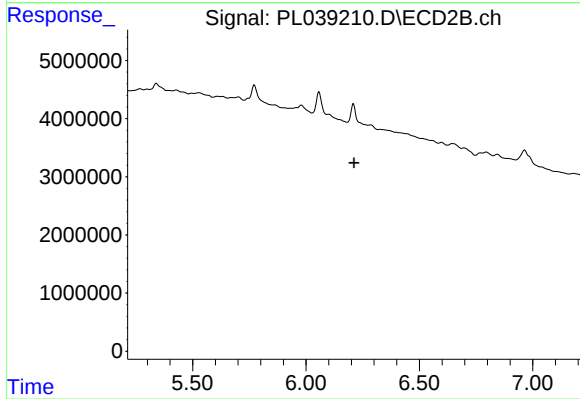


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

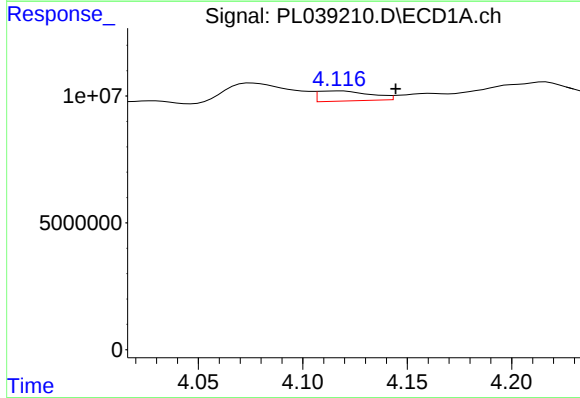


#23 Chlordane-1

R.T.: 4.118 min
Delta R.T.: -0.027 min
Response: 6924999
Conc: 21.87 ng/ml

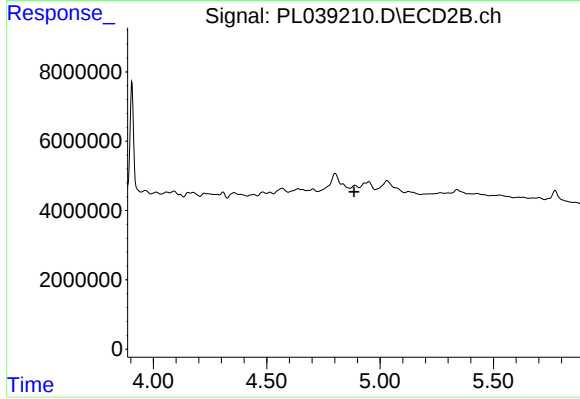

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

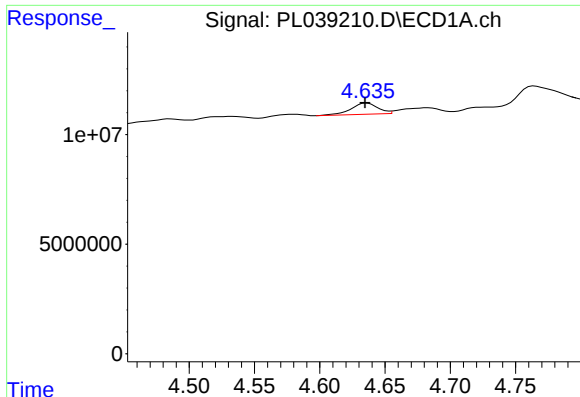

#24 Chlordane-2


R.T.: 4.636 min
Delta R.T.: 0.002 min
Response: 7387900
Conc: 21.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

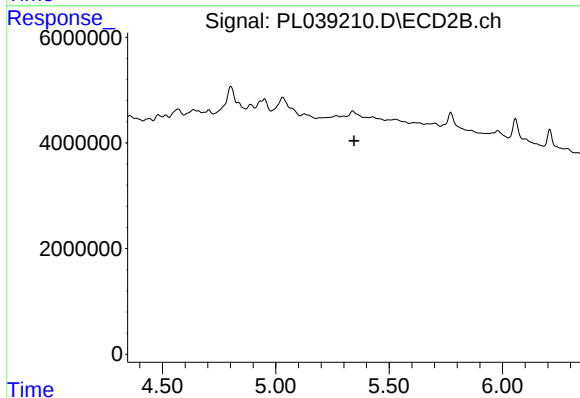


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

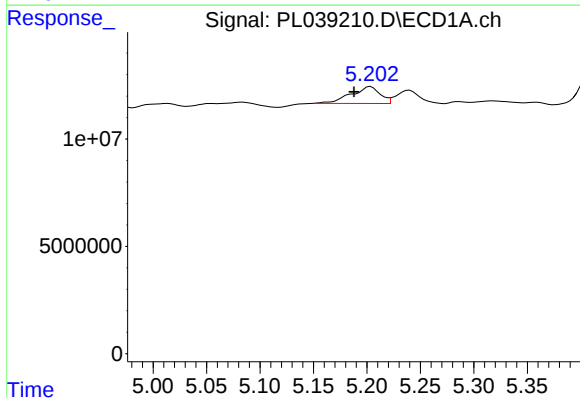


#25 Chlordane-3

R.T.: 5.204 min
Delta R.T.: 0.016 min
Response: 14777816
Conc: 13.53 ng/ml

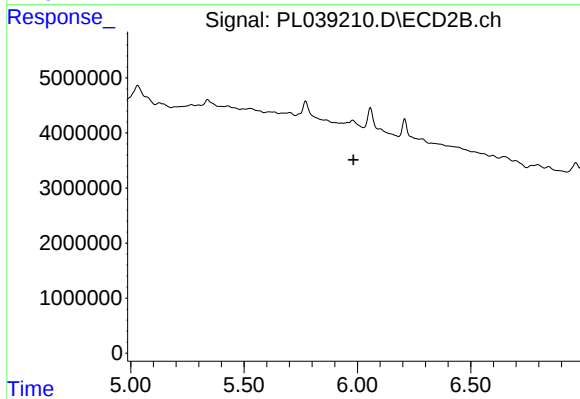

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

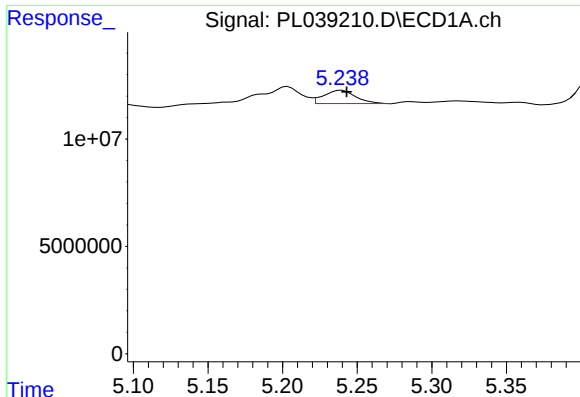

#26 Chlordane-4


R.T.: 5.240 min
Delta R.T.: -0.003 min
Response: 9205073
Conc: 9.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

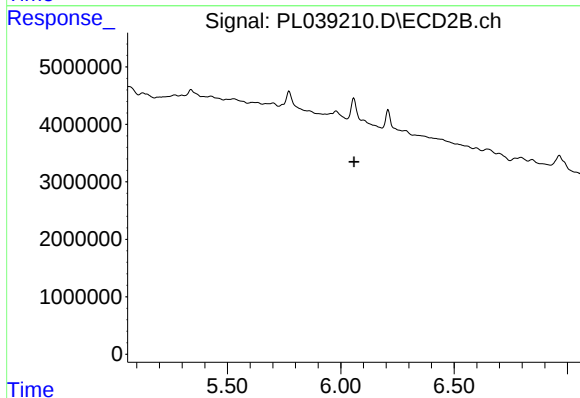


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.058 min
Response: 0
Conc: N.D.

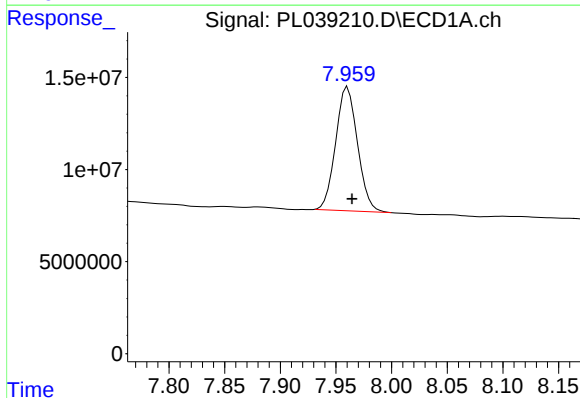

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 91664043
Conc: 13.05 ng/ml

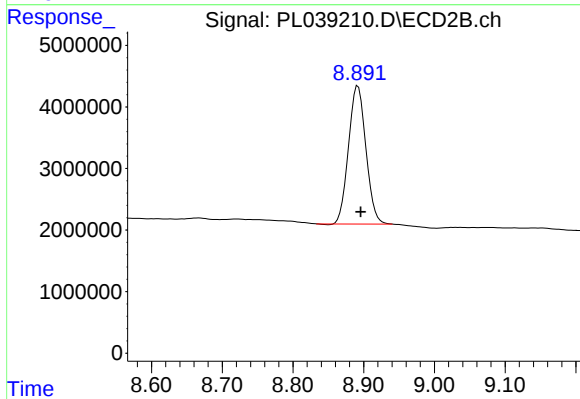

#28 Decachlorobiphenyl

R.T.: 8.892 min
Delta R.T.: -0.004 min
Response: 38334686
Conc: 16.52 ng/ml