

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
 Data File : PL039220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 18:57
 Operator : AJ\SJ
 Sample : J4499-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 04:37:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.906	78807883	32376581	11.274	12.077
28)	SA Decachlor...	7.961	8.894	90126388	35210786	12.832	15.173
Target Compounds							
2)	A alpha-BHC	3.688f	0.000	17421623	0	1.474	N.D. #
6)	B beta-BHC	4.217f	0.000	11499807	0	2.475	N.D. #
12)	B 4,4'-DDE	5.410	6.211	50136465	16735903	5.236	5.413
13)	MA Dieldrin	5.533	0.000	10541094	0	1.081	N.D. #
14)	MA Endrin	5.848f	0.000	2478237	0	0.277	N.D. #
15)	B Endosulfa...	6.047	0.000	5361401	0	0.617	N.D. #
17)	MA 4,4'-DDT	6.152	0.000	34364984	0	4.533	N.D. #
18)	B Endrin al...	6.190f	0.000	1205802	0	0.178	N.D. #
20)	A Methoxychlor	6.676	0.000	7533552	0	1.841	N.D. #
23)	Chlordane-1	4.075	0.000	22840514	0	72.146	N.D. #
27)	Chlordane-5	6.047	0.000	5361401	0	16.531	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
Data File : PL039220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 18:57
Operator : AJ\SJ
Sample : J4499-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:37:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

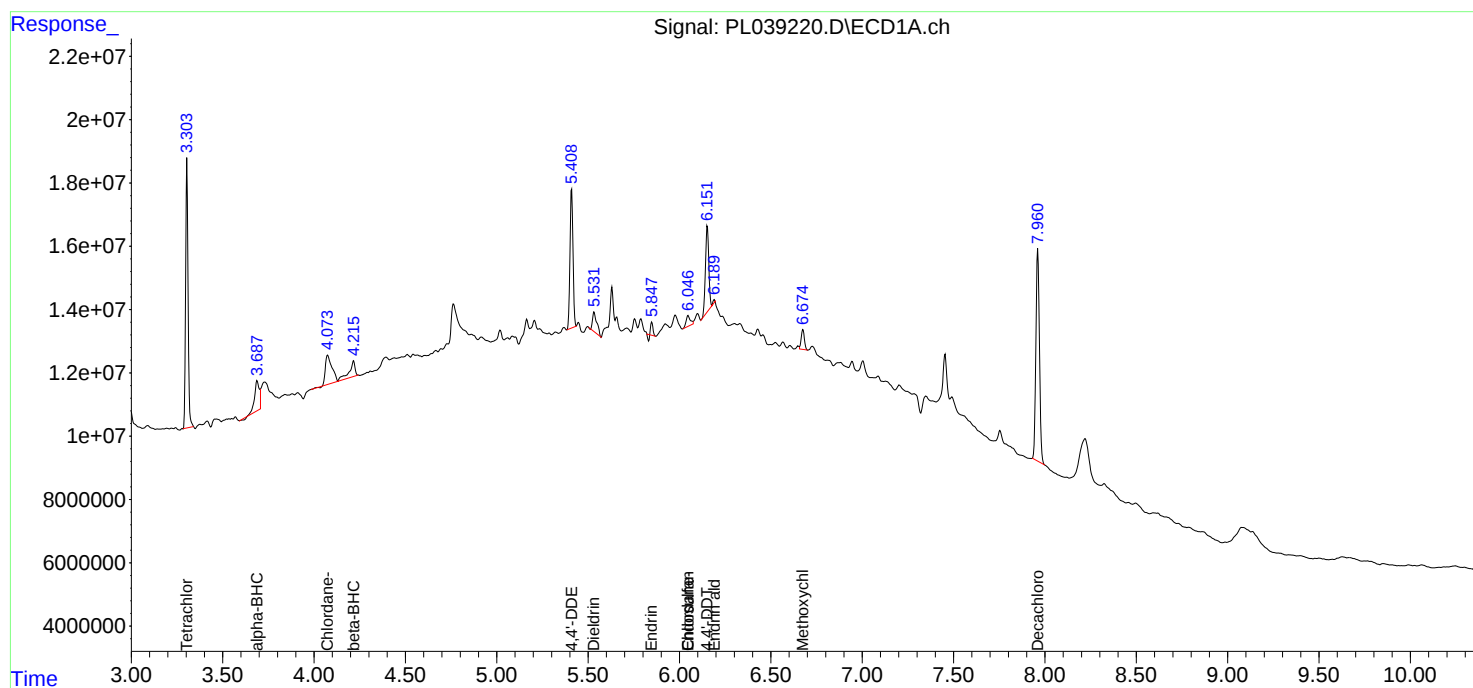


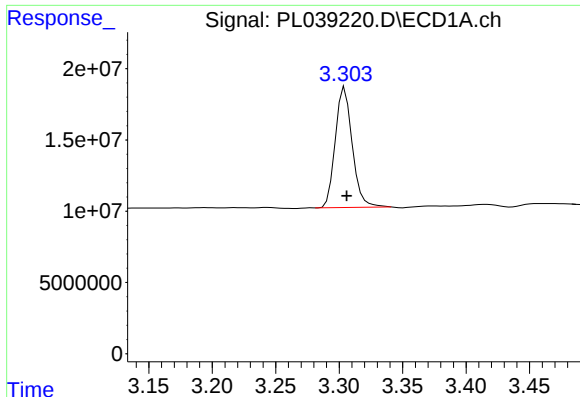

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 78807883
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

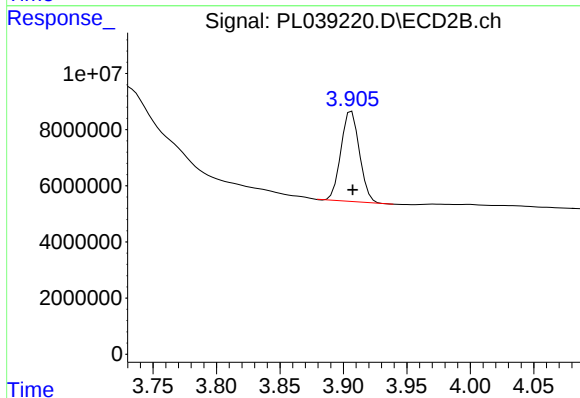


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 32376581
Conc: 12.08 ng/ml

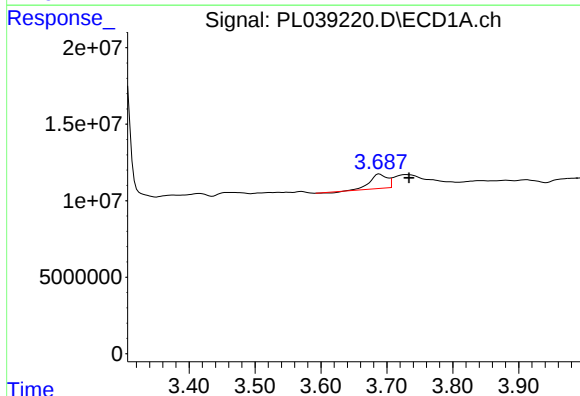


#2 alpha-BHC

R.T.: 3.688 min
Delta R.T.: -0.045 min
Response: 17421623
Conc: 1.47 ng/ml

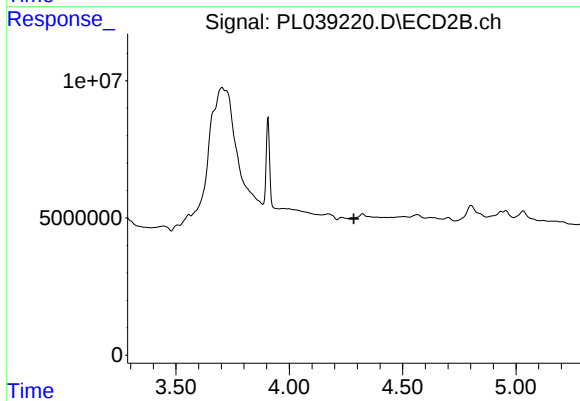

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

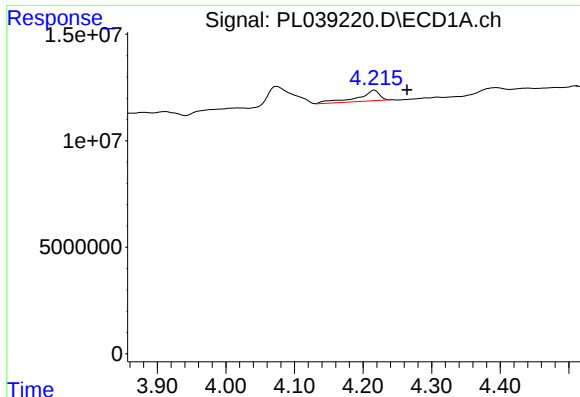

#6 beta-BHC


R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 11499807
Conc: 2.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

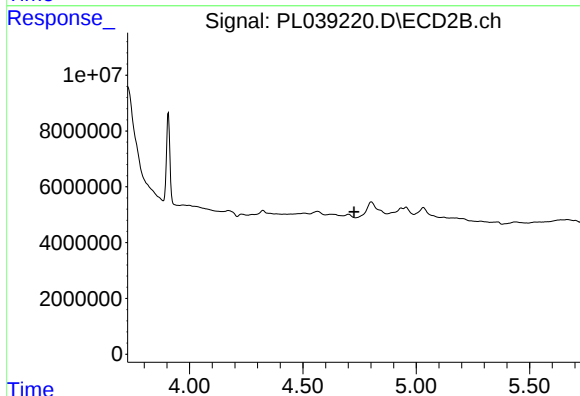


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

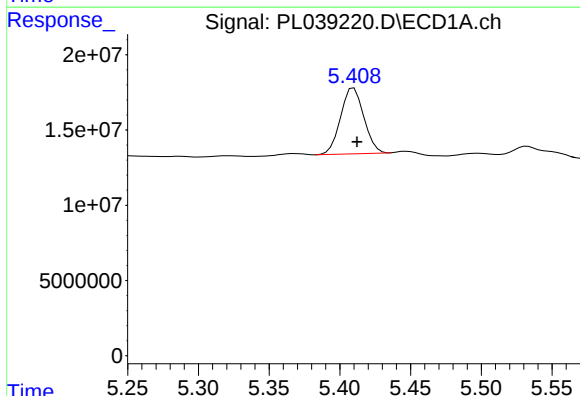


#12 4,4'-DDE

R.T.: 5.410 min
Delta R.T.: -0.002 min
Response: 50136465
Conc: 5.24 ng/ml

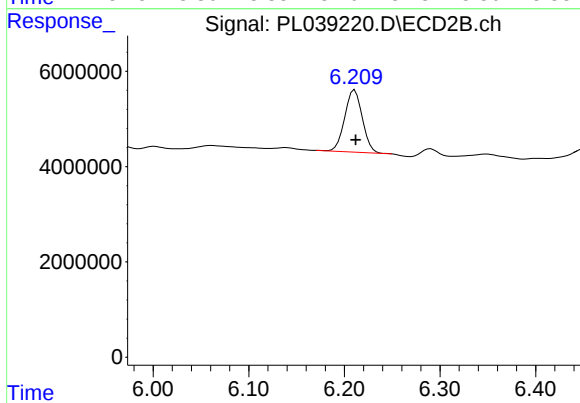

#12 4,4'-DDE


R.T.: 6.211 min
Delta R.T.: -0.001 min
Response: 16735903
Conc: 5.41 ng/ml

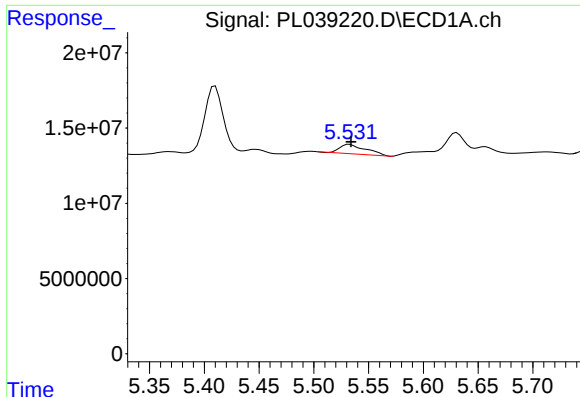

#13 Dieldrin


R.T.: 5.533 min
Delta R.T.: -0.001 min
Response: 10541094
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

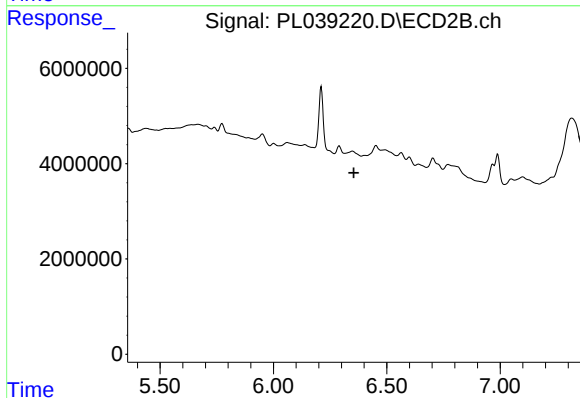


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

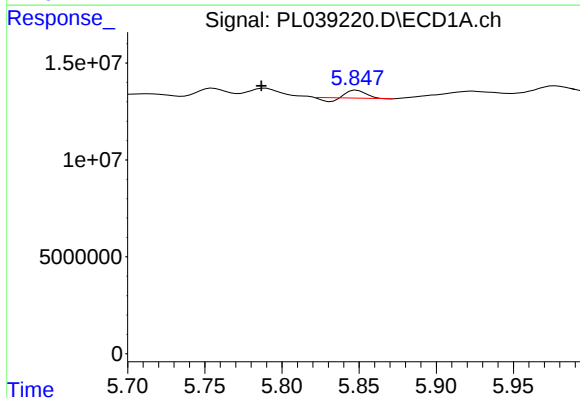


#14 Endrin

R.T.: 5.848 min
Delta R.T.: 0.062 min
Response: 2478237
Conc: 0.28 ng/ml

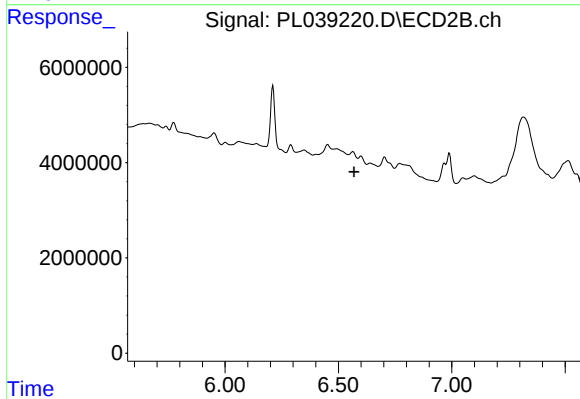

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.570 min
Response: 0
Conc: N.D.

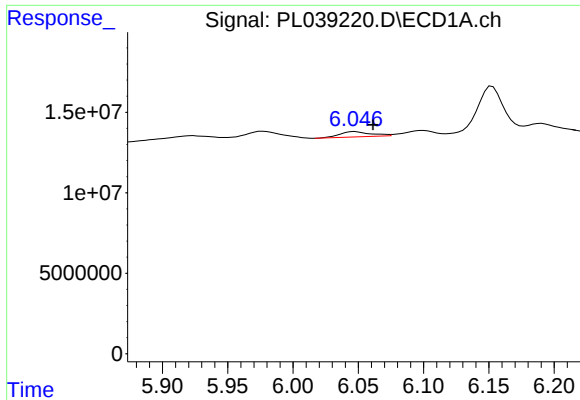

#15 Endosulfan II


R.T.: 6.047 min
Delta R.T.: -0.014 min
Response: 5361401
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

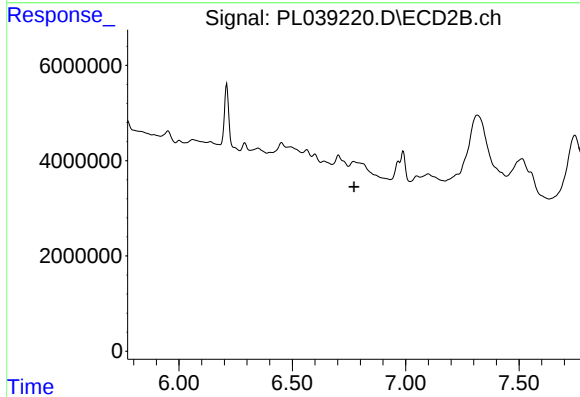


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

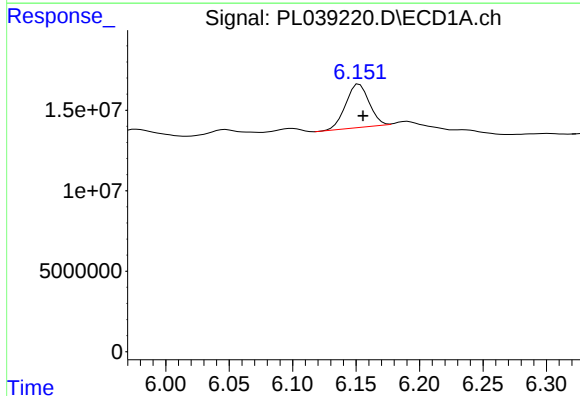


#17 4,4'-DDT

R.T.: 6.152 min
Delta R.T.: -0.003 min
Response: 34364984
Conc: 4.53 ng/ml

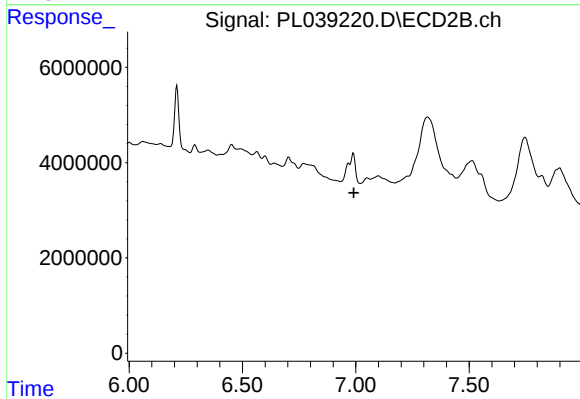

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

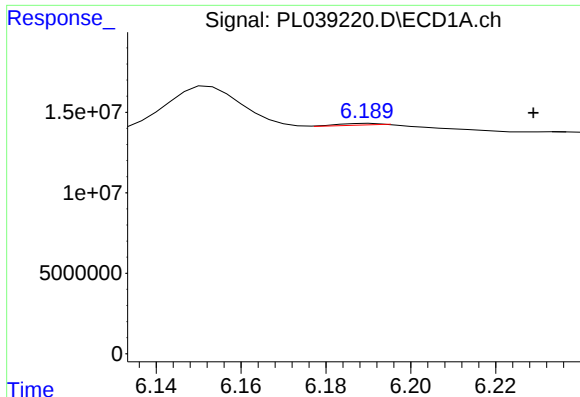

#18 Endrin aldehyde


R.T.: 6.190 min
Delta R.T.: -0.039 min
Response: 1205802
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

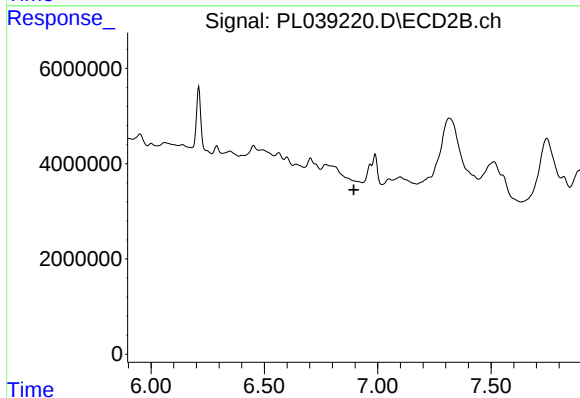


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

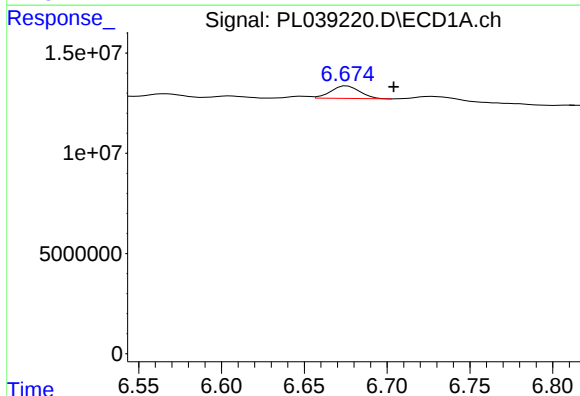


#20 Methoxychlor

R.T.: 6.676 min
Delta R.T.: -0.028 min
Response: 7533552
Conc: 1.84 ng/ml

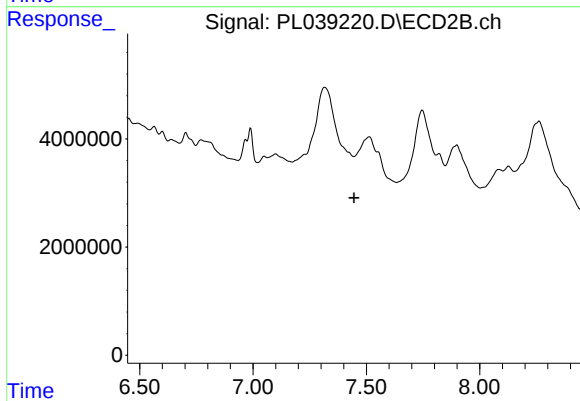

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

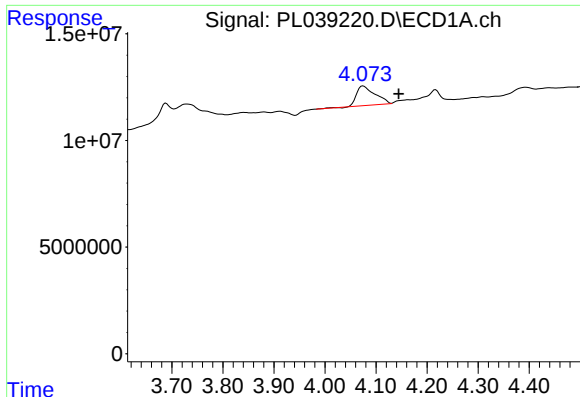

#23 Chlordane-1


R.T.: 4.075 min
Delta R.T.: -0.070 min
Response: 22840514
Conc: 72.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

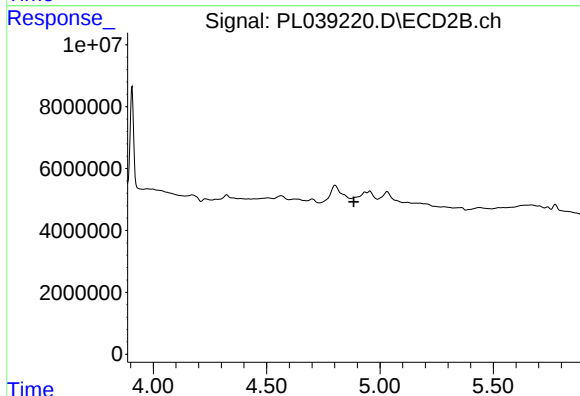


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

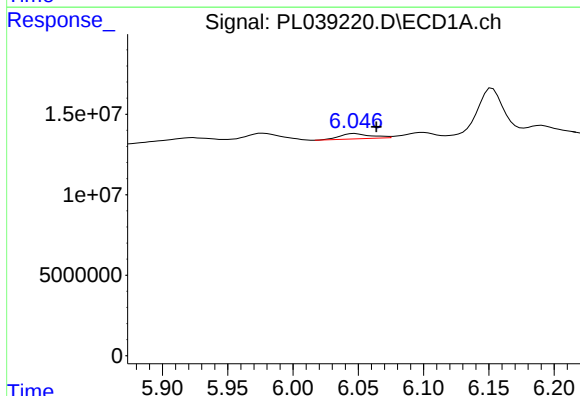


#27 Chlordane-5

R.T.: 6.047 min
Delta R.T.: -0.017 min
Response: 5361401
Conc: 16.53 ng/ml

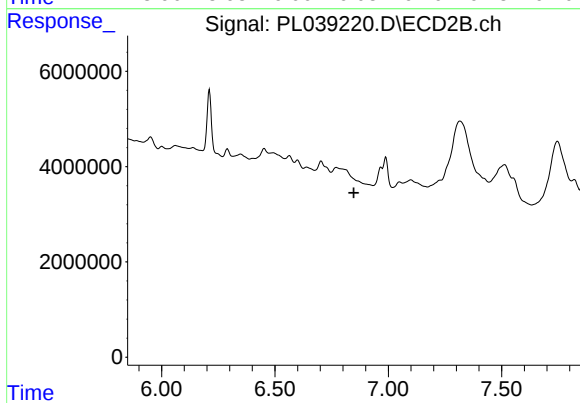

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

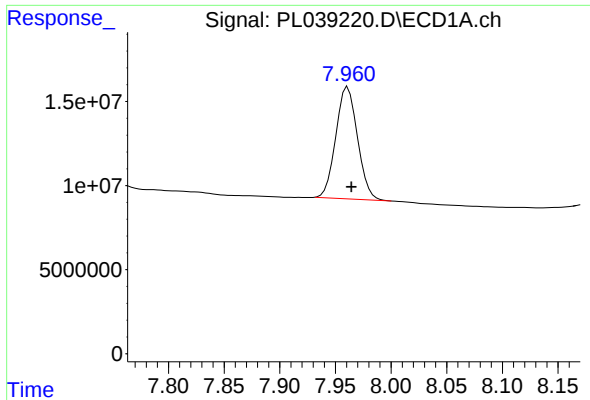

#28 Decachlorobiphenyl


R.T.: 7.961 min

Delta R.T.: -0.003 min

Response: 90126388

Conc: 12.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

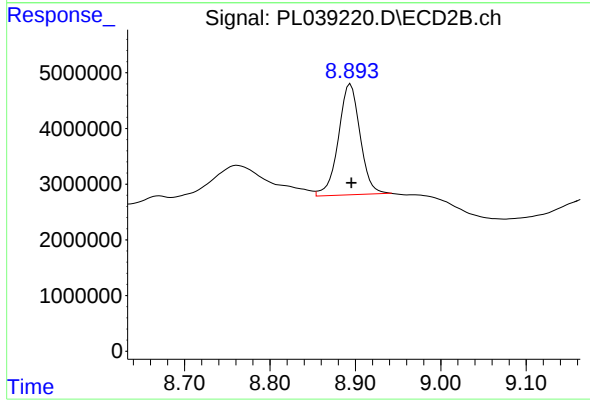

#28 Decachlorobiphenyl

R.T.: 8.894 min

Delta R.T.: -0.001 min

Response: 35210786

Conc: 15.17 ng/ml