

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
 Data File : PL039236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2018 22:44
 Operator : AJ\SJ
 Sample : J4500-16
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 04:38:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	120.8E6	49058701	17.277	18.299
28)	SA Decachlor...	7.962	8.894	122.5E6	47470593	17.445	20.456
Target Compounds							
3)	MA gamma-BHC...	4.047f	0.000	4424388	0	0.417	N.D. #
6)	B beta-BHC	4.219f	0.000	15007315	0	3.230	N.D. #
7)	B delta-BHC	0.000	4.932	0	9776195	N.D.	2.455 #
19)	B Endosulfa...	6.457	0.000	19036372	0	2.340	N.D. #
20)	A Methoxychlor	6.638f	0.000	26323064	0	6.432	N.D. #
23)	Chlordane-1	0.000	4.932	0	9776195	N.D.	78.250 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081618\
Data File : PL039236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2018 22:44
Operator : AJ\SJ
Sample : J4500-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 04:38:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

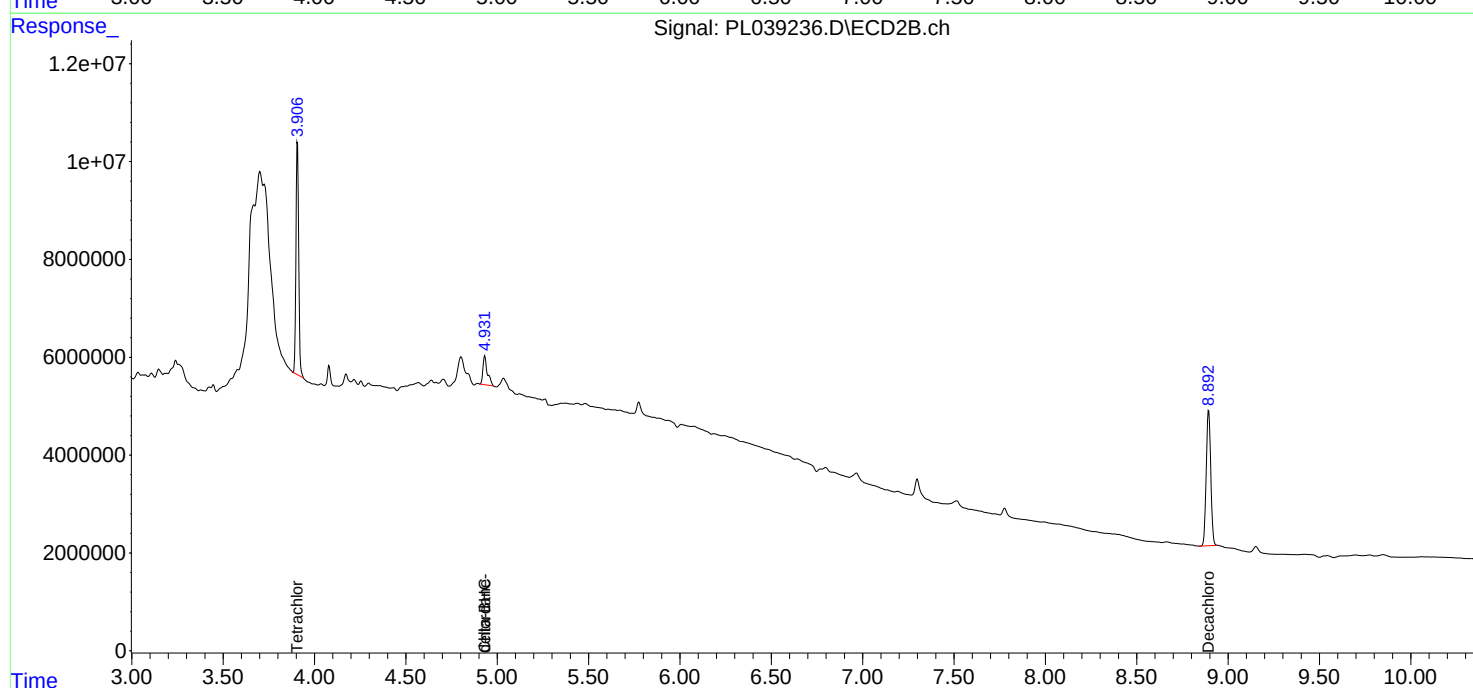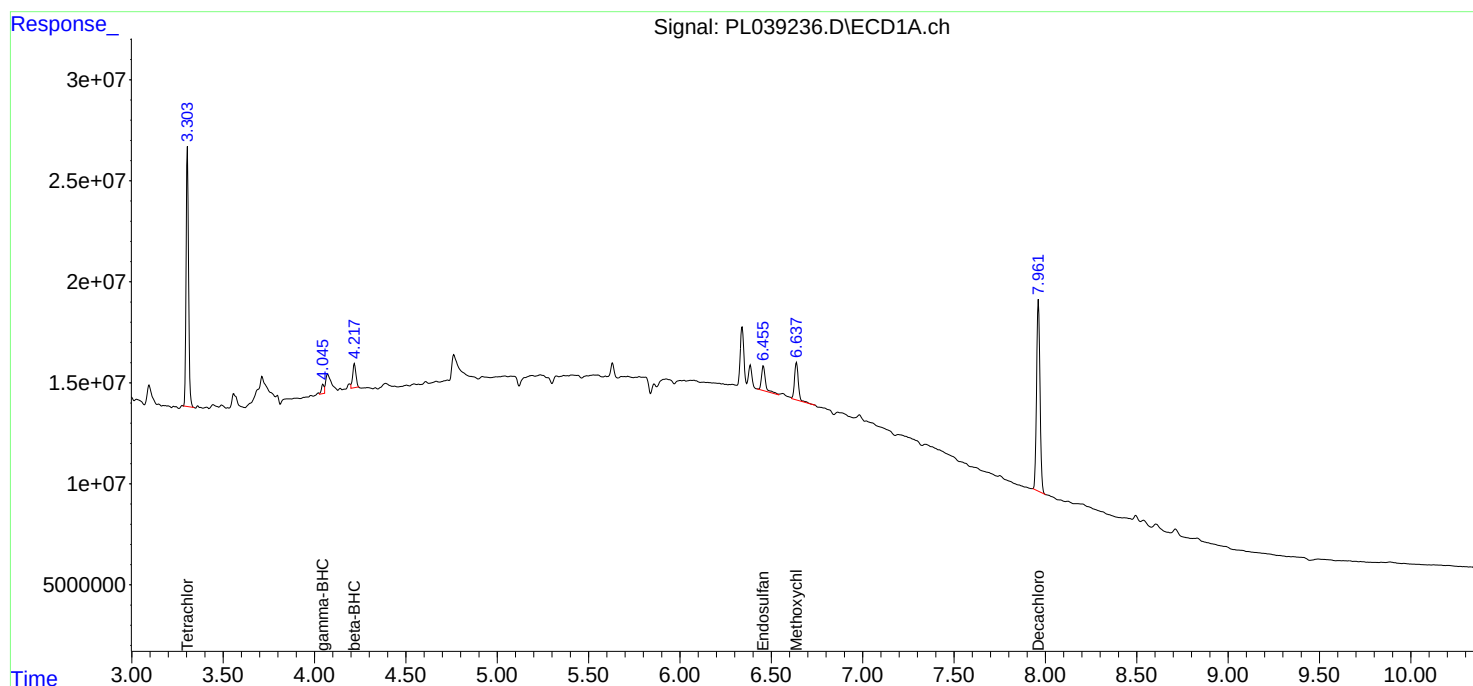


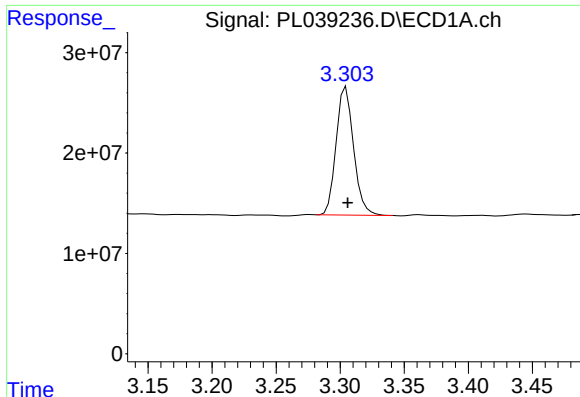

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 120776068
Conc: 17.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

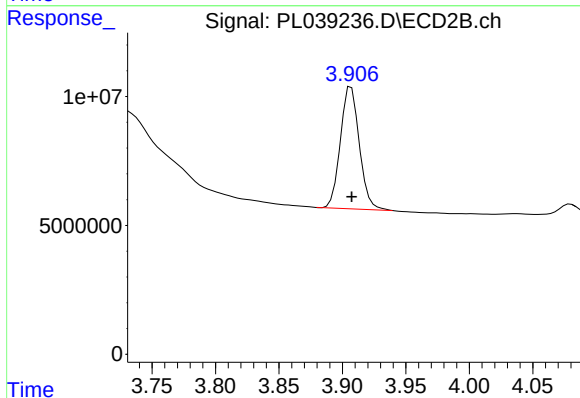


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 49058701
Conc: 18.30 ng/ml

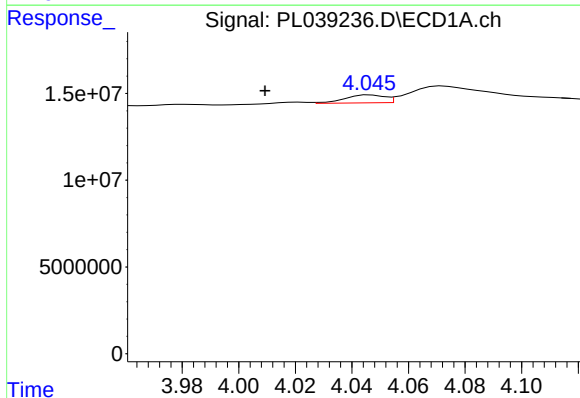


#3 gamma-BHC (Lindane)

R.T.: 4.047 min
Delta R.T.: 0.037 min
Response: 4424388
Conc: 0.42 ng/ml

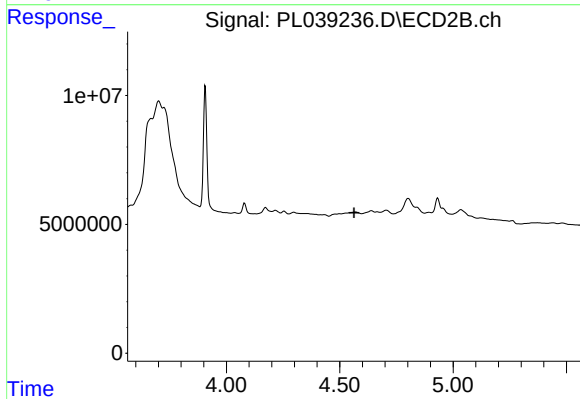

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

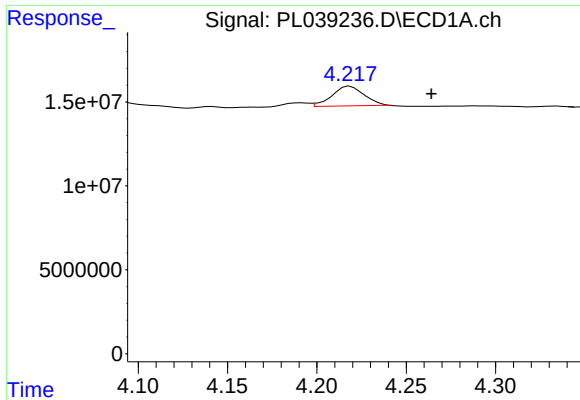

#6 beta-BHC


R.T.: 4.219 min
Delta R.T.: -0.045 min
Response: 15007315
Conc: 3.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

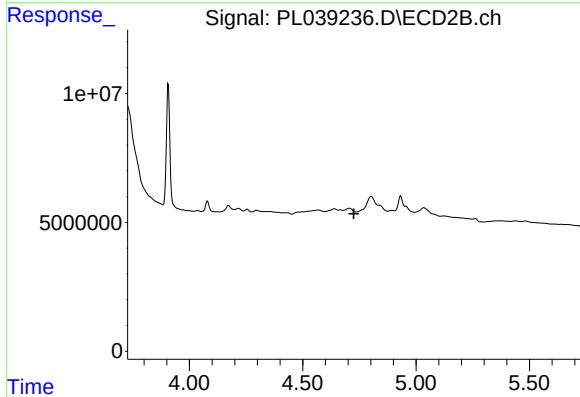


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

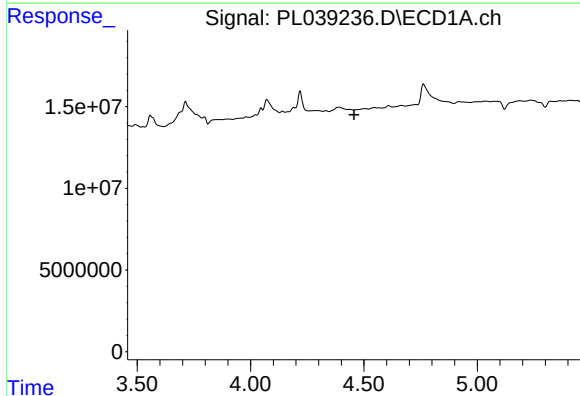


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

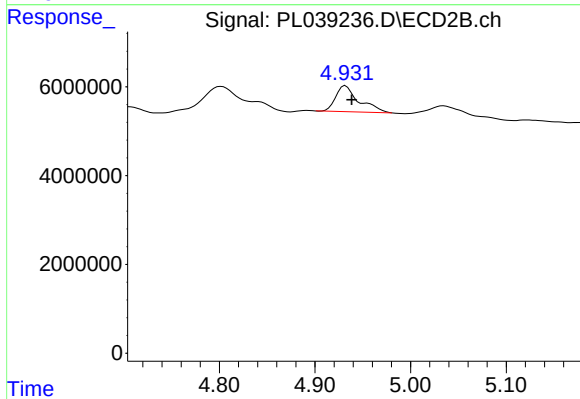

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 9776195
Conc: 2.46 ng/ml

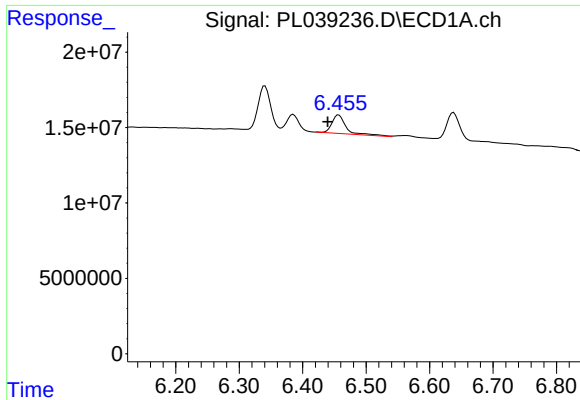

#19 Endosulfan Sulfate


R.T.: 6.457 min
Delta R.T.: 0.017 min
Response: 19036372
Conc: 2.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

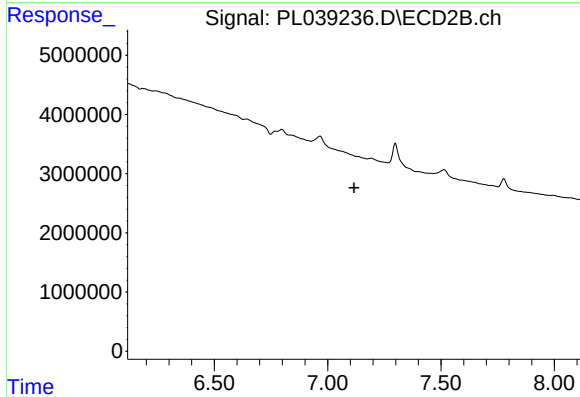


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

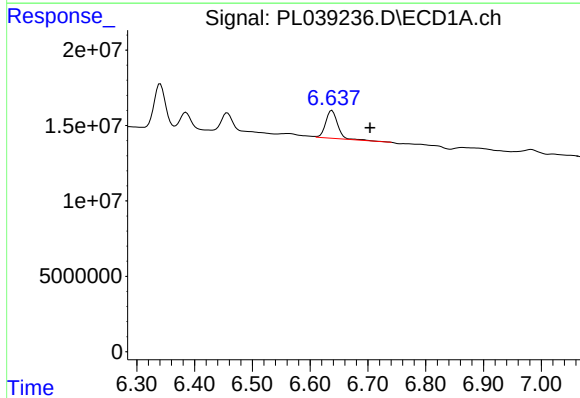


#20 Methoxychlor

R.T.: 6.638 min
Delta R.T.: -0.066 min
Response: 26323064
Conc: 6.43 ng/ml

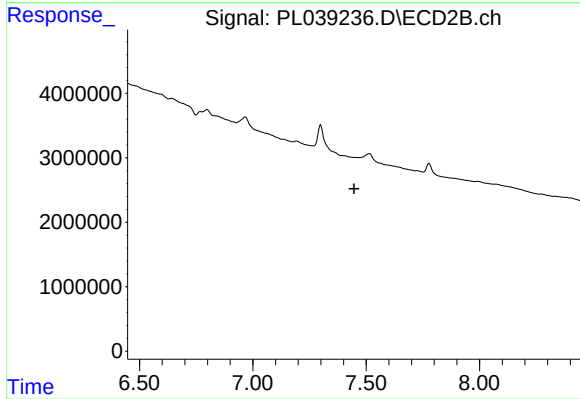

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

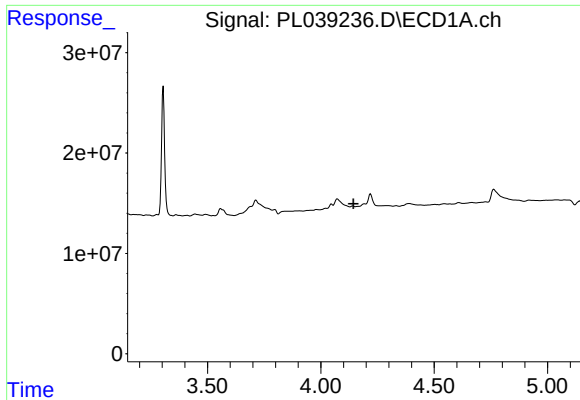

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

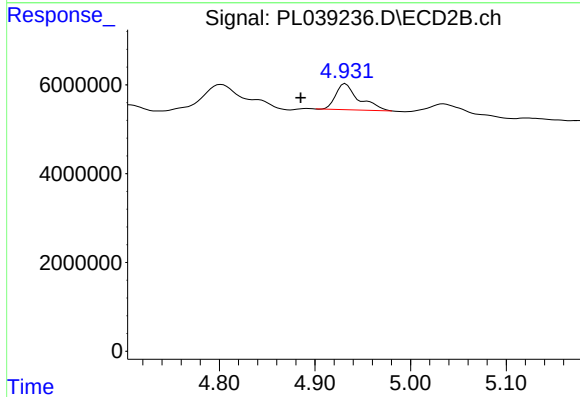


#23 Chlordane-1

R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 9776195
Conc: 78.25 ng/ml

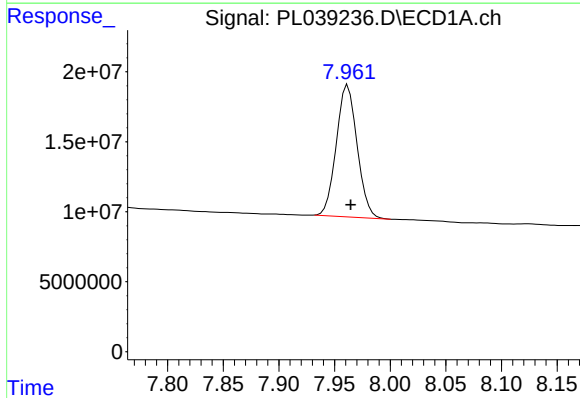

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.002 min
Response: 122526263
Conc: 17.45 ng/ml

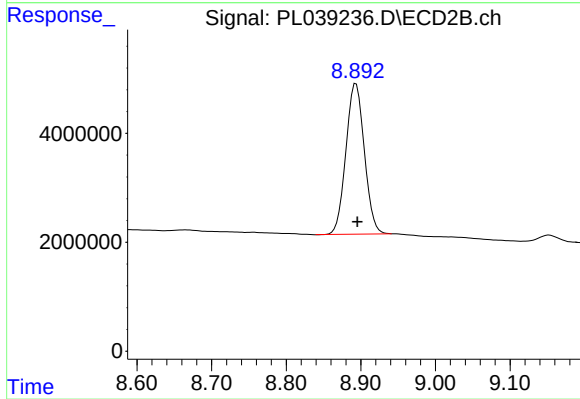

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 47470593
Conc: 20.46 ng/ml