

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
 Data File : PL051566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 08:52
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:44:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.926	261.6E6	63996107	26.038	22.430
28)	SA Decachlor...	7.976	8.952	263.8E6	67914209	26.054	24.016
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	5213006	N.D.	3.015 #
8)	B Heptachlo...	4.986	0.000	4949105	0	0.335	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
Data File : PL051566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 08:52
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:44:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

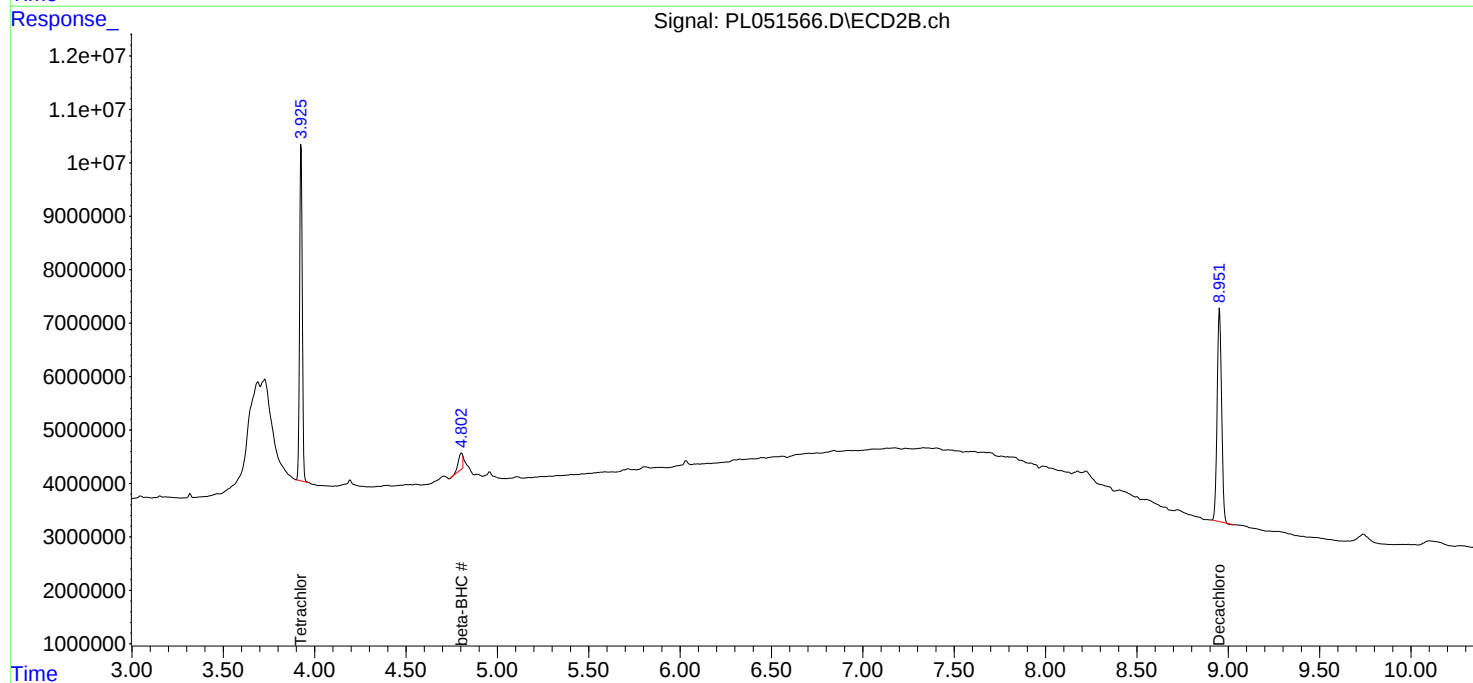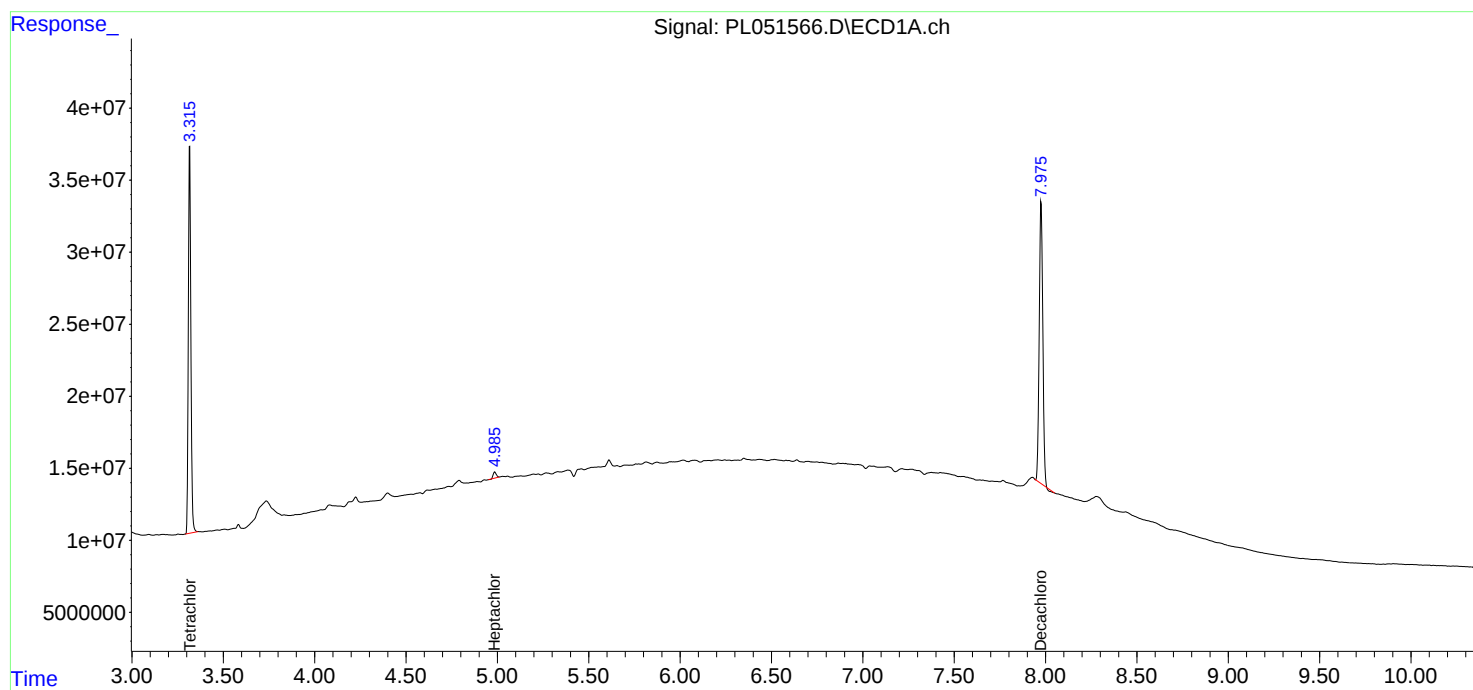


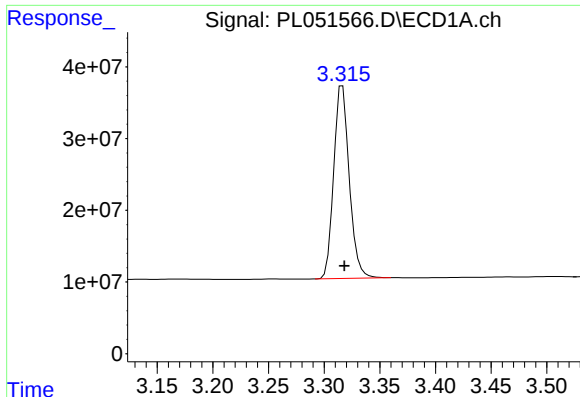

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 261622656
Conc: 26.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

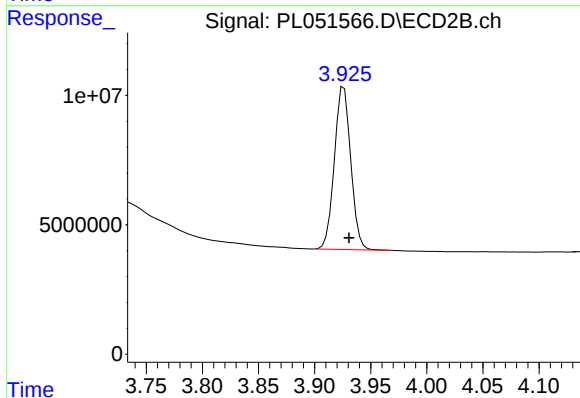


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 63996107
Conc: 22.43 ng/ml

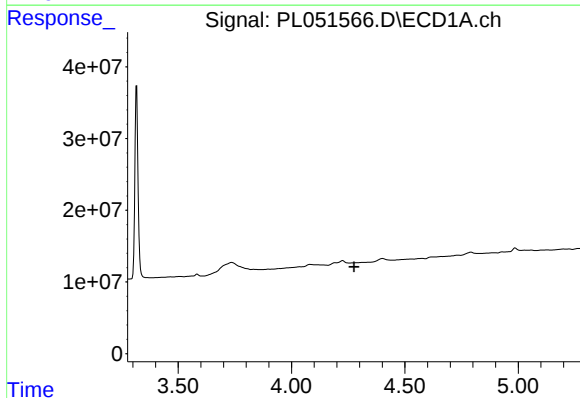


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

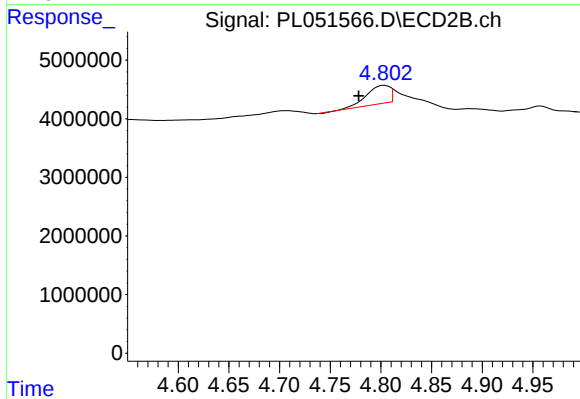

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 5213006
Conc: 3.02 ng/ml

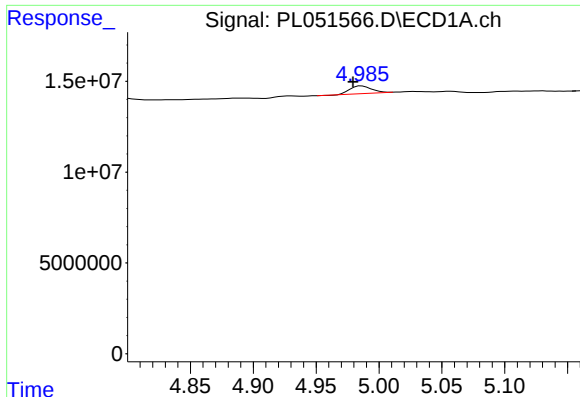

#8 Heptachlor epoxide


R.T.: 4.986 min
Delta R.T.: 0.007 min
Response: 4949105
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

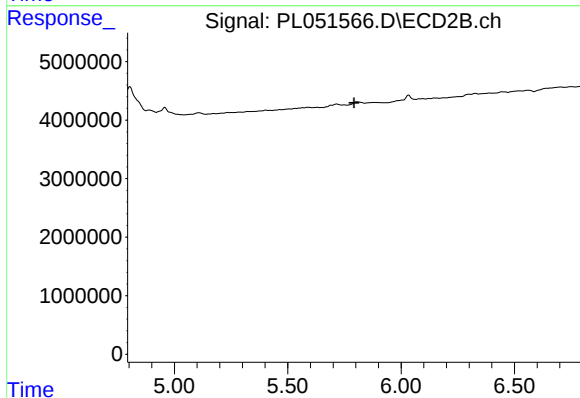


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

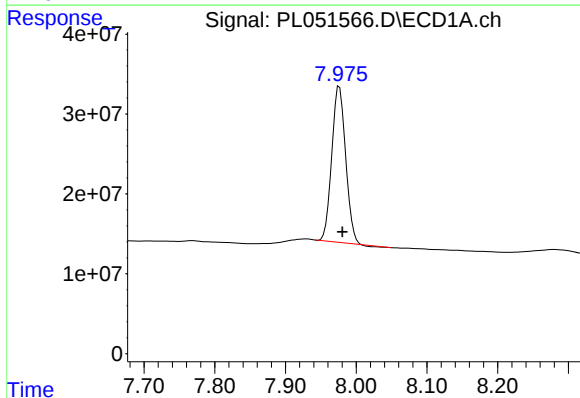

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.004 min
Response: 263807224
Conc: 26.05 ng/ml

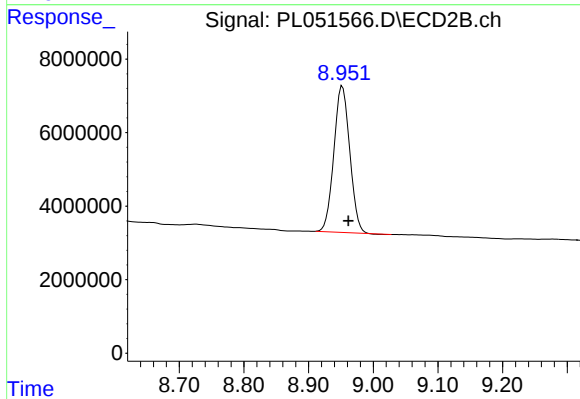

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: -0.009 min
Response: 67914209
Conc: 24.02 ng/ml