

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
 Data File : PL051570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 10:50
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:45:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	3.927	237.1E6	62821995	23.594	22.018
28)	SA Decachlor...	7.983	8.957	273.0E6	68175013	26.965	24.108
Target Compounds							
3)	MA gamma-BHC...	0.000	4.622f	0	1737913	N.D.	0.449 #
8)	B Heptachlo...	4.996f	0.000	5584325	0	0.378	N.D. #
10)	B gamma-Chl...	5.204	0.000	8277968	0	0.524	N.D. #
11)	B alpha-Chl...	5.272	0.000	3211515	0	0.211	N.D. #
25)	Chlordane-3	5.204	0.000	8277968	0	5.914	N.D. #
26)	Chlordane-4	5.272	0.000	3211515	0	2.435	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
Data File : PL051570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 10:50
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:45:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

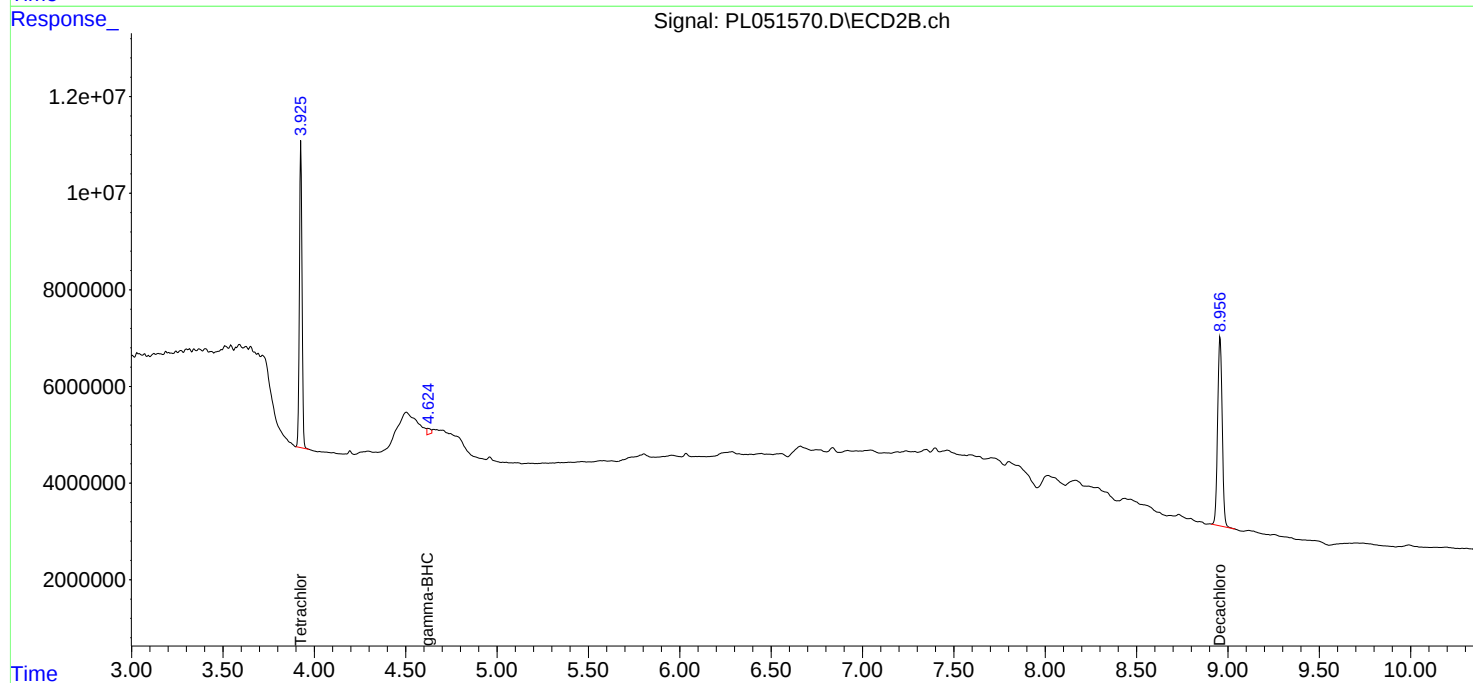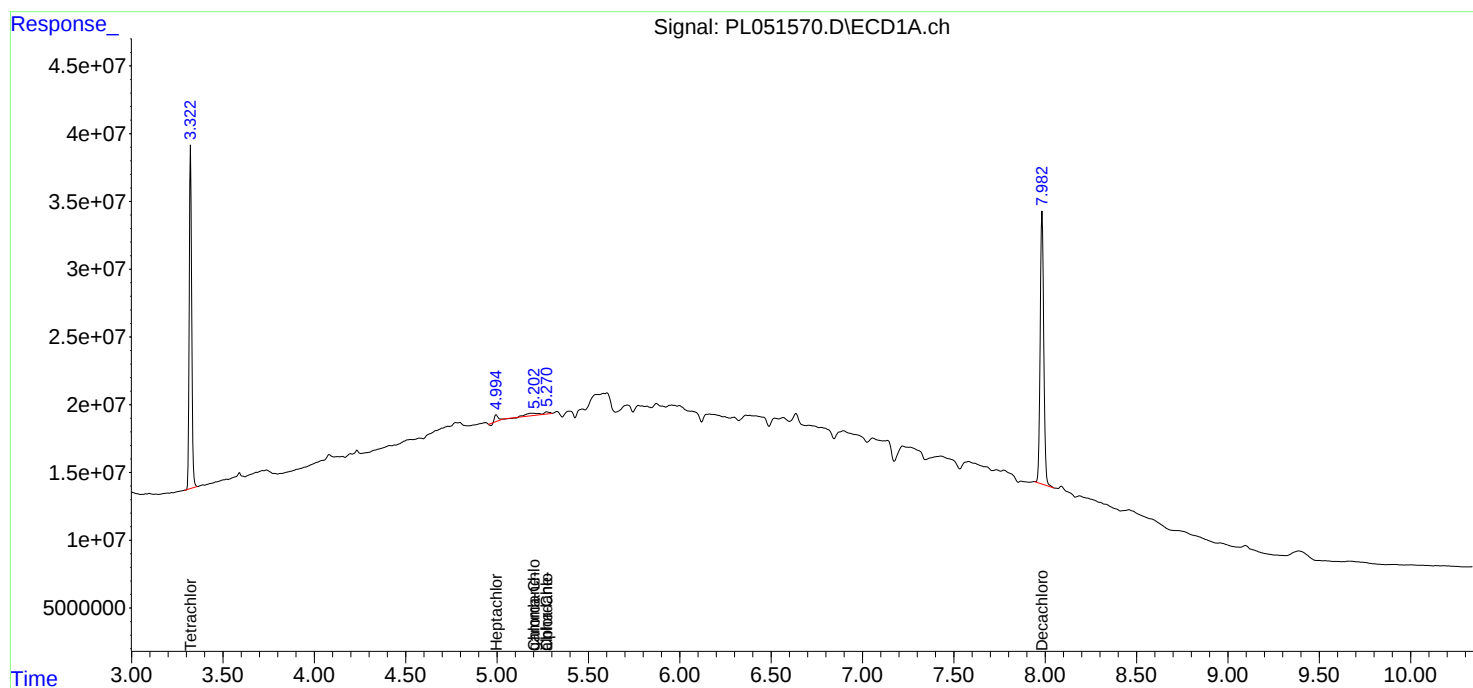


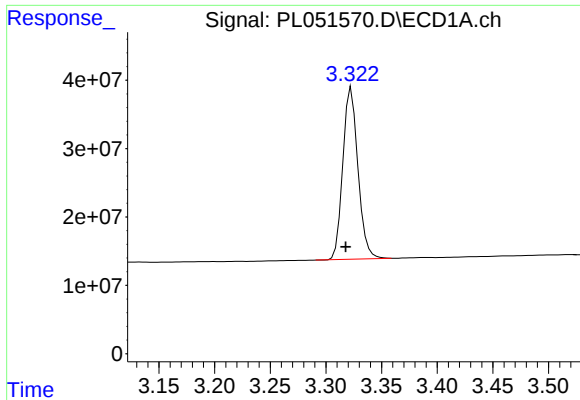

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.005 min
Response: 237073075
Conc: 23.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

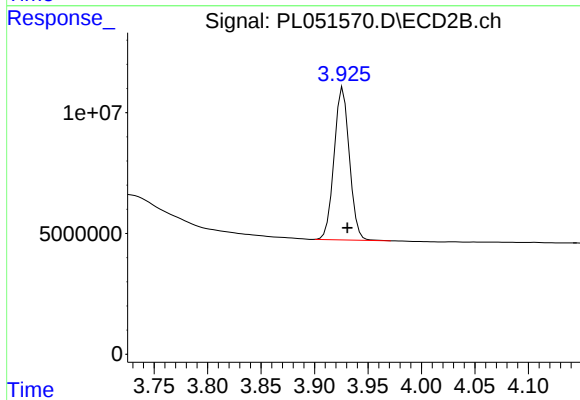


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 62821995
Conc: 22.02 ng/ml

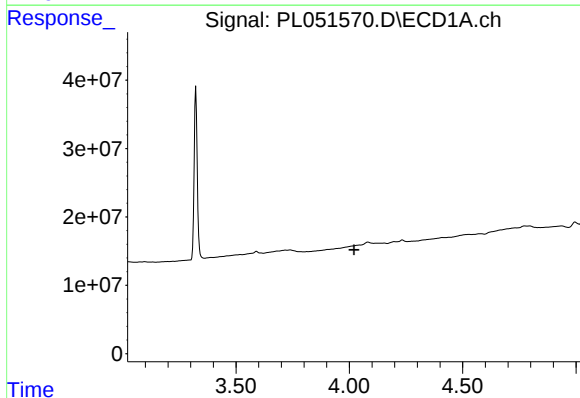


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.021 min
Response: 0
Conc: N.D.

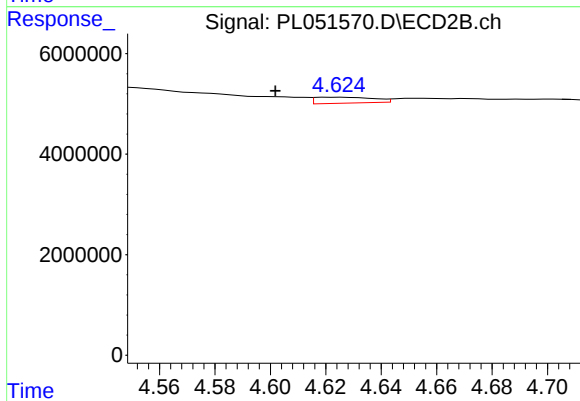

#3 gamma-BHC (Lindane)


R.T.: 4.622 min
Delta R.T.: 0.020 min
Response: 1737913
Conc: 0.45 ng/ml

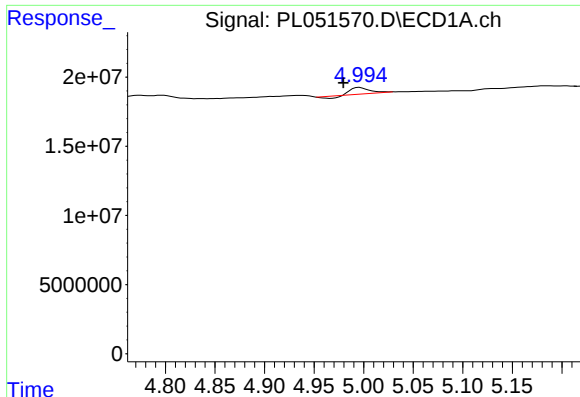

#8 Heptachlor epoxide


R.T.: 4.996 min
Delta R.T.: 0.016 min
Response: 5584325
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

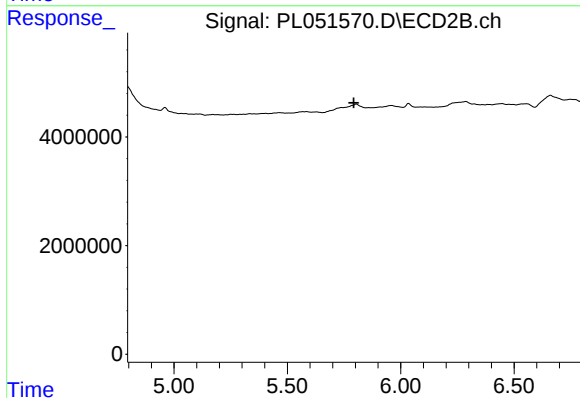


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.793 min
Response: 0
Conc: N.D.

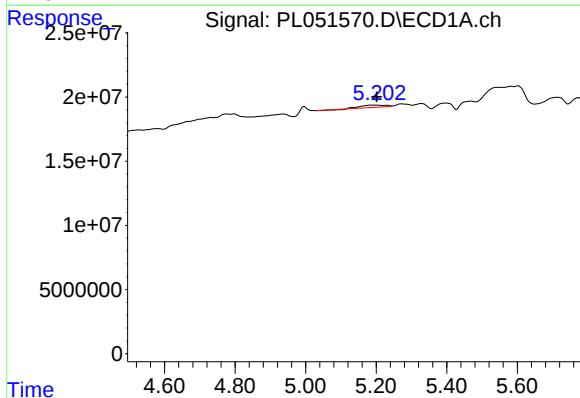


#10 gamma-Chlordane

R.T.: 5.204 min
Delta R.T.: 0.003 min
Response: 8277968
Conc: 0.52 ng/ml

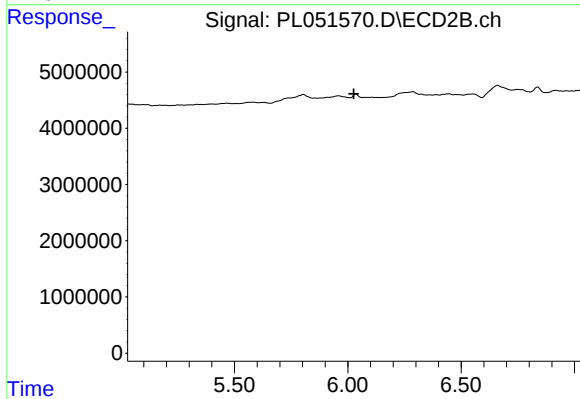

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

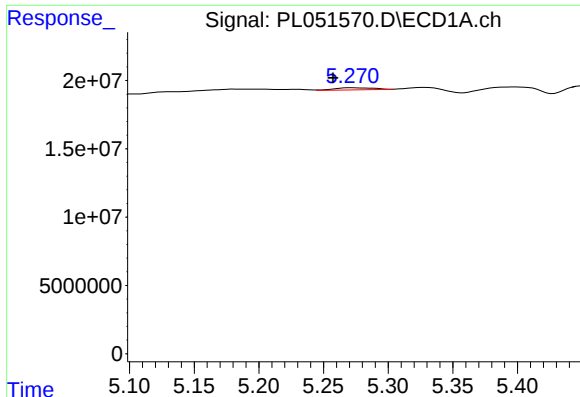

#11 alpha-Chlordane


R.T.: 5.272 min
Delta R.T.: 0.014 min
Response: 3211515
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

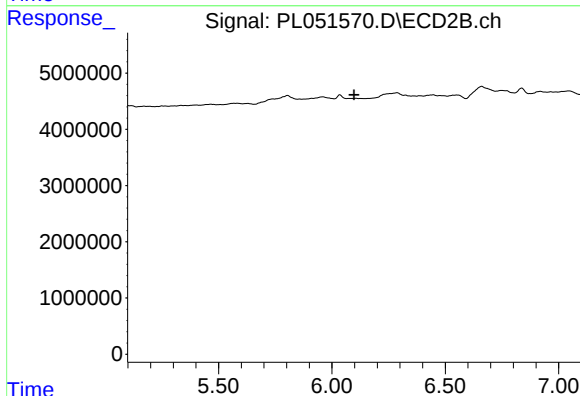


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

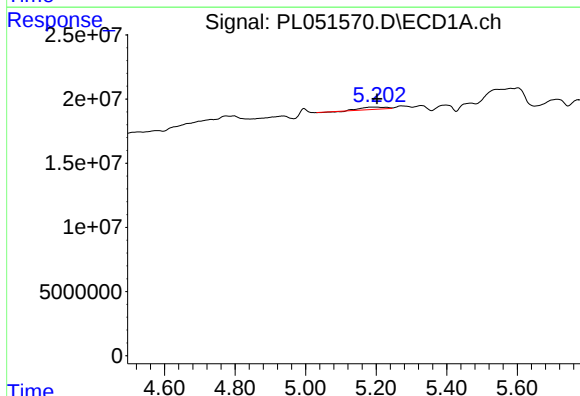


#25 Chlordane-3

R.T.: 5.204 min
Delta R.T.: 0.002 min
Response: 8277968
Conc: 5.91 ng/ml

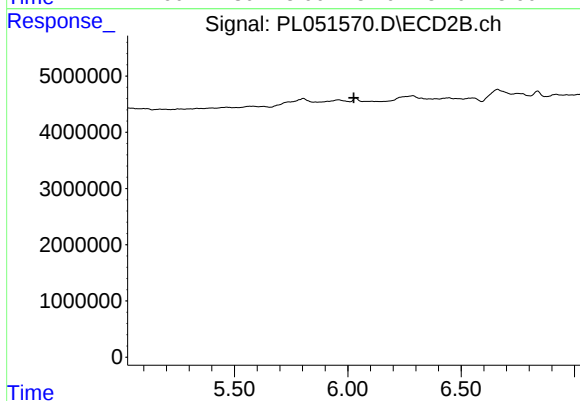

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

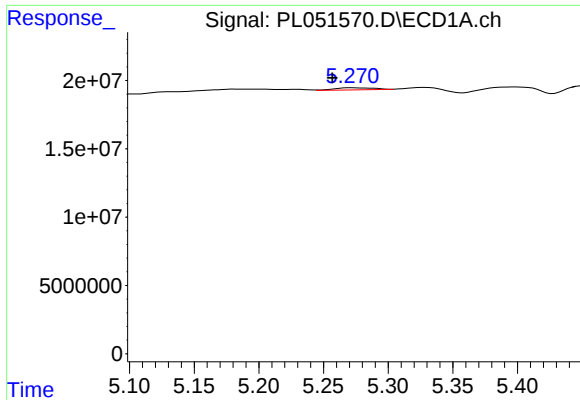

#26 Chlordane-4


R.T.: 5.272 min
Delta R.T.: 0.015 min
Response: 3211515
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

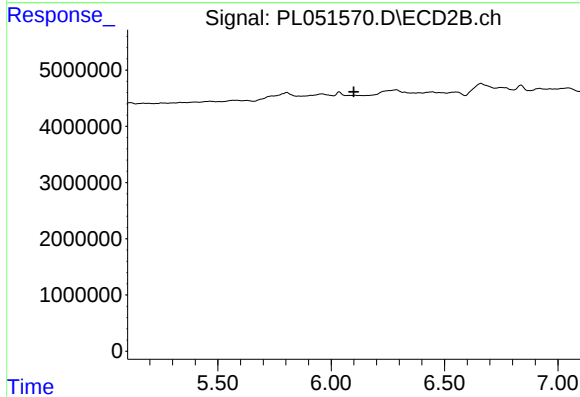


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

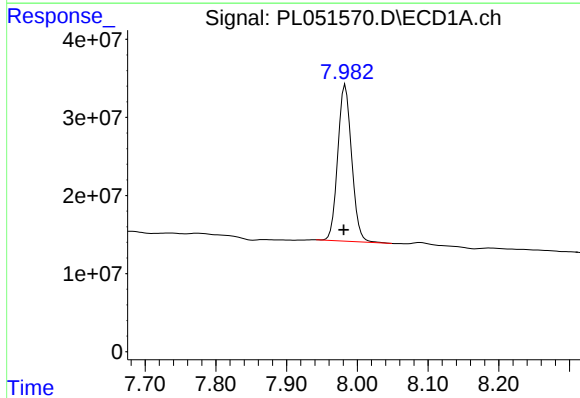

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: 0.003 min
Response: 273033062
Conc: 26.97 ng/ml

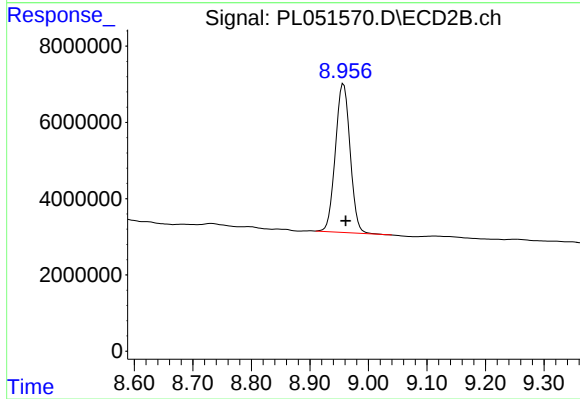

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.004 min
Response: 68175013
Conc: 24.11 ng/ml