

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
 Data File : PL051583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 16:20
 Operator : SG\AJ
 Sample : K4377-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RBR-29

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:47:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	191.0E6	47818830	19.009	16.760
28)	SA Decachlor...	7.973	8.953	122.2E6	31934563	12.065	11.293
Target Compounds							
2)	A alpha-BHC	0.000	4.338f	0	3012839	N.D.	0.730 #
6)	B beta-BHC	0.000	4.800f	0	4137795	N.D.	2.393 #
15)	B Endosulfa...	0.000	6.846	0	5724577	N.D.	1.801 #
20)	A Methoxychlor	6.685f	0.000	21371029	0	3.425	N.D. #
22)	Mirex	0.000	8.117f	0	11443748	N.D.	4.982 #
23)	Chlordane-1	4.184f	0.000	318959	0	0.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
Data File : PL051583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 16:20
Operator : SG\AJ
Sample : K4377-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RBR-29

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:47:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

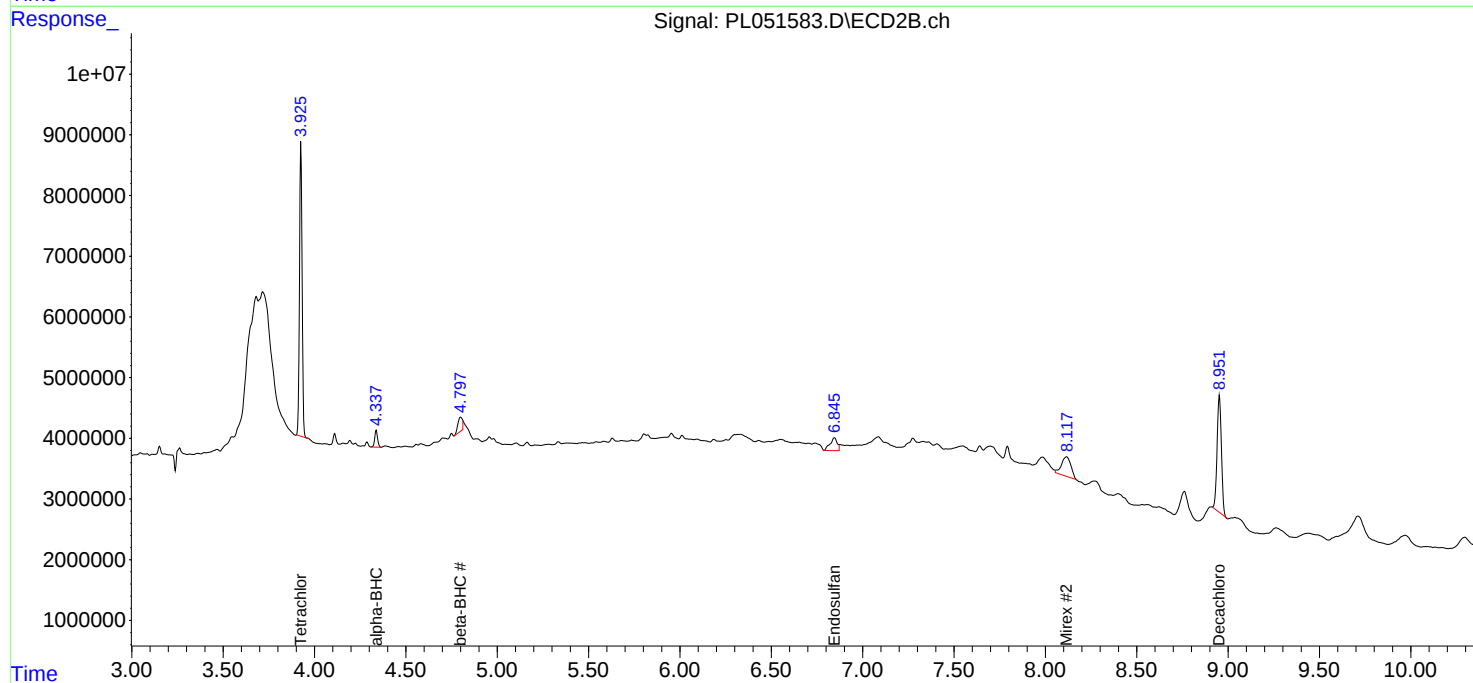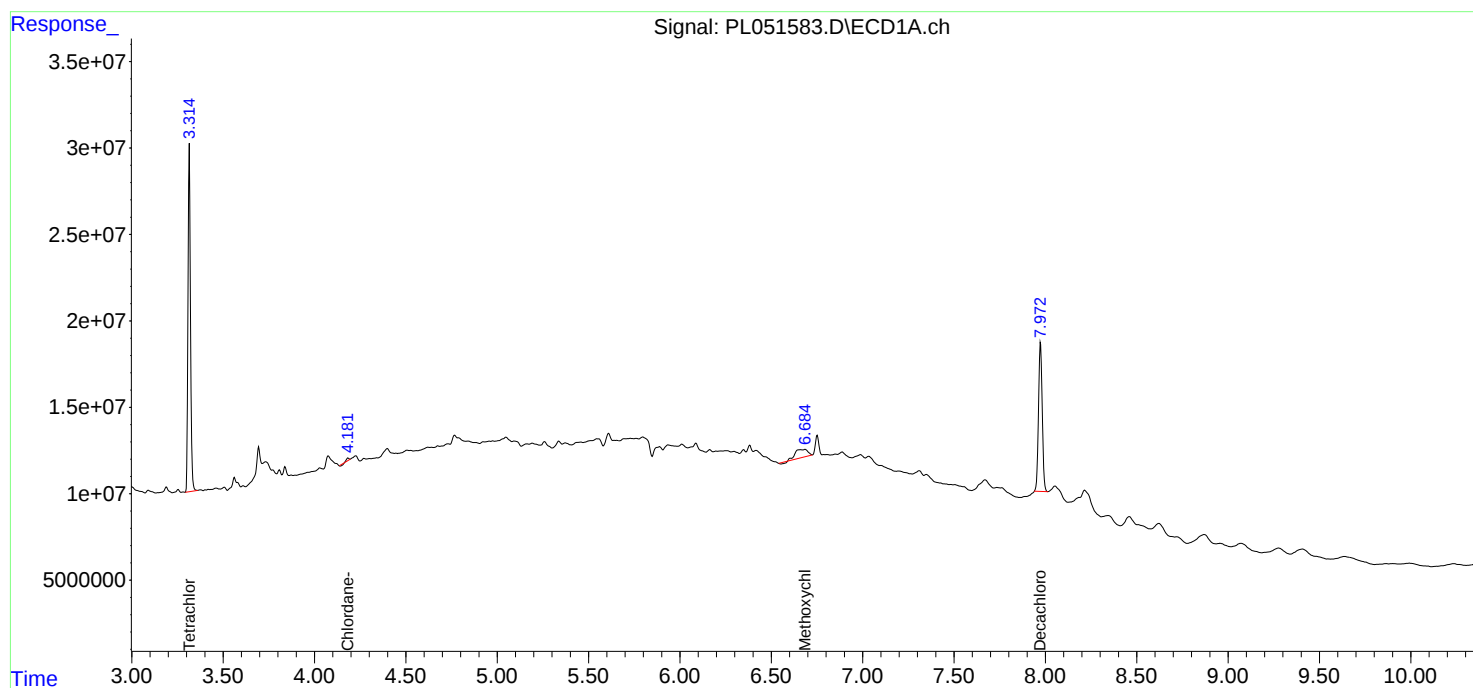


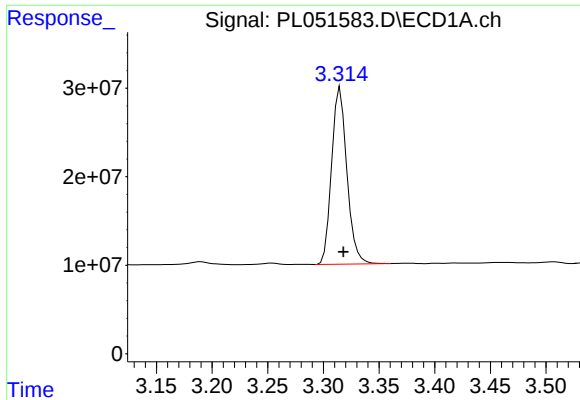

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 190997467
Conc: 19.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-29

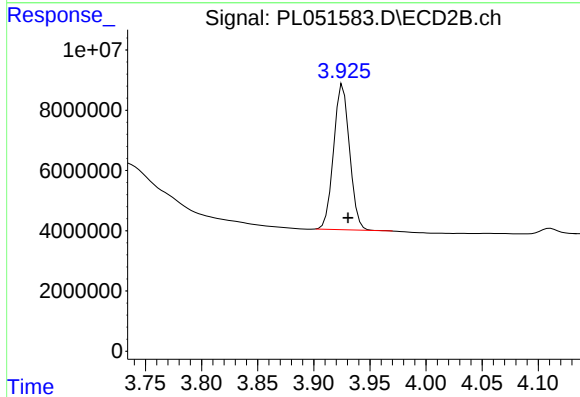


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 47818830
Conc: 16.76 ng/ml

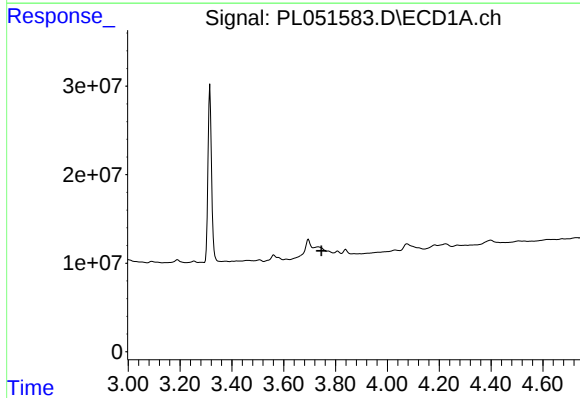


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.746 min
Response: 0
Conc: N.D.

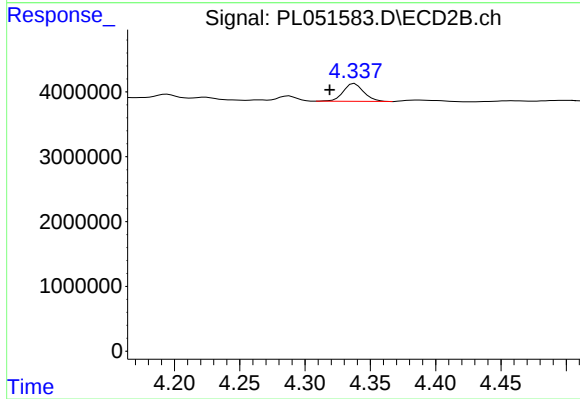

#2 alpha-BHC


R.T.: 4.338 min
Delta R.T.: 0.019 min
Response: 3012839
Conc: 0.73 ng/ml

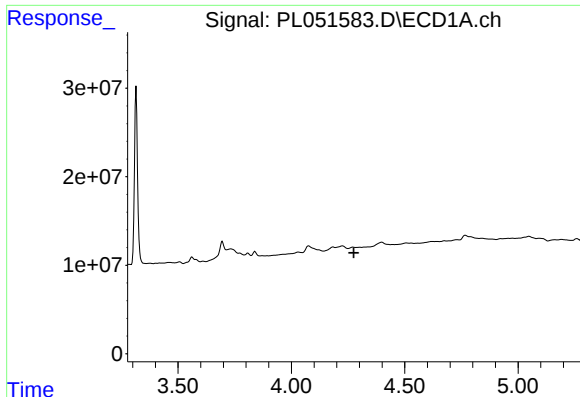

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RBR-29

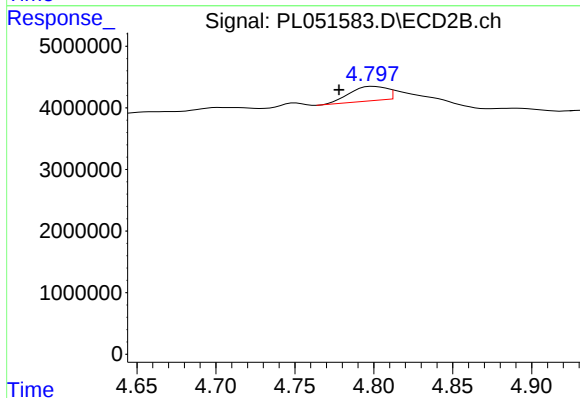


#6 beta-BHC

R.T.: 4.800 min
Delta R.T.: 0.022 min
Response: 4137795
Conc: 2.39 ng/ml

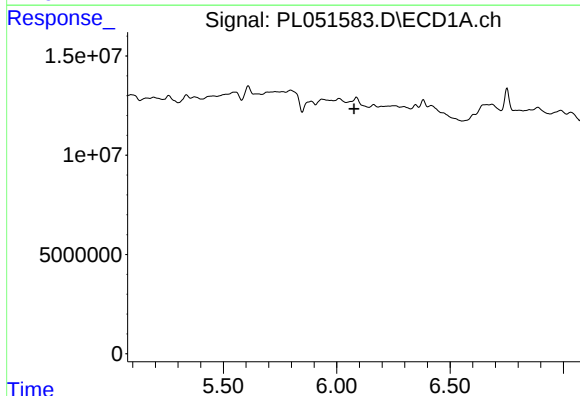


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

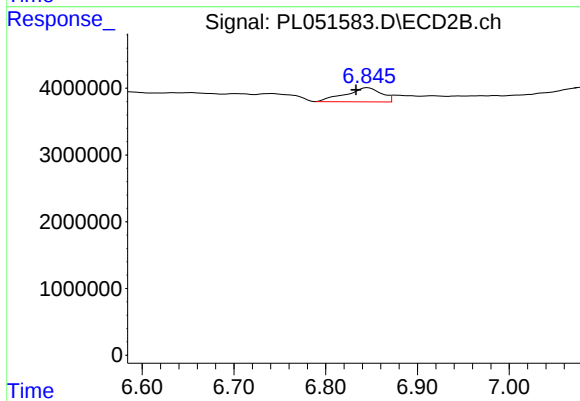

#15 Endosulfan II


R.T.: 6.846 min
Delta R.T.: 0.013 min
Response: 5724577
Conc: 1.80 ng/ml

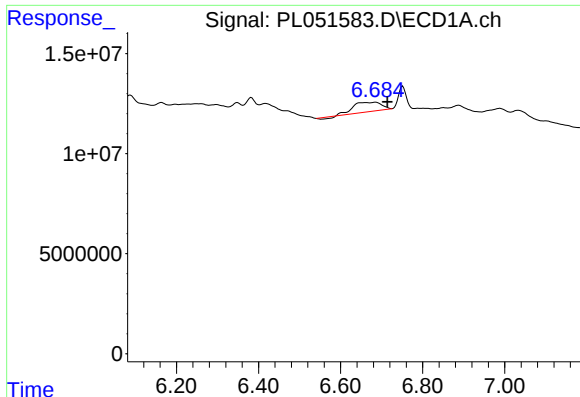

#20 Methoxychlor


R.T.: 6.685 min
Delta R.T.: -0.029 min
Response: 21371029
Conc: 3.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-29

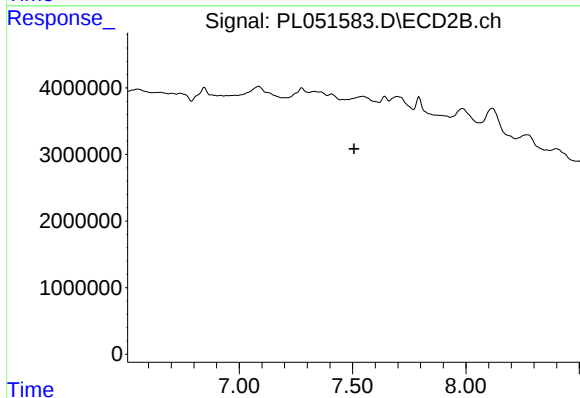


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

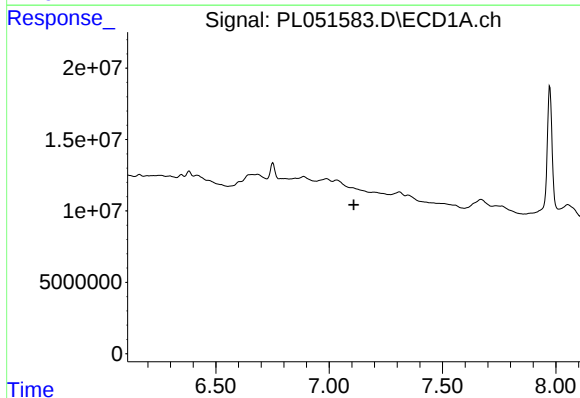


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.109 min
Response: 0
Conc: N.D.

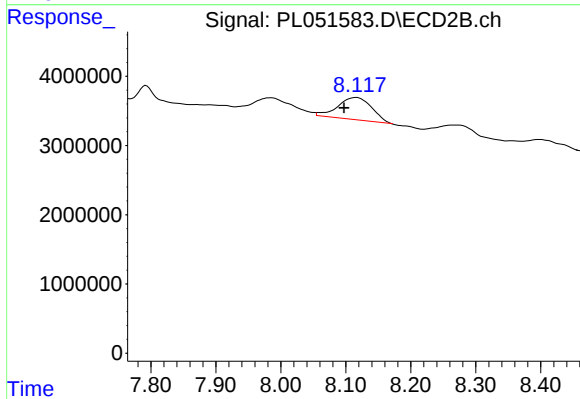

#22 Mirex


R.T.: 8.117 min
Delta R.T.: 0.019 min
Response: 11443748
Conc: 4.98 ng/ml

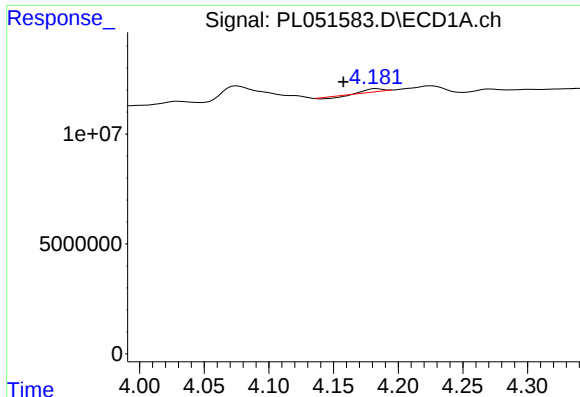

#23 Chlordane-1


R.T.: 4.184 min
Delta R.T.: 0.026 min
Response: 318959
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-29

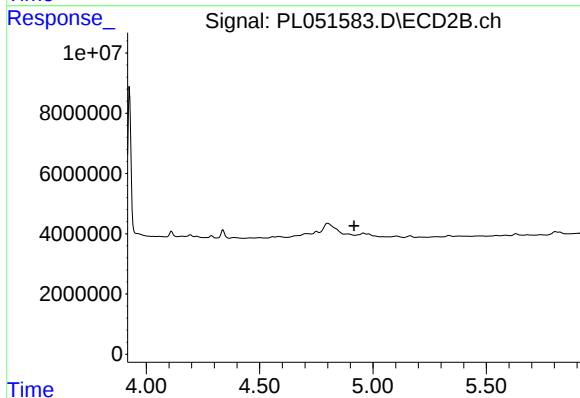


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.916 min
Response: 0
Conc: N.D.

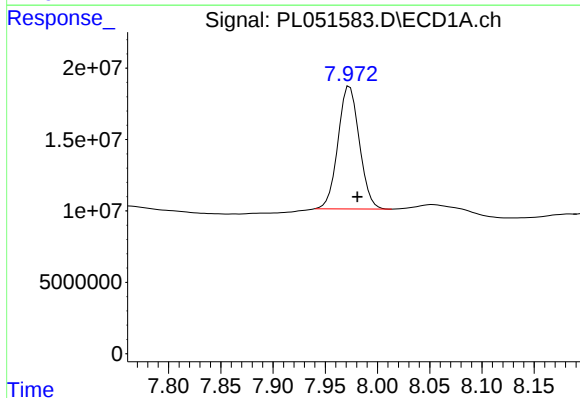

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.007 min
Response: 122160261
Conc: 12.06 ng/ml

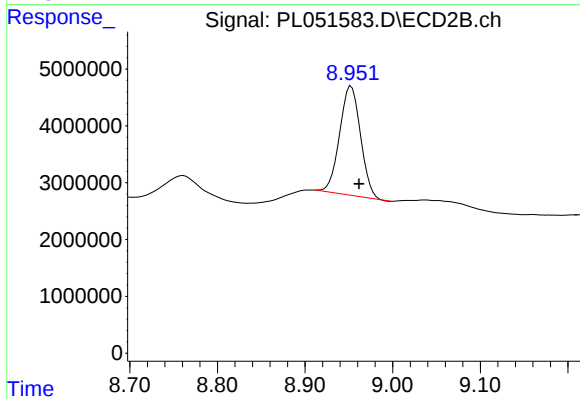

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 31934563
Conc: 11.29 ng/ml