

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
 Data File : PL051588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 17:31
 Operator : SG\AJ
 Sample : K4365-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0603-COMP-BH-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:48:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	188.5E6	48026890	18.756	16.833
28)	SA Decachlor...	7.973	8.953	110.2E6	30614732	10.882	10.826
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	1381469	N.D.	0.799 #
9)	A Endosulfan I	5.331f	0.000	2631371	0	0.181	N.D. #
10)	B gamma-Chl...	5.217f	0.000	19209147	0	1.217	N.D. #
11)	B alpha-Chl...	5.260	0.000	10482282	0	0.687	N.D. #
25)	Chlordane-3	5.217	0.000	19209147	0	13.723	N.D. #
26)	Chlordane-4	5.260	0.000	10482282	0	7.947	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
Data File : PL051588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 17:31
Operator : SG\AJ
Sample : K4365-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0603-COMP-BH-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:48:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

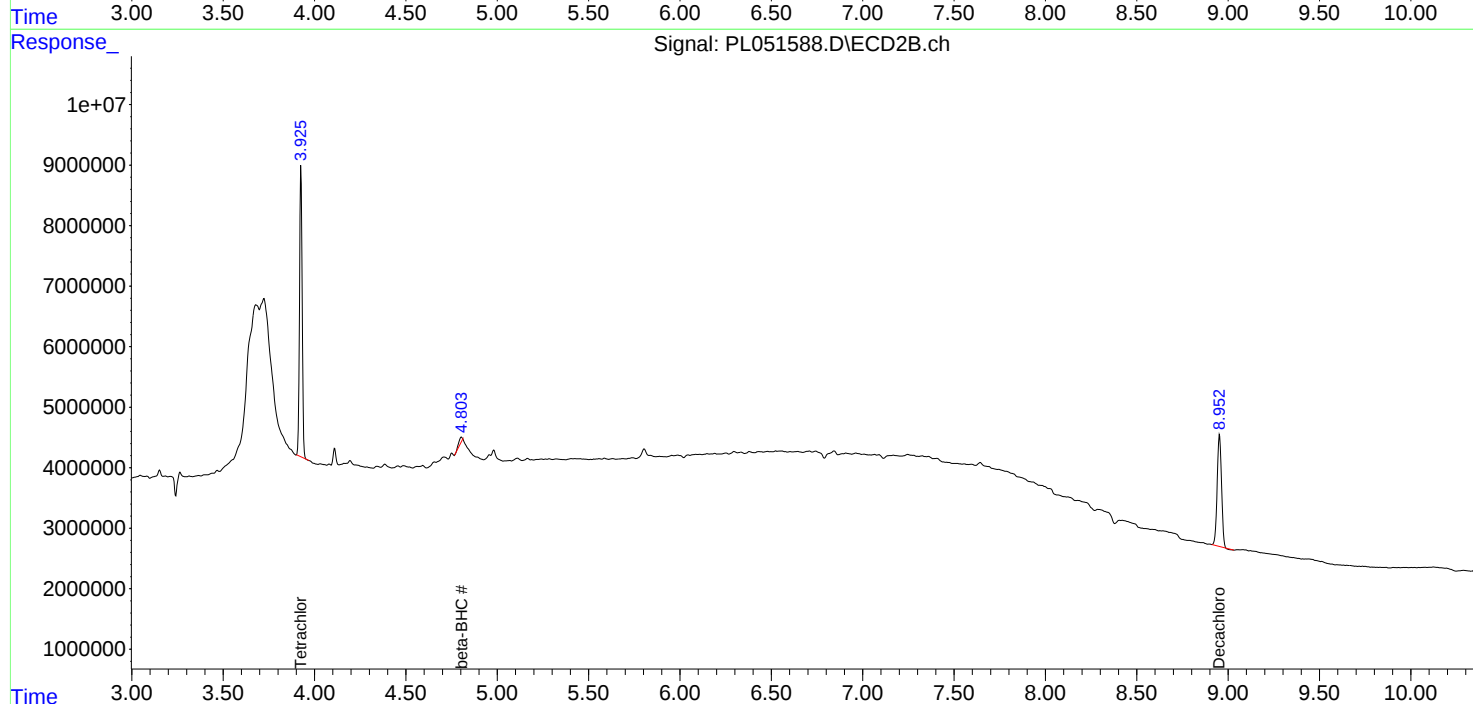


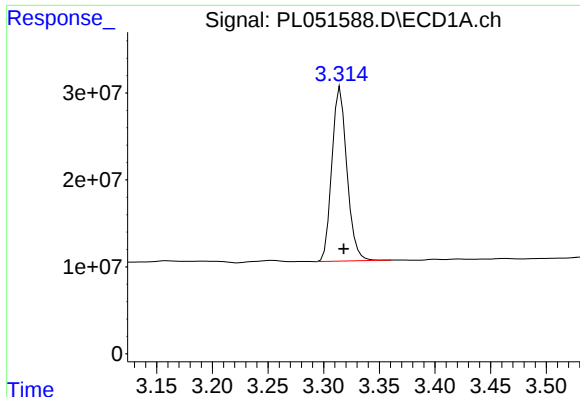

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 188460814
Conc: 18.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
0603-COMP-BH-4

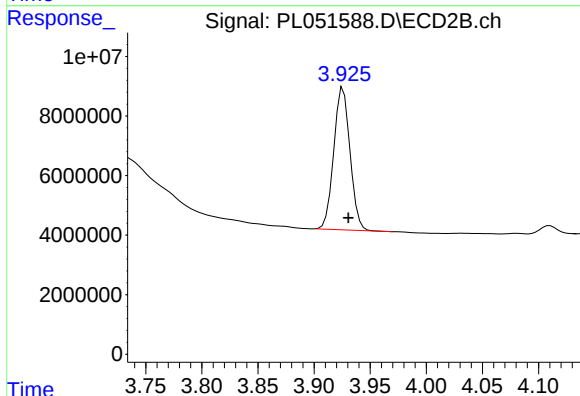


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 48026890
Conc: 16.83 ng/ml

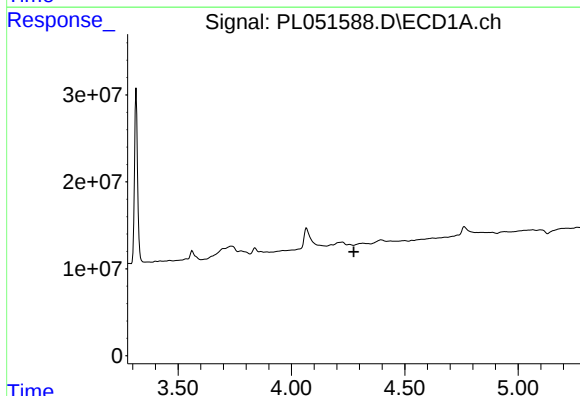


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

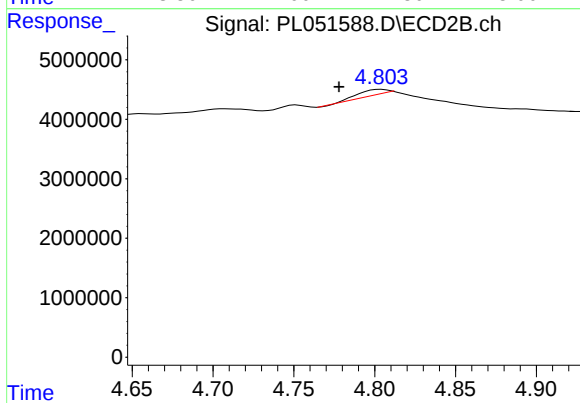

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 1381469
Conc: 0.80 ng/ml

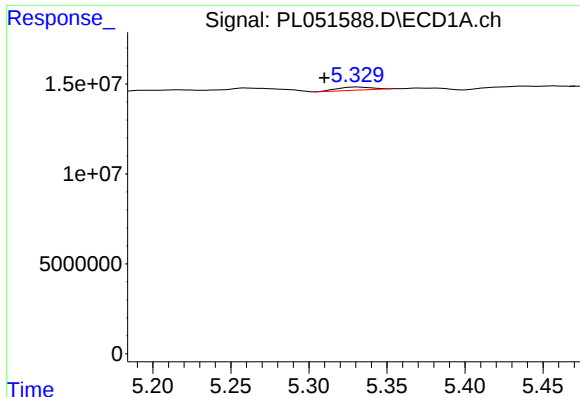

#9 Endosulfan I


R.T.: 5.331 min
Delta R.T.: 0.021 min
Response: 2631371
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
0603-COMP-BH-4

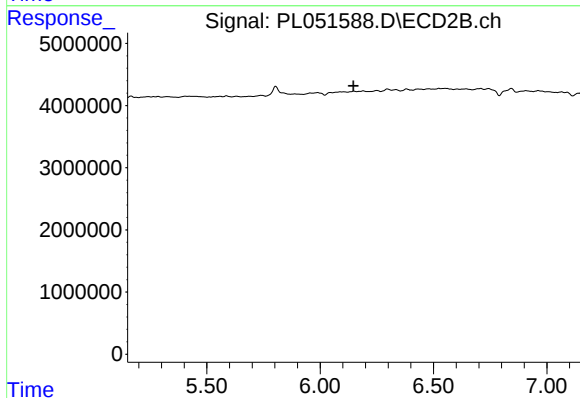


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

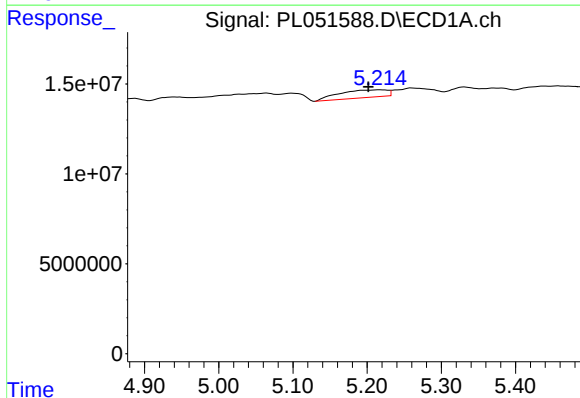


#10 gamma-Chlordane

R.T.: 5.217 min
Delta R.T.: 0.015 min
Response: 19209147
Conc: 1.22 ng/ml

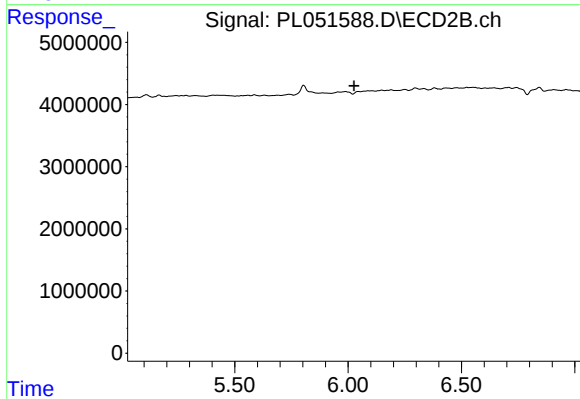

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

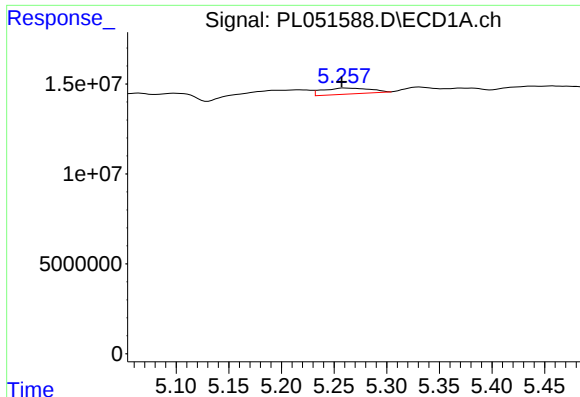

#11 alpha-Chlordane


R.T.: 5.260 min
Delta R.T.: 0.003 min
Response: 10482282
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
0603-COMP-BH-4

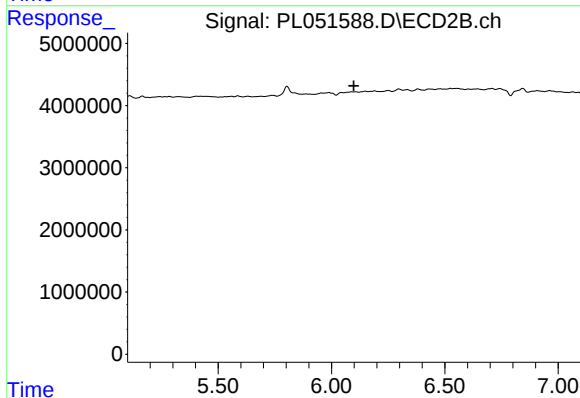


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

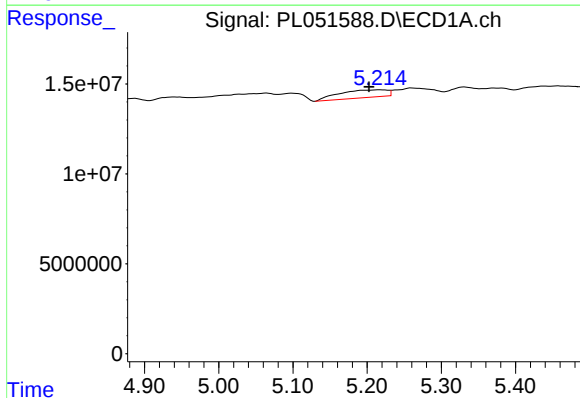


#25 Chlordane-3

R.T.: 5.217 min
Delta R.T.: 0.014 min
Response: 19209147
Conc: 13.72 ng/ml

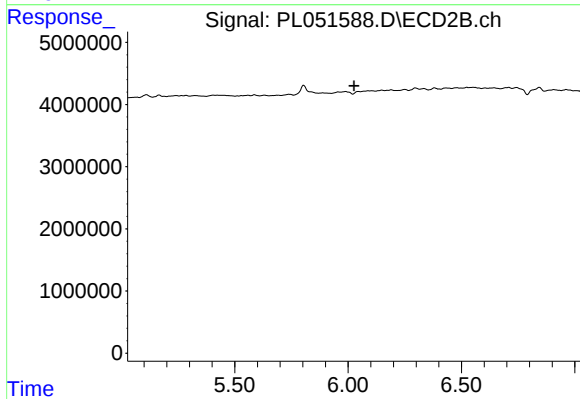

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

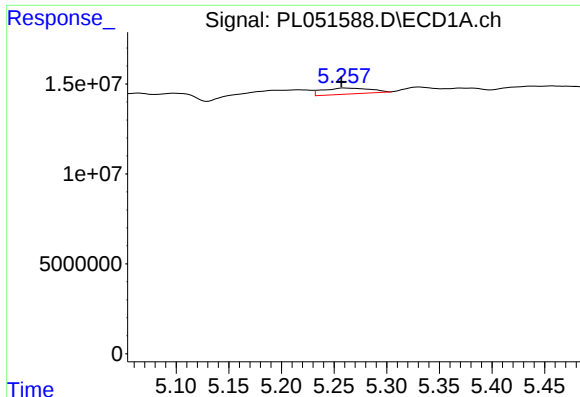

#26 Chlordane-4


R.T.: 5.260 min
Delta R.T.: 0.004 min
Response: 10482282
Conc: 7.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
0603-COMP-BH-4

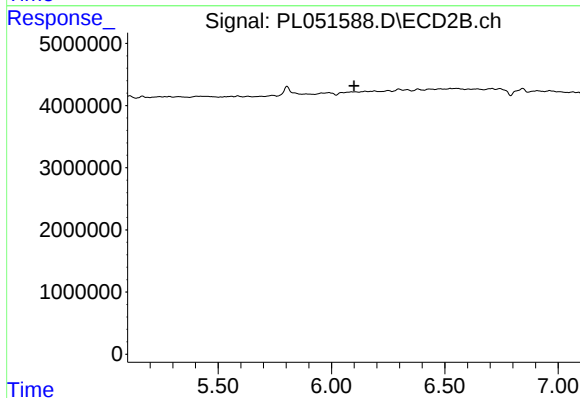


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

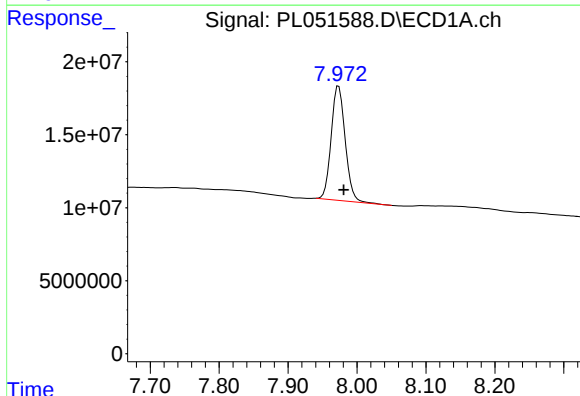

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.007 min
Response: 110185998
Conc: 10.88 ng/ml

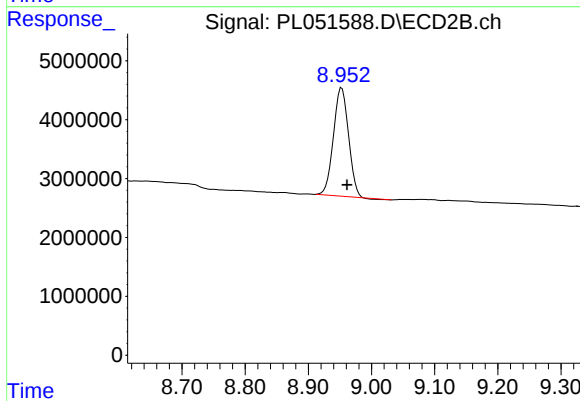

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 30614732
Conc: 10.83 ng/ml