

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
 Data File : PL051598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 19:53
 Operator : SG\AJ
 Sample : K3616-14
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-081519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:50:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	237.7E6	67409622	23.662	23.626
28)	SA Decachlor...	7.973	8.953	184.3E6	49773828	18.200	17.601
Target Compounds							
5)	MB Aldrin	4.573f	0.000	6690955	0	0.432	N.D. #
8)	B Heptachlo...	0.000	5.802	0	6097876	N.D.	1.594 #
9)	A Endosulfan I	5.330f	0.000	5387929	0	0.370	N.D. #
10)	B gamma-Chl...	5.192	0.000	22530768	0	1.428	N.D. #
11)	B alpha-Chl...	5.258	0.000	36172224	0	2.371	N.D. #
15)	B Endosulfa...	0.000	6.842	0	4712312	N.D.	1.482 #
25)	Chlordane-3	5.192	0.000	22530768	0	16.096	N.D. #
26)	Chlordane-4	5.258	0.000	36172224	0	27.424	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081619\
Data File : PL051598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 19:53
Operator : SG\AJ
Sample : K3616-14
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:50:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

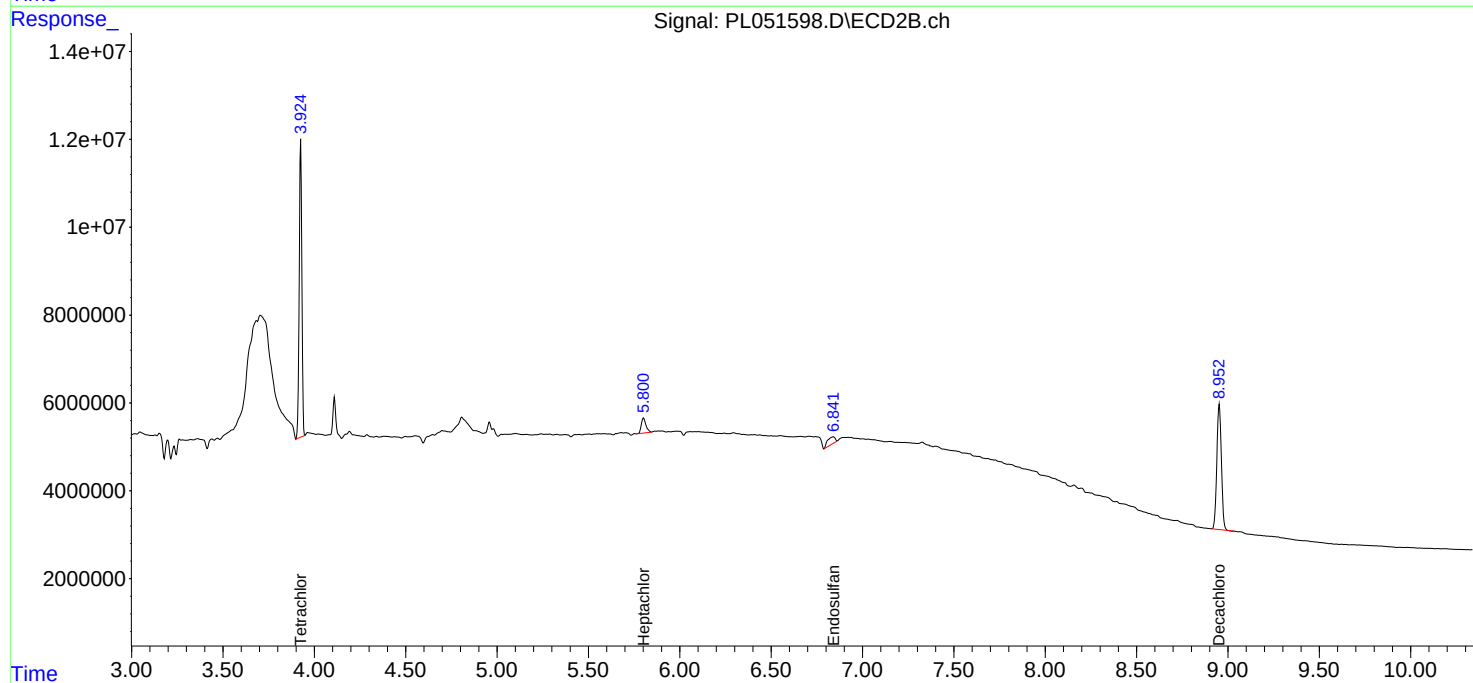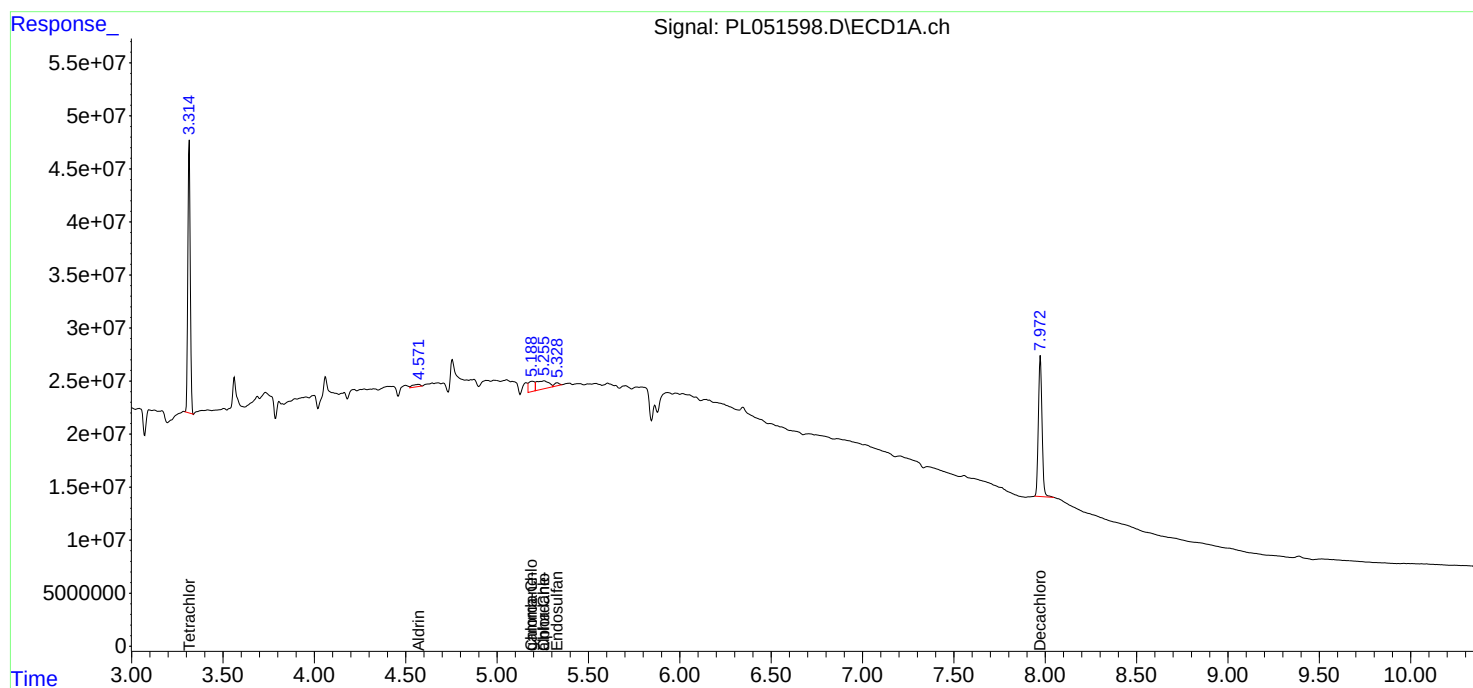


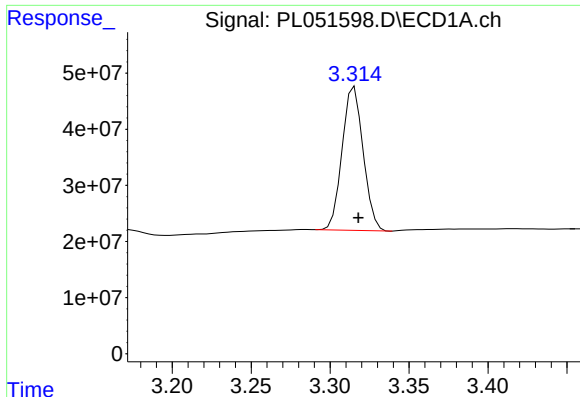

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 237749920
Conc: 23.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

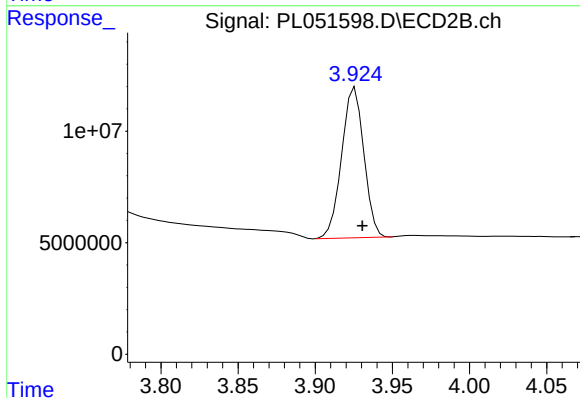


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 67409622
Conc: 23.63 ng/ml

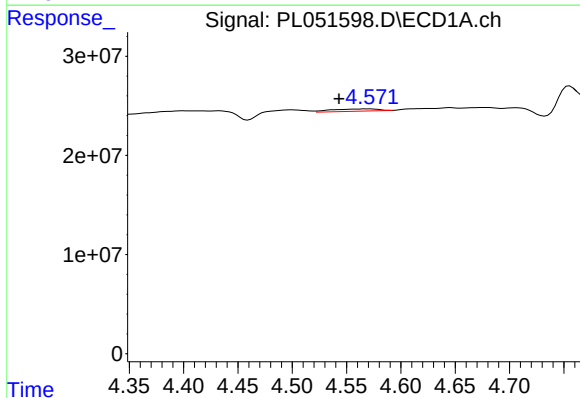


#5 Aldrin

R.T.: 4.573 min
Delta R.T.: 0.030 min
Response: 6690955
Conc: 0.43 ng/ml

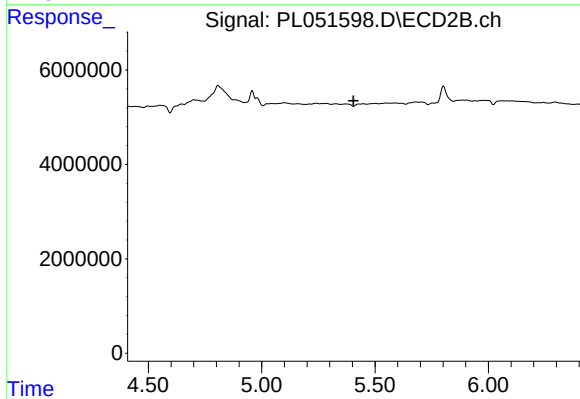

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

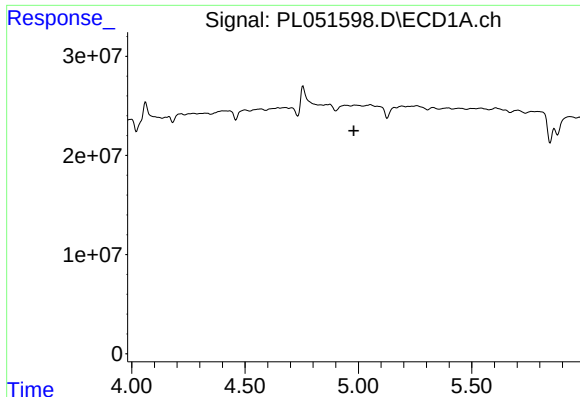

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

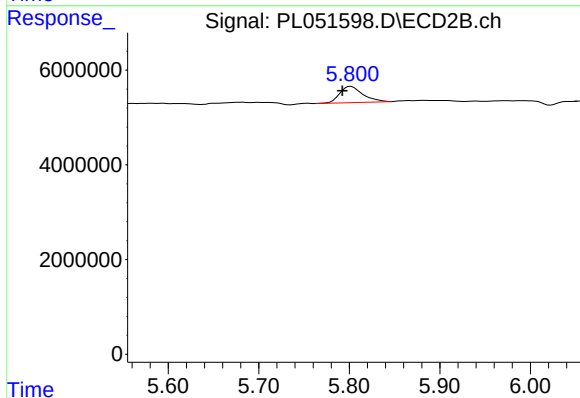


#8 Heptachlor epoxide

R.T.: 5.802 min
Delta R.T.: 0.009 min
Response: 6097876
Conc: 1.59 ng/ml

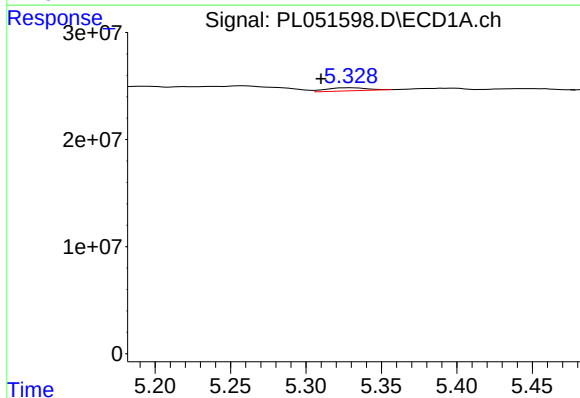


#9 Endosulfan I

R.T.: 5.330 min
Delta R.T.: 0.020 min
Response: 5387929
Conc: 0.37 ng/ml

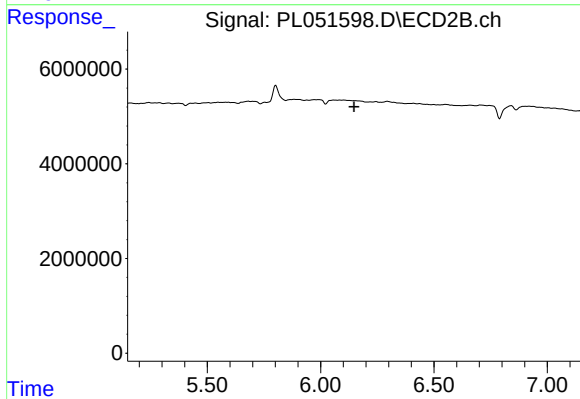

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

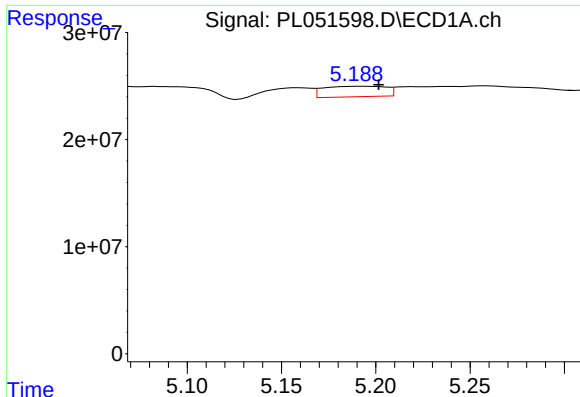

#10 gamma-Chlordane


R.T.: 5.192 min
Delta R.T.: -0.009 min
Response: 22530768
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

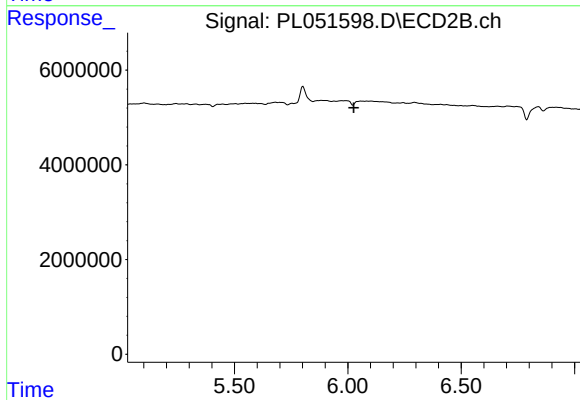


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

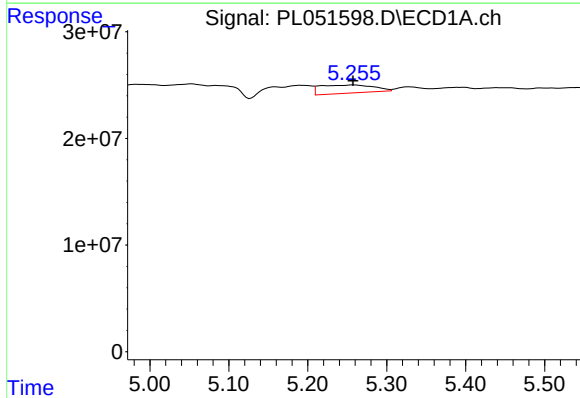


#11 alpha-Chlordane

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 36172224
Conc: 2.37 ng/ml

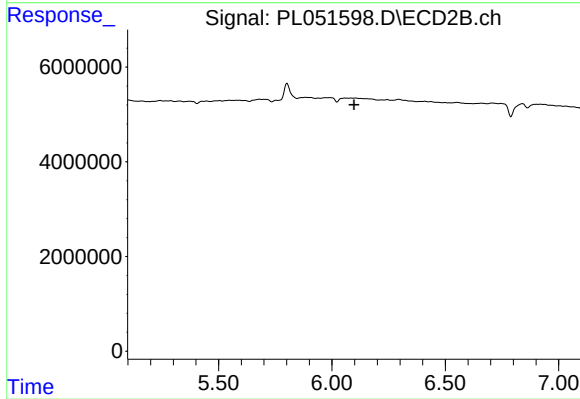

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

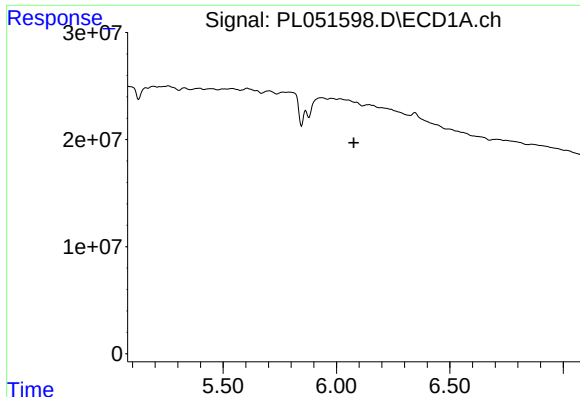

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

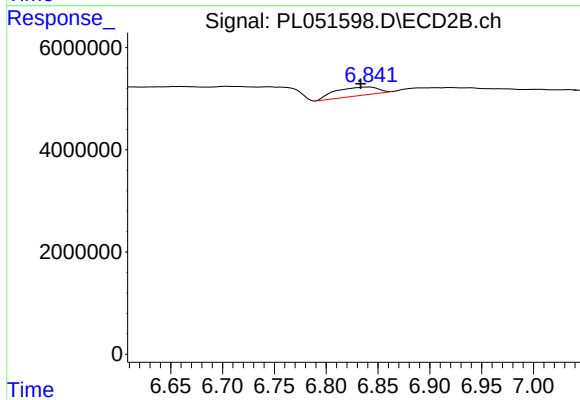


#15 Endosulfan II

R.T.: 6.842 min
Delta R.T.: 0.008 min
Response: 4712312
Conc: 1.48 ng/ml

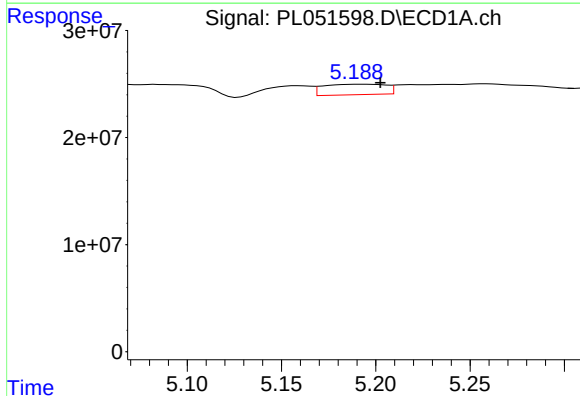


#25 Chlordane-3

R.T.: 5.192 min
Delta R.T.: -0.010 min
Response: 22530768
Conc: 16.10 ng/ml

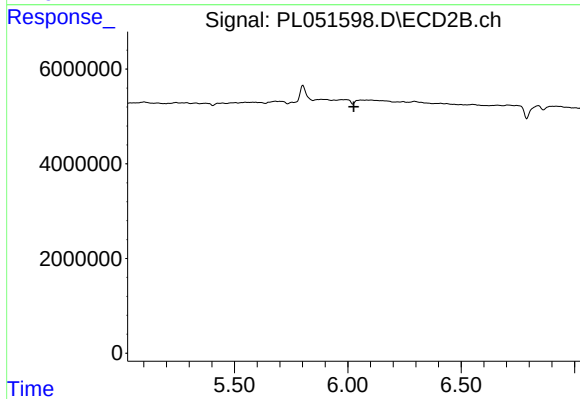

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

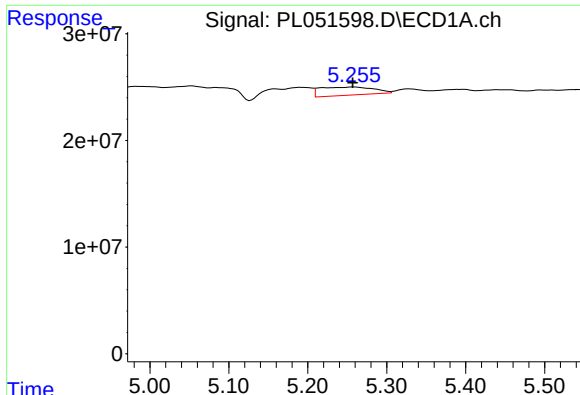

#26 Chlordane-4


R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 36172224
Conc: 27.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-081519-B

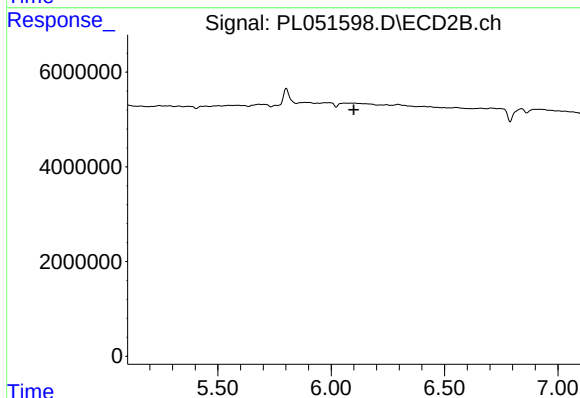


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

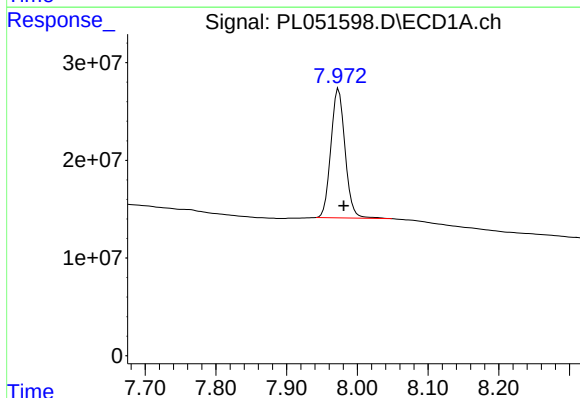

#28 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.007 min
Response: 184282323
Conc: 18.20 ng/ml

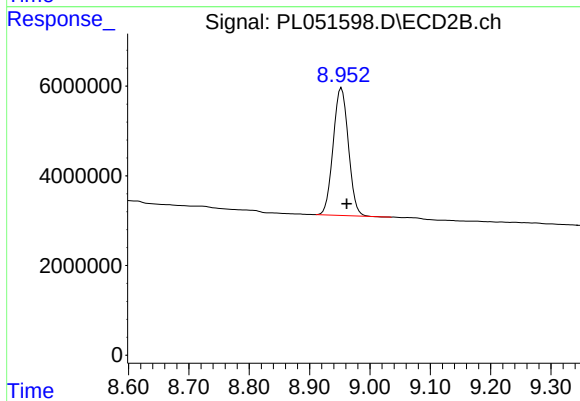

#28 Decachlorobiphenyl

R.T.: 8.953 min
Delta R.T.: -0.009 min
Response: 49773828
Conc: 17.60 ng/ml