

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081624\
 Data File : PL091169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2024 19:55
 Operator : AR\AJ
 Sample : P3617-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VCPS-B5-081424-10-14

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/19/2024
 Supervised By :Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 07:54:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 13:09:19 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.785	35490498	32082596	16.529	16.436
28) SA Decachlor...	9.053	7.925	16950498	19932620	11.118m	10.523

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081624\
Data File : PL091169.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2024 19:55
Operator : AR\AJ
Sample : P3617-12
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VCPS-B5-081424-10-14


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/19/2024
Supervised By : Ankita Jodhani 08/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 07:54:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081324.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 13:09:19 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

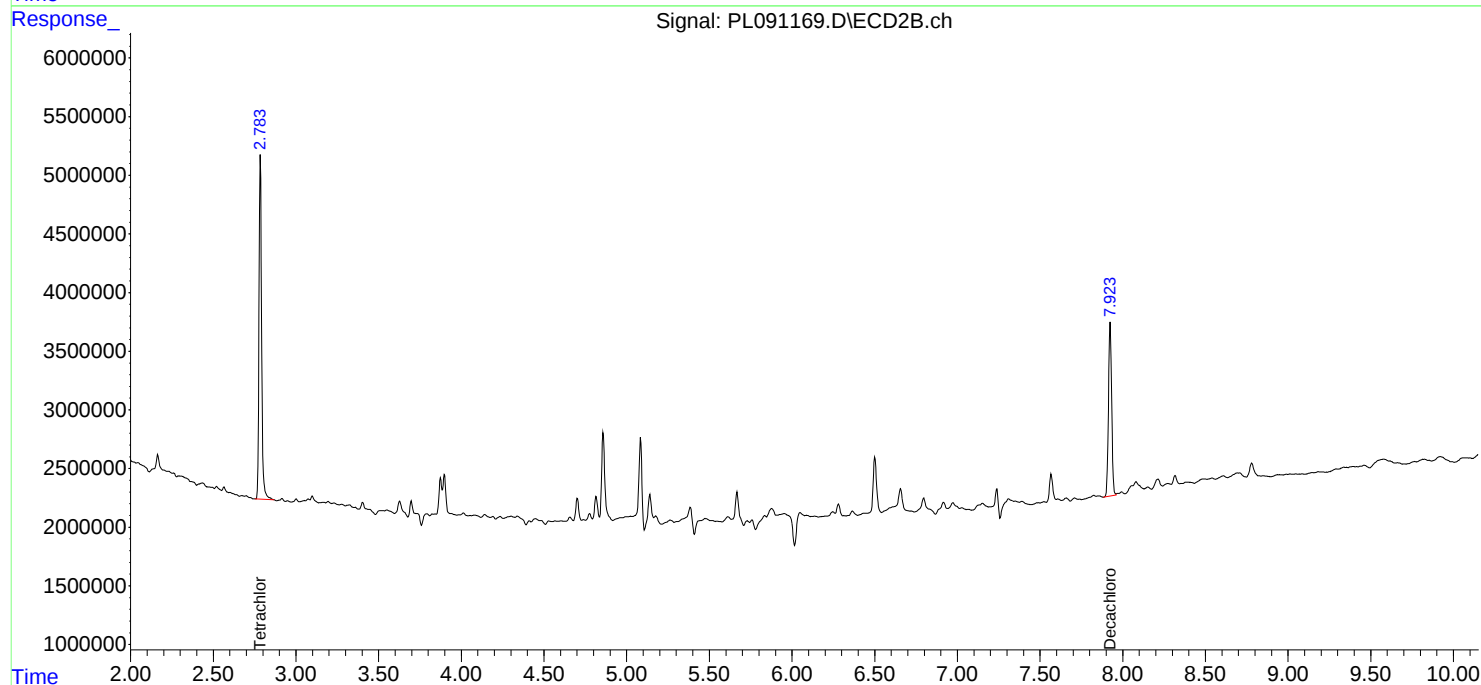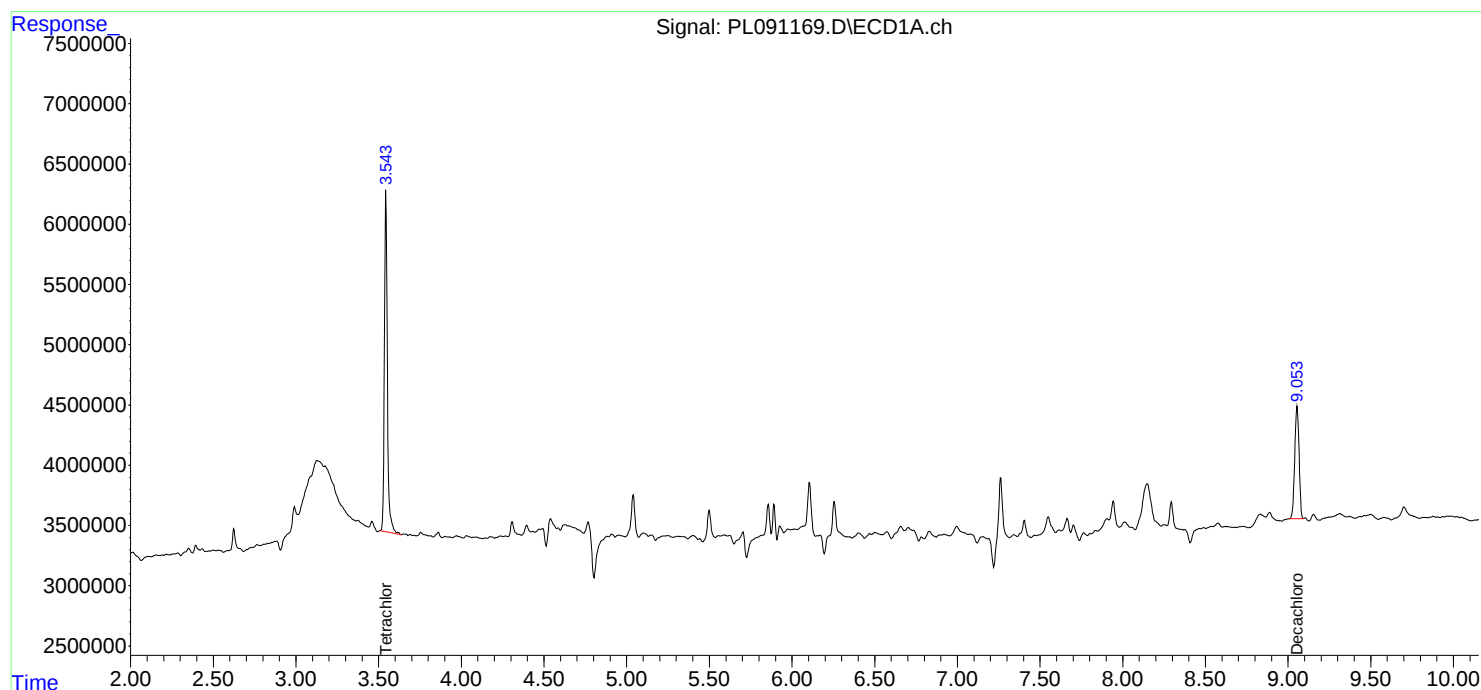

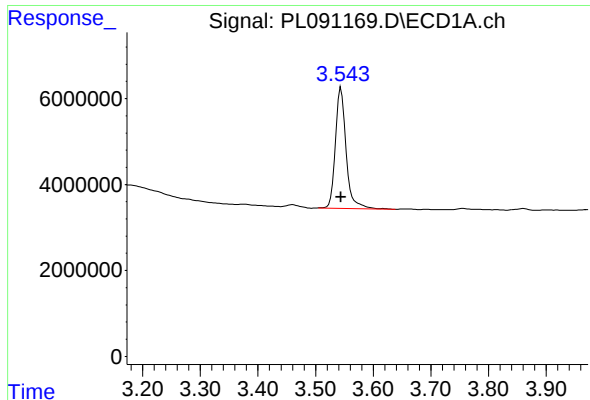


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 35490498
Conc: 16.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
VCPS-B5-081424-10-14


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/19/2024
Supervised By :Ankita Jodhani 08/19/2024

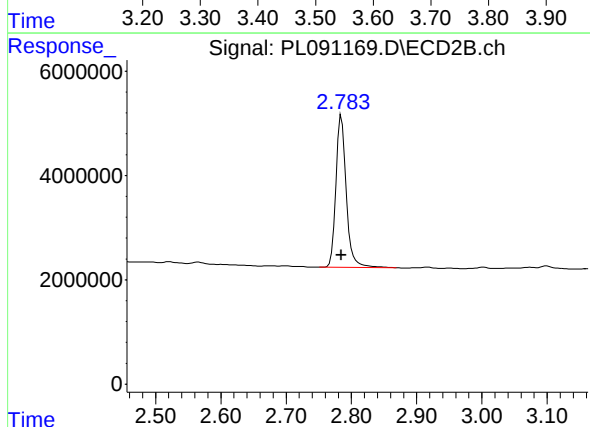


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: 0.000 min
Response: 32082596
Conc: 16.44 ng/ml

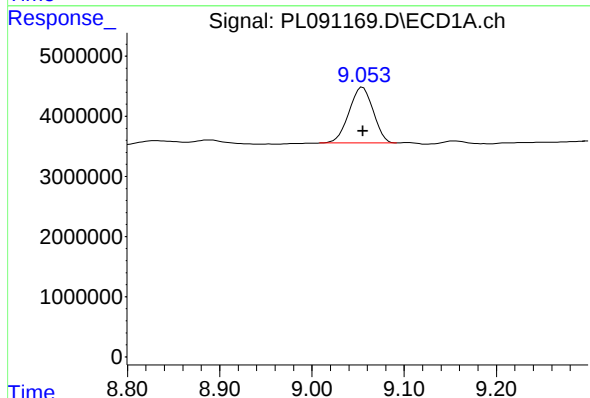

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.002 min
Response: 16950498
Conc: 11.12 ng/ml m

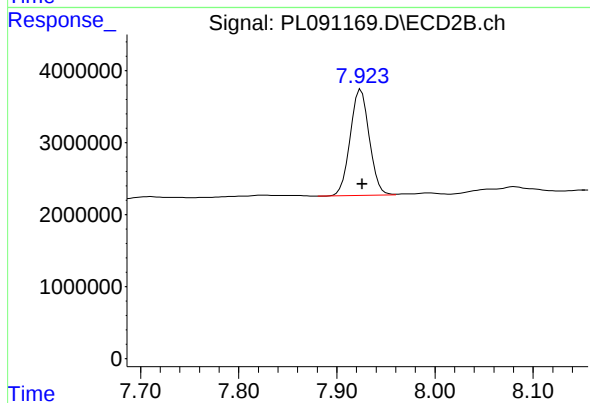

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.001 min
Response: 19932620
Conc: 10.52 ng/ml