

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081625\
 Data File : PL096839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2025 21:15
 Operator : AR\AJ
 Sample : Q2815-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TW-22M-W

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:57:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.826	90354924	85851950	28.406	17.969 #
28)	SA Decachlor...	9.004	7.987	29279186	53534074	12.278	12.340
Target Compounds							
4)	MA Heptachlor	4.921f	0.000	32926209	0	7.923	N.D. #
9)	A Endosulfan I	0.000	5.178	0	81096586	N.D.	14.661 #
11)	B alpha-Chl...	5.996	5.103	11436760	7016053	2.967	1.189 #
12)	B 4,4'-DDE	6.137f	5.305	58713135	23424148	18.284	4.248 #
14)	MA Endrin	0.000	5.714	0	5202198	N.D.	0.962 #
17)	MA 4,4'-DDT	6.982	6.120	7635862	32723031	2.663	6.469 #
18)	B Endrin al...	0.000	6.166	0	13730005	N.D.	3.777 #
23)	Chlordane-1	0.000	3.826	0	22493702	N.D.	107.298 #
26)	Chlordane-4	5.996	5.103	11436760	7016053	13.818	11.274



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081625\
Data File : PL096839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 21:15
Operator : AR\AJ
Sample : Q2815-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 05:57:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

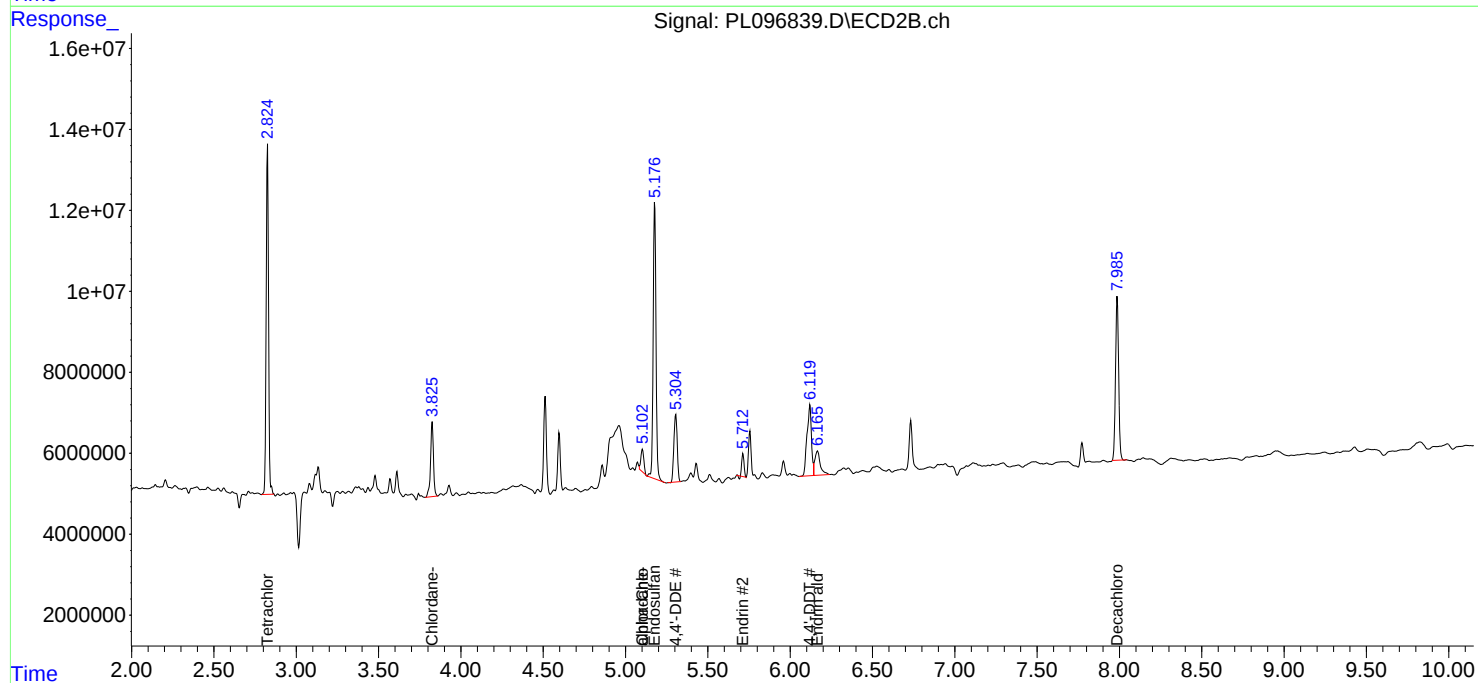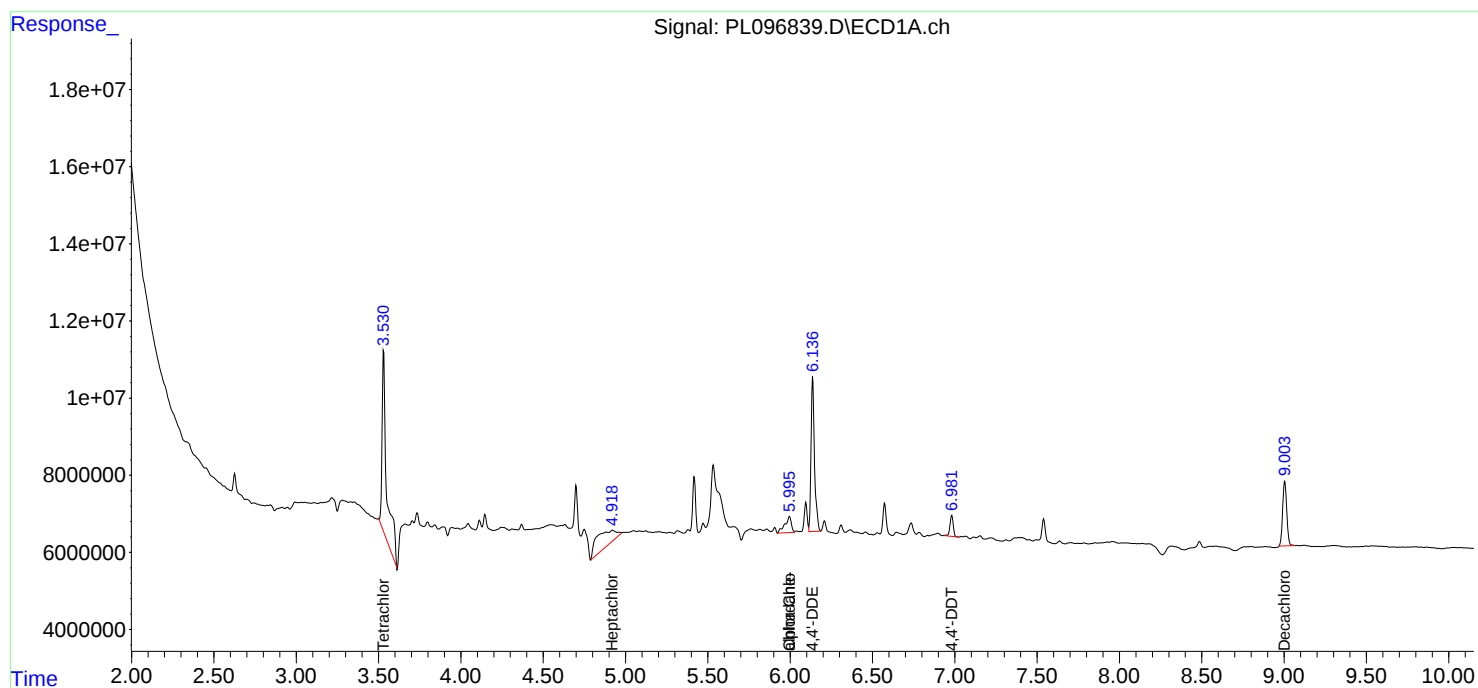


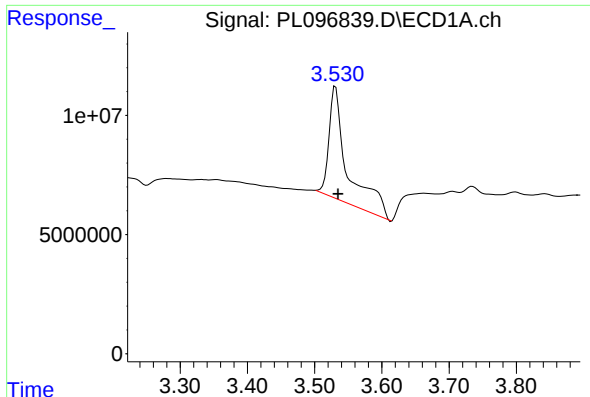

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: -0.004 min
Response: 90354924
Conc: 28.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

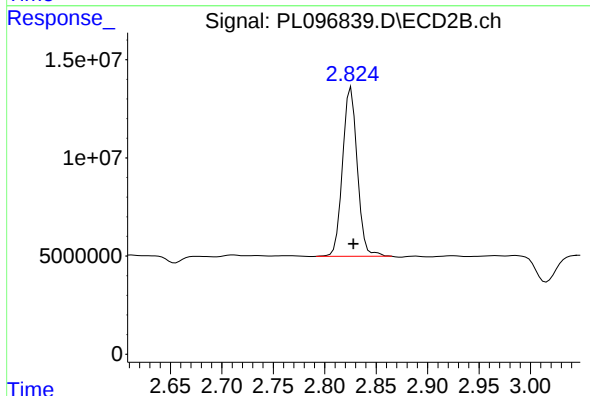


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 85851950
Conc: 17.97 ng/ml

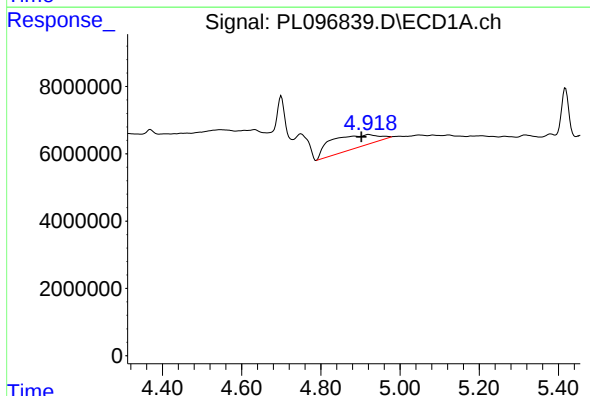


#4 Heptachlor

R.T.: 4.921 min
Delta R.T.: 0.018 min
Response: 32926209
Conc: 7.92 ng/ml

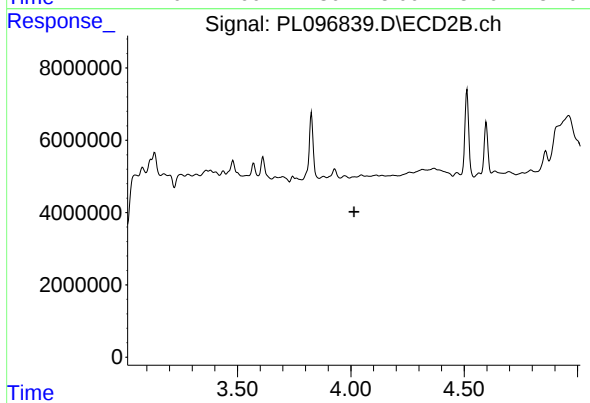

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.014 min
Response: 0
Conc: N.D.

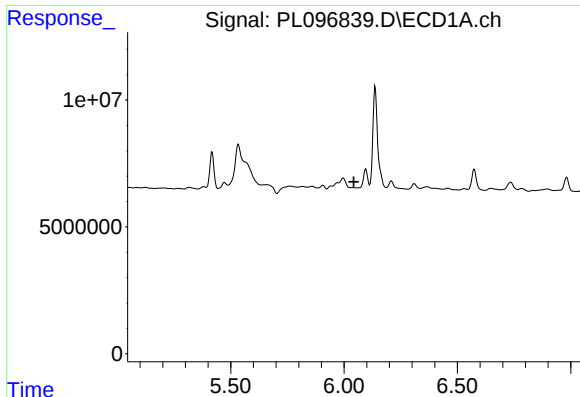

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.044 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

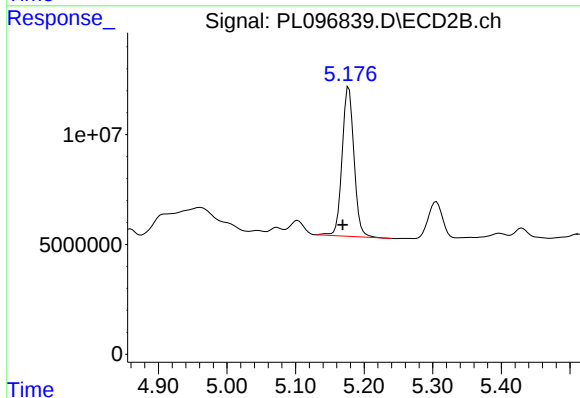


#9 Endosulfan I

R.T.: 5.178 min
Delta R.T.: 0.009 min
Response: 81096586
Conc: 14.66 ng/ml

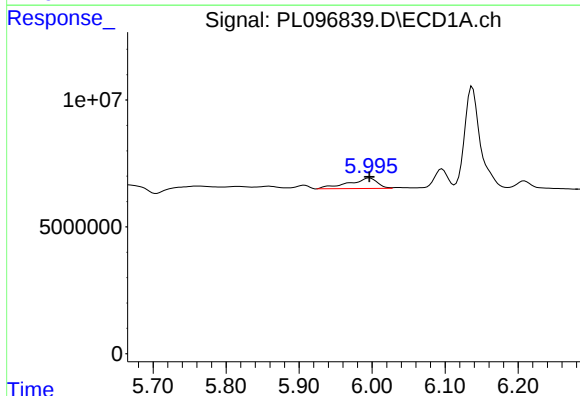


#11 alpha-Chlordane

R.T.: 5.996 min
Delta R.T.: 0.000 min
Response: 11436760
Conc: 2.97 ng/ml

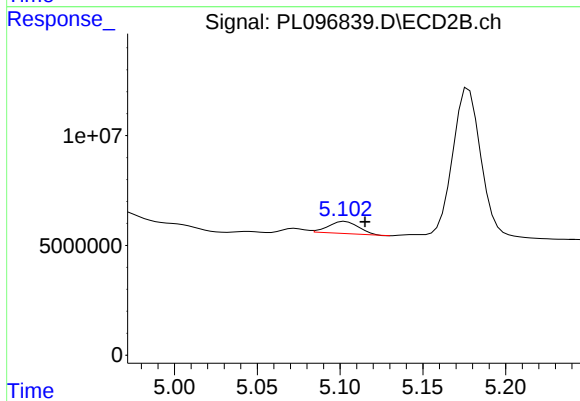

#11 alpha-Chlordane


R.T.: 5.103 min
Delta R.T.: -0.012 min
Response: 7016053
Conc: 1.19 ng/ml

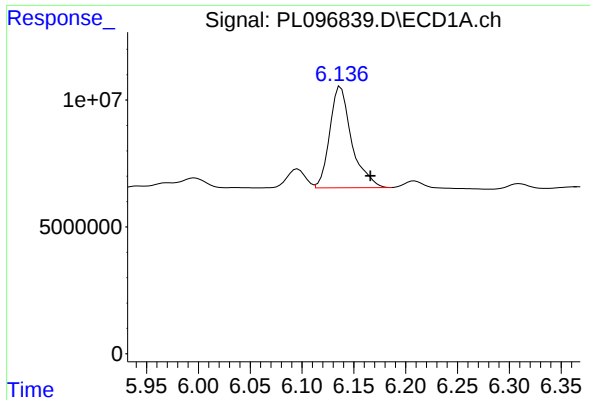

#12 4,4'-DDE


R.T.: 6.137 min
Delta R.T.: -0.029 min
Response: 58713135
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

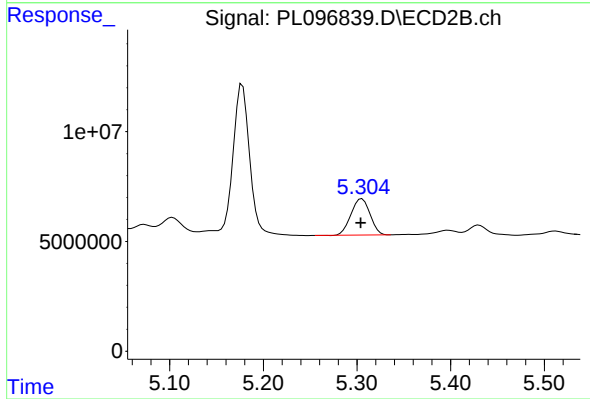


#12 4,4'-DDE

R.T.: 5.305 min
Delta R.T.: 0.001 min
Response: 23424148
Conc: 4.25 ng/ml

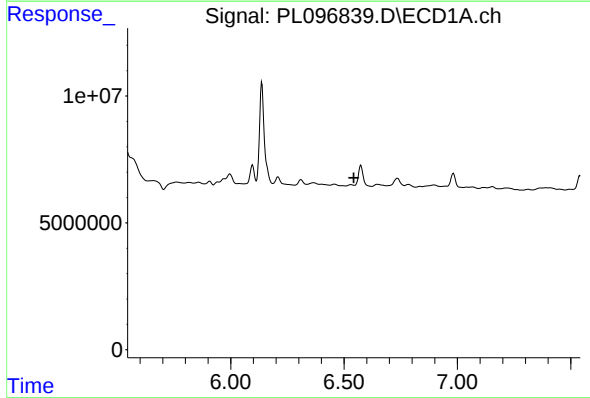


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

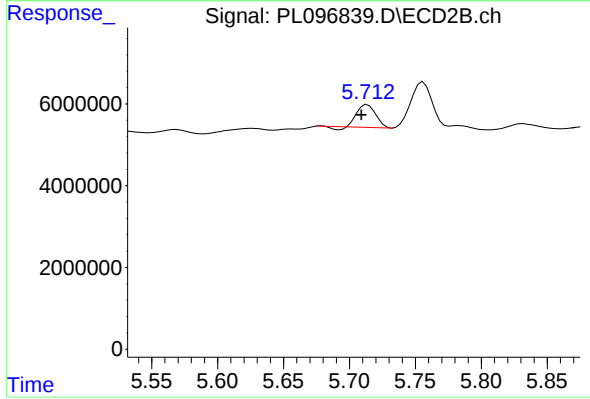

#14 Endrin


R.T.: 5.714 min
Delta R.T.: 0.005 min
Response: 5202198
Conc: 0.96 ng/ml

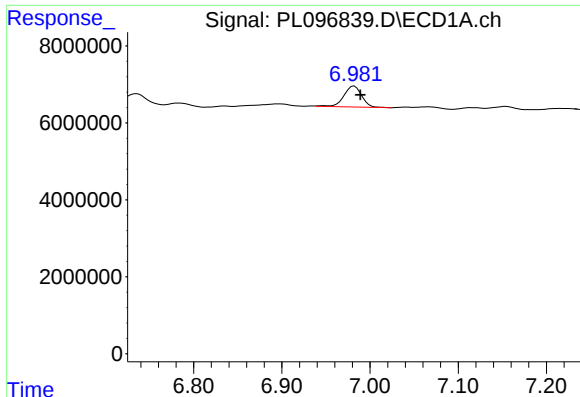

#17 4,4'-DDT


R.T.: 6.982 min
Delta R.T.: -0.007 min
Response: 7635862
Conc: 2.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

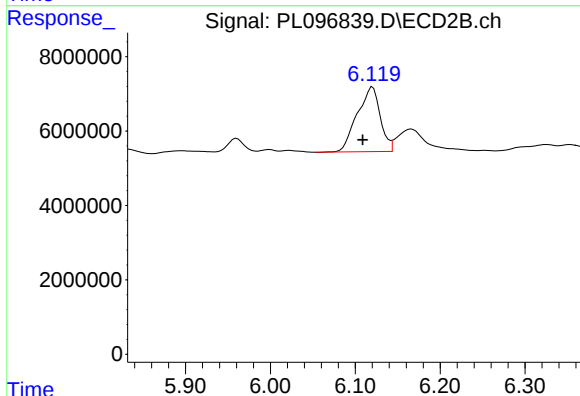


#17 4,4'-DDT

R.T.: 6.120 min
Delta R.T.: 0.011 min
Response: 32723031
Conc: 6.47 ng/ml

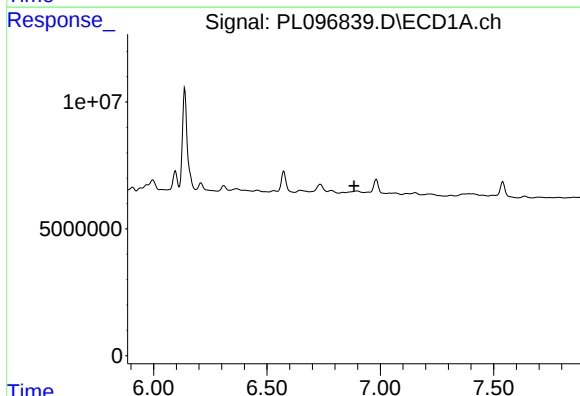


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.884 min
Response: 0
Conc: N.D.

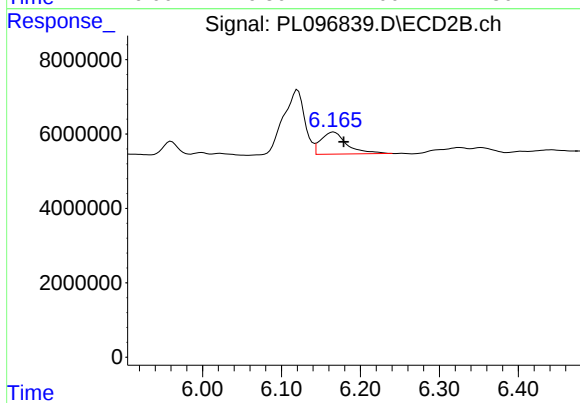

#18 Endrin aldehyde


R.T.: 6.166 min
Delta R.T.: -0.013 min
Response: 13730005
Conc: 3.78 ng/ml

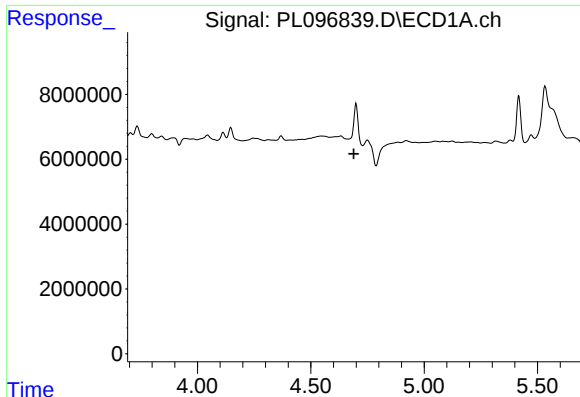

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.690 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

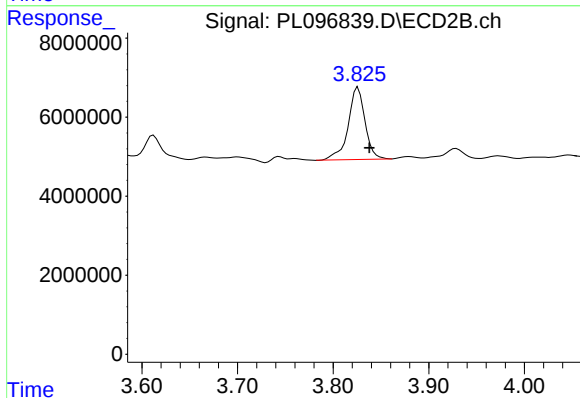


#23 Chlordane-1

R.T.: 3.826 min
Delta R.T.: -0.012 min
Response: 22493702
Conc: 107.30 ng/ml

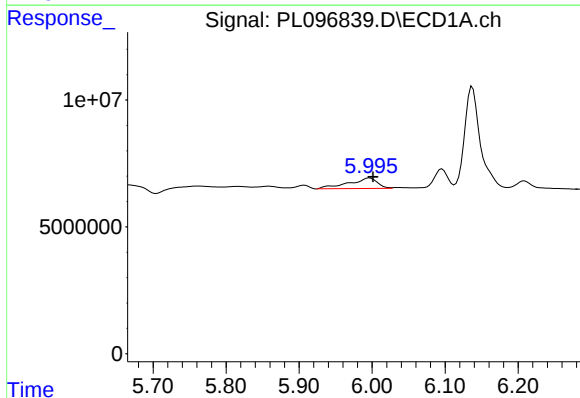


#26 Chlordane-4

R.T.: 5.996 min
Delta R.T.: -0.005 min
Response: 11436760
Conc: 13.82 ng/ml

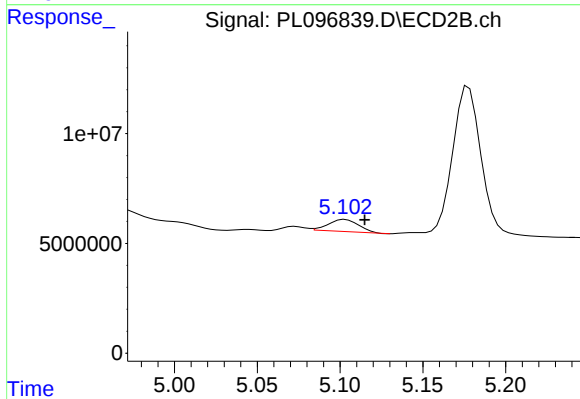

#26 Chlordane-4


R.T.: 5.103 min
Delta R.T.: -0.012 min
Response: 7016053
Conc: 11.27 ng/ml

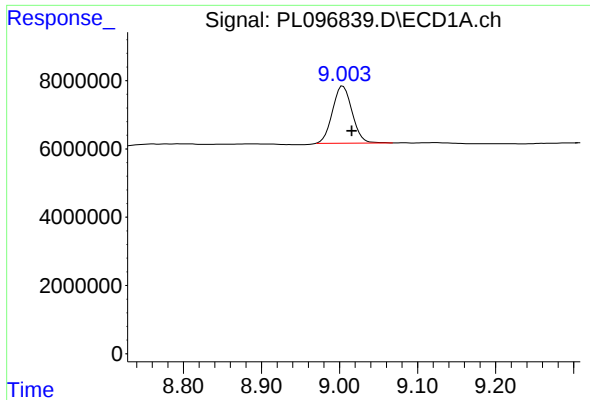

#28 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: -0.011 min
Response: 29279186
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-22M-W

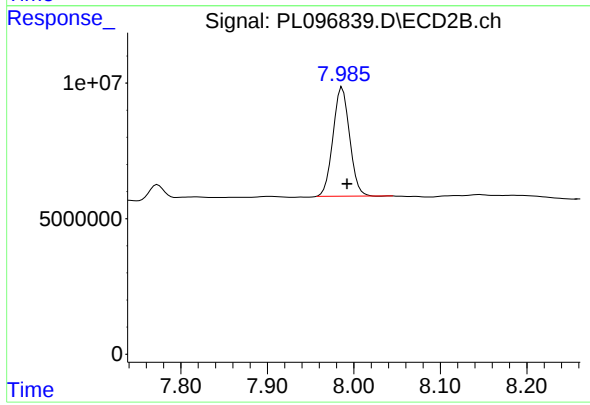

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 53534074
Conc: 12.34 ng/ml