

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 13:21
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 22:42:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.306	3.907	168.3E6	71716962	24.081	26.751
28)	SA Decachlor...	7.963	8.893	153.4E6	58309068	21.836	25.127
Target Compounds							
3)	MA gamma-BHC...	4.048f	0.000	411.4E6	0	38.791	N.D. #
7)	B delta-BHC	0.000	4.946	0	35059581	N.D.	8.805 #
8)	B Heptachlo...	4.919f	5.772	5859743	30995122	0.614	9.216 #
10)	B gamma-Chl...	5.138f	0.000	18628142	0	1.886	N.D. #
15)	B Endosulfa...	6.016f	0.000	24141871	0	2.776	N.D. #
23)	Chlordane-1	4.179	4.946	6174677	35059581	19.504	280.623 #
25)	Chlordane-3	5.138	0.000	18628142	0	17.055	N.D. #
27)	Chlordane-5	6.016	0.000	24141871	0	74.436	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 13:21
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 22:42:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

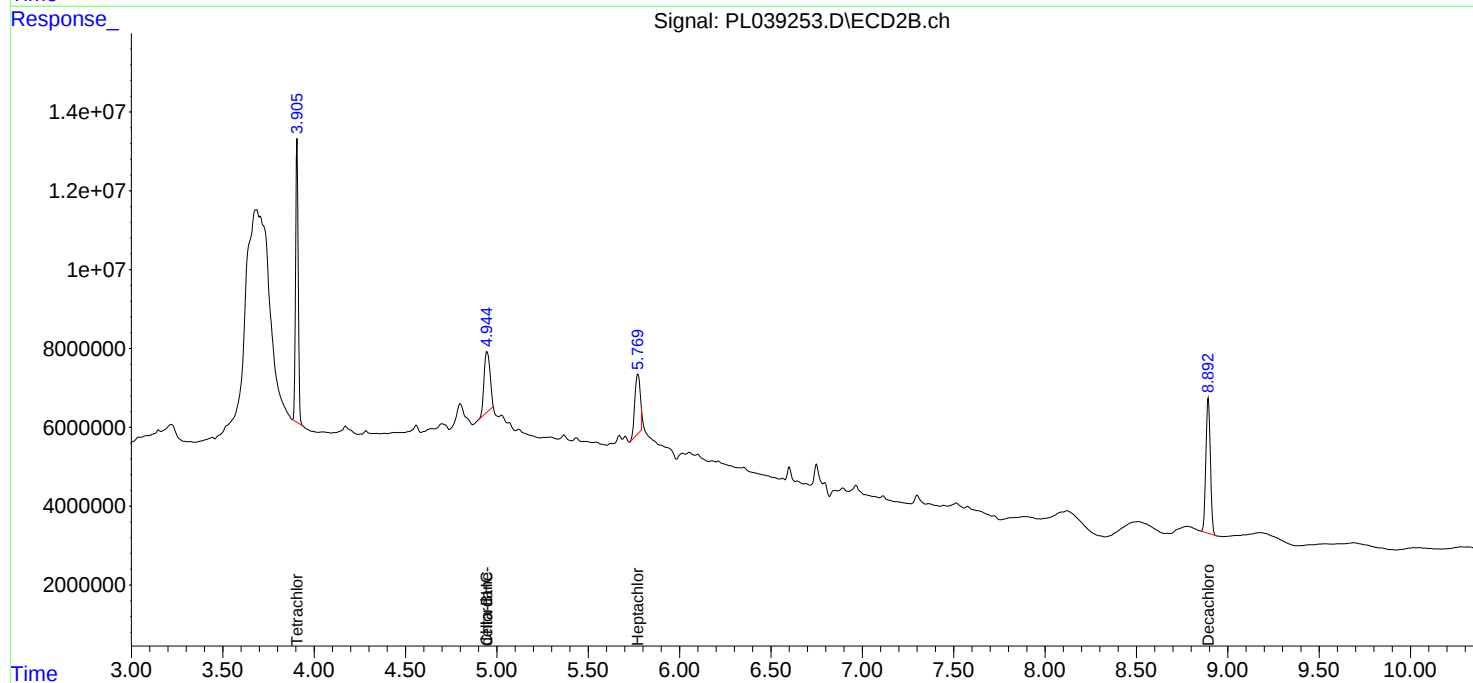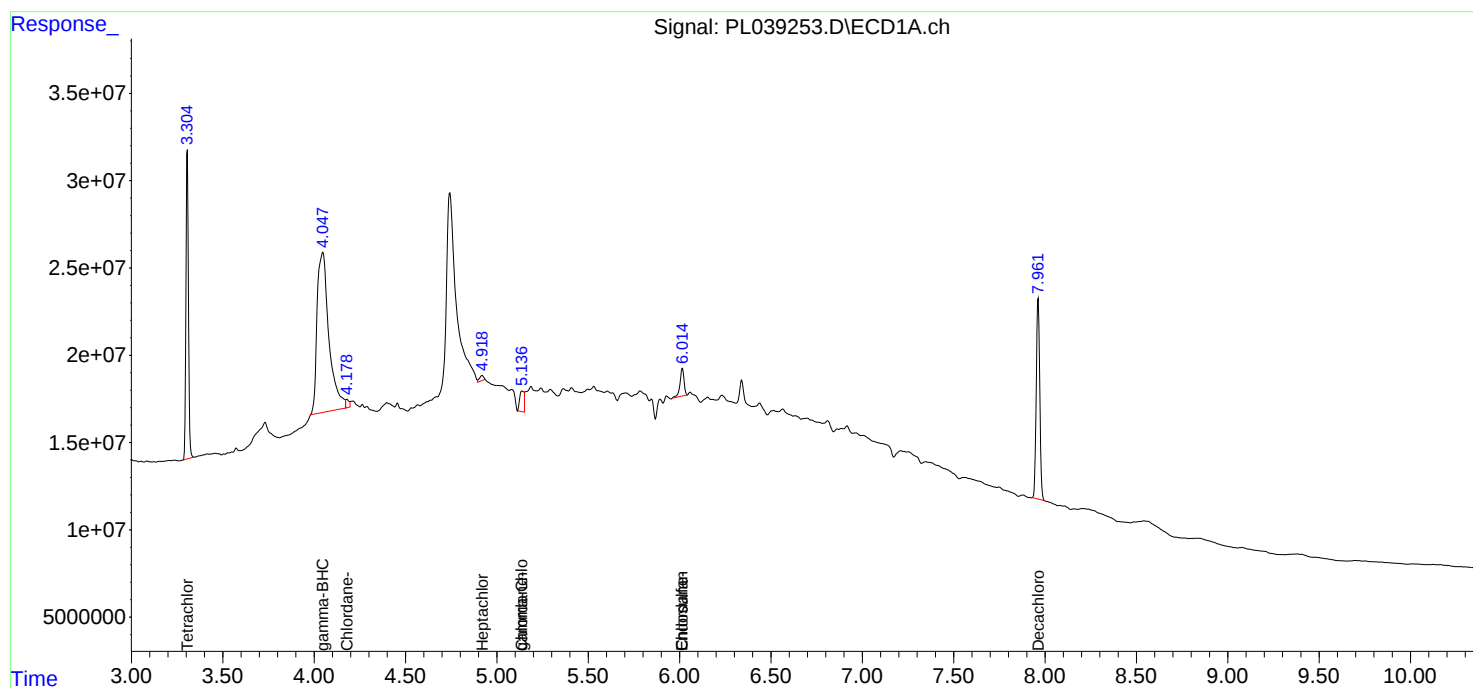


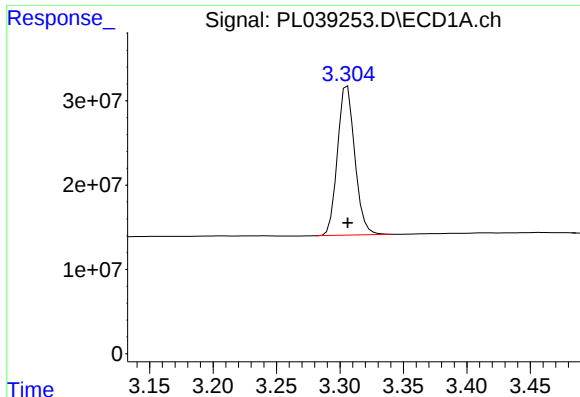

#1 Tetrachloro-m-xylene


R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 168339144
Conc: 24.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

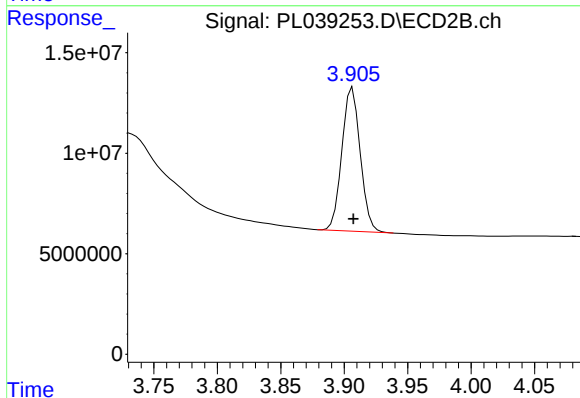


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 71716962
Conc: 26.75 ng/ml

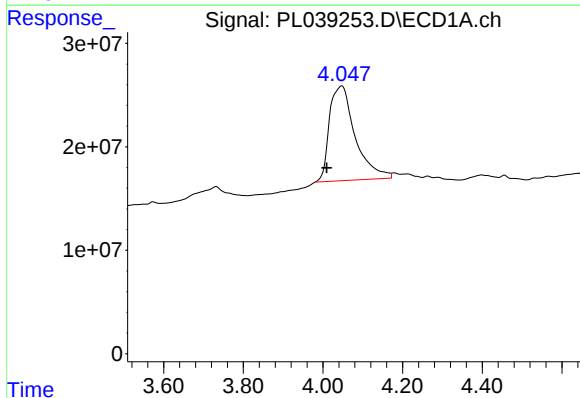


#3 gamma-BHC (Lindane)

R.T.: 4.048 min
Delta R.T.: 0.039 min
Response: 411439321
Conc: 38.79 ng/ml

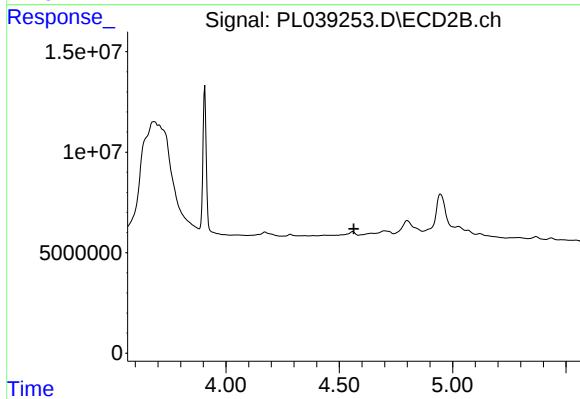

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

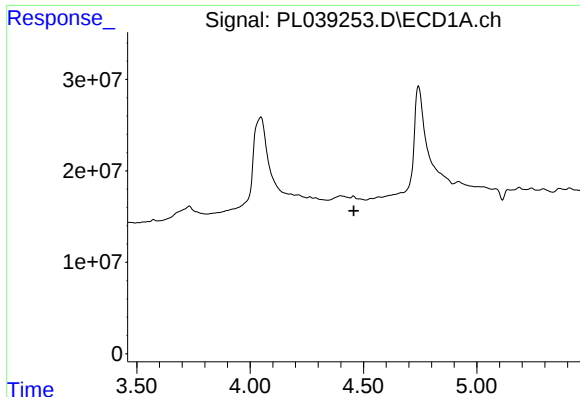

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

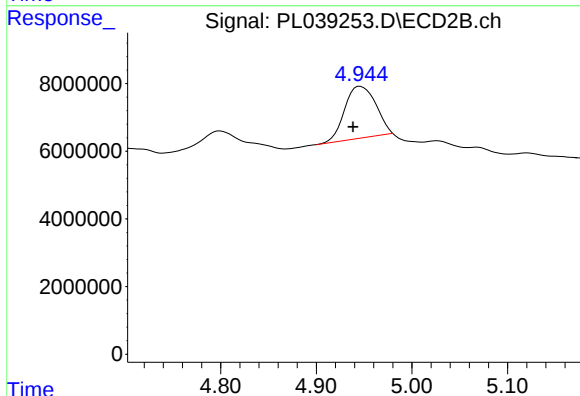


#7 delta-BHC

R.T.: 4.946 min
Delta R.T.: 0.007 min
Response: 35059581
Conc: 8.81 ng/ml

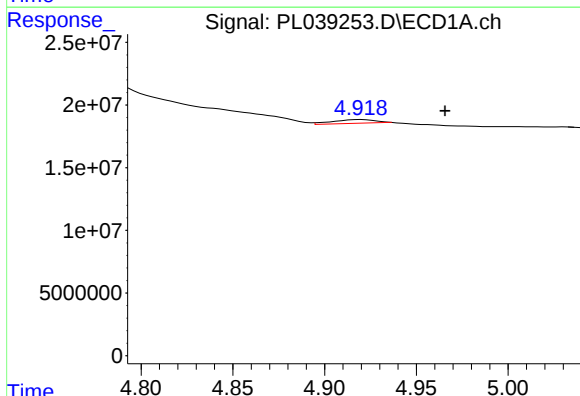


#8 Heptachlor epoxide

R.T.: 4.919 min
Delta R.T.: -0.046 min
Response: 5859743
Conc: 0.61 ng/ml

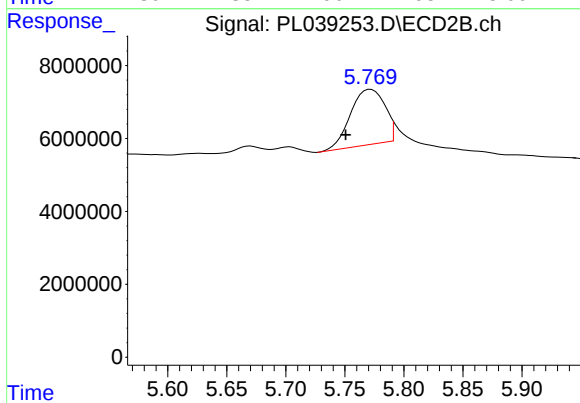

#8 Heptachlor epoxide


R.T.: 5.772 min
Delta R.T.: 0.021 min
Response: 30995122
Conc: 9.22 ng/ml

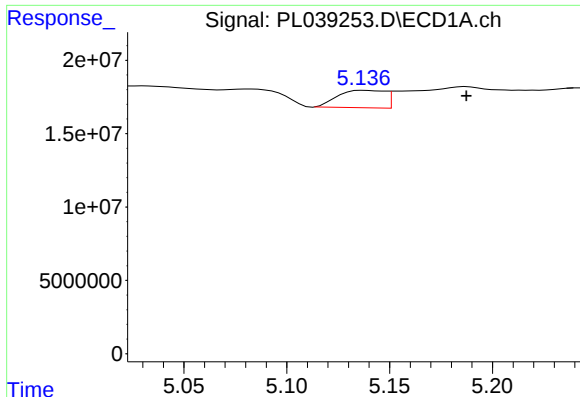

#10 gamma-Chlordane


R.T.: 5.138 min
Delta R.T.: -0.050 min
Response: 18628142
Conc: 1.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

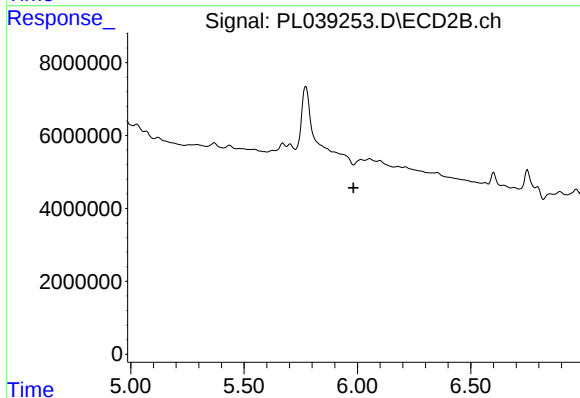


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

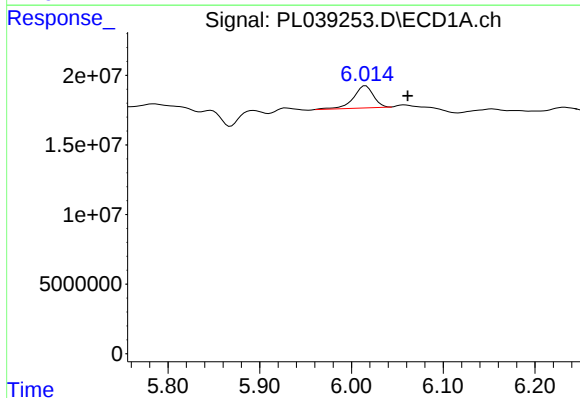


#15 Endosulfan II

R.T.: 6.016 min
Delta R.T.: -0.046 min
Response: 24141871
Conc: 2.78 ng/ml

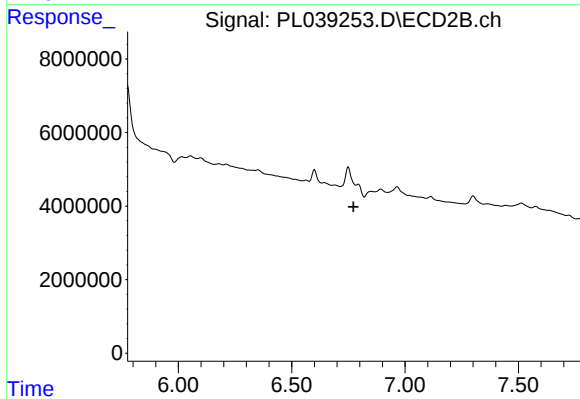

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

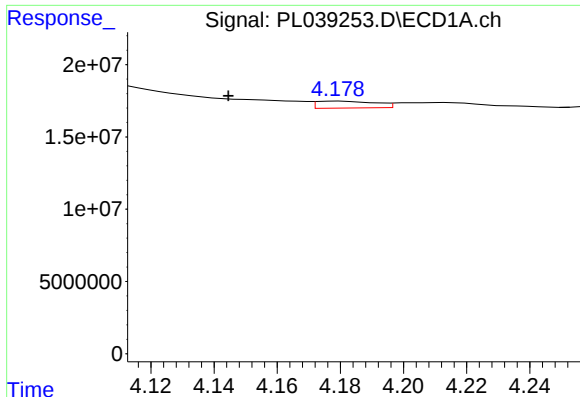

#23 Chlordane-1


R.T.: 4.179 min
Delta R.T.: 0.035 min
Response: 6174677
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

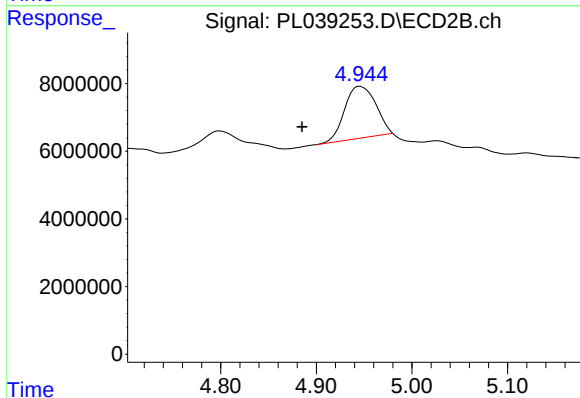


#23 Chlordane-1

R.T.: 4.946 min
Delta R.T.: 0.061 min
Response: 35059581
Conc: 280.62 ng/ml

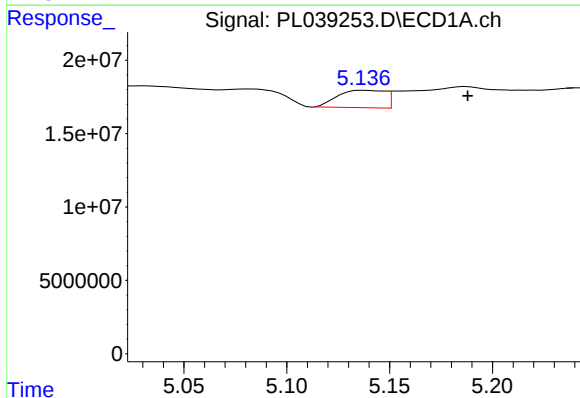


#25 Chlordane-3

R.T.: 5.138 min
Delta R.T.: -0.050 min
Response: 18628142
Conc: 17.05 ng/ml

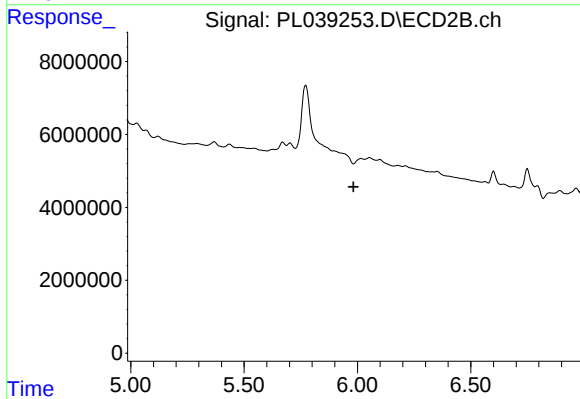

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

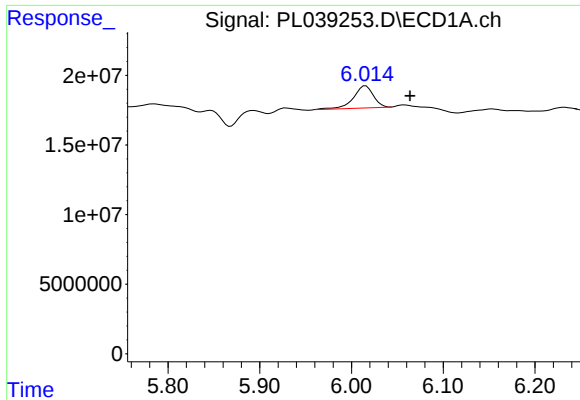

#27 Chlordane-5


R.T.: 6.016 min
Delta R.T.: -0.048 min
Response: 24141871
Conc: 74.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

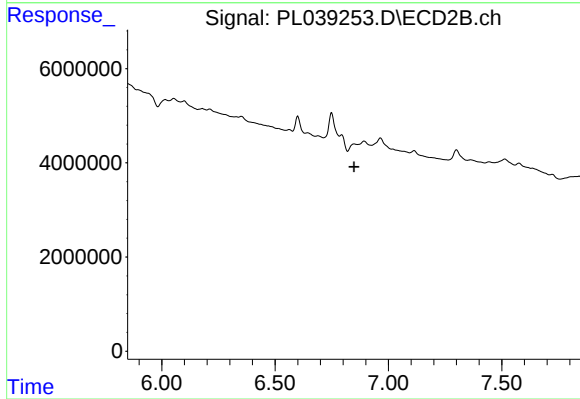


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

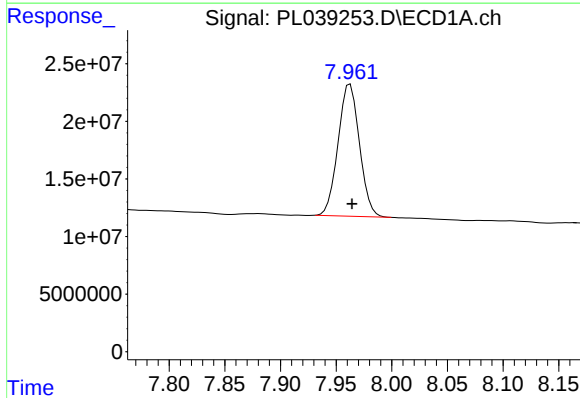

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 153360412
Conc: 21.84 ng/ml

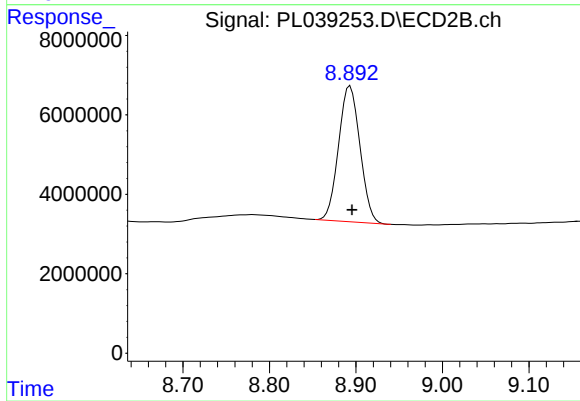

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 58309068
Conc: 25.13 ng/ml