

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 18:19
 Operator : AJ\SJ
 Sample : PB112168TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 22:49:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.906	130.4E6	54419803	18.650	20.299
28)	SA Decachlor...	7.961	8.893	129.0E6	50650054	18.363	21.826
Target Compounds							
3)	MA gamma-BHC...	4.058f	0.000	90048696	0	8.490	N.D. #
6)	B beta-BHC	4.216f	0.000	12923673	0	2.782	N.D. #
7)	B delta-BHC	0.000	4.952	0	10811766	N.D.	2.715 #
8)	B Heptachlo...	4.920f	5.772	2430623	7758777	0.255	2.307 #
17)	MA 4,4'-DDT	6.159	0.000	10261453	0	1.354	N.D. #
18)	B Endrin al...	6.159f	0.000	10261453	0	1.514	N.D. #
20)	A Methoxychlor	6.635f	0.000	15465261	0	3.779	N.D. #
23)	Chlordane-1	0.000	4.952	0	10811766	N.D.	86.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 18:19
Operator : AJ\SJ
Sample : PB112168TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 22:49:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

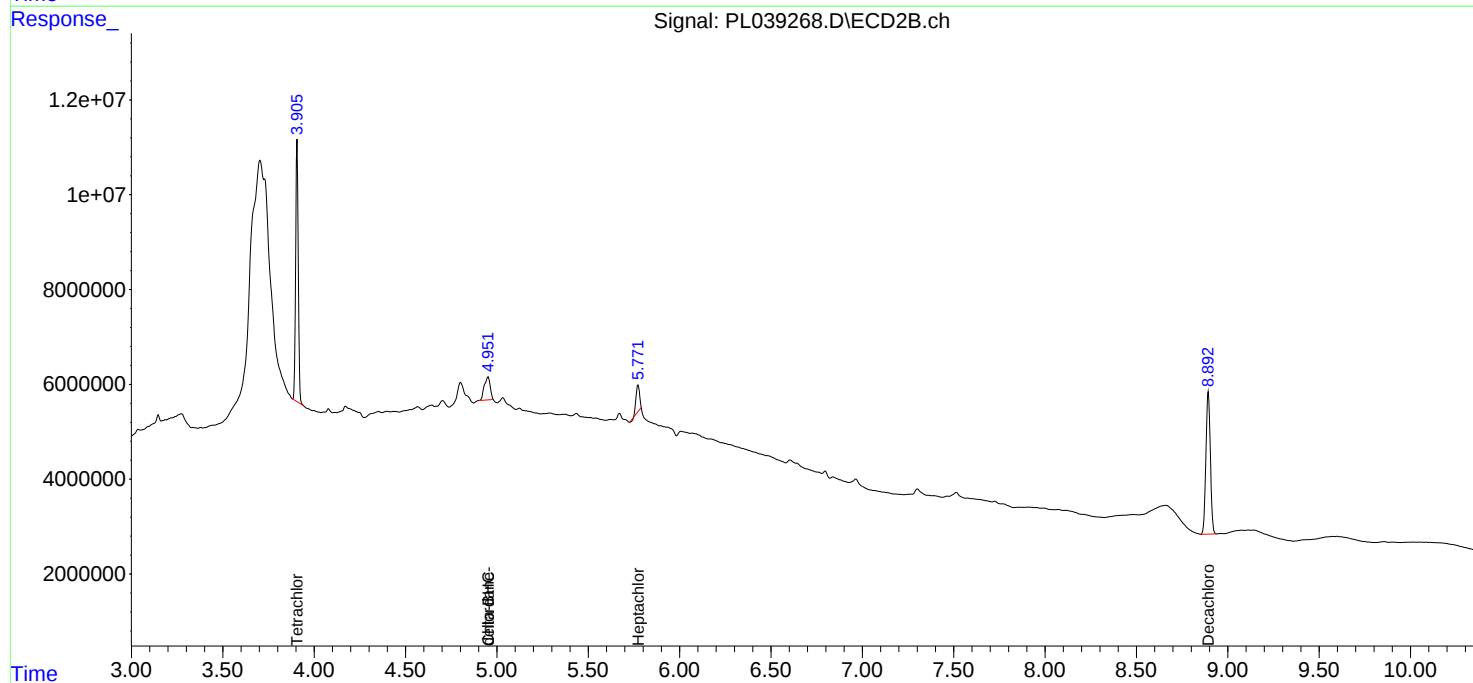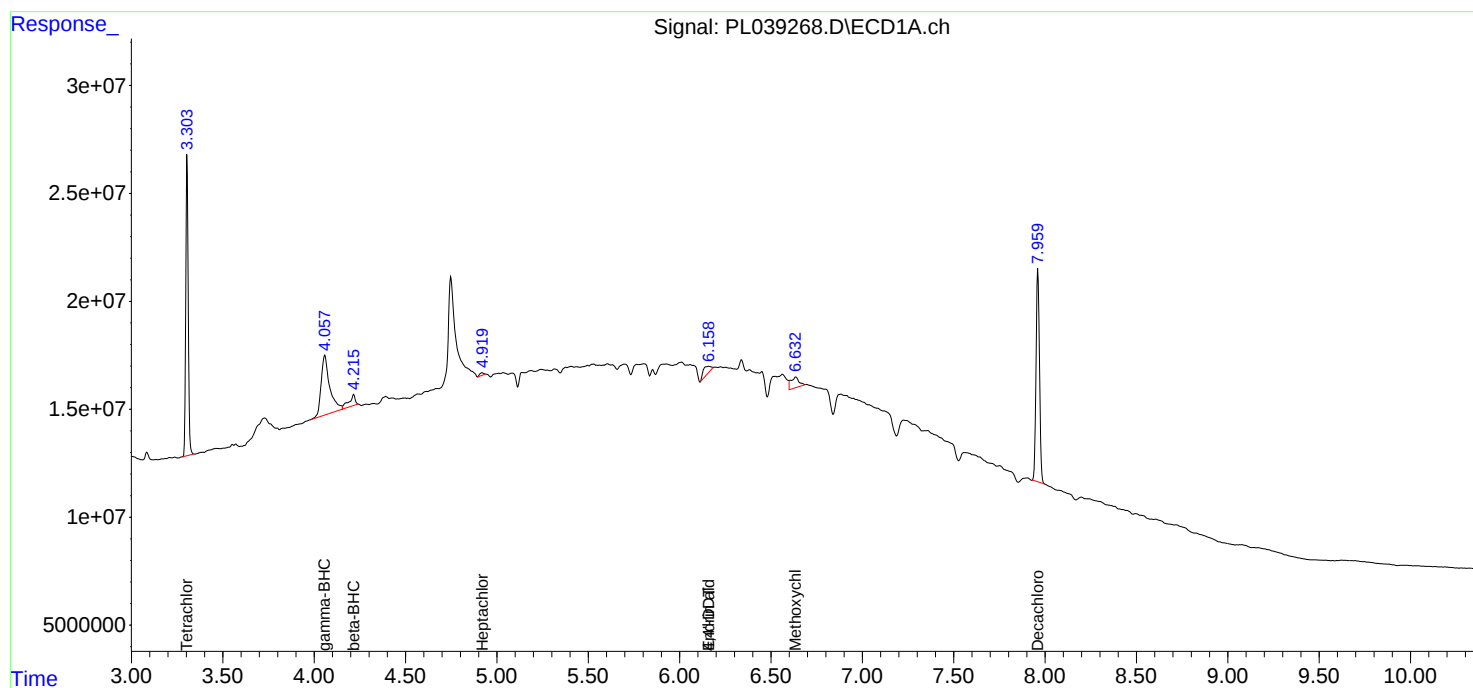


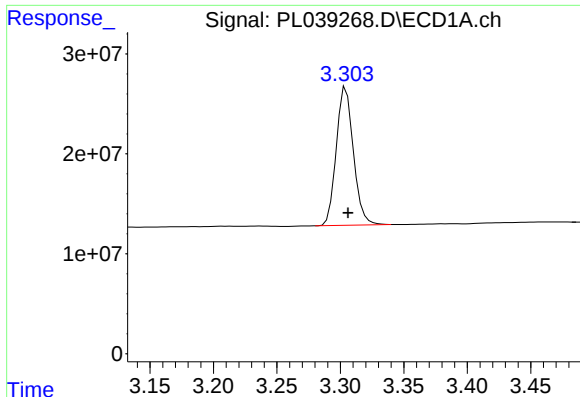

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 130373828
Conc: 18.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

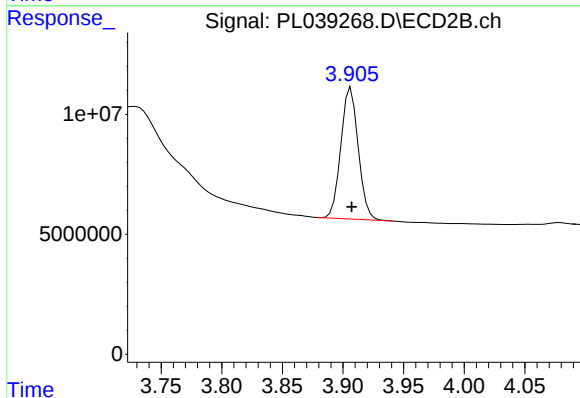


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 54419803
Conc: 20.30 ng/ml

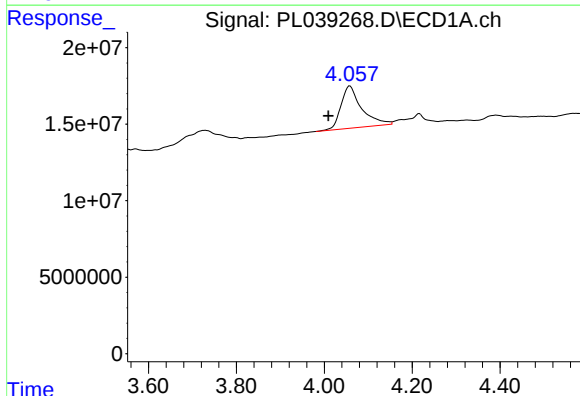


#3 gamma-BHC (Lindane)

R.T.: 4.058 min
Delta R.T.: 0.049 min
Response: 90048696
Conc: 8.49 ng/ml

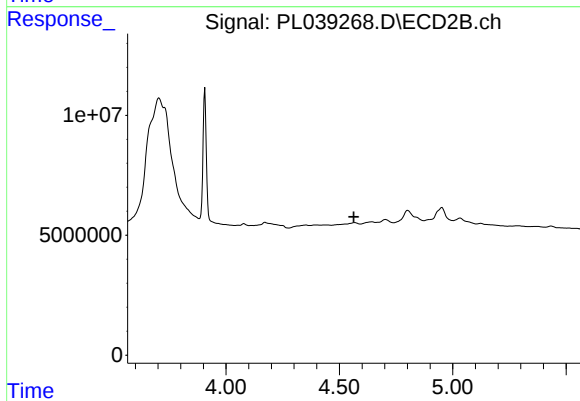

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

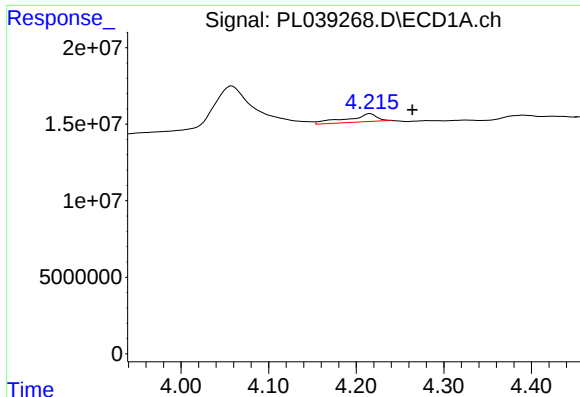

#6 beta-BHC


R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 12923673
Conc: 2.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

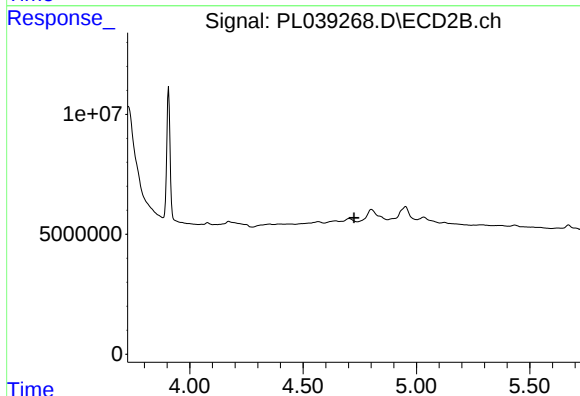


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

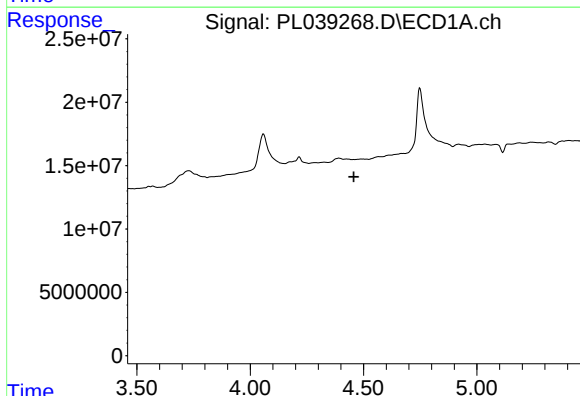


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

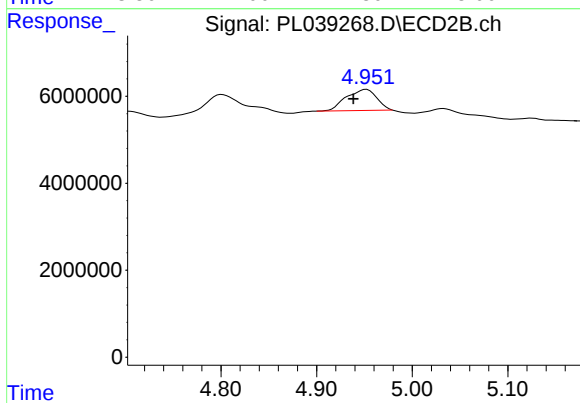

#7 delta-BHC


R.T.: 4.952 min
Delta R.T.: 0.014 min
Response: 10811766
Conc: 2.72 ng/ml

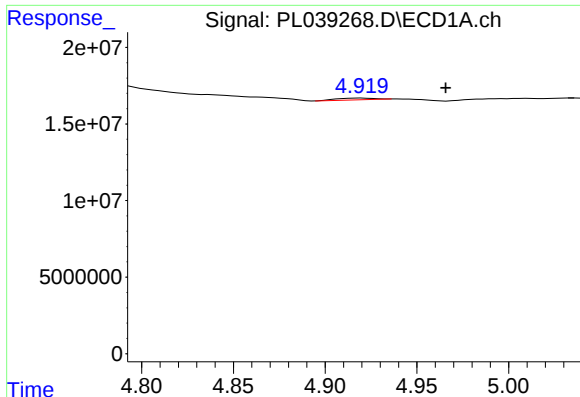

#8 Heptachlor epoxide


R.T.: 4.920 min
Delta R.T.: -0.046 min
Response: 2430623
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

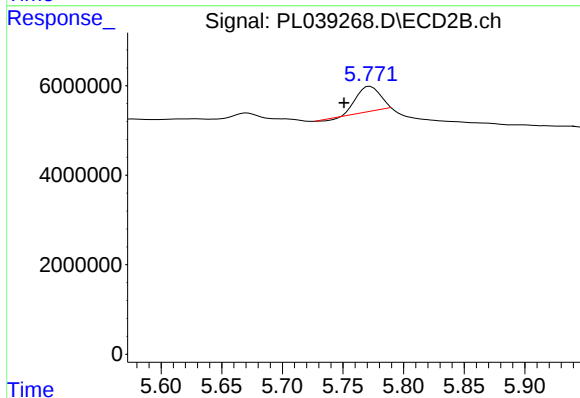


#8 Heptachlor epoxide

R.T.: 5.772 min
Delta R.T.: 0.022 min
Response: 7758777
Conc: 2.31 ng/ml

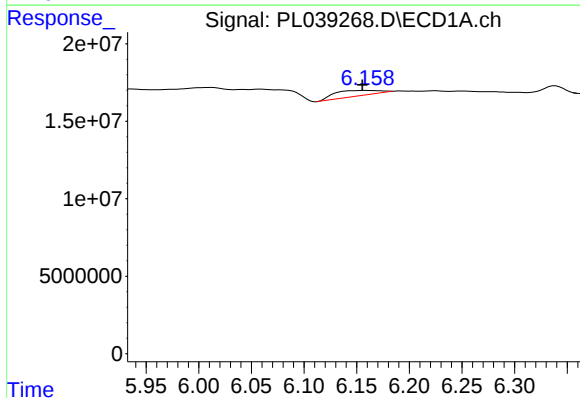


#17 4,4'-DDT

R.T.: 6.159 min
Delta R.T.: 0.004 min
Response: 10261453
Conc: 1.35 ng/ml

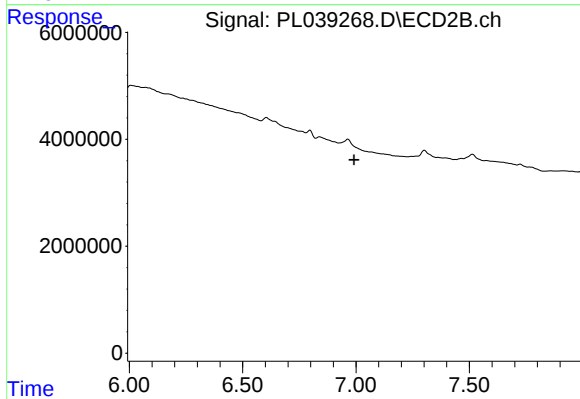

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

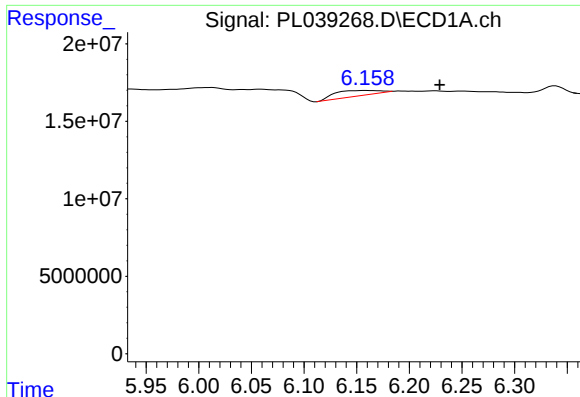

#18 Endrin aldehyde


R.T.: 6.159 min
Delta R.T.: -0.070 min
Response: 10261453
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

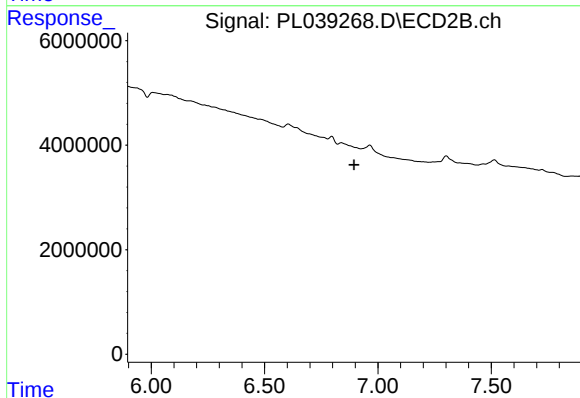


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

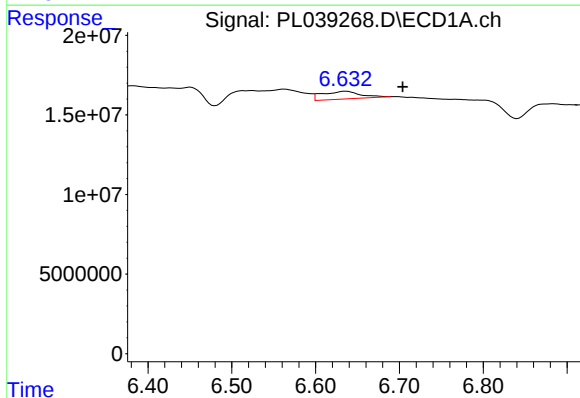


#20 Methoxychlor

R.T.: 6.635 min
Delta R.T.: -0.069 min
Response: 15465261
Conc: 3.78 ng/ml

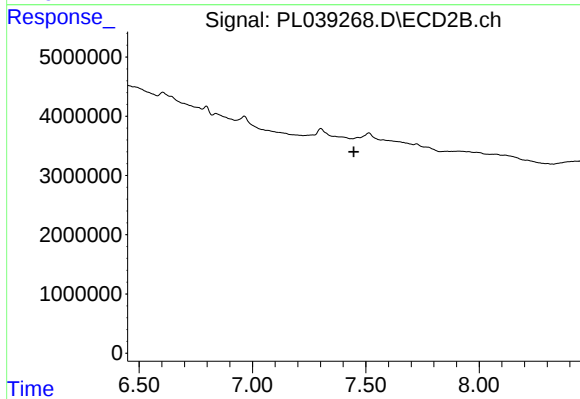

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

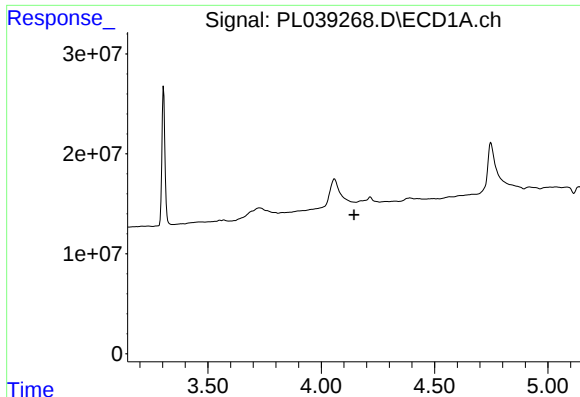

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

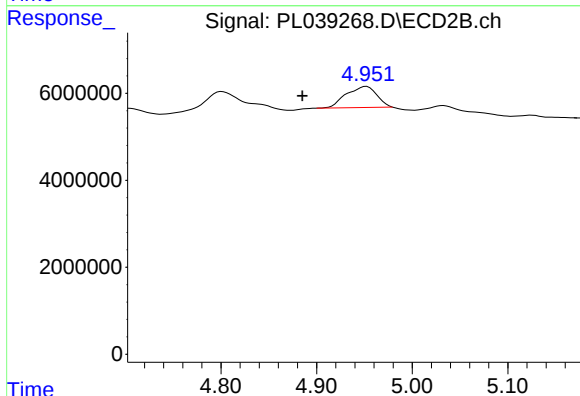


#23 Chlordane-1

R.T.: 4.952 min
Delta R.T.: 0.067 min
Response: 10811766
Conc: 86.54 ng/ml

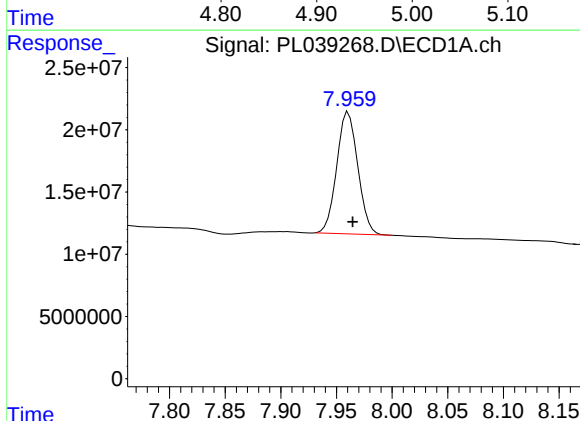

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 128970879
Conc: 18.36 ng/ml

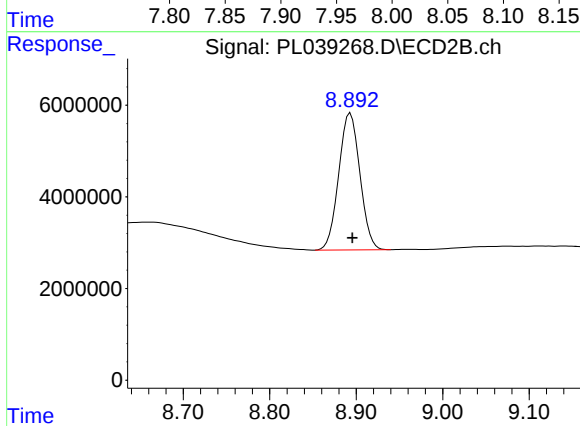

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: -0.002 min
Response: 50650054
Conc: 21.83 ng/ml