

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 21:38
 Operator : AJ\SJ
 Sample : J4521-27
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 22:54:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	154.1E6	65252035	22.051	24.340
28)	SA Decachlor...	7.962	8.895	145.6E6	56056863	20.734	24.156
Target Compounds							
3)	MA gamma-BHC...	4.059f	0.000	51534749	0	4.859	N.D. #
6)	B beta-BHC	4.218f	0.000	14530658	0	3.128	N.D. #
7)	B delta-BHC	0.000	4.933	0	10395922	N.D.	2.611 #
8)	B Heptachlo...	4.917f	5.774	2032841	4680759	0.213	1.392 #
10)	B gamma-Chl...	5.134f	0.000	9659422	0	0.978	N.D. #
17)	MA 4,4'-DDT	6.161	0.000	10318484	0	1.361	N.D. #
18)	B Endrin al...	6.161f	0.000	10318484	0	1.523	N.D. #
20)	A Methoxychlor	6.637f	0.000	16978992	0	4.149	N.D. #
23)	Chlordane-1	0.000	4.933	0	10395922	N.D.	83.211 #
25)	Chlordane-3	5.134	0.000	9659422	0	8.843	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 21:38
Operator : AJ\SJ
Sample : J4521-27
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 22:54:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

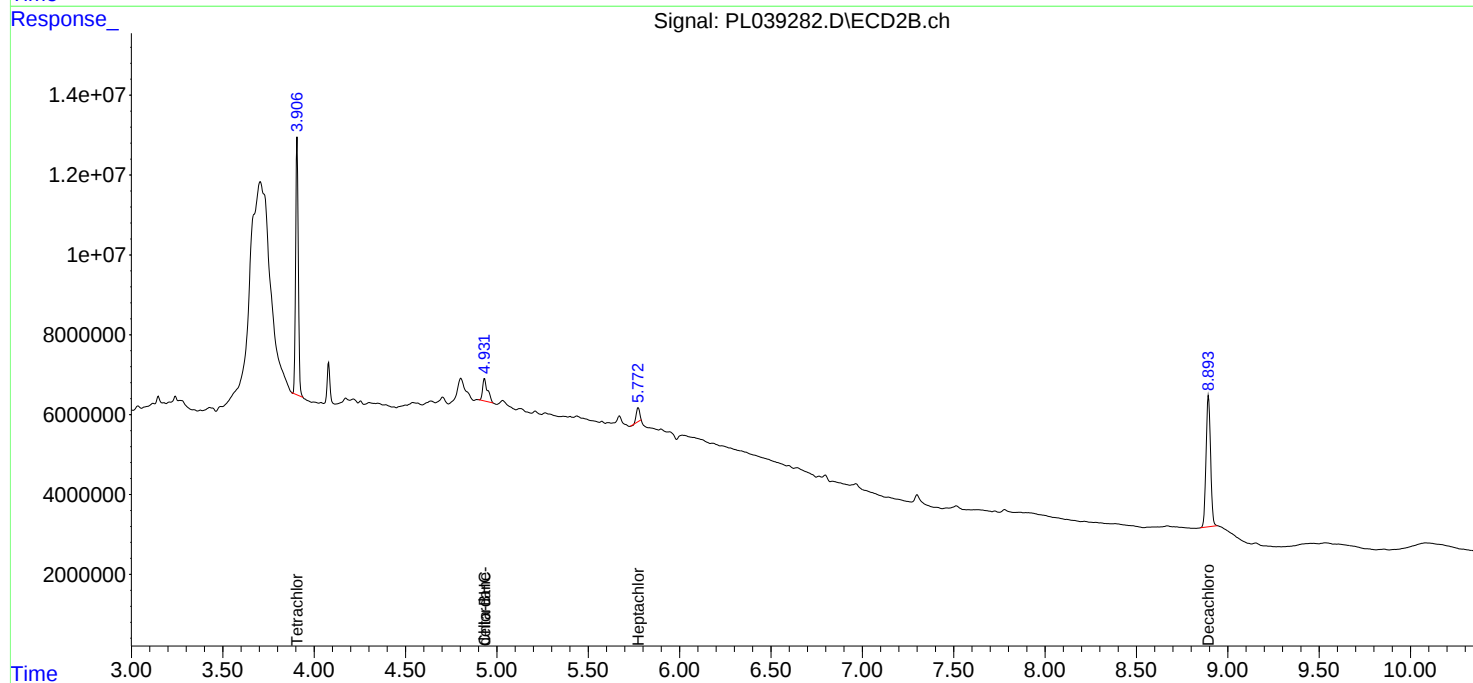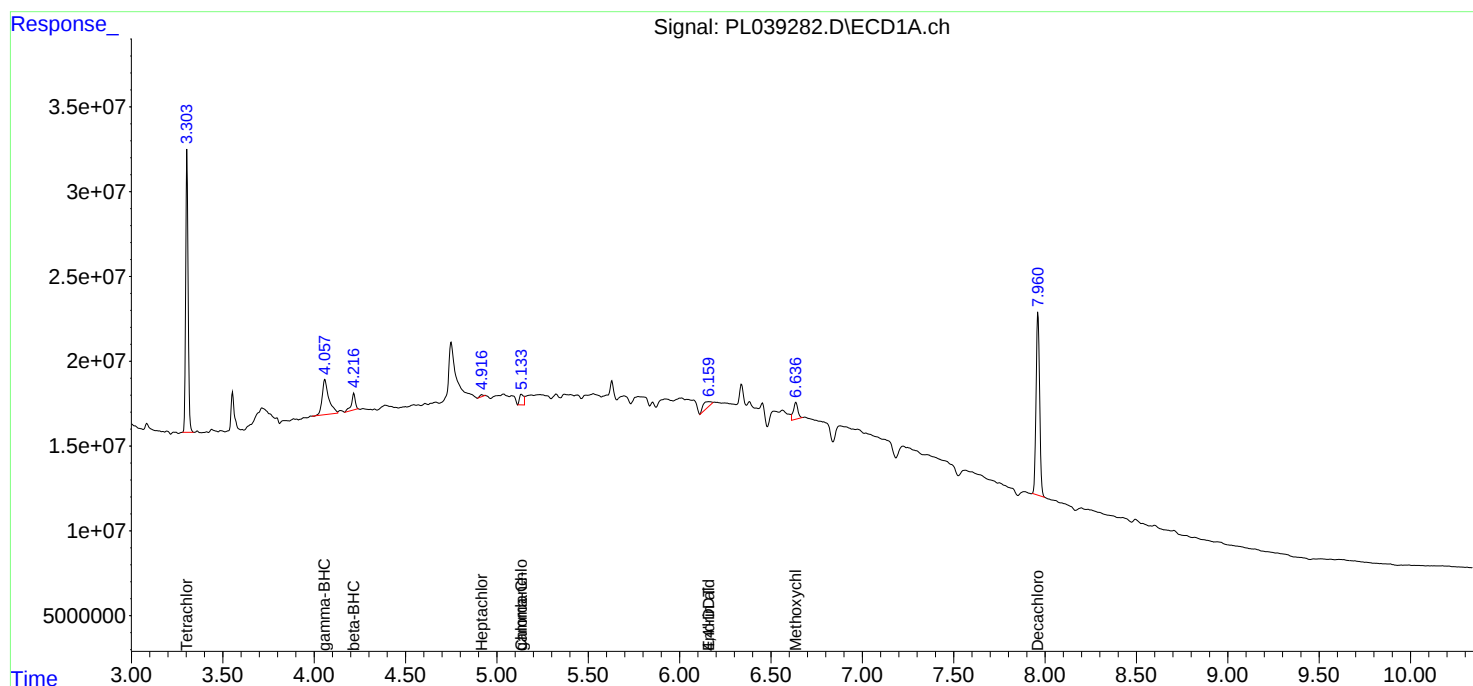


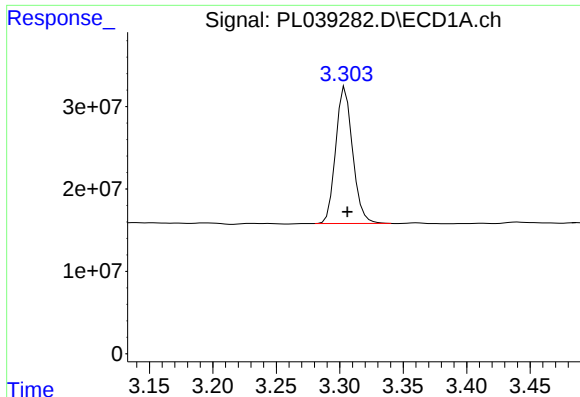

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 154147911
Conc: 22.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

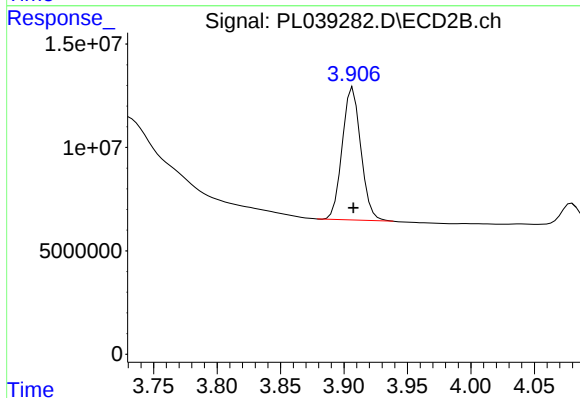


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 65252035
Conc: 24.34 ng/ml

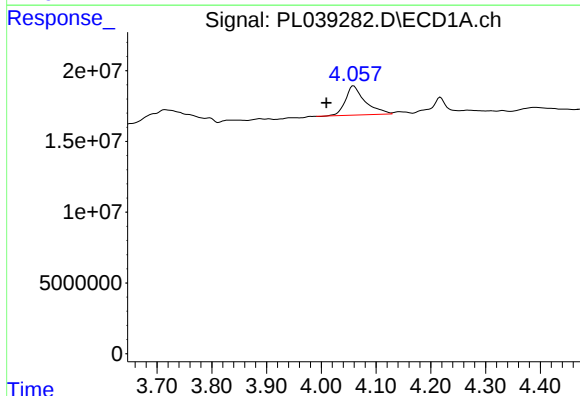


#3 gamma-BHC (Lindane)

R.T.: 4.059 min
Delta R.T.: 0.050 min
Response: 51534749
Conc: 4.86 ng/ml

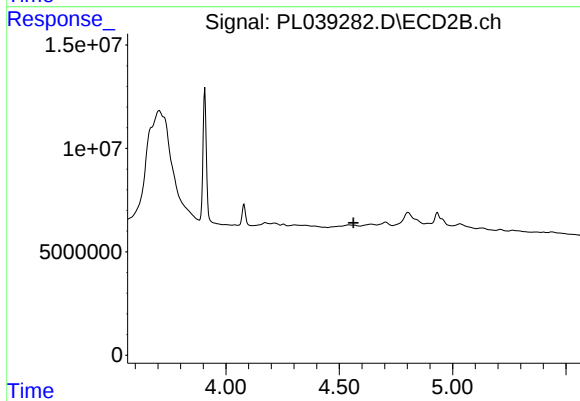

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

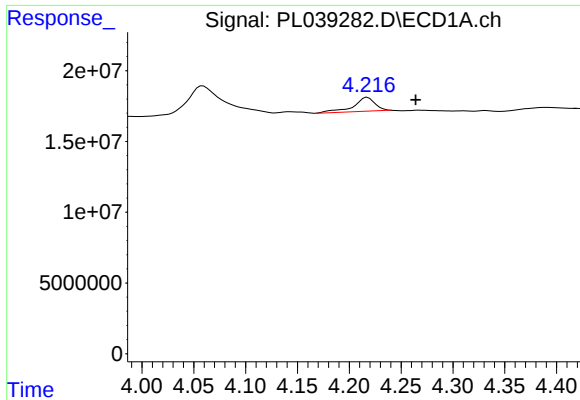

#6 beta-BHC


R.T.: 4.218 min
Delta R.T.: -0.046 min
Response: 14530658
Conc: 3.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

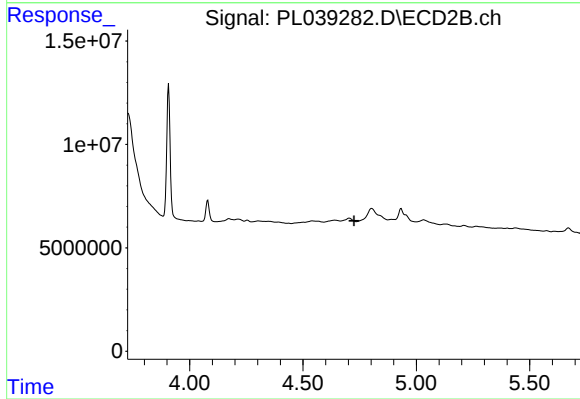


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

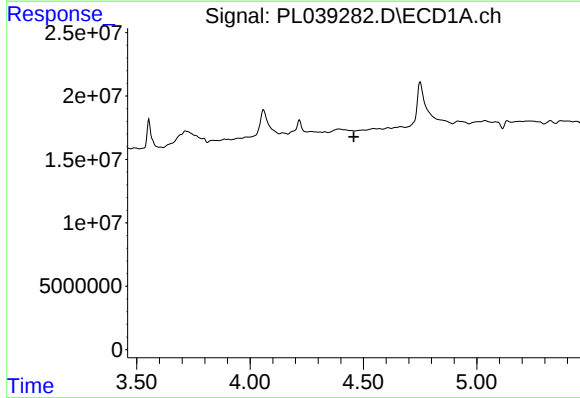


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

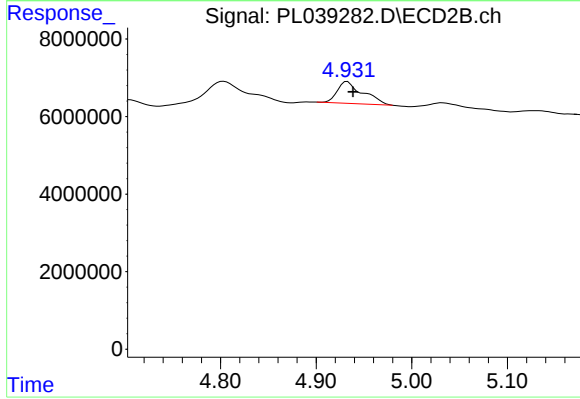

#7 delta-BHC


R.T.: 4.933 min
Delta R.T.: -0.006 min
Response: 10395922
Conc: 2.61 ng/ml

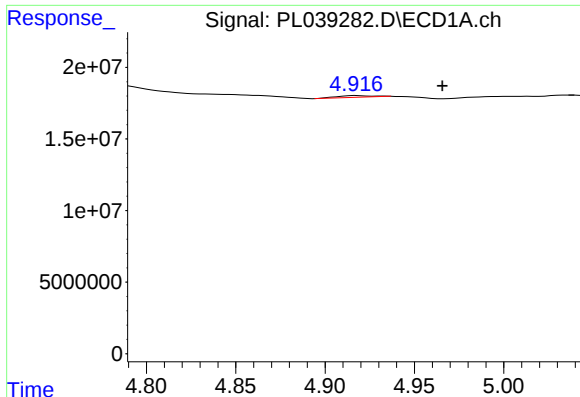

#8 Heptachlor epoxide


R.T.: 4.917 min
Delta R.T.: -0.048 min
Response: 2032841
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

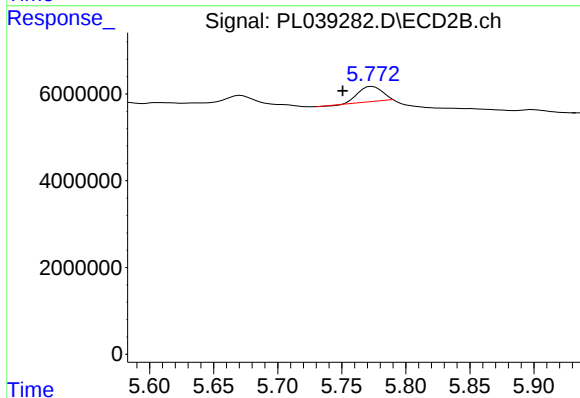


#8 Heptachlor epoxide

R.T.: 5.774 min
Delta R.T.: 0.023 min
Response: 4680759
Conc: 1.39 ng/ml

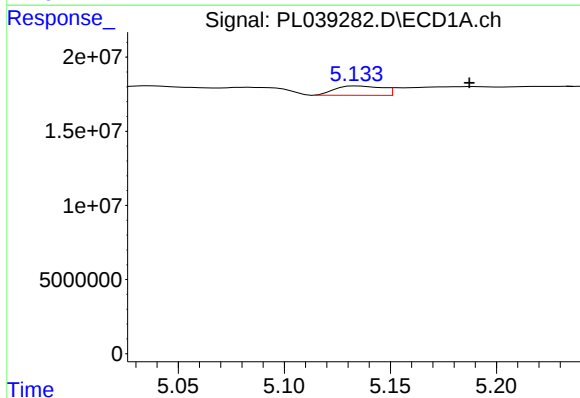


#10 gamma-Chlordane

R.T.: 5.134 min
Delta R.T.: -0.053 min
Response: 9659422
Conc: 0.98 ng/ml

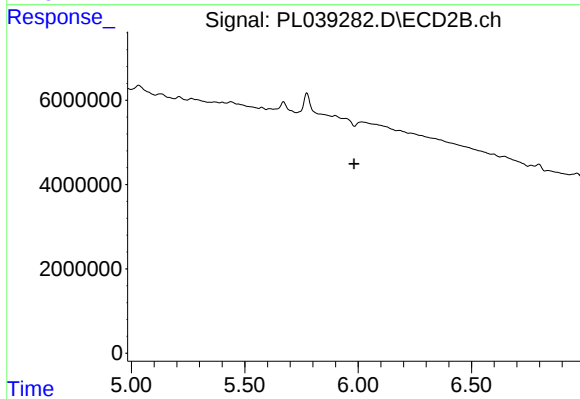

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.983 min
Response: 0
Conc: N.D.

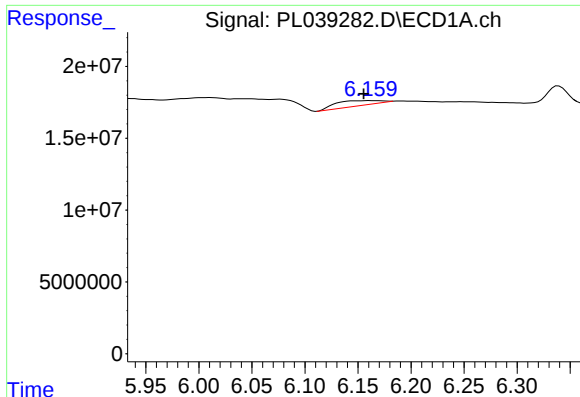

#17 4,4'-DDT


R.T.: 6.161 min
Delta R.T.: 0.006 min
Response: 10318484
Conc: 1.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

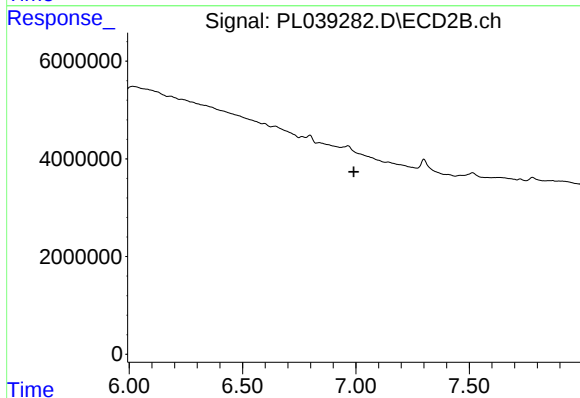


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

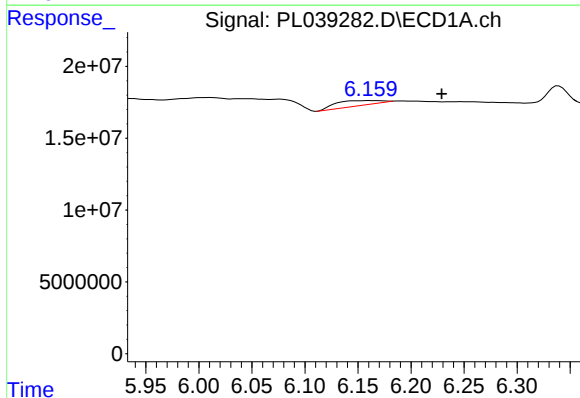


#18 Endrin aldehyde

R.T.: 6.161 min
Delta R.T.: -0.068 min
Response: 10318484
Conc: 1.52 ng/ml

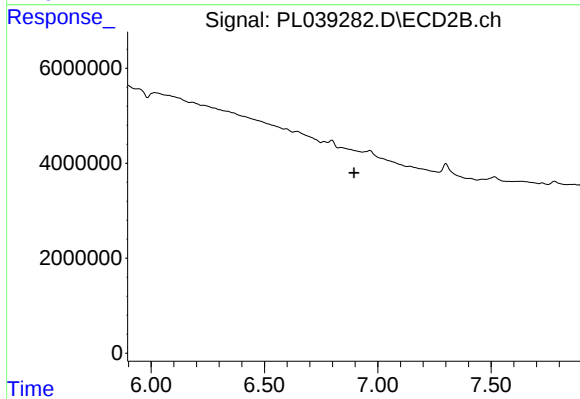

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

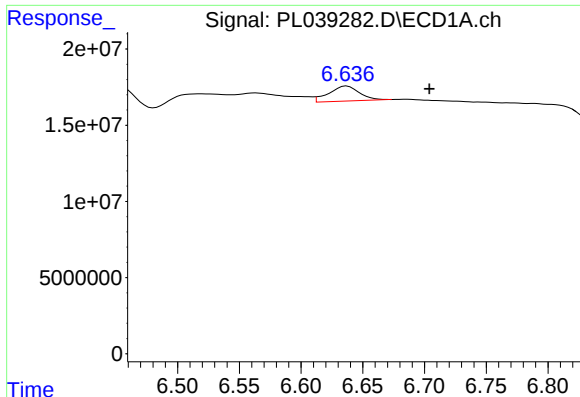

#20 Methoxychlor


R.T.: 6.637 min
Delta R.T.: -0.067 min
Response: 16978992
Conc: 4.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

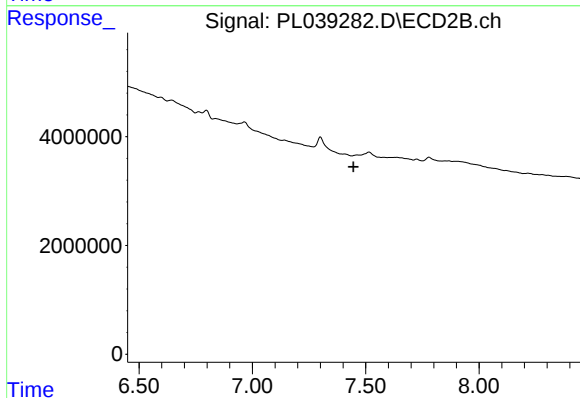


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

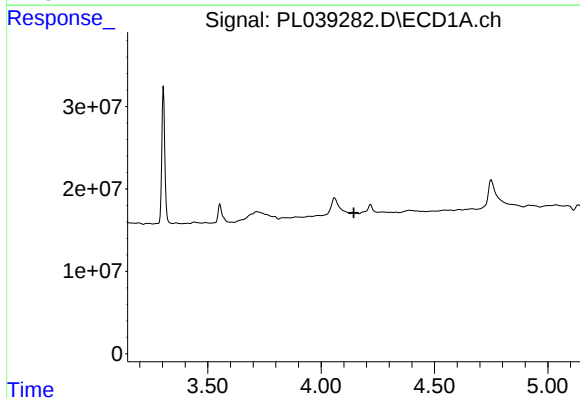


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.145 min
Response: 0
Conc: N.D.

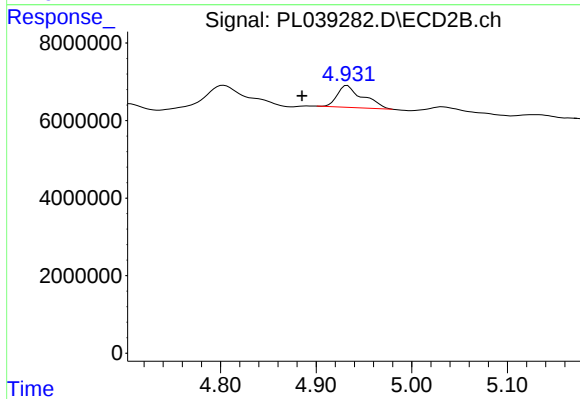

#23 Chlordane-1


R.T.: 4.933 min
Delta R.T.: 0.047 min
Response: 10395922
Conc: 83.21 ng/ml

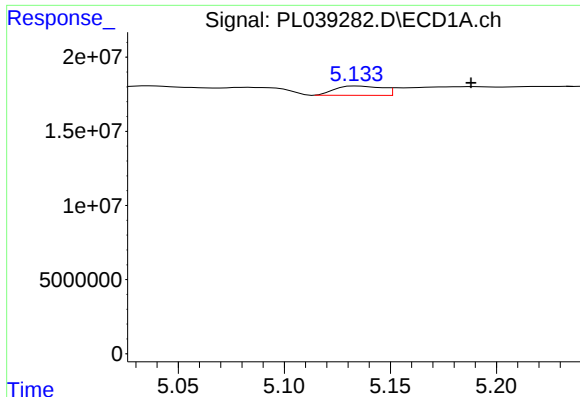

#25 Chlordane-3


R.T.: 5.134 min
Delta R.T.: -0.054 min
Response: 9659422
Conc: 8.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

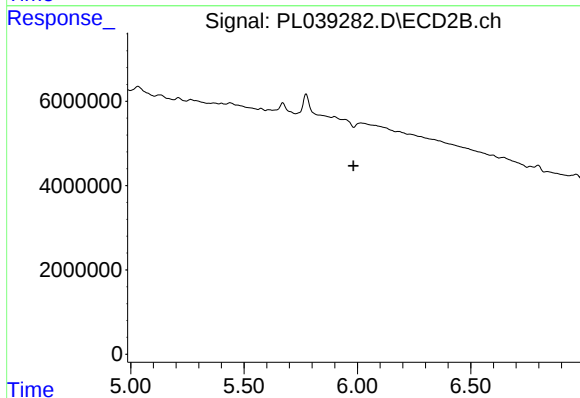


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

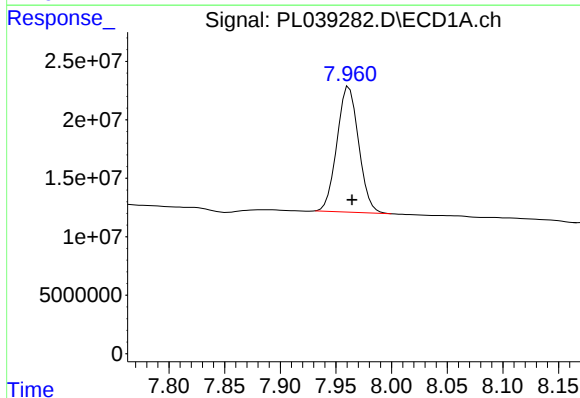

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 145621079
Conc: 20.73 ng/ml

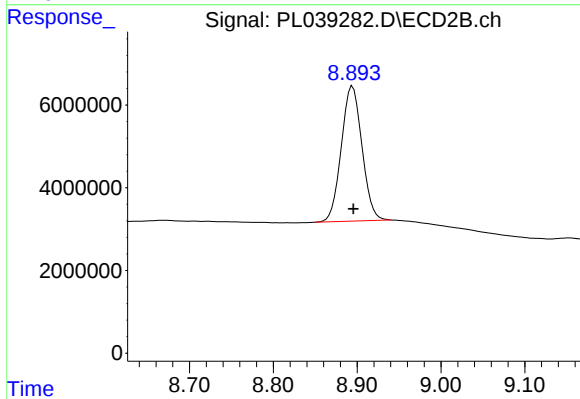

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 56056863
Conc: 24.16 ng/ml