

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 22:06
 Operator : AJ\SJ
 Sample : J4523-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 22:54:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	134.8E6	57781492	19.290	21.553
28)	SA Decachlor...	7.962	8.895	86271795	32864203	12.283	14.162
Target Compounds							
2)	A alpha-BHC	3.729	0.000	12162176	0	1.029	N.D. #
3)	MA gamma-BHC...	4.055f	0.000	83263522	0	7.850	N.D. #
6)	B beta-BHC	4.220f	0.000	13934623	0	3.000	N.D. #
7)	B delta-BHC	0.000	4.932	0	7246591	N.D.	1.820 #
8)	B Heptachlo...	0.000	5.774	0	4551840	N.D.	1.353 #
17)	MA 4,4'-DDT	6.159	0.000	30000699	0	3.958	N.D. #
19)	B Endosulfa...	6.509f	0.000	21325892	0	2.621	N.D. #
20)	A Methoxychlor	6.637f	0.000	17592736	0	4.299	N.D. #
23)	Chlordane-1	0.000	4.932	0	7246591	N.D.	58.003 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 22:06
Operator : AJ\SJ
Sample : J4523-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 22:54:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

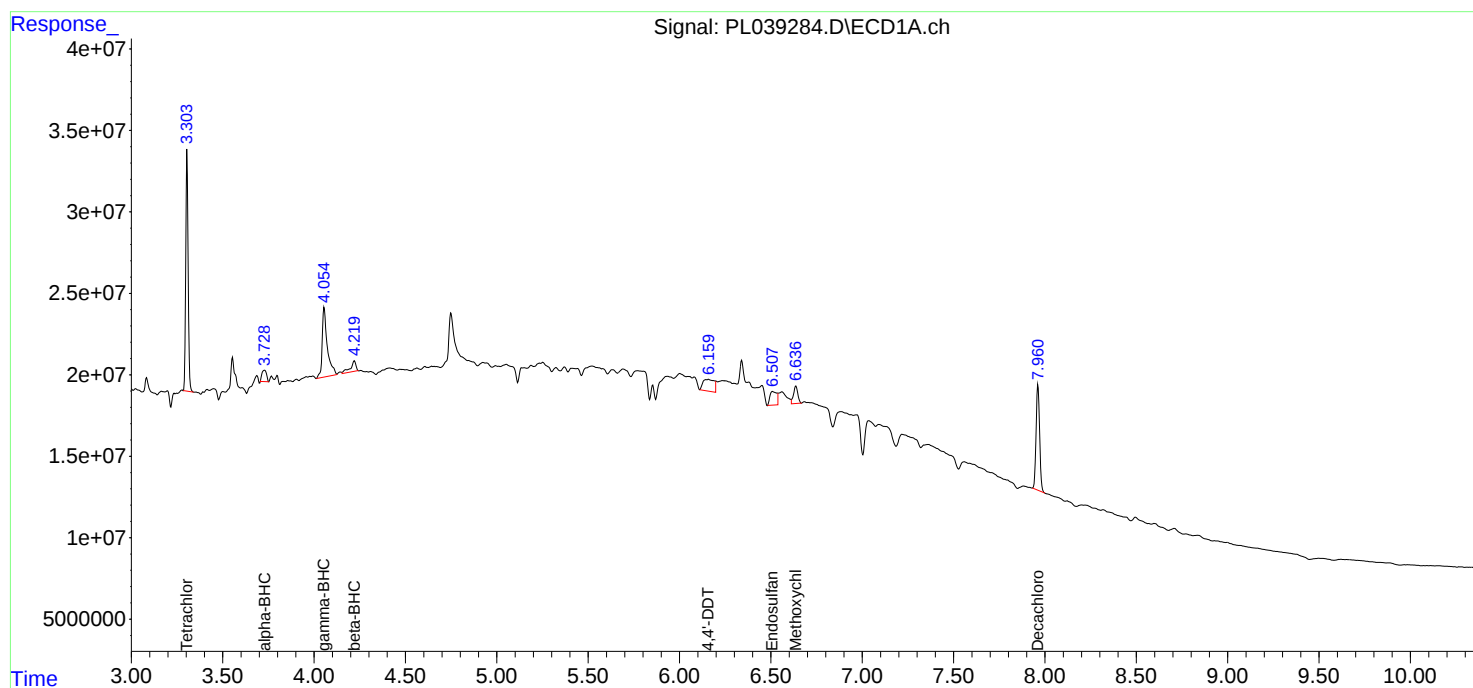


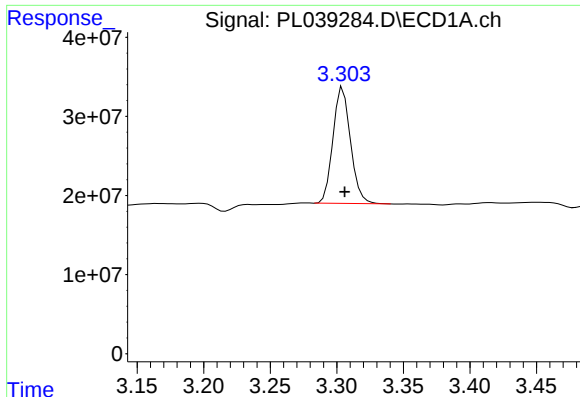

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 134847864
Conc: 19.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

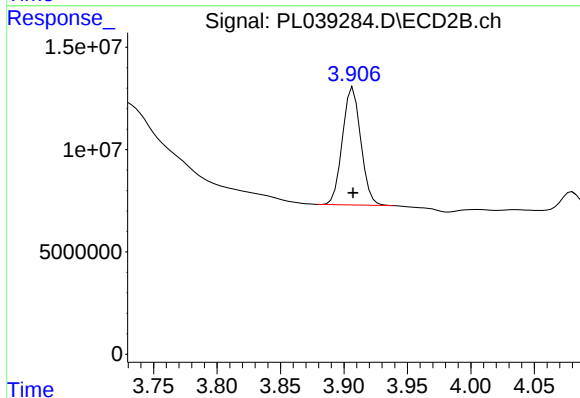


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 57781492
Conc: 21.55 ng/ml

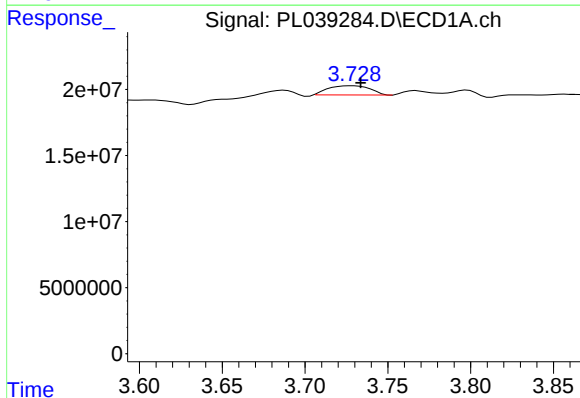


#2 alpha-BHC

R.T.: 3.729 min
Delta R.T.: -0.005 min
Response: 12162176
Conc: 1.03 ng/ml

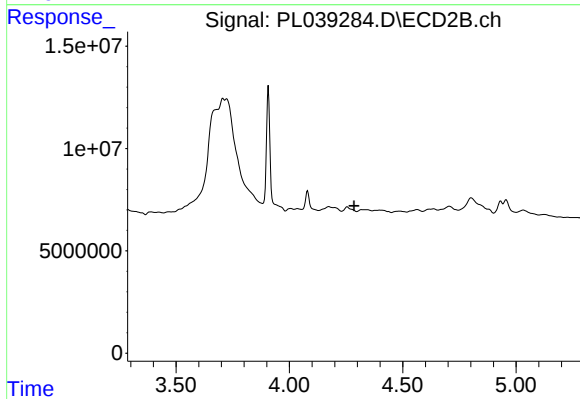

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

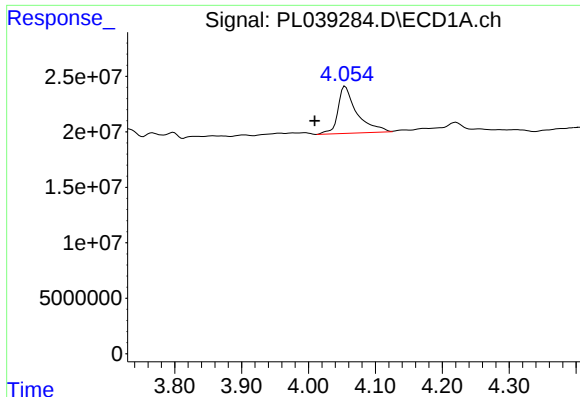

#3 gamma-BHC (Lindane)


R.T.: 4.055 min
Delta R.T.: 0.046 min
Response: 83263522
Conc: 7.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

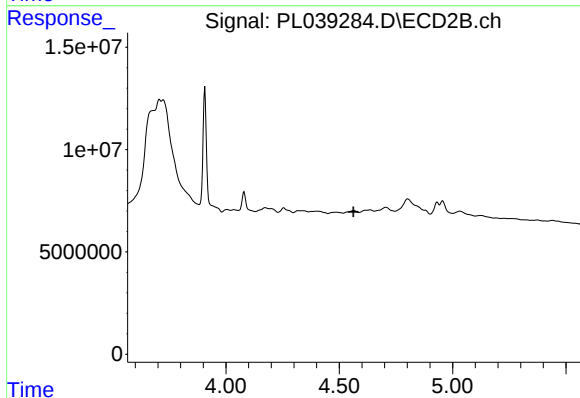


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

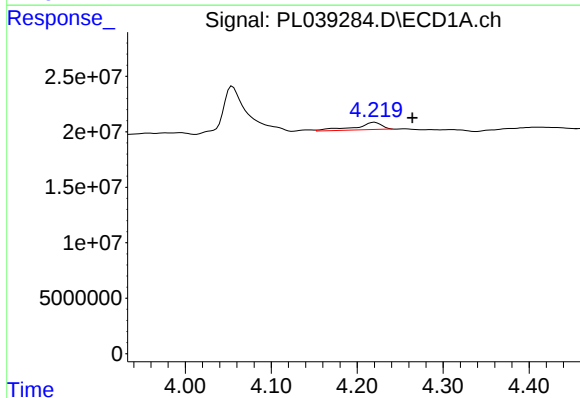


#6 beta-BHC

R.T.: 4.220 min
Delta R.T.: -0.044 min
Response: 13934623
Conc: 3.00 ng/ml

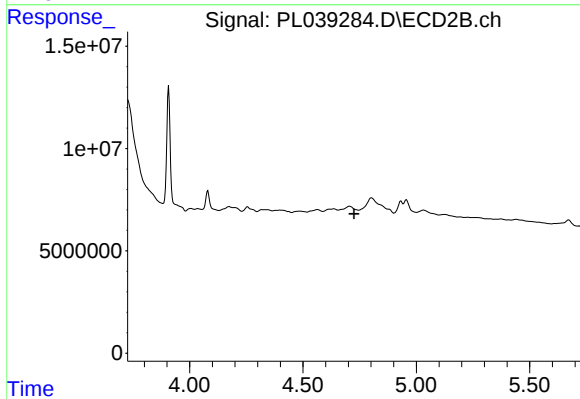

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

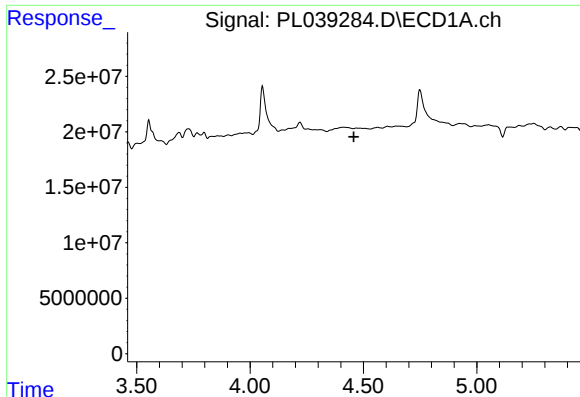

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

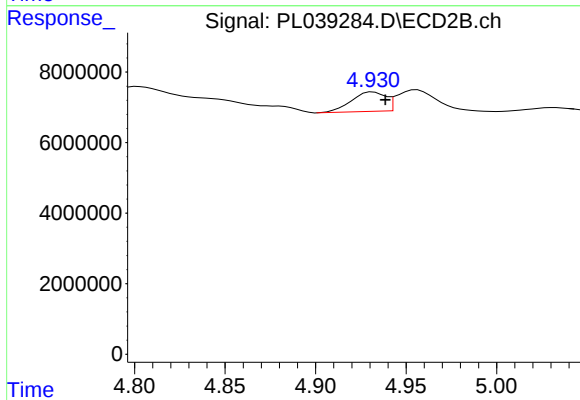


#7 delta-BHC

R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 7246591
Conc: 1.82 ng/ml

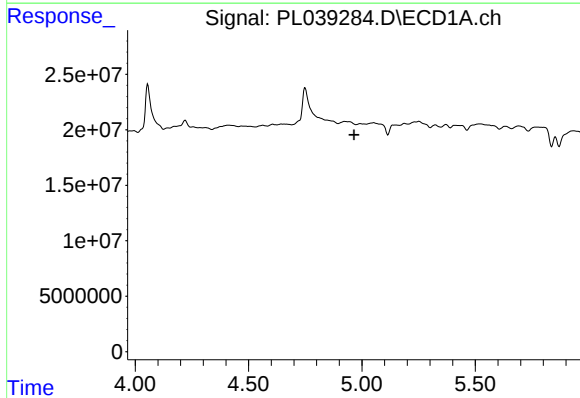


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

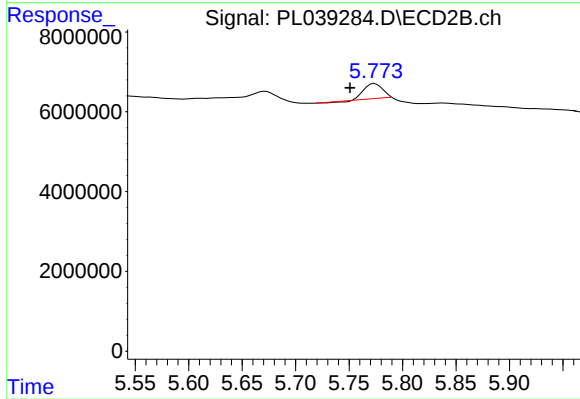

#8 Heptachlor epoxide


R.T.: 5.774 min
Delta R.T.: 0.023 min
Response: 4551840
Conc: 1.35 ng/ml

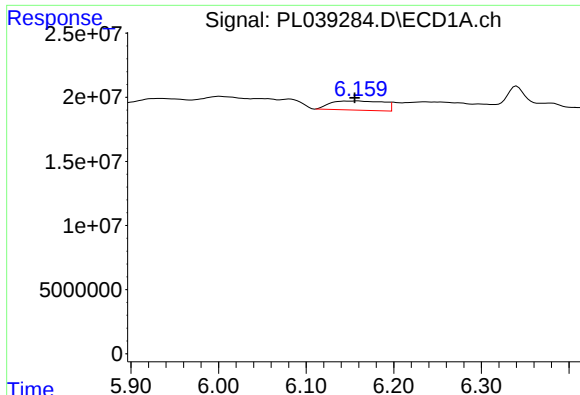

#17 4,4'-DDT


R.T.: 6.159 min
Delta R.T.: 0.003 min
Response: 30000699
Conc: 3.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

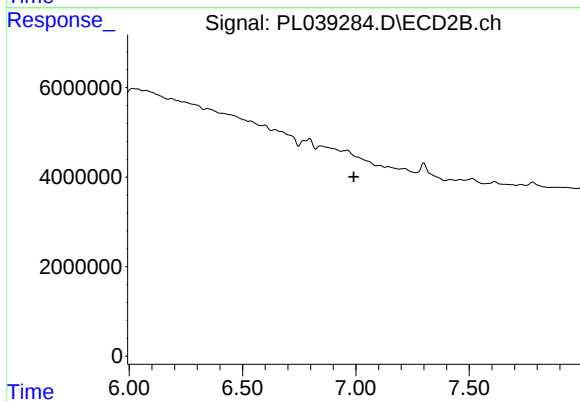


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

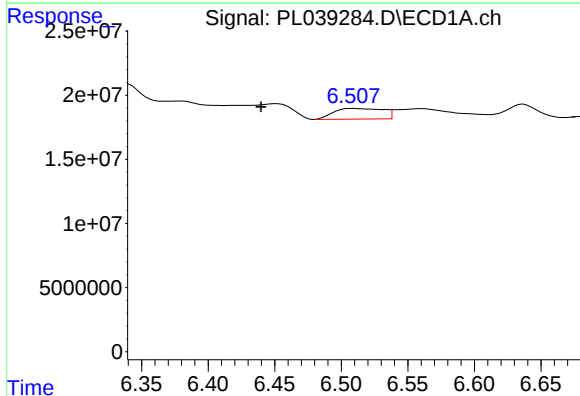


#19 Endosulfan Sulfate

R.T.: 6.509 min
Delta R.T.: 0.069 min
Response: 21325892
Conc: 2.62 ng/ml

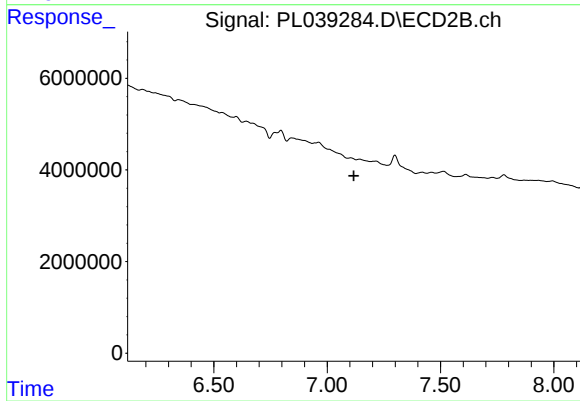

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

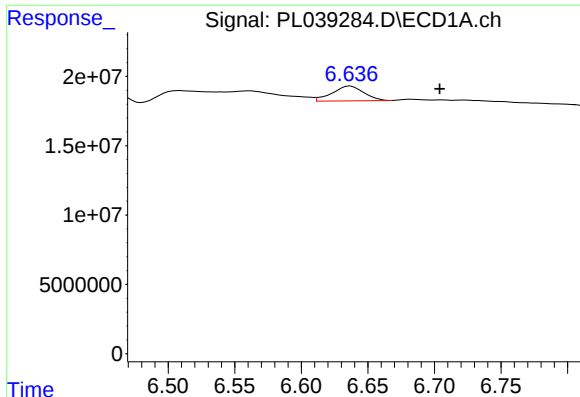

#20 Methoxychlor


R.T.: 6.637 min
Delta R.T.: -0.067 min
Response: 17592736
Conc: 4.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

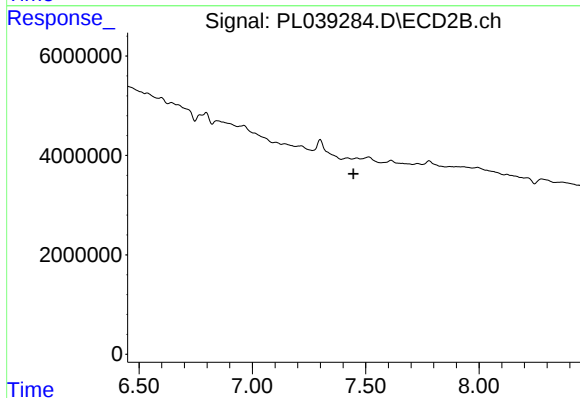


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

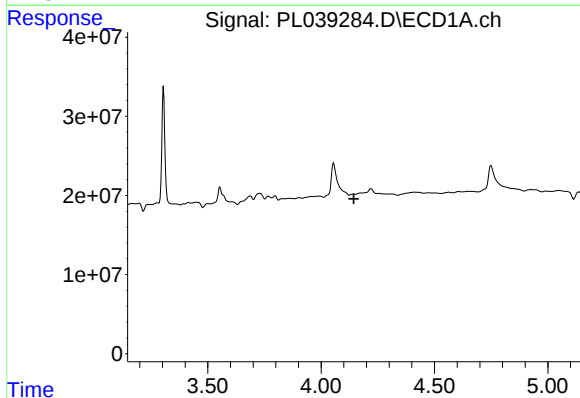


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.145 min
Response: 0
Conc: N.D.

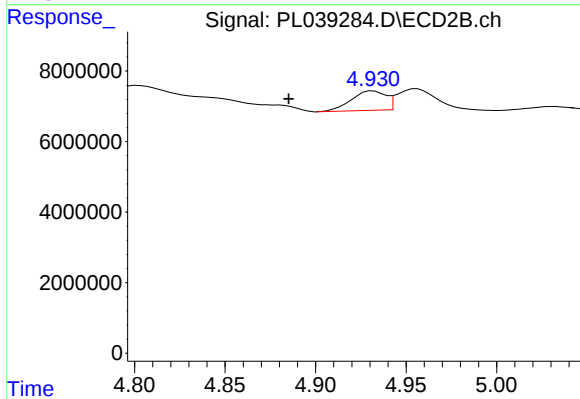

#23 Chlordane-1


R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 7246591
Conc: 58.00 ng/ml

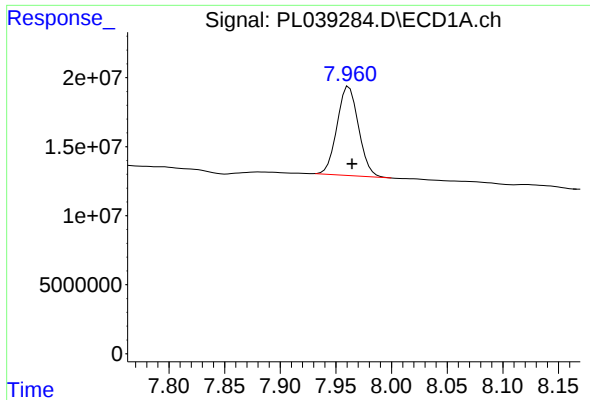

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 86271795
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

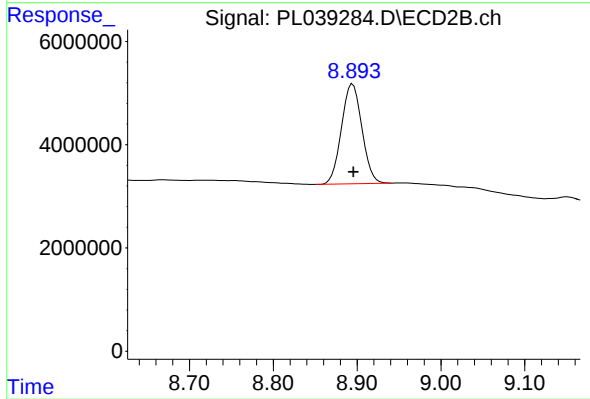

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 32864203
Conc: 14.16 ng/ml