

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2018 01:27
 Operator : AJ\SJ
 Sample : J4521-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:13:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.306	3.906	81134922	34800546	11.607	12.981
28)	SA Decachlor...	7.964	8.895	78786558	32044616	11.218	13.809
Target Compounds							
6)	B beta-BHC	4.218f	0.000	10986102	0	2.365	N.D. #
8)	B Heptachlo...	4.921f	5.774	1512558	4211166	0.158	1.252 #
10)	B gamma-Chl...	5.136f	0.000	8825752	0	0.894	N.D. #
16)	A 4,4'-DDD	5.857f	0.000	543921	0	0.068	N.D. #
17)	MA 4,4'-DDT	6.151	0.000	3553156	0	0.469	N.D. #
18)	B Endrin al...	6.191f	0.000	827952	0	0.122	N.D. #
24)	Chlordane-2	4.668	0.000	5053921	0	14.457	N.D. #
25)	Chlordane-3	5.136	0.000	8825752	0	8.080	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2018 01:27
Operator : AJ\SJ
Sample : J4521-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:13:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

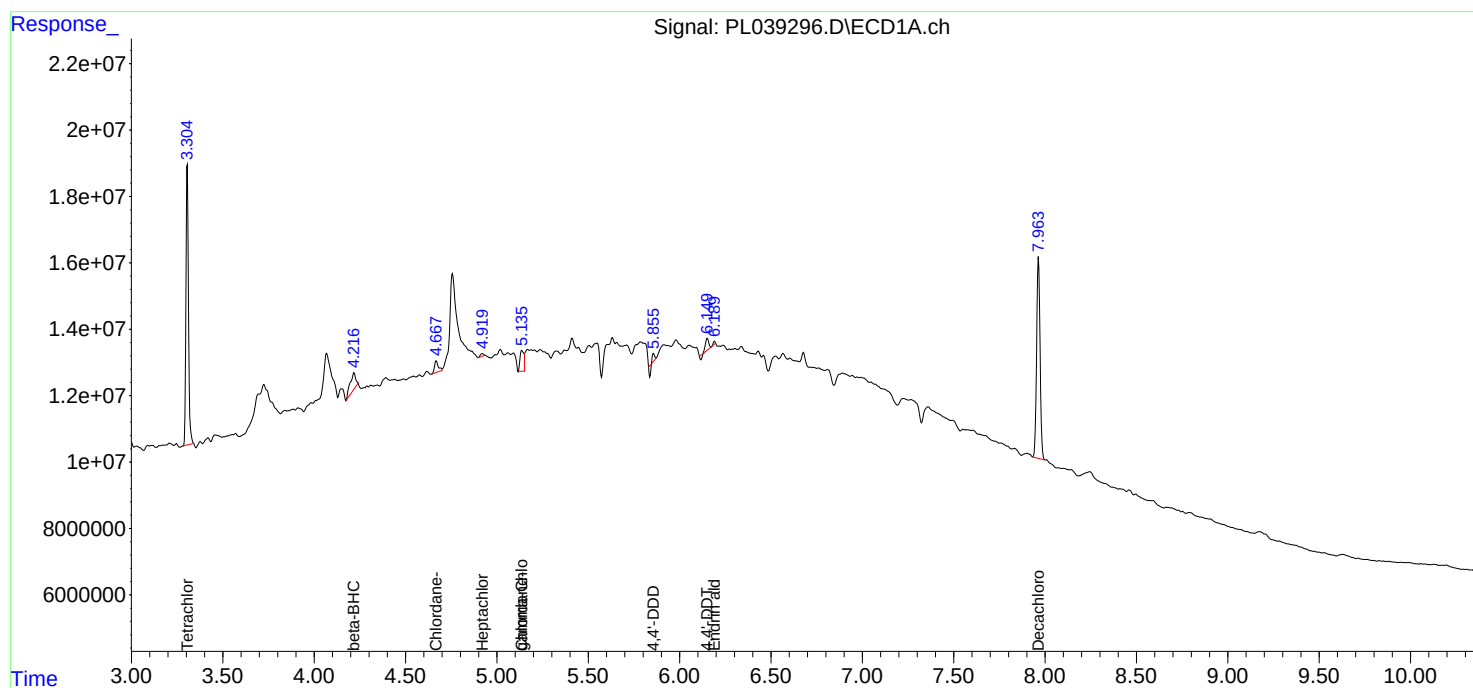


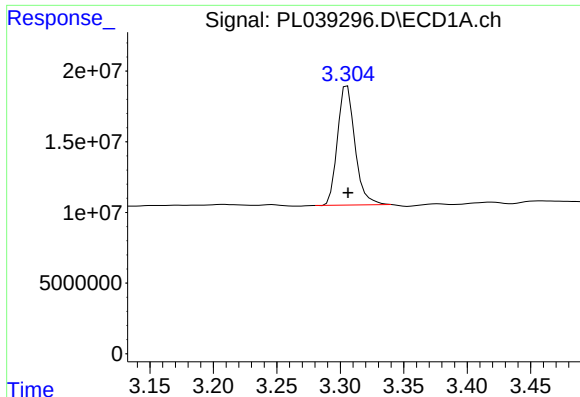

#1 Tetrachloro-m-xylene


R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 81134922
Conc: 11.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

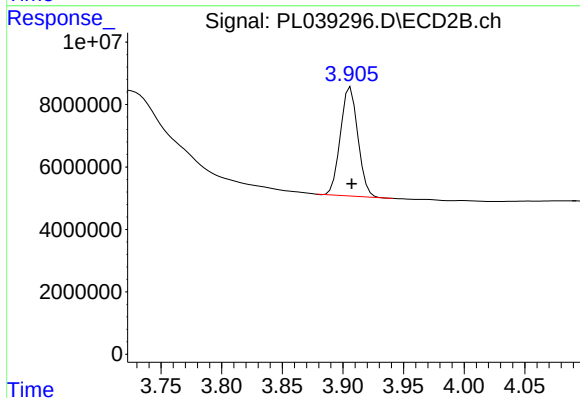


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 34800546
Conc: 12.98 ng/ml

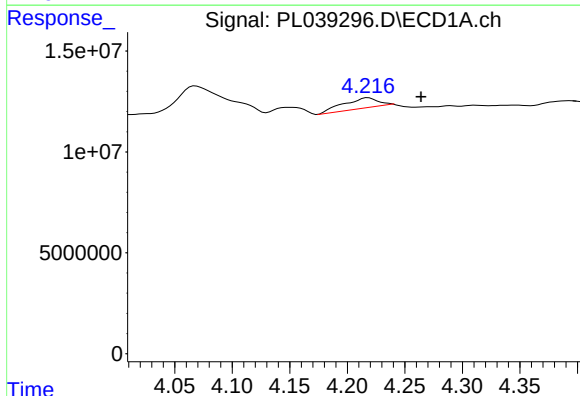


#6 beta-BHC

R.T.: 4.218 min
Delta R.T.: -0.046 min
Response: 10986102
Conc: 2.36 ng/ml

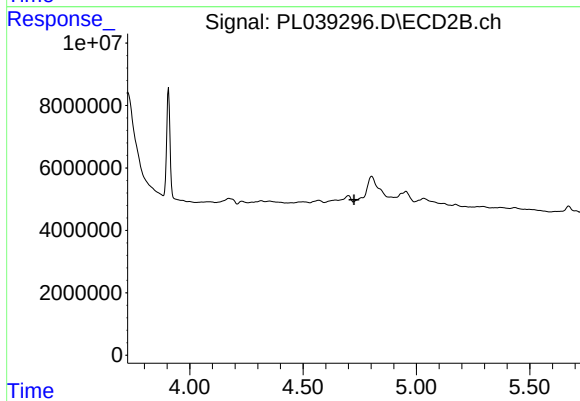

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

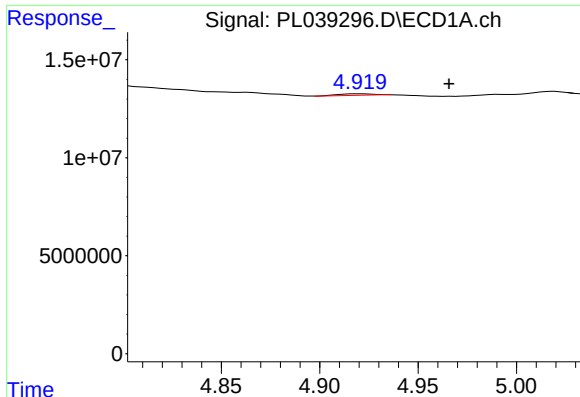

#8 Heptachlor epoxide


R.T.: 4.921 min
Delta R.T.: -0.045 min
Response: 1512558
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

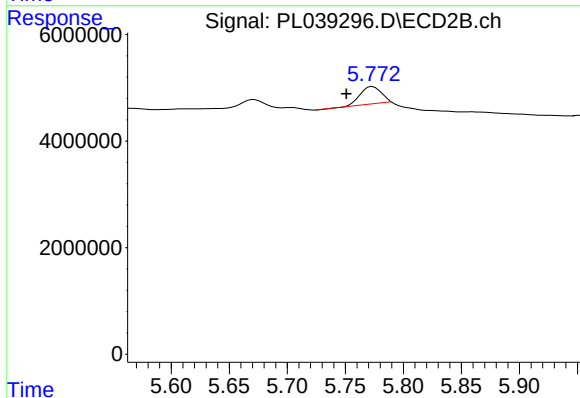


#8 Heptachlor epoxide

R.T.: 5.774 min
Delta R.T.: 0.023 min
Response: 4211166
Conc: 1.25 ng/ml

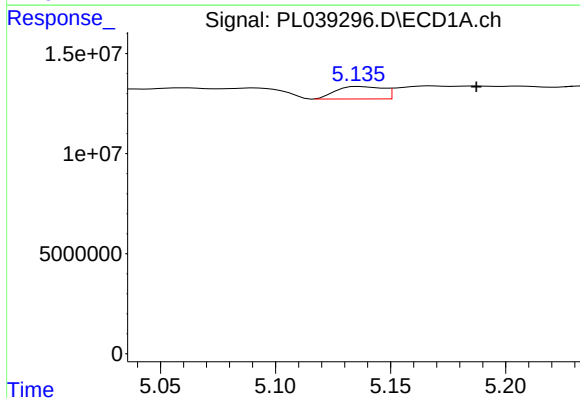


#10 gamma-Chlordane

R.T.: 5.136 min
Delta R.T.: -0.051 min
Response: 8825752
Conc: 0.89 ng/ml

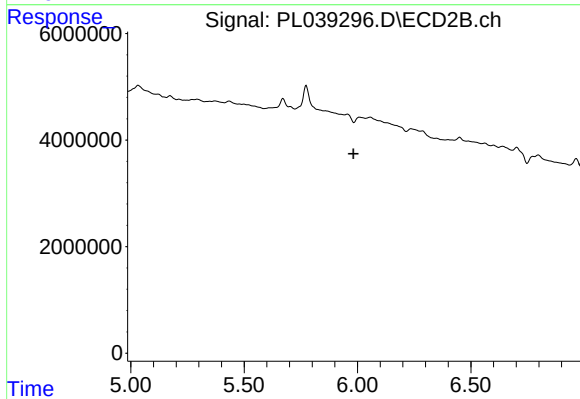

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

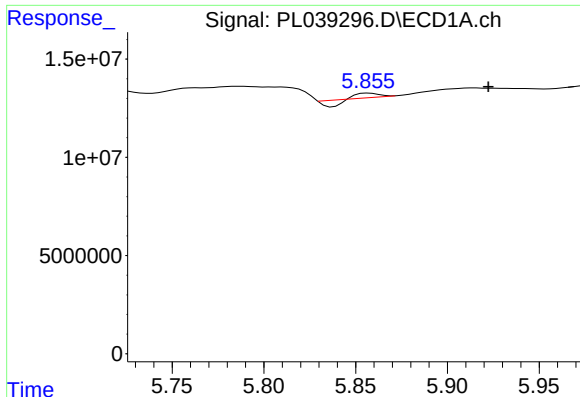

#16 4,4'-DDD

R.T.: 5.857 min
Delta R.T.: -0.066 min
Response: 543921
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

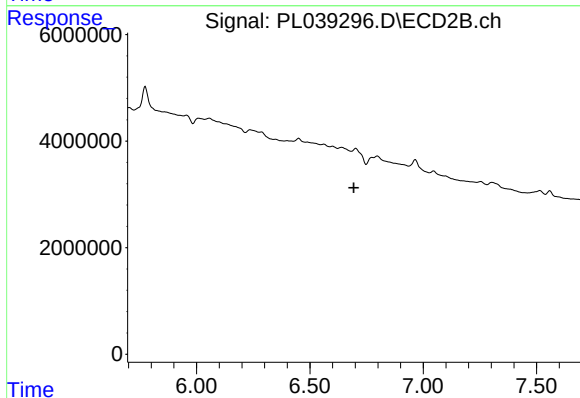


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.693 min
Response: 0
Conc: N.D.


#17 4,4'-DDT

R.T.: 6.151 min
Delta R.T.: -0.004 min
Response: 3553156
Conc: 0.47 ng/ml

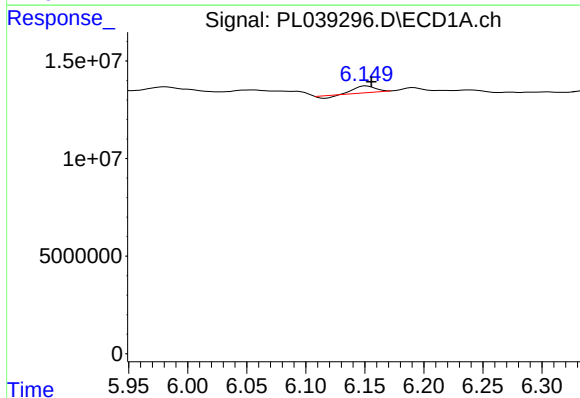

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

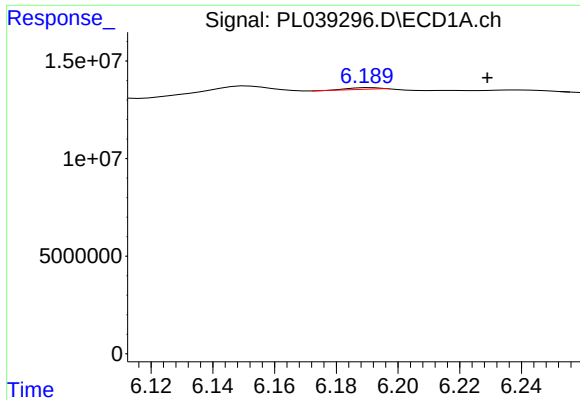

#18 Endrin aldehyde


R.T.: 6.191 min
Delta R.T.: -0.038 min
Response: 827952
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

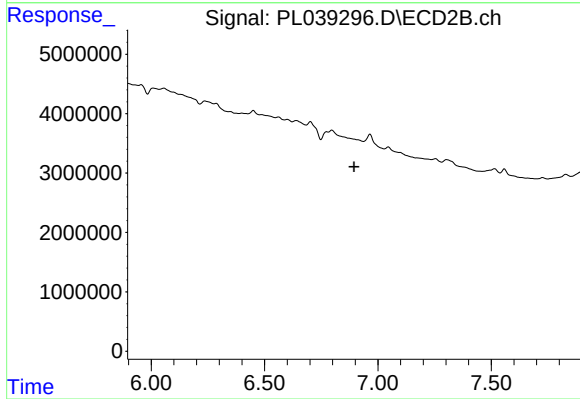


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

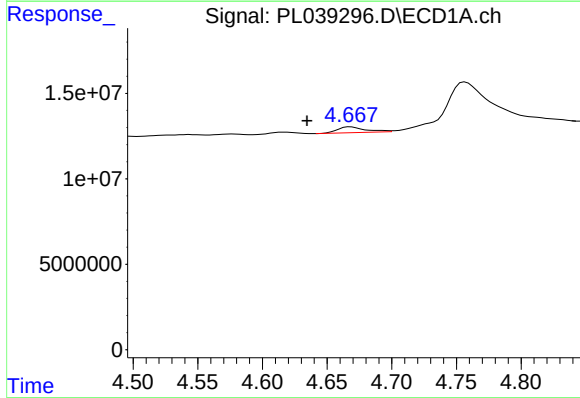


#24 Chlordane-2

R.T.: 4.668 min
Delta R.T.: 0.033 min
Response: 5053921
Conc: 14.46 ng/ml

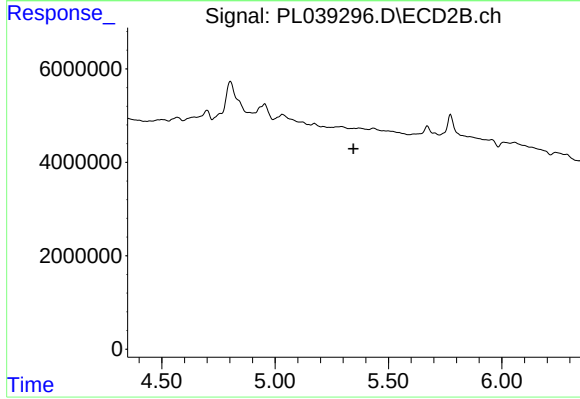

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

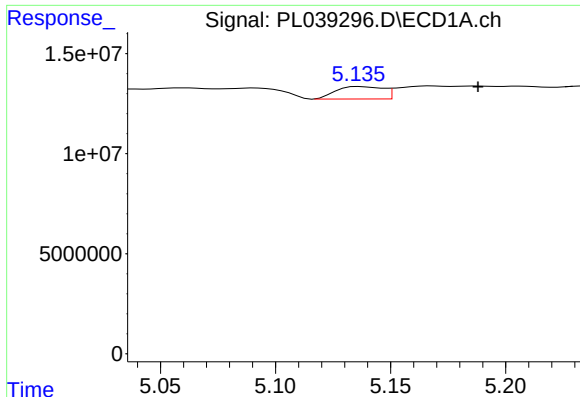

#25 Chlordane-3


R.T.: 5.136 min
Delta R.T.: -0.052 min
Response: 8825752
Conc: 8.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

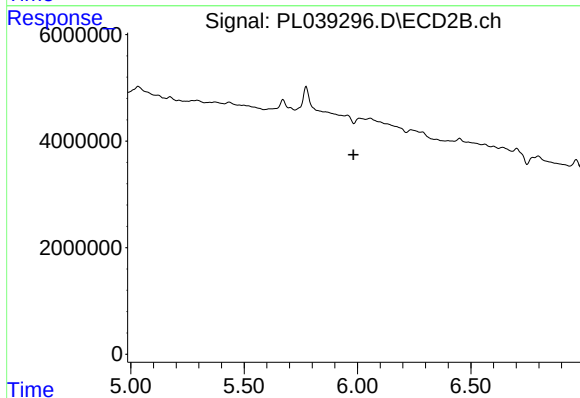


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

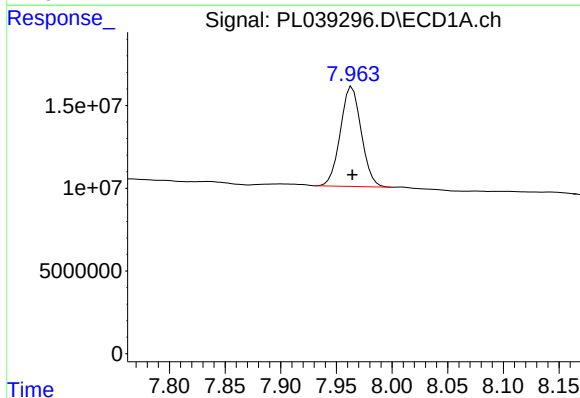

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 78786558
Conc: 11.22 ng/ml

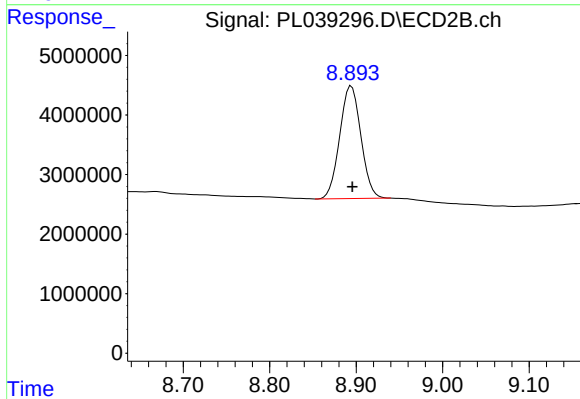

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: -0.001 min
Response: 32044616
Conc: 13.81 ng/ml