

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039299.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2018 02:10
 Operator : AJ\SJ
 Sample : J4521-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:14:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	81097841	31420590	11.601	11.720
28)	SA Decachlor...	7.963	8.895	83607488	34005402	11.904	14.654
Target Compounds							
6)	B beta-BHC	4.216f	0.000	24070366	0	5.181	N.D. #
8)	B Heptachlo...	4.919f	5.774	2388528	7334092	0.250	2.181 #
10)	B gamma-Chl...	5.134f	0.000	8862424	0	0.897	N.D. #
12)	B 4,4'-DDE	5.410	0.000	5164905	0	0.539	N.D. #
17)	MA 4,4'-DDT	6.151	0.000	5096067	0	0.672	N.D. #
23)	Chlordane-1	4.152	0.000	17031942	0	53.799	N.D. #
24)	Chlordane-2	4.666	0.000	20793061	0	59.478	N.D. #
25)	Chlordane-3	5.134	0.000	8862424	0	8.114	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039299.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2018 02:10
Operator : AJ\SJ
Sample : J4521-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:14:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

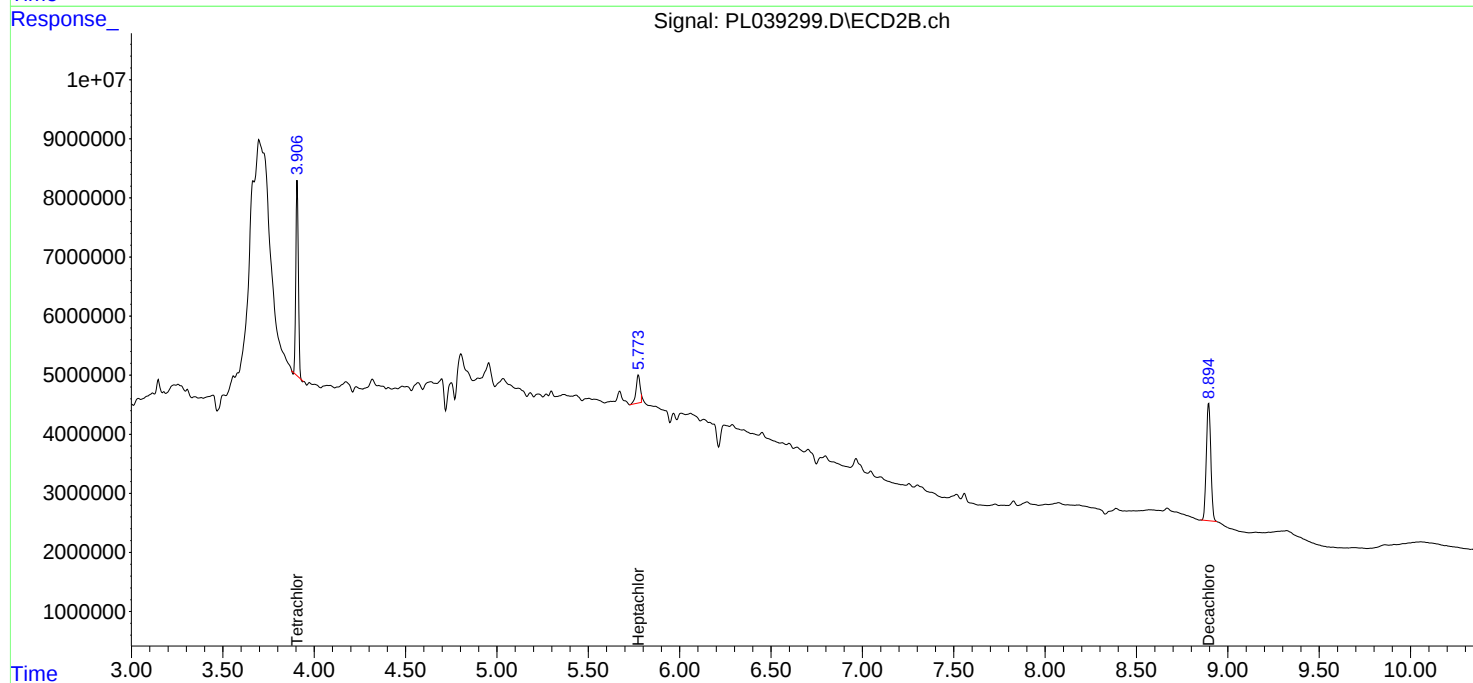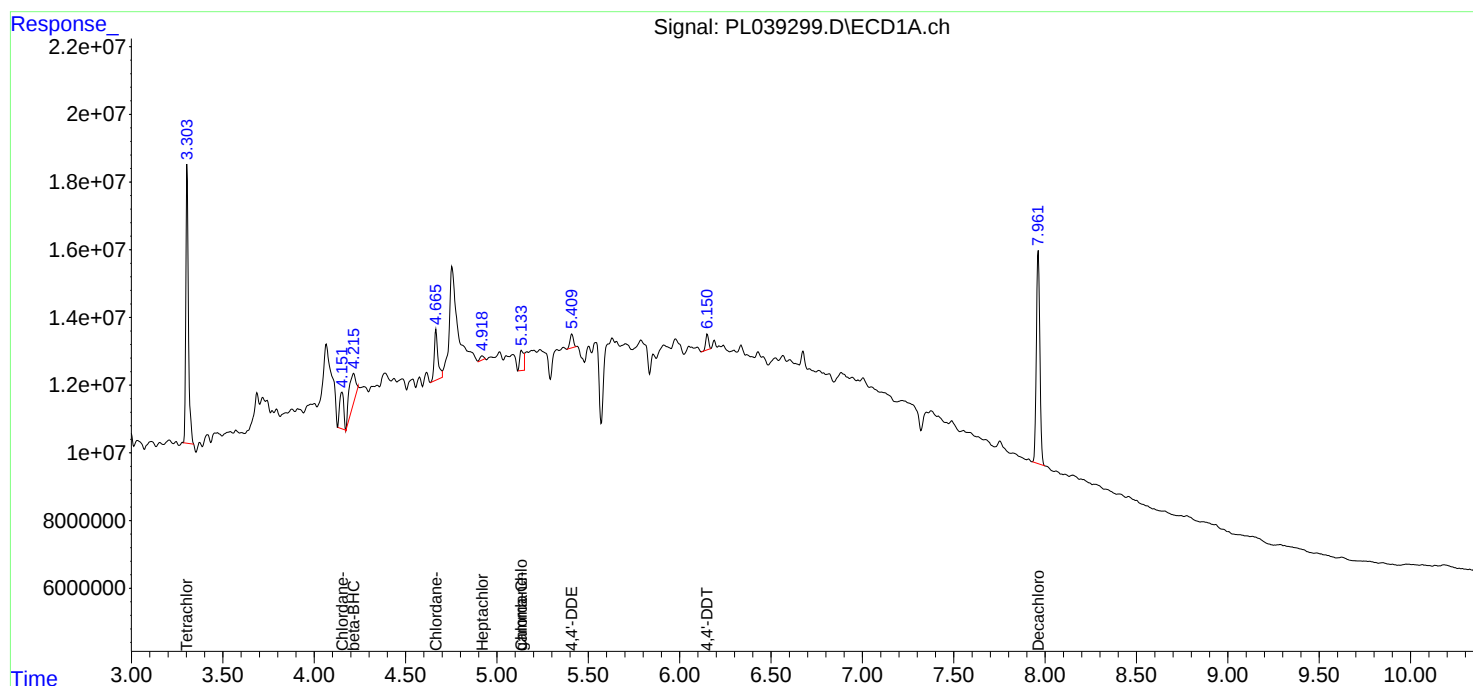


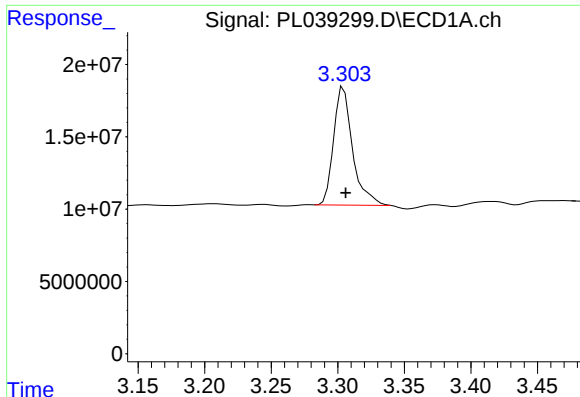

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 81097841
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

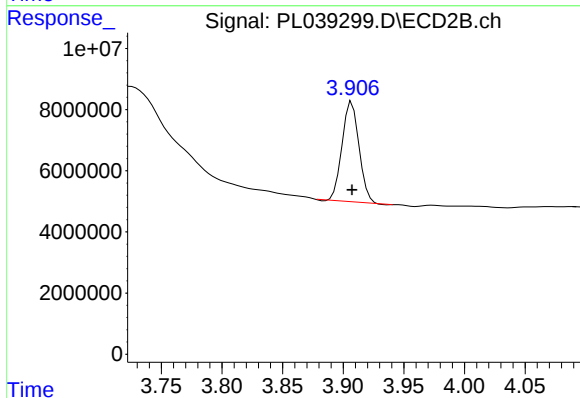


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 31420590
Conc: 11.72 ng/ml

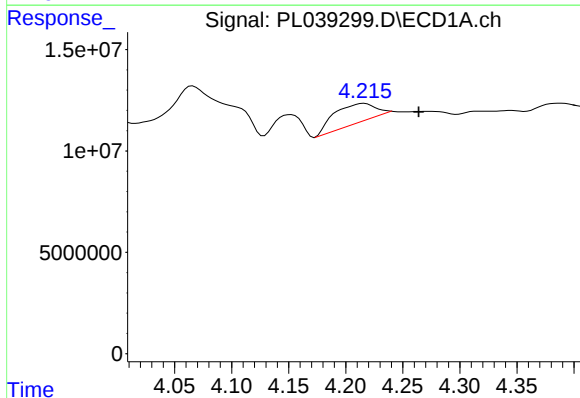


#6 beta-BHC

R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 24070366
Conc: 5.18 ng/ml

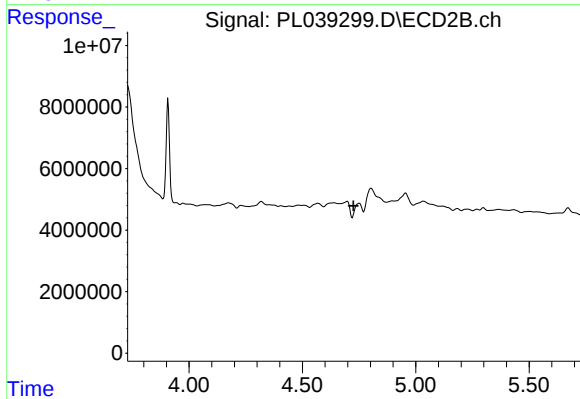

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

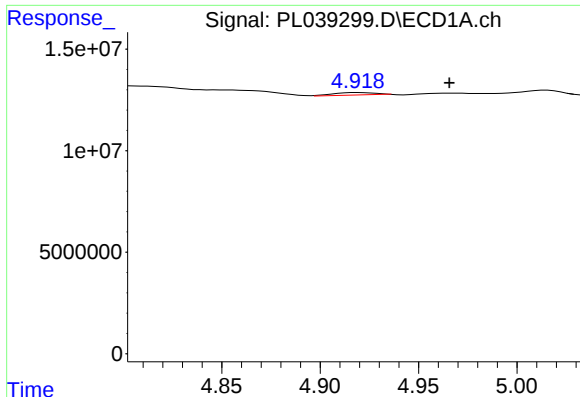

#8 Heptachlor epoxide


R.T.: 4.919 min
Delta R.T.: -0.047 min
Response: 2388528
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

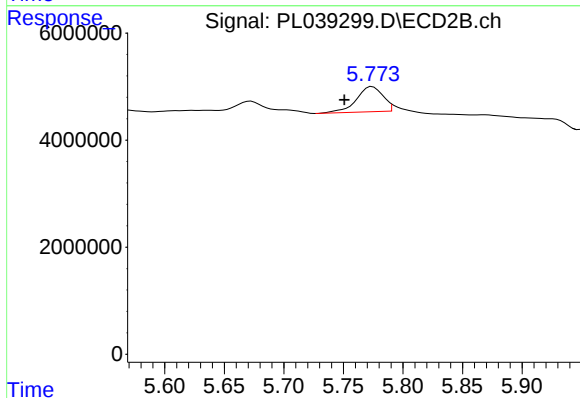


#8 Heptachlor epoxide

R.T.: 5.774 min
Delta R.T.: 0.023 min
Response: 7334092
Conc: 2.18 ng/ml

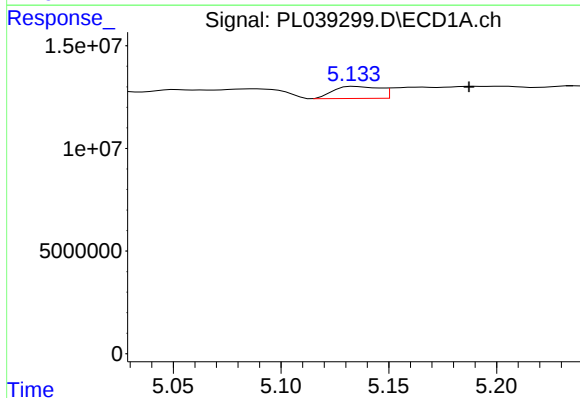


#10 gamma-Chlordane

R.T.: 5.134 min
Delta R.T.: -0.053 min
Response: 8862424
Conc: 0.90 ng/ml

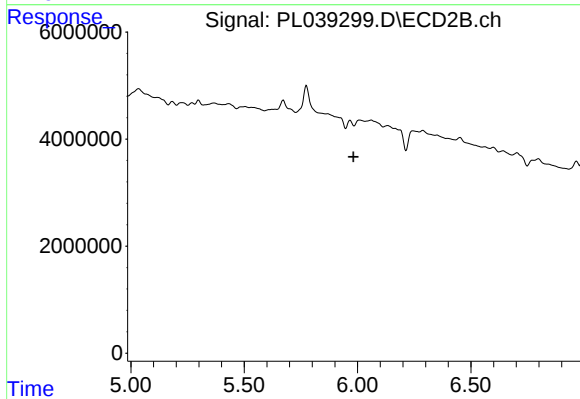

#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

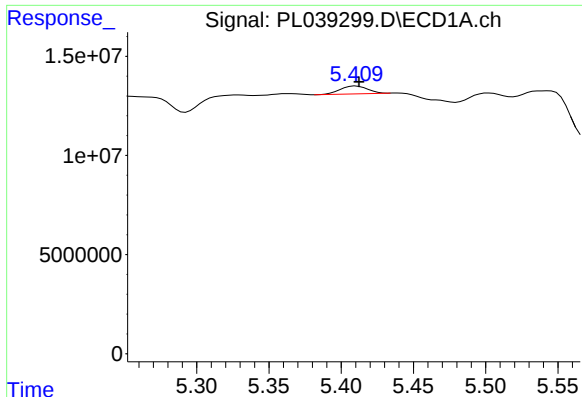

#12 4,4'-DDE

R.T.: 5.410 min
Delta R.T.: -0.002 min
Response: 5164905
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.212 min
Response: 0
Conc: N.D.

#17 4,4'-DDT

R.T.: 6.151 min
Delta R.T.: -0.004 min
Response: 5096067
Conc: 0.67 ng/ml

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

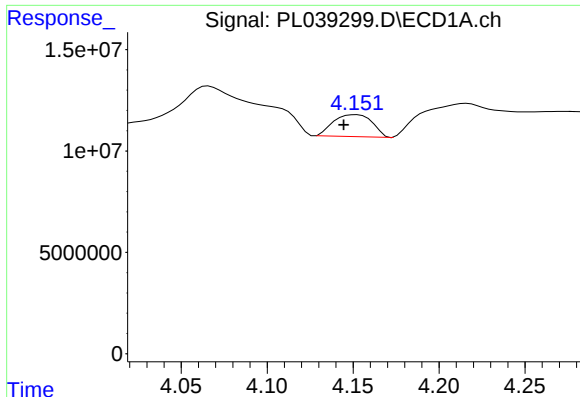

#23 Chlordane-1


R.T.: 4.152 min
Delta R.T.: 0.007 min
Response: 17031942
Conc: 53.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

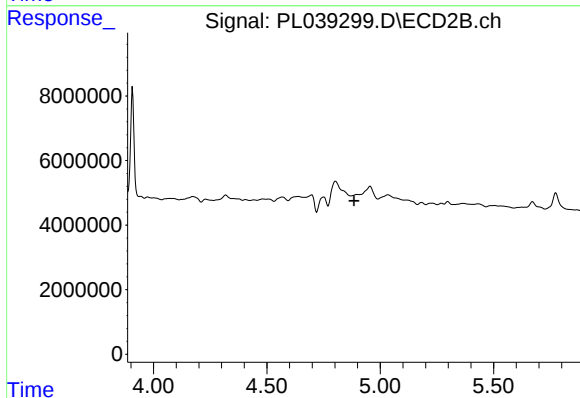


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

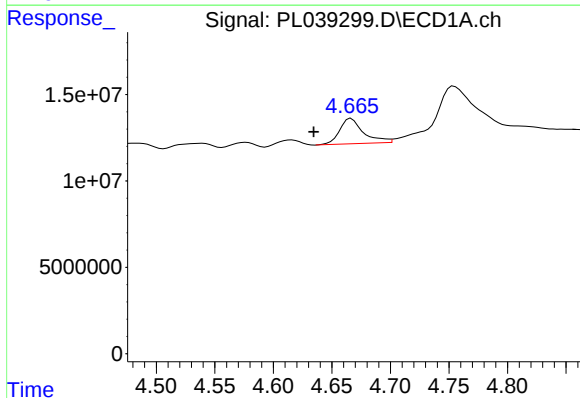


#24 Chlordane-2

R.T.: 4.666 min
Delta R.T.: 0.032 min
Response: 20793061
Conc: 59.48 ng/ml

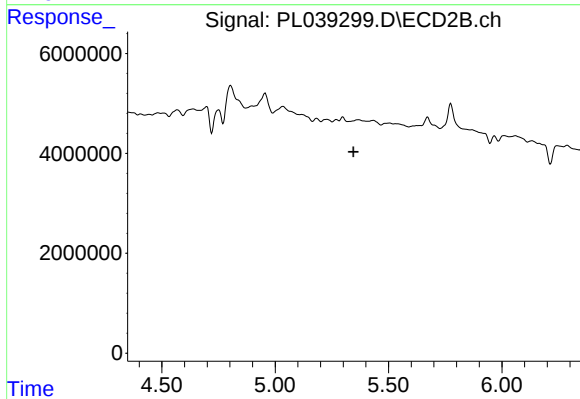

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

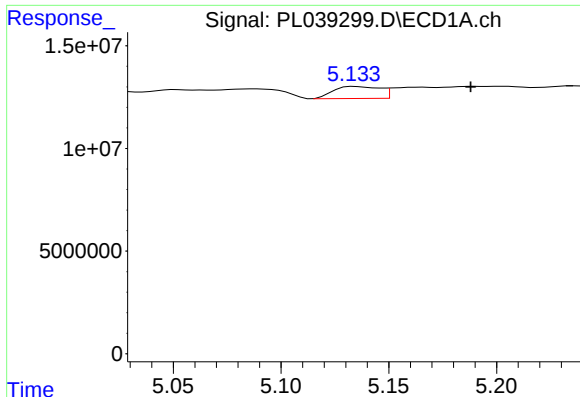

#25 Chlordane-3


R.T.: 5.134 min
Delta R.T.: -0.054 min
Response: 8862424
Conc: 8.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

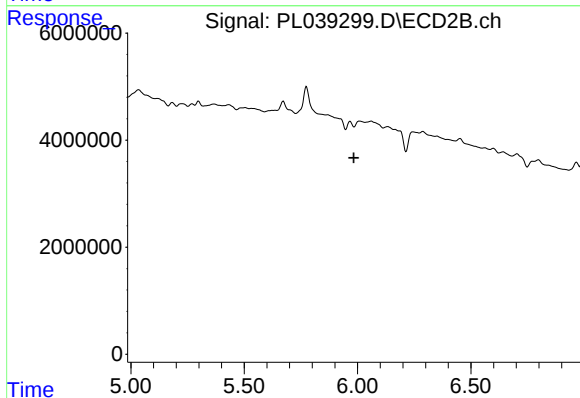


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

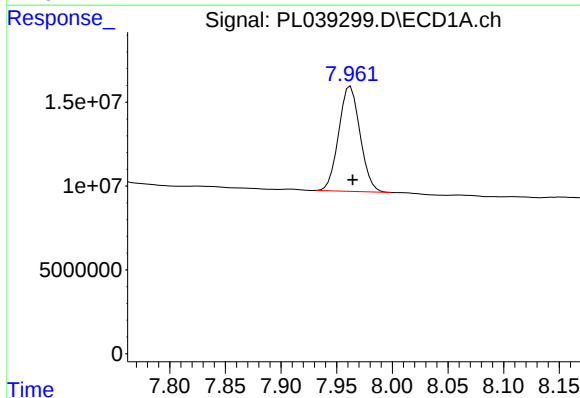

#28 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: -0.002 min
Response: 83607488
Conc: 11.90 ng/ml

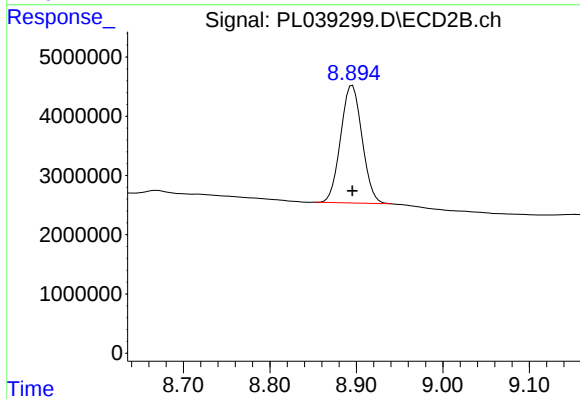

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.000 min
Response: 34005402
Conc: 14.65 ng/ml