

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
 Data File : PL039262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2018 16:54
 Operator : AJ\SJ
 Sample : J4516-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ND-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 8/20/2018 12:58:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 22:46:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.905	132.3E6	54905475	18.919	20.480m
28)	SA Decachlor...	7.961	8.894	130.1E6	51376939	18.521	22.139

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081718\
Data File : PL039262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2018 16:54
Operator : AJ\SJ
Sample : J4516-06
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ND-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/20/2018 12:58:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 22:46:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

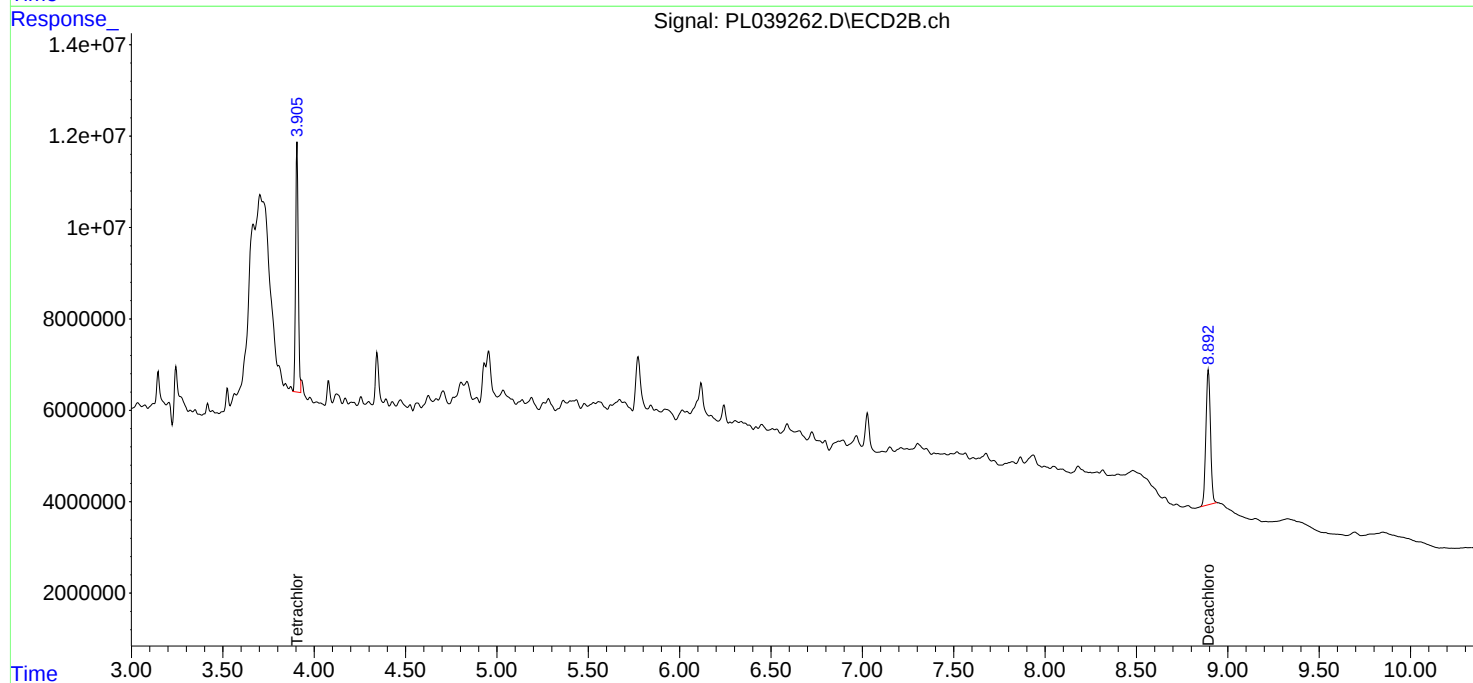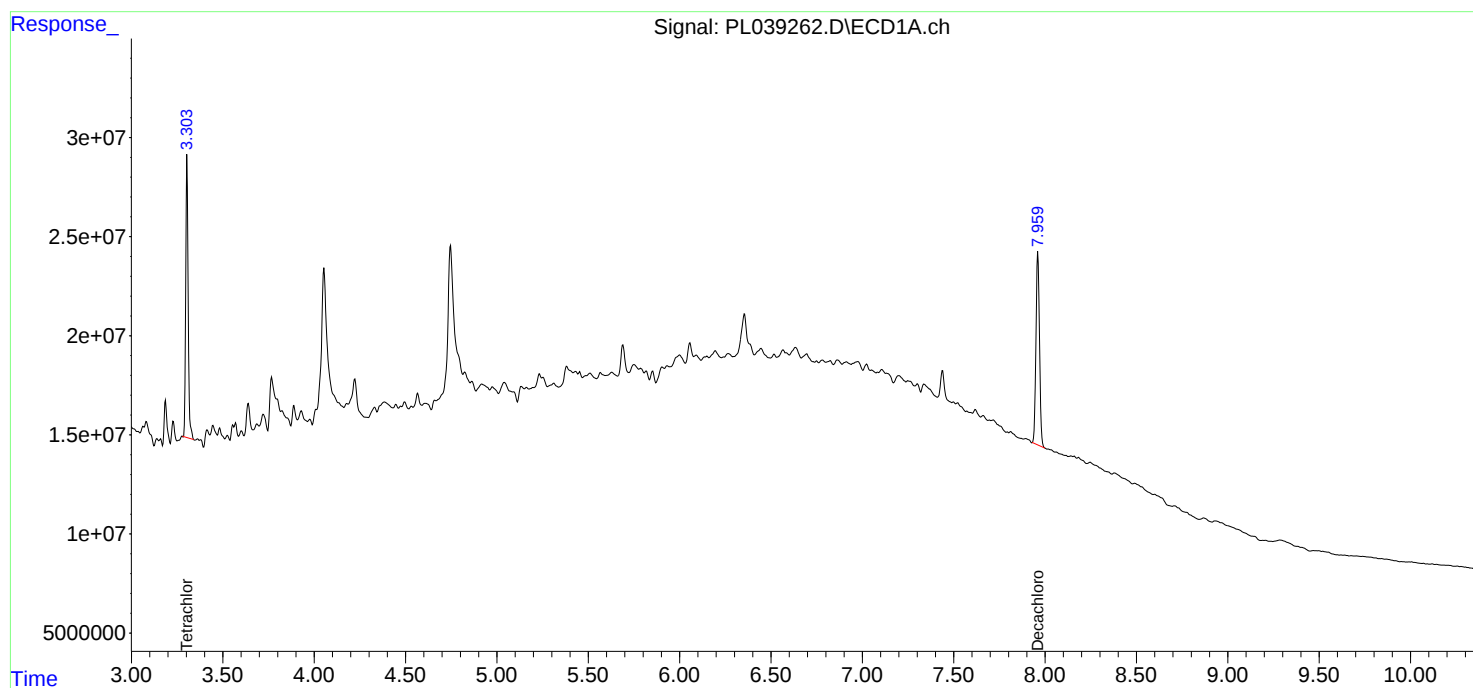

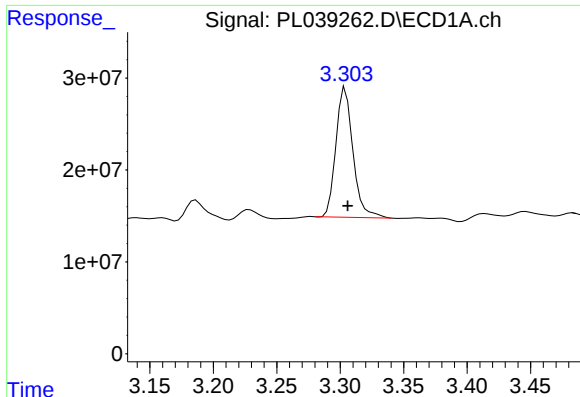


#1 Tetrachloro-m-xylene

R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 132253510
Conc: 18.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
ND-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
8/20/2018 12:58:53 PM

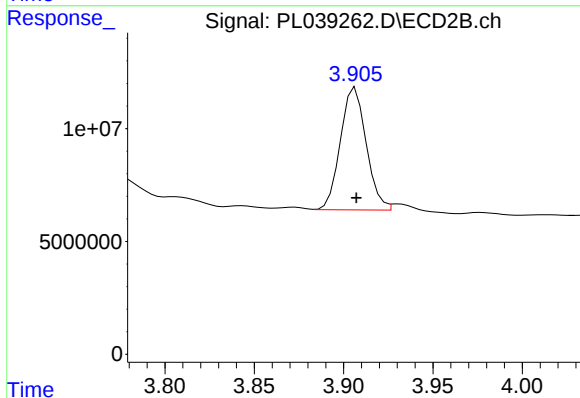


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 54905475
Conc: 20.48 ng/ml m

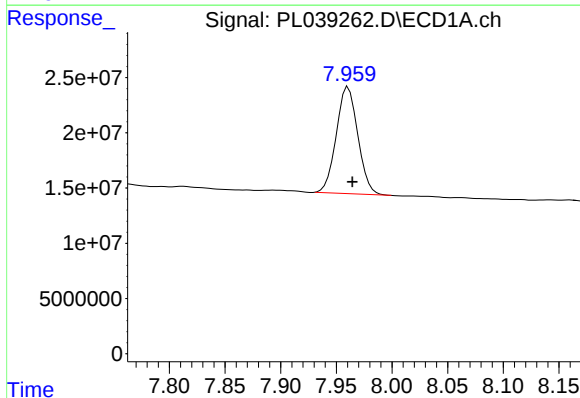

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.004 min
Response: 130083301
Conc: 18.52 ng/ml

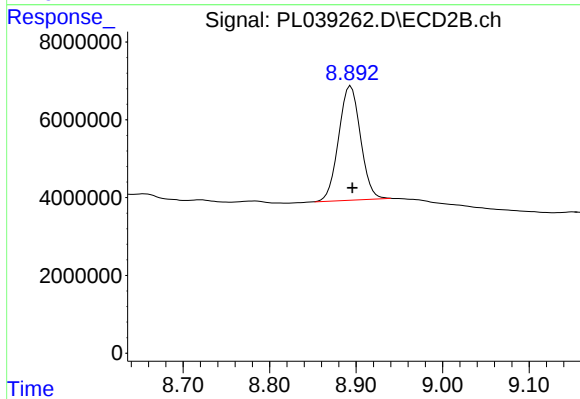

#28 Decachlorobiphenyl

R.T.: 8.894 min
Delta R.T.: -0.002 min
Response: 51376939
Conc: 22.14 ng/ml