

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
 Data File : PL060774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 13:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 16:30:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.009	36975743	62885575	19.723	23.649
28)	SA Decachlor...	8.216	9.098	26402676	35447252	14.465	18.893 #
Target Compounds							
24)	Chlordane-2	0.000	5.458f	0	2649669	N.D.	26.865 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
Data File : PL060774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 13:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 16:30:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

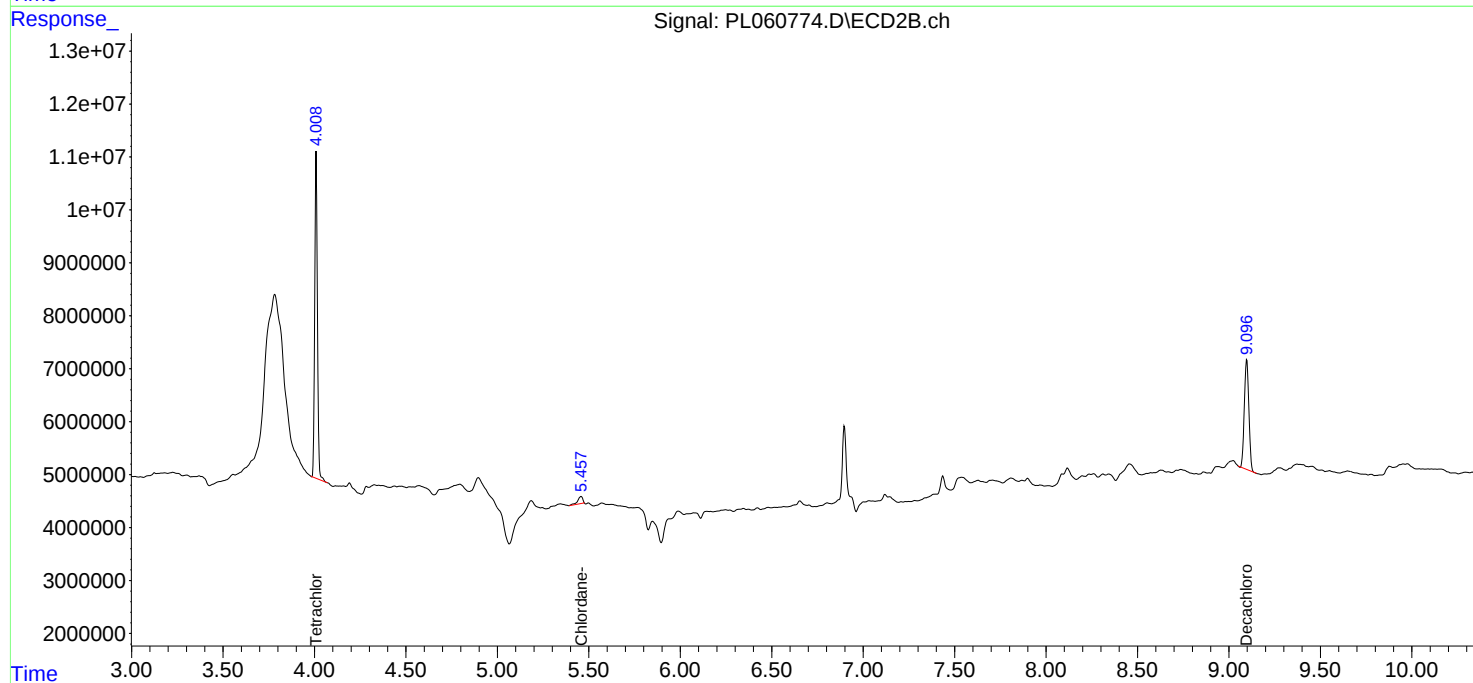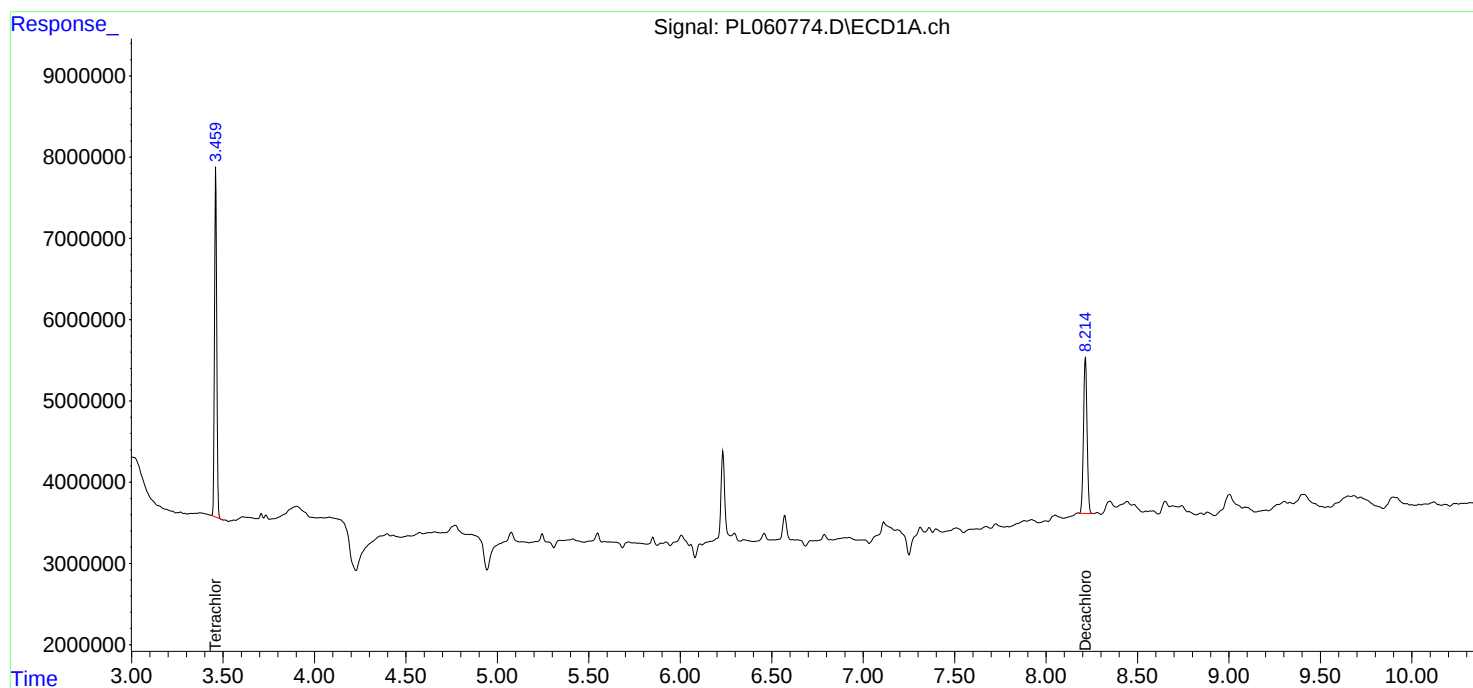


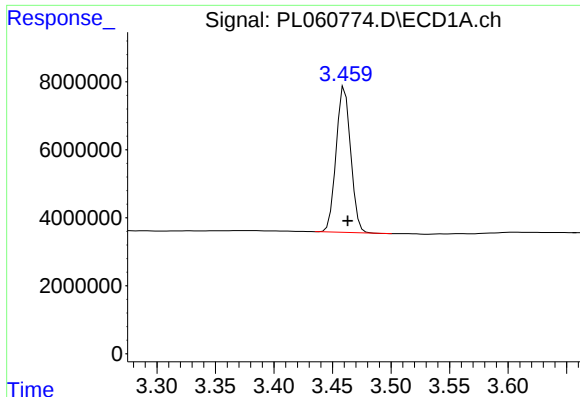

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: -0.002 min
Response: 36975743
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

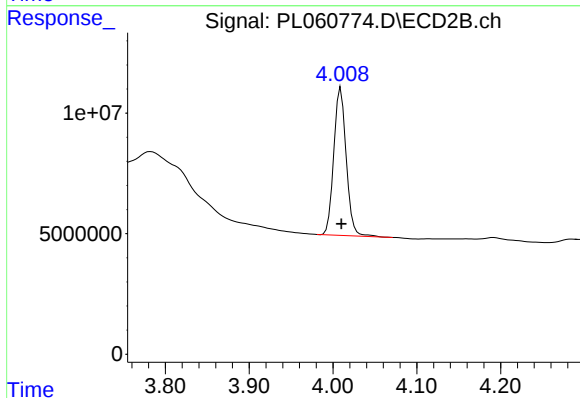


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 62885575
Conc: 23.65 ng/ml

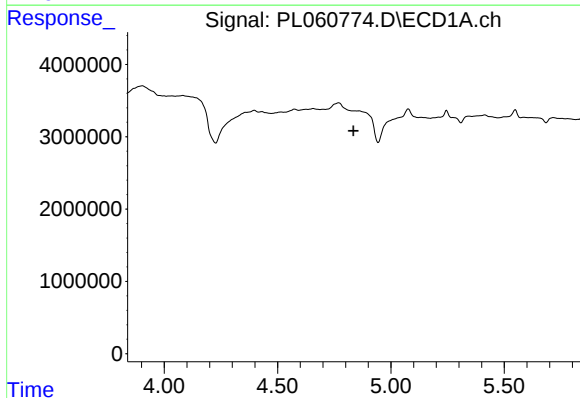


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.835 min
Response: 0
Conc: N.D.

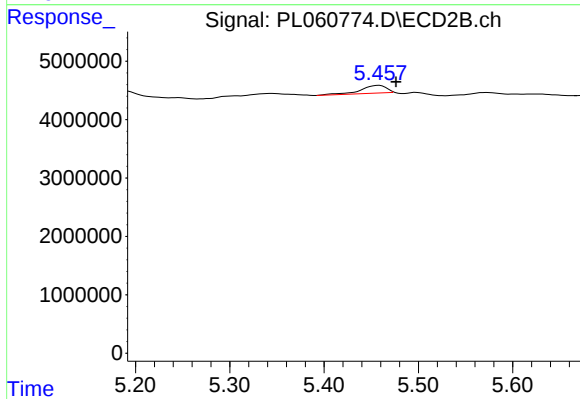

#24 Chlordane-2


R.T.: 5.458 min
Delta R.T.: -0.018 min
Response: 2649669
Conc: 26.87 ng/ml

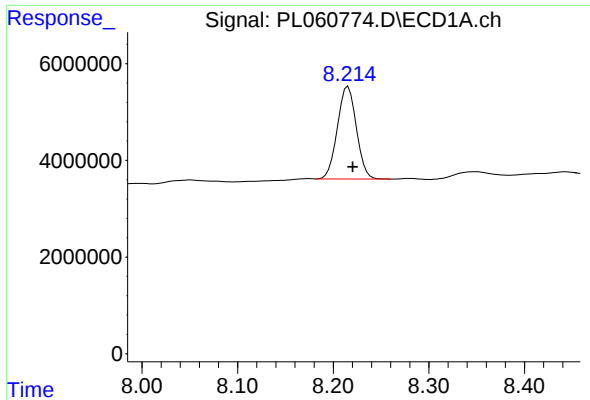

#28 Decachlorobiphenyl

R.T.: 8.216 min
Delta R.T.: -0.005 min
Response: 26402676
Conc: 14.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

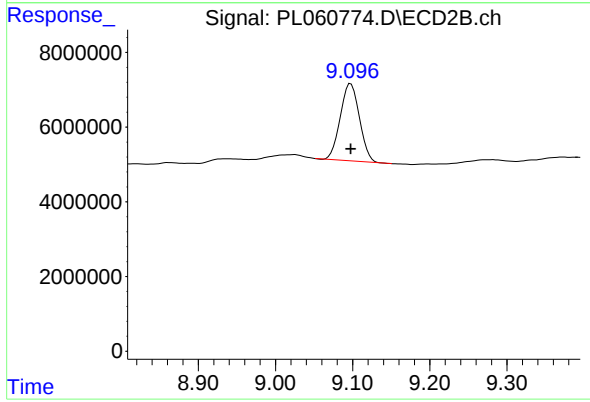

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 35447252
Conc: 18.89 ng/ml