

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
 Data File : PL060770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 12:25
 Operator : DD\AJ
 Sample : L3508-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-08-081420

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:39:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 08:22:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	27737773	34721810	14.796	13.058
28)	SA Decachlor...	8.220	9.100	21447870	25831289	11.750	13.768
Target Compounds							
10)	B gamma-Chl...	5.403	6.124	1376739	2427301	0.649m	0.803m
11)	B alpha-Chl...	5.461	6.198	1556958	3296502	0.734m	1.072 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
Data File : PL060770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 12:25
Operator : DD\AJ
Sample : L3508-19
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-08-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 08:22:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

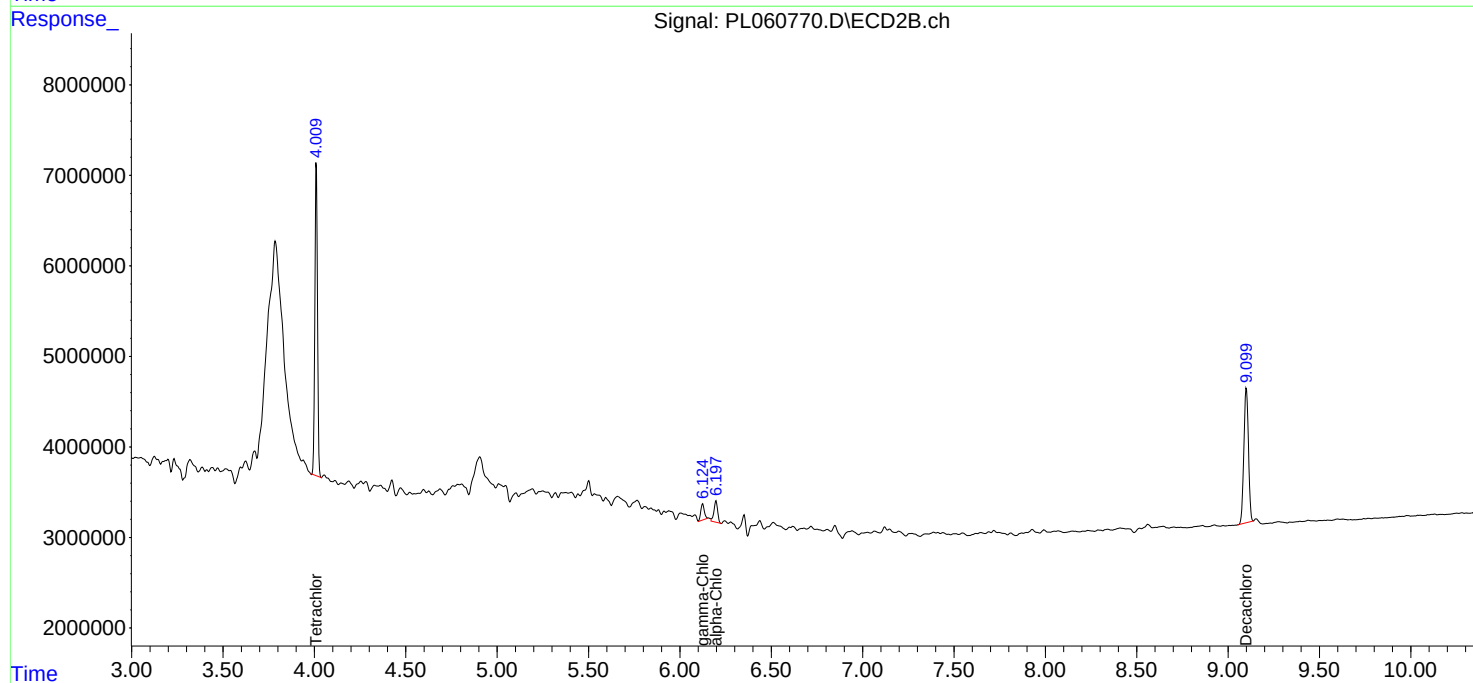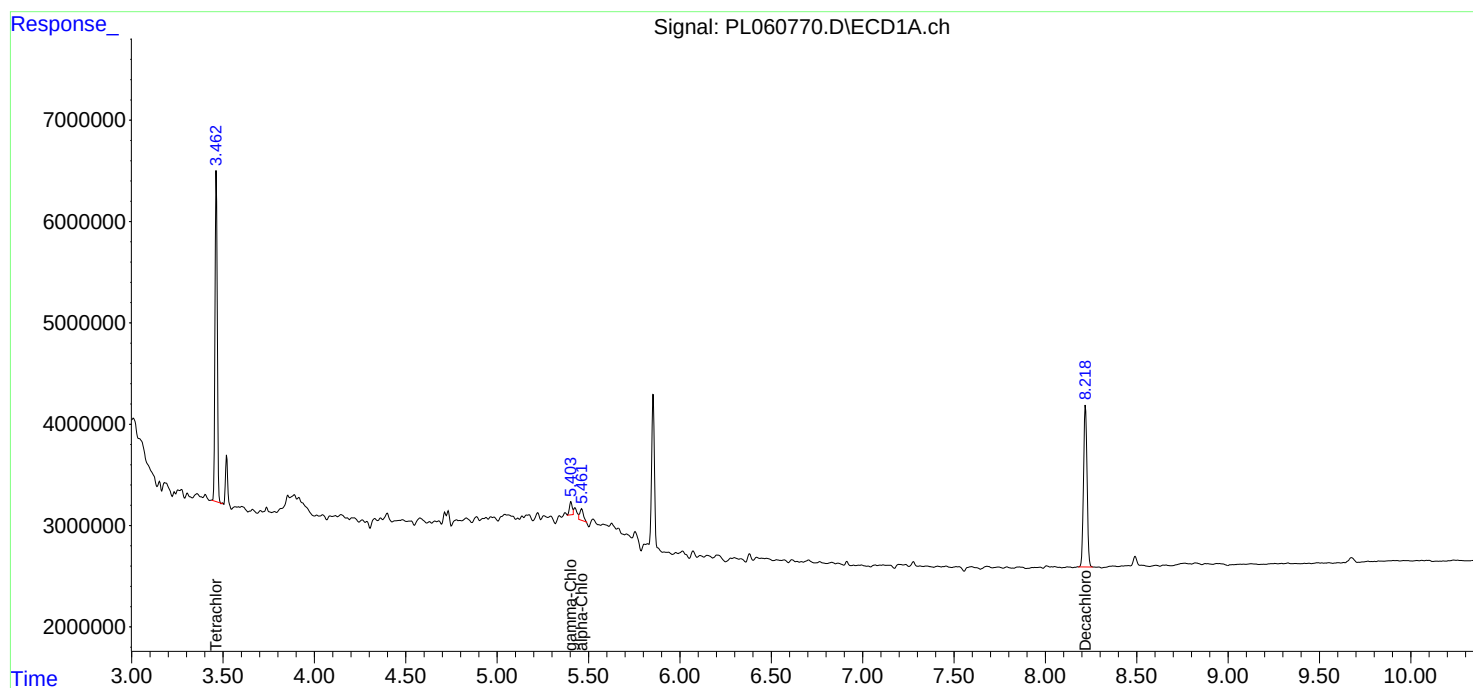

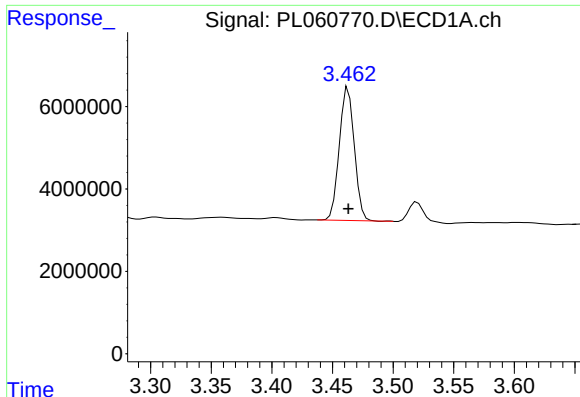


#1 Tetrachloro-m-xylene

R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 27737773
Conc: 14.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-08-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:41 PM

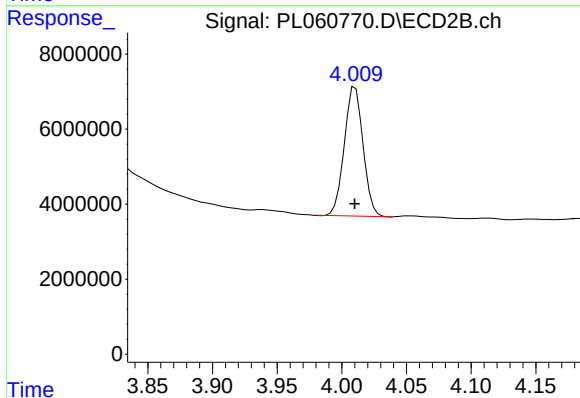


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 34721810
Conc: 13.06 ng/ml

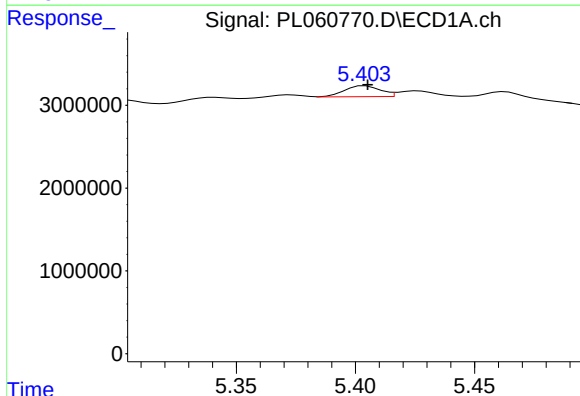


#10 gamma-Chlordane

R.T.: 5.403 min
Delta R.T.: -0.003 min
Response: 1376739
Conc: 0.65 ng/ml m

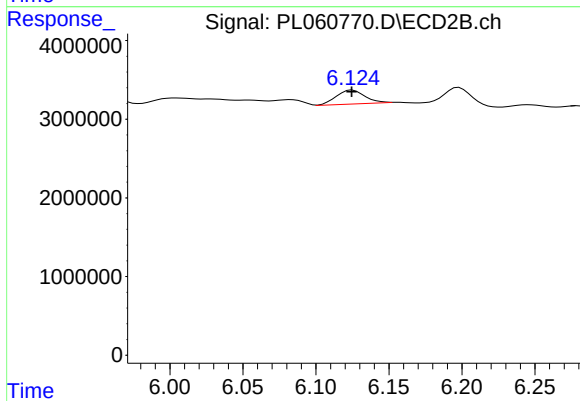

#10 gamma-Chlordane

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 2427301
Conc: 0.80 ng/ml m

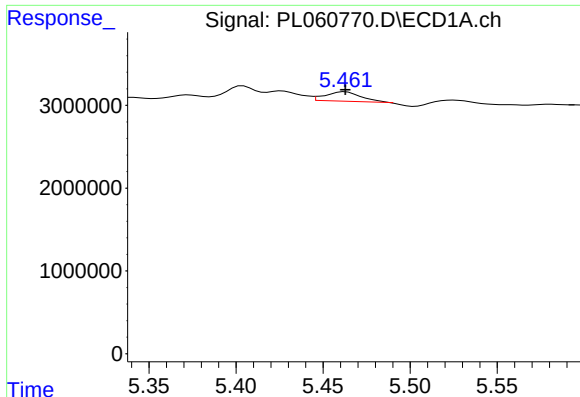


#11 alpha-Chlordane

R.T.: 5.461 min
Delta R.T.: -0.001 min
Response: 1556958
Conc: 0.73 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-08-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:41 PM

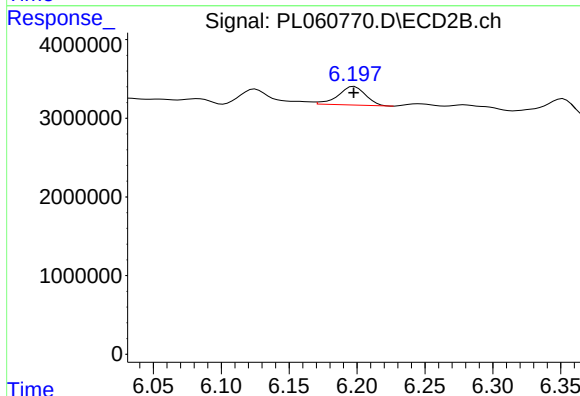


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 3296502
Conc: 1.07 ng/ml

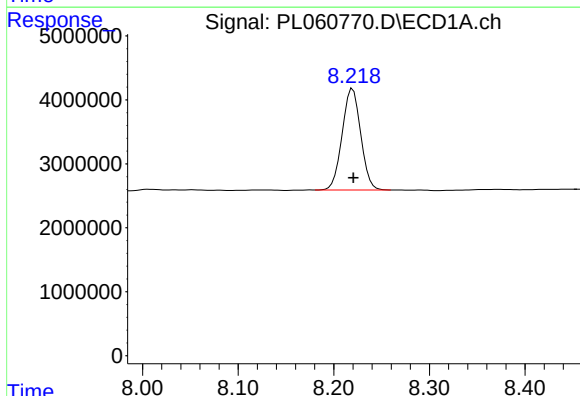

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 21447870
Conc: 11.75 ng/ml

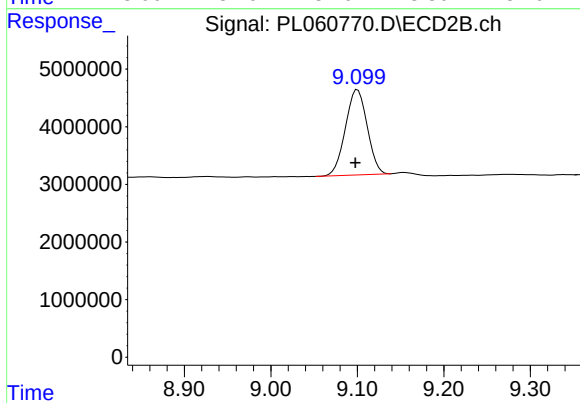

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.003 min
Response: 25831289
Conc: 13.77 ng/ml