

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
 Data File : PL060771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2020 12:39
 Operator : DD\AJ
 Sample : L3500-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-081420

Manual Integrations
 APPROVED

Ankita
 8/18/2020 3:39:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 08:41:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.011	24353572	32153209	12.991	12.092
28)	SA Decachlor...	8.219	9.099	19577542	24305191	10.726	12.954
Target Compounds							
17)	MA 4,4'-DDT	6.380	7.146	1159390	954306	0.701m	0.437m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081720\
Data File : PL060771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2020 12:39
Operator : DD\AJ
Sample : L3500-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-02-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 08:41:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

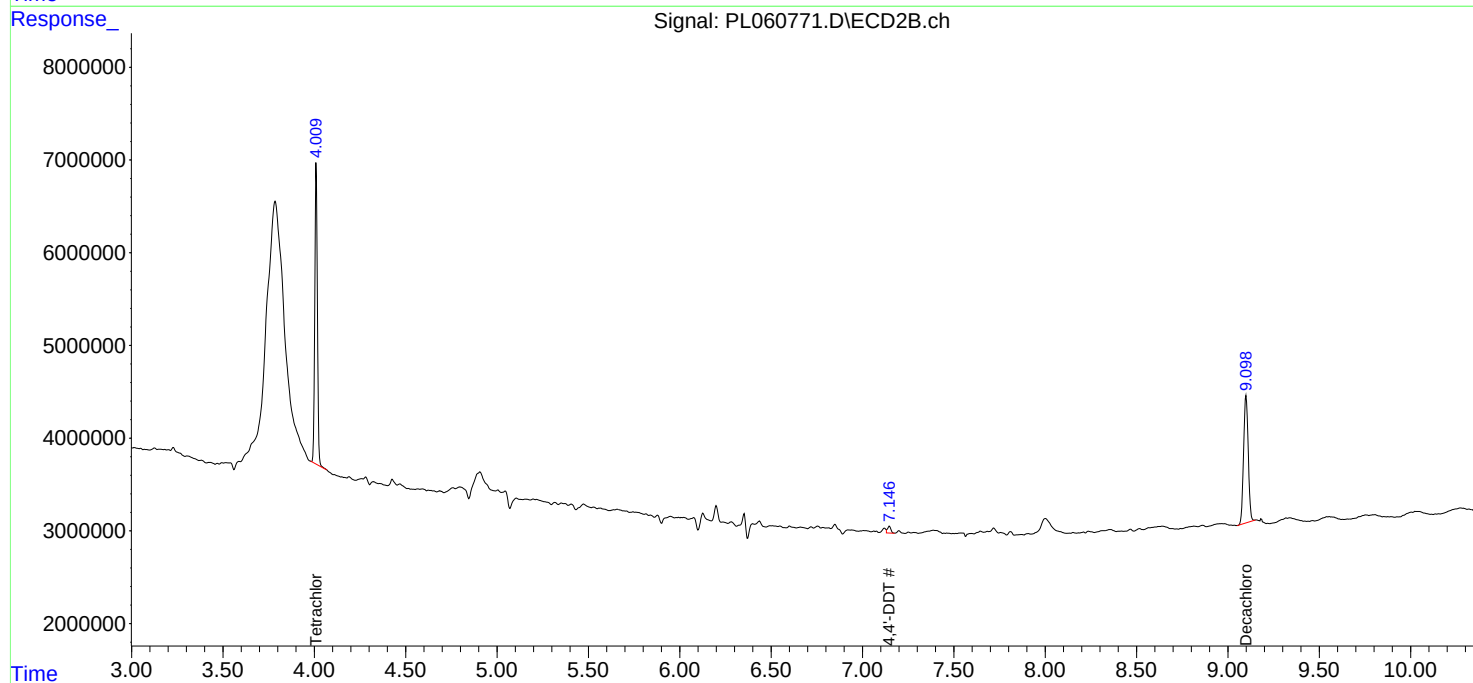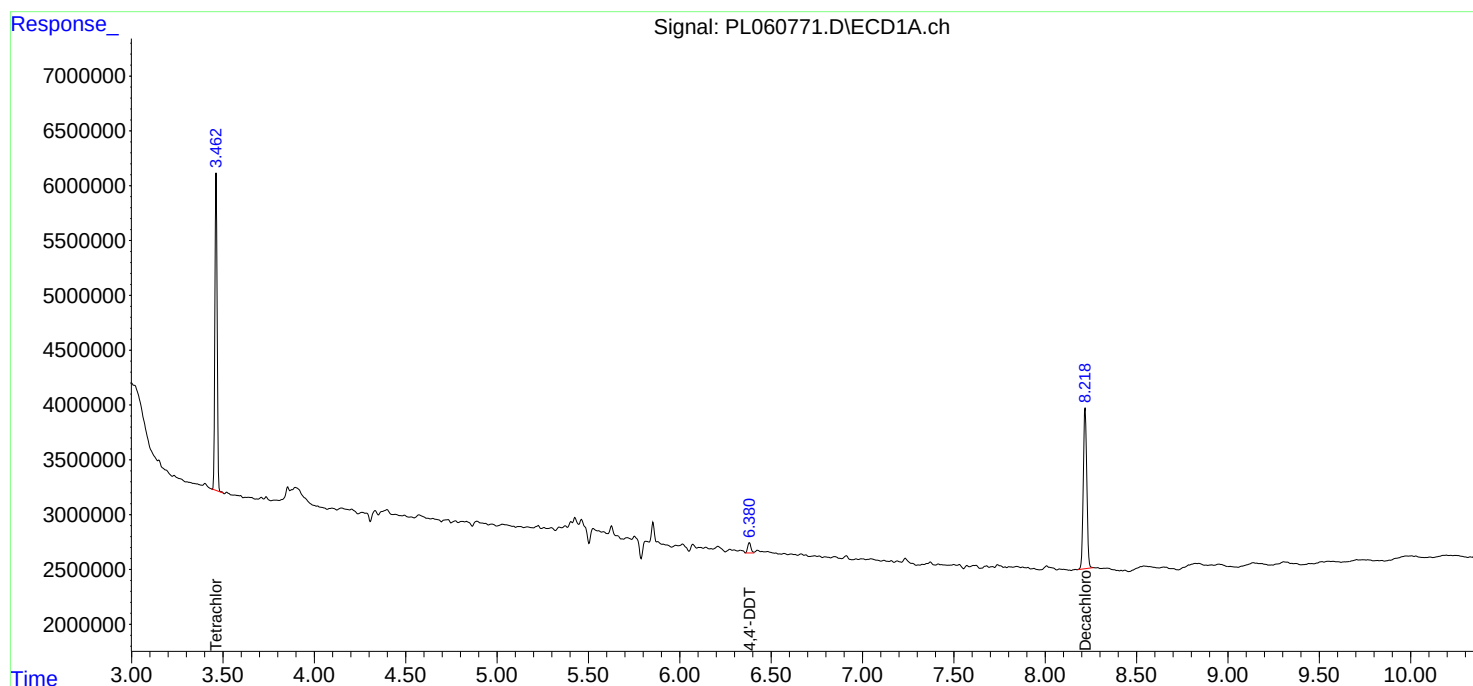

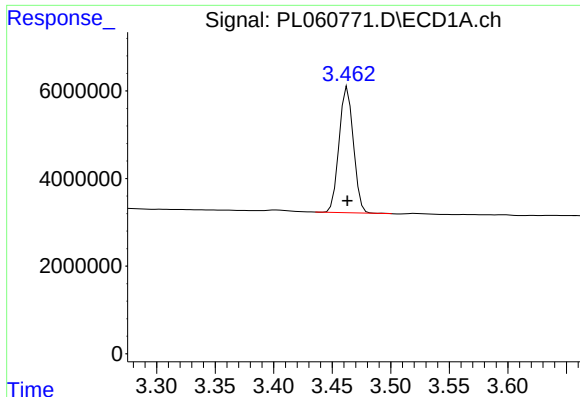


#1 Tetrachloro-m-xylene

R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 24353572
Conc: 12.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-081420


Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:42 PM

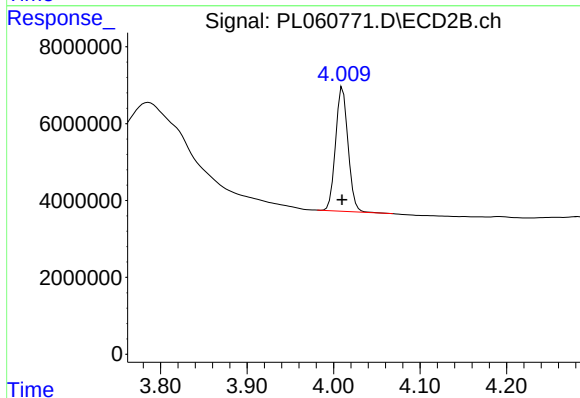


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 32153209
Conc: 12.09 ng/ml

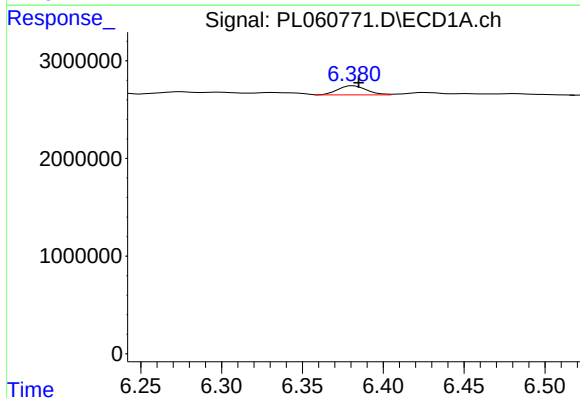


#17 4,4'-DDT

R.T.: 6.380 min
Delta R.T.: -0.005 min
Response: 1159390
Conc: 0.70 ng/ml m

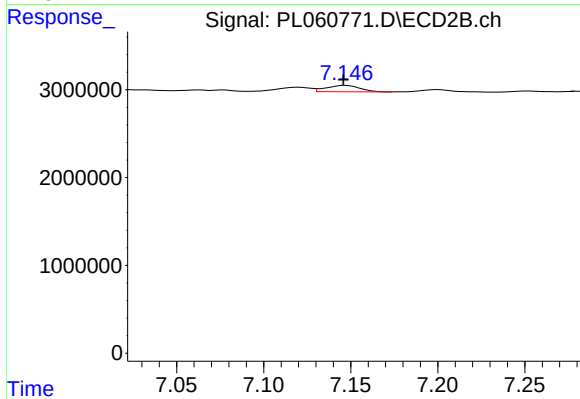

#17 4,4'-DDT

R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 954306
Conc: 0.44 ng/ml m

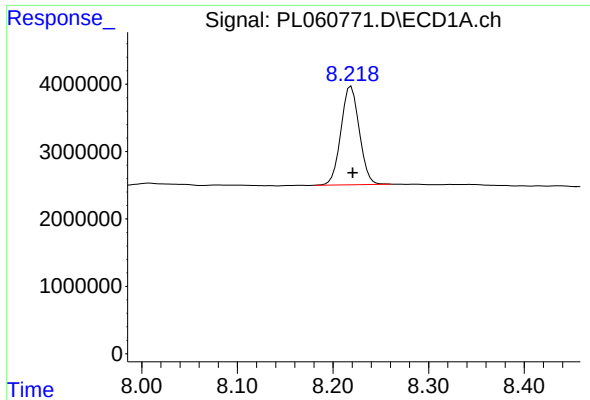


#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.002 min
Response: 19577542
Conc: 10.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-081420

Manual Integrations
APPROVED

Ankita
8/18/2020 3:39:42 PM

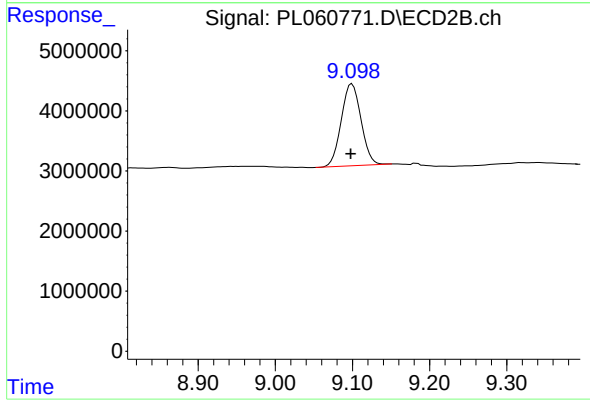

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.002 min
Response: 24305191
Conc: 12.95 ng/ml