

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 09:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 16:18:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.569	8519003	23824217	20.595	23.464
28)	SA Decachlor...	10.405	11.493	13100804	23279343	22.796	23.993
Target Compounds							
4)	MA Heptachlor	6.152f	0.000	1337323	0	2.277	N.D. #
6)	B beta-BHC	6.152	0.000	1337323	0	4.744	N.D. #
8)	B Heptachlo...	0.000	8.039	0	136238	N.D.	0.118 #
15)	B Endosulfa...	0.000	9.219f	0	268811	N.D.	0.293 #
23)	Chlordane-1	0.000	6.974f	0	48637	N.D.	1.153 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 09:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 16:18:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

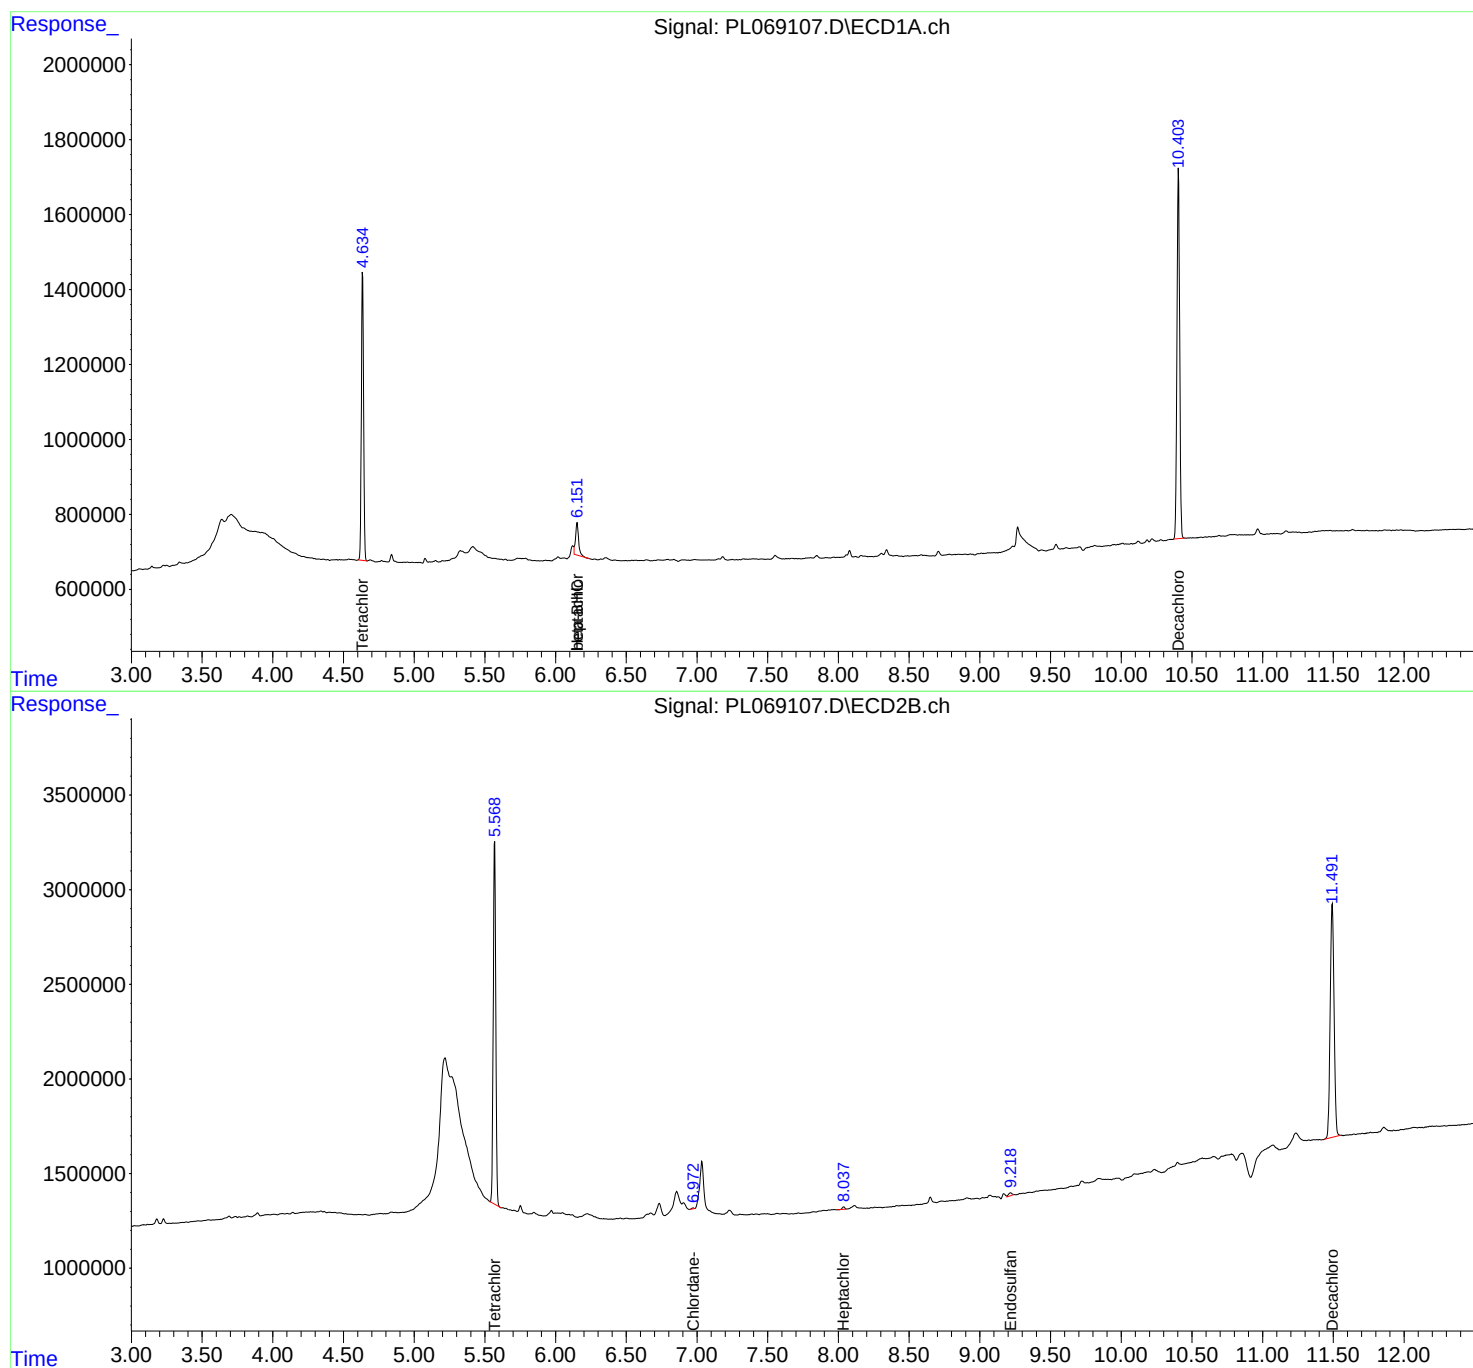


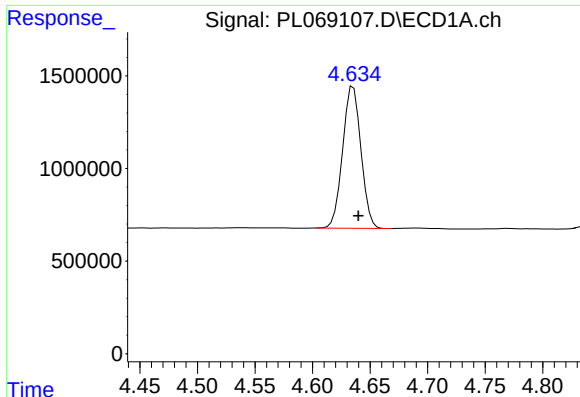

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.005 min
Response: 8519003
Conc: 20.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

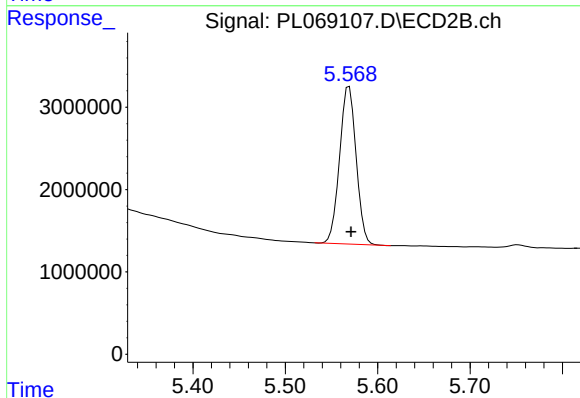


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 23824217
Conc: 23.46 ng/ml

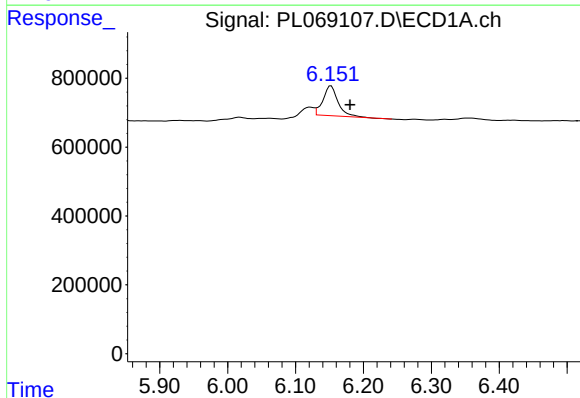


#4 Heptachlor

R.T.: 6.152 min
Delta R.T.: -0.028 min
Response: 1337323
Conc: 2.28 ng/ml

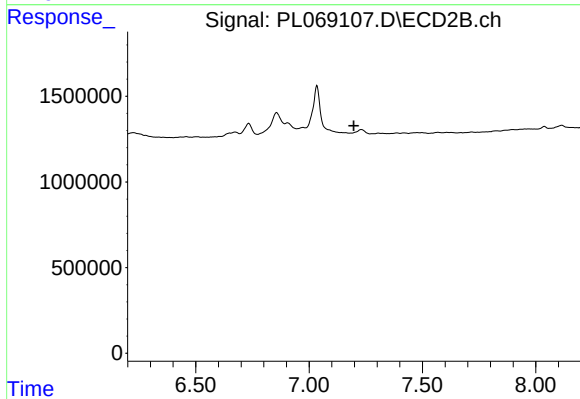

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

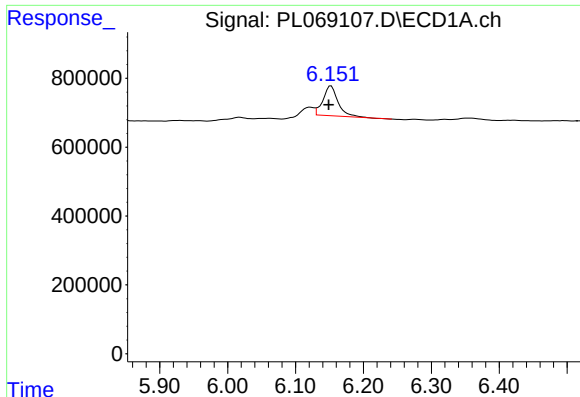

#6 beta-BHC


R.T.: 6.152 min
Delta R.T.: 0.004 min
Response: 1337323
Conc: 4.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

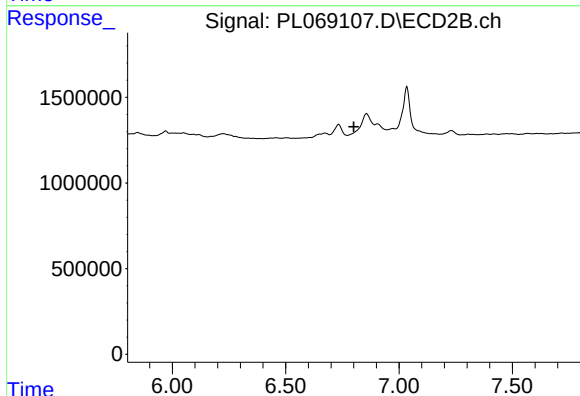


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

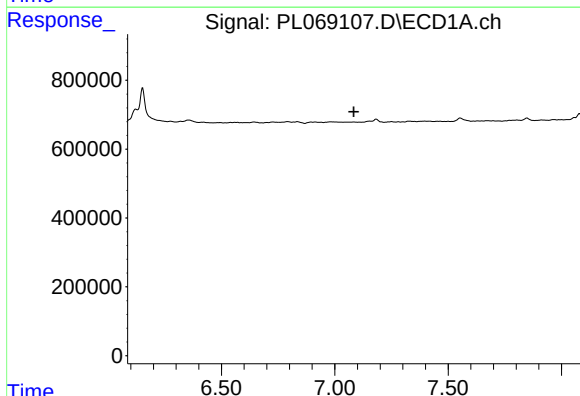


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

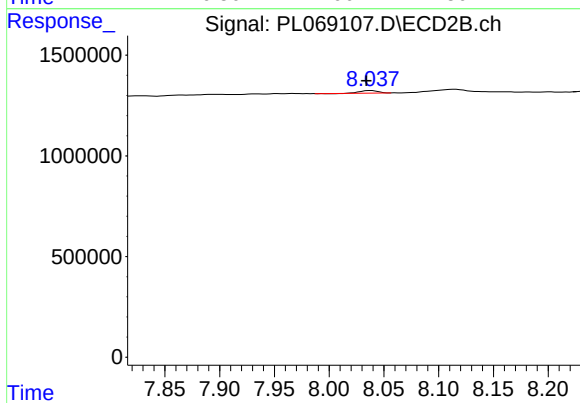

#8 Heptachlor epoxide


R.T.: 8.039 min
Delta R.T.: 0.005 min
Response: 136238
Conc: 0.12 ng/ml

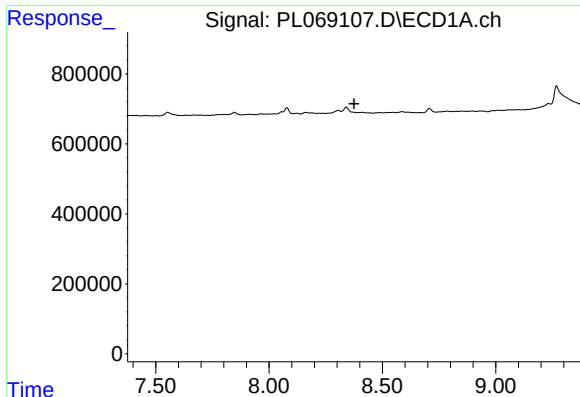

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

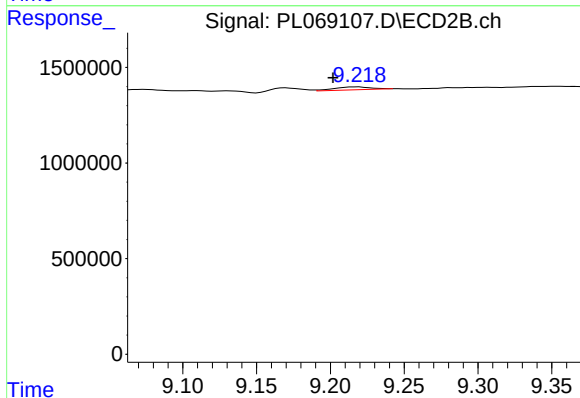


#15 Endosulfan II

R.T.: 9.219 min
Delta R.T.: 0.017 min
Response: 268811
Conc: 0.29 ng/ml

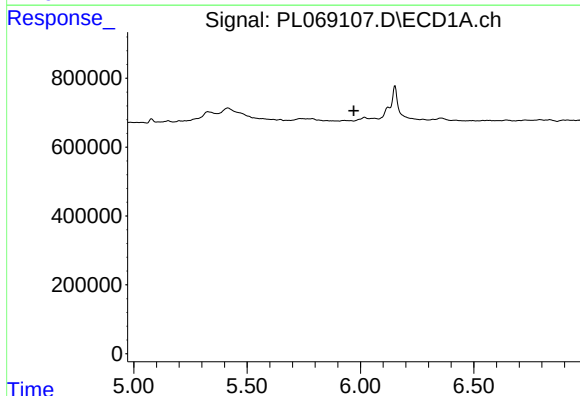


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

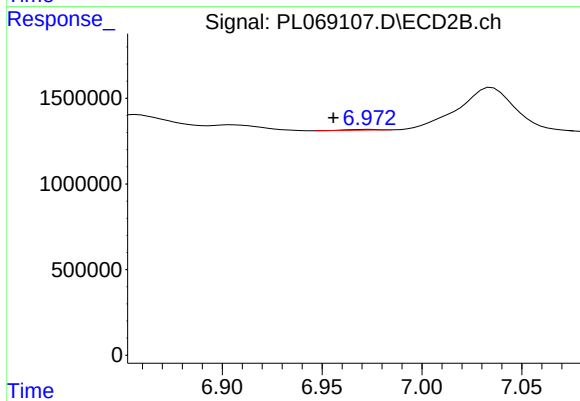

#23 Chlordane-1


R.T.: 6.974 min
Delta R.T.: 0.018 min
Response: 48637
Conc: 1.15 ng/ml

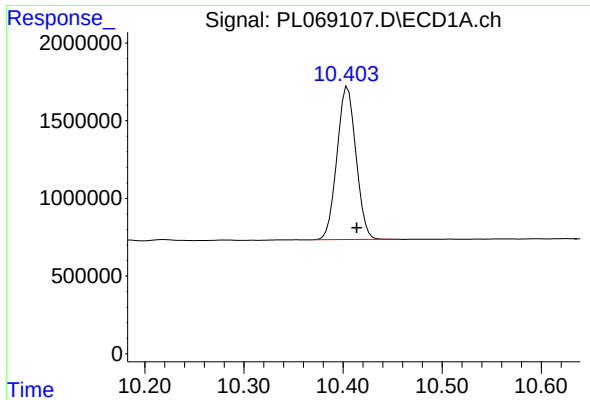

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 13100804
Conc: 22.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

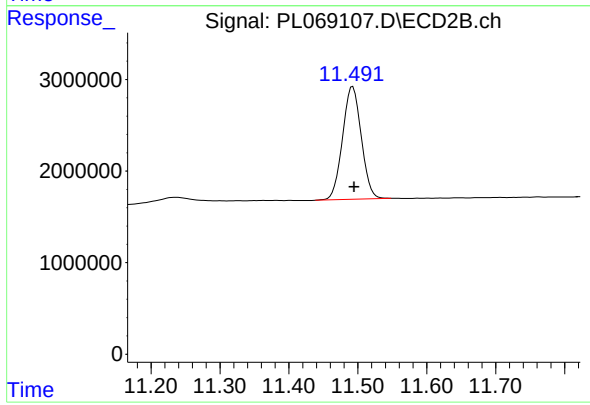

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: -0.002 min
Response: 23279343
Conc: 23.99 ng/ml