

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2021 22:41
 Operator : AR\AJ
 Sample : M3431-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:32:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.566	6536192	18684007	15.802	18.402
28)	SA Decachlor...	10.400	11.485	9299471	18068020	16.182	18.622
Target Compounds							
12)	B 4,4'-DDE	7.635	8.559	436964	787692	0.905	0.745
17)	MA 4,4'-DDT	8.480	9.422	326135	572637	0.672	0.605



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2021 22:41
Operator : AR\AJ
Sample : M3431-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:32:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

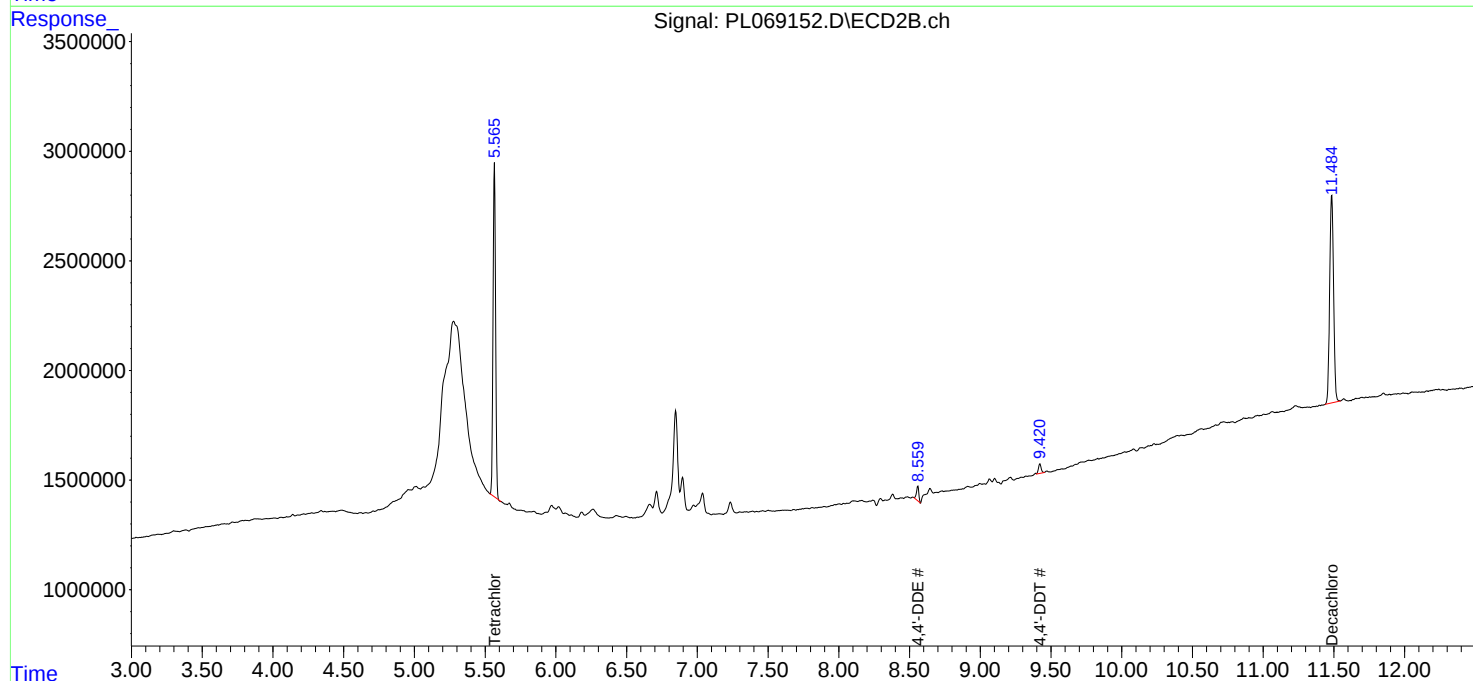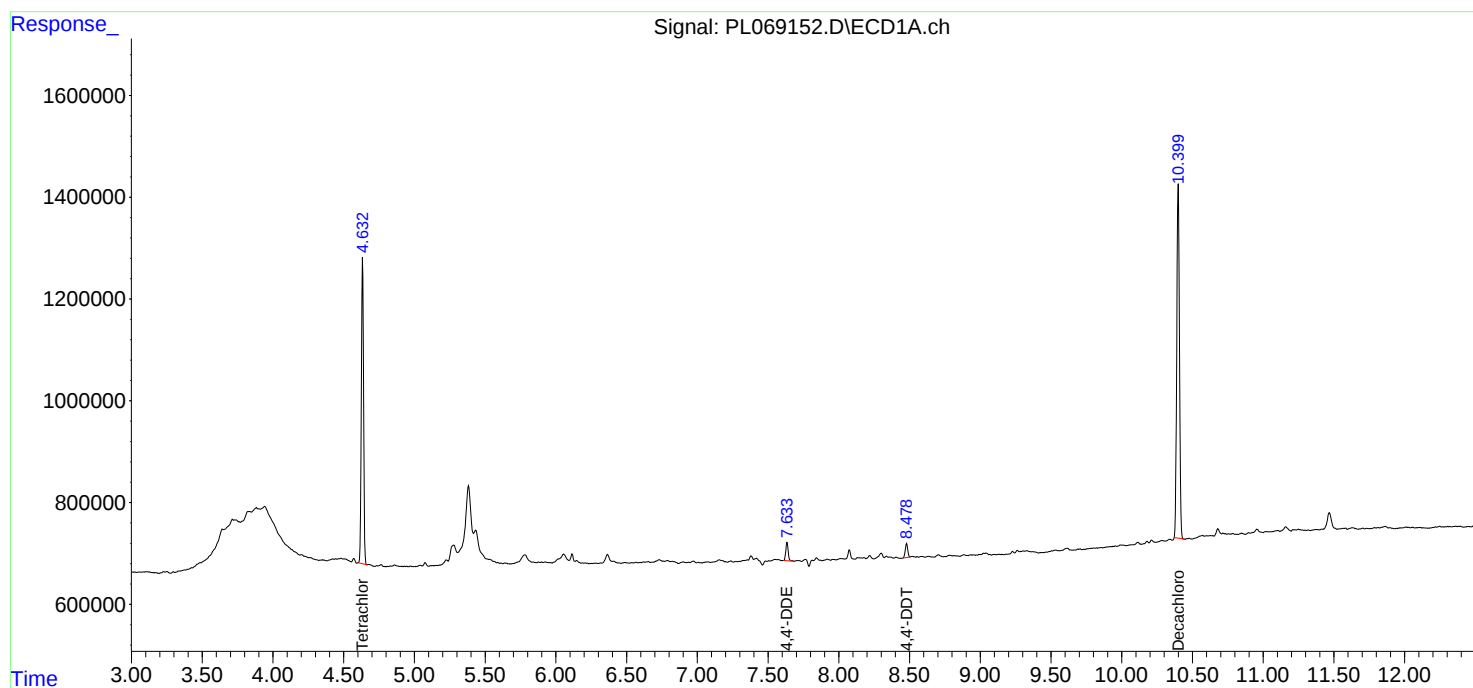


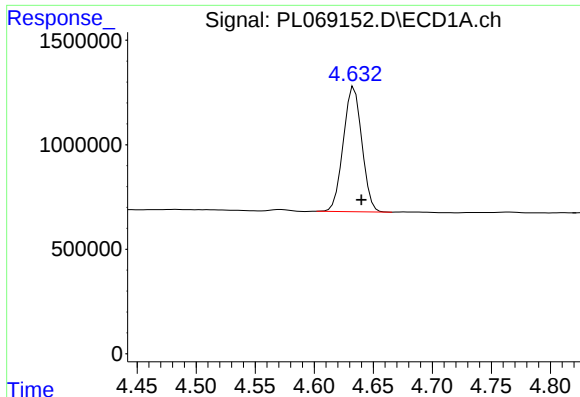

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 6536192
Conc: 15.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
3

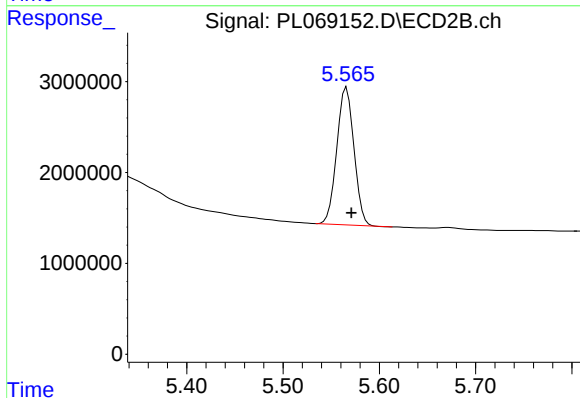


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 18684007
Conc: 18.40 ng/ml

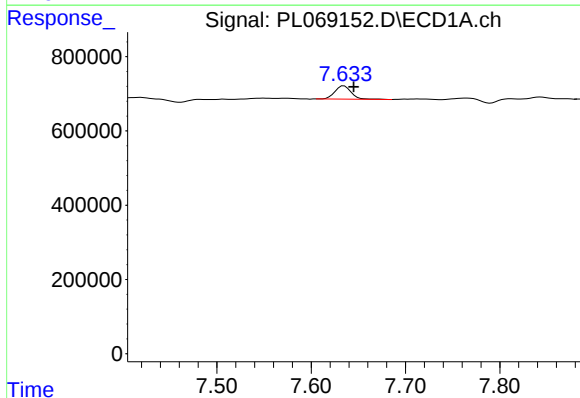


#12 4,4'-DDE

R.T.: 7.635 min
Delta R.T.: -0.010 min
Response: 436964
Conc: 0.90 ng/ml

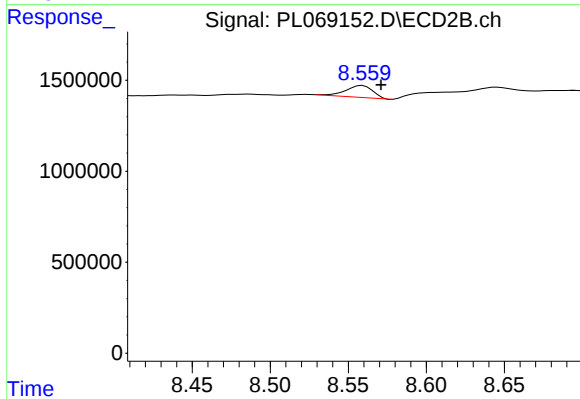

#12 4,4'-DDE


R.T.: 8.559 min
Delta R.T.: -0.012 min
Response: 787692
Conc: 0.75 ng/ml

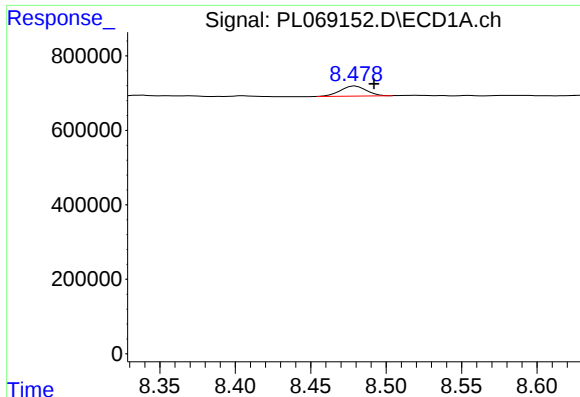

#17 4,4'-DDT


R.T.: 8.480 min
Delta R.T.: -0.012 min
Response: 326135
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
3

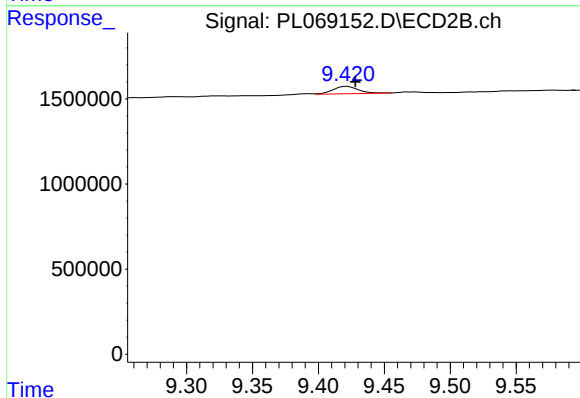


#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.006 min
Response: 572637
Conc: 0.61 ng/ml

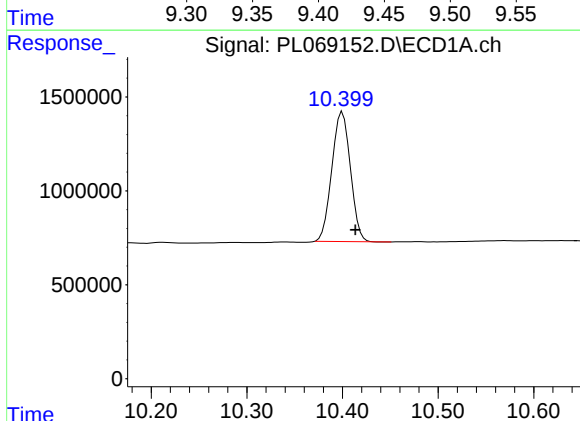

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.014 min
Response: 9299471
Conc: 16.18 ng/ml

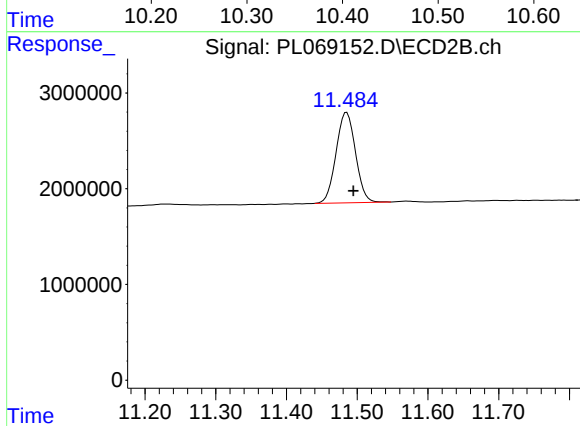

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.009 min
Response: 18068020
Conc: 18.62 ng/ml