

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069159.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 02:02
 Operator : AR\AJ
 Sample : M3431-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:34:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.566	7043669	20258721	17.028	19.953
28)	SA Decachlor...	10.399	11.484	10103336	18885951	17.580	19.465
Target Compounds							
12)	B 4,4'-DDE	7.634	8.559	479552	760197	0.993	0.719 #
17)	MA 4,4'-DDT	8.479	9.421	340124	591743	0.700	0.625



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069159.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 02:02
Operator : AR\AJ
Sample : M3431-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:34:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

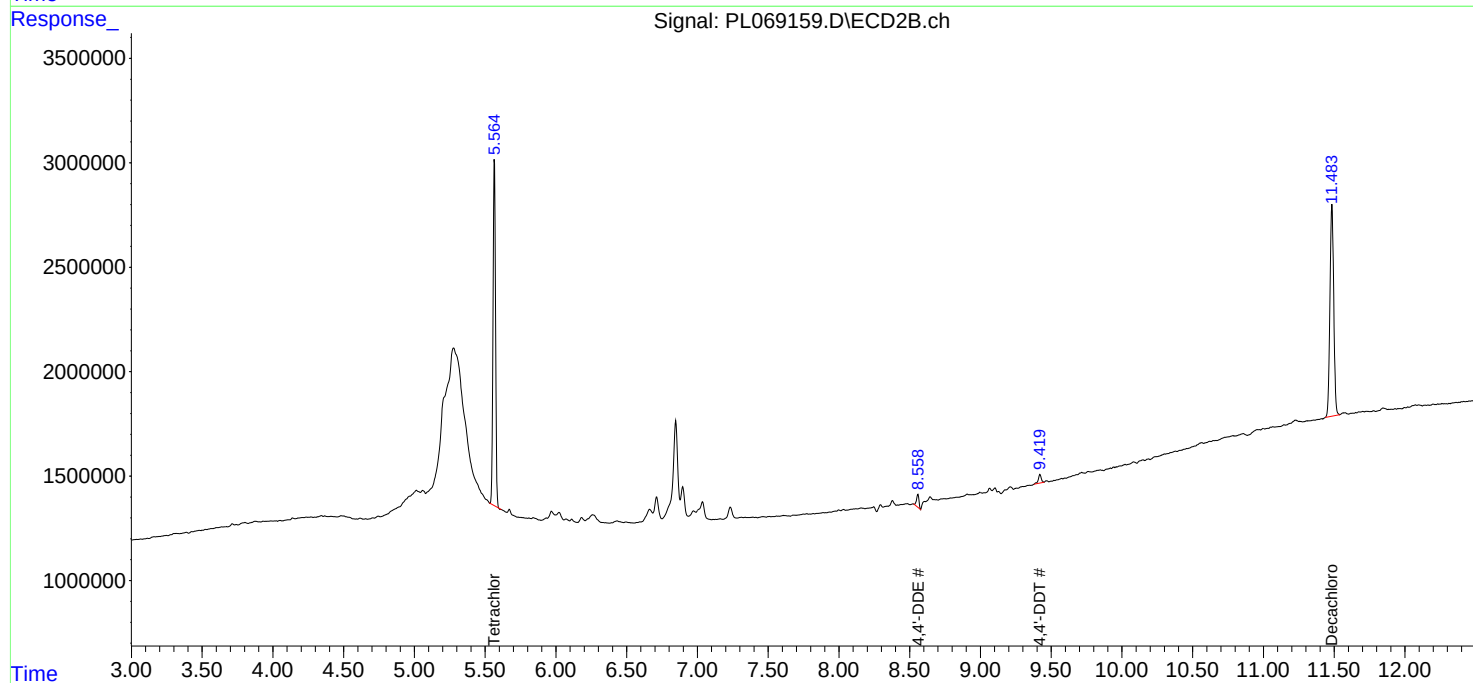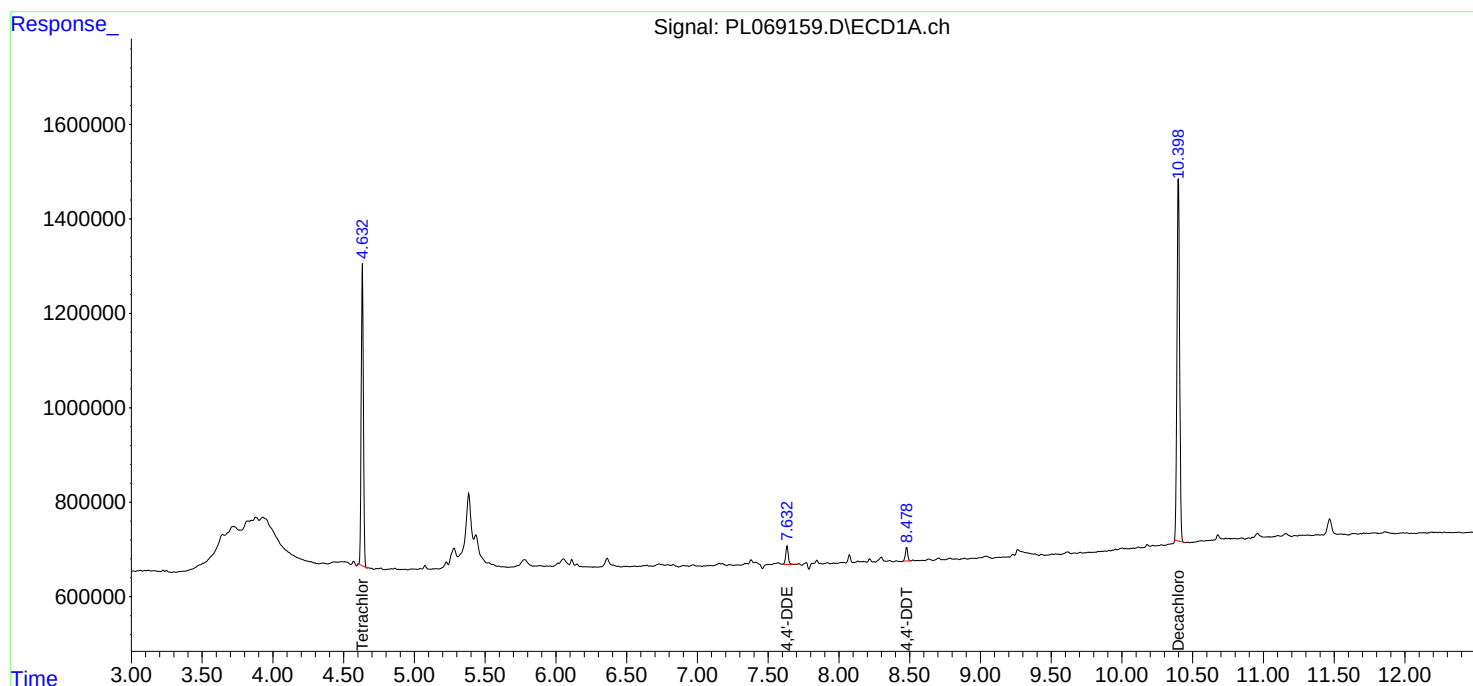


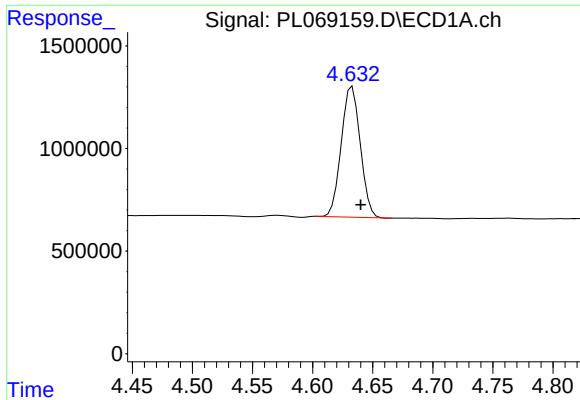

#1 Tetrachloro-m-xylene


R.T.: 4.633 min
Delta R.T.: -0.007 min
Response: 7043669
Conc: 17.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
6

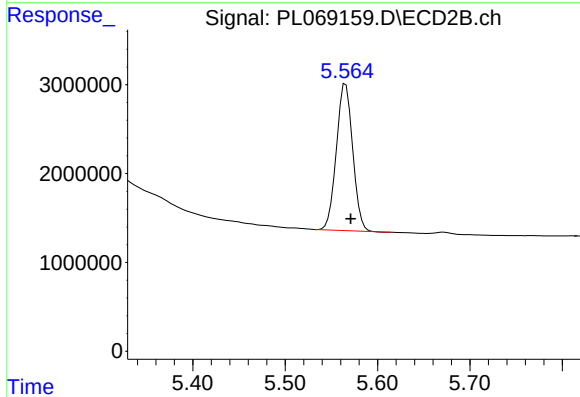


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.006 min
Response: 20258721
Conc: 19.95 ng/ml

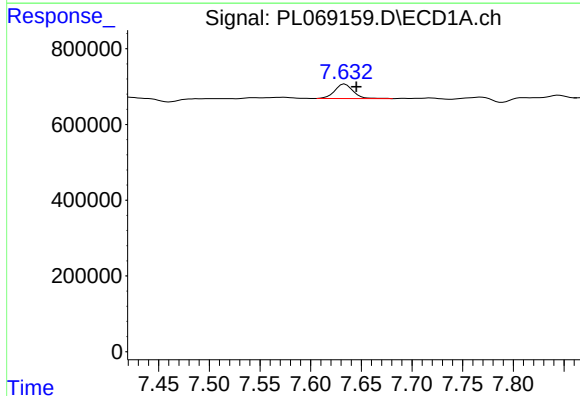


#12 4,4'-DDE

R.T.: 7.634 min
Delta R.T.: -0.011 min
Response: 479552
Conc: 0.99 ng/ml

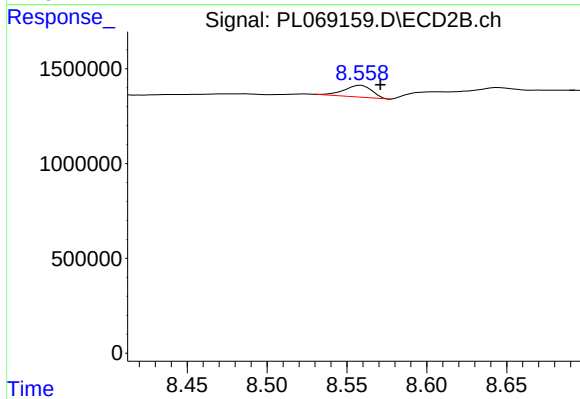

#12 4,4'-DDE


R.T.: 8.559 min
Delta R.T.: -0.012 min
Response: 760197
Conc: 0.72 ng/ml

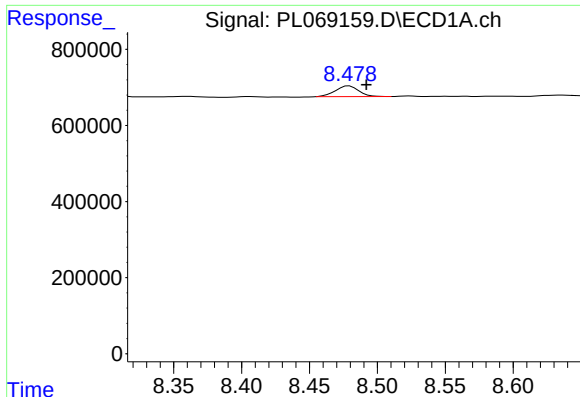

#17 4,4'-DDT


R.T.: 8.479 min
Delta R.T.: -0.013 min
Response: 340124
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
6

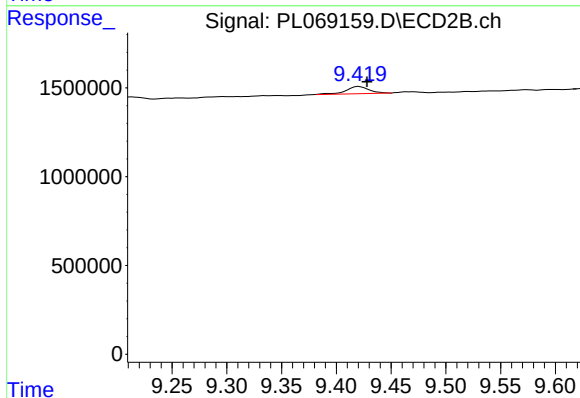


#17 4,4'-DDT

R.T.: 9.421 min
Delta R.T.: -0.007 min
Response: 591743
Conc: 0.63 ng/ml

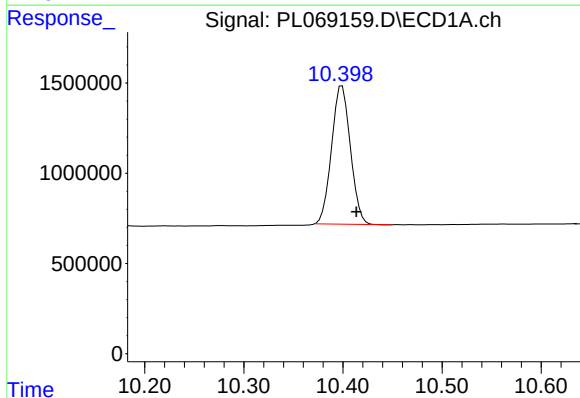

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.014 min
Response: 10103336
Conc: 17.58 ng/ml

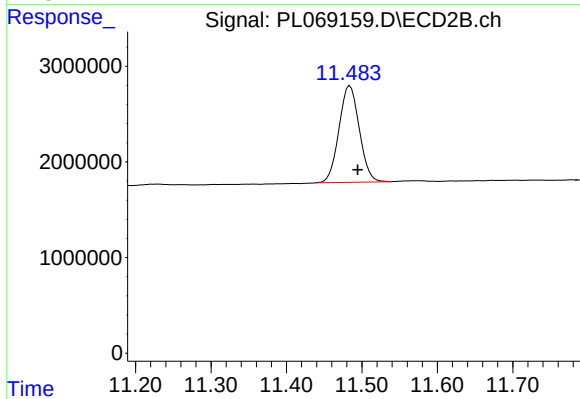

#28 Decachlorobiphenyl

R.T.: 11.484 min
Delta R.T.: -0.011 min
Response: 18885951
Conc: 19.47 ng/ml