

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 02:35
 Operator : AR\AJ
 Sample : M3398-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2021-08-10-FD-01

Manual Integrations
 APPROVED

mohammad
 8/18/2021 4:17:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:35:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.633	5.566	10225440	29808725	24.721	29.359
28)	SA Decachlor...	10.399	11.485	12317056	23125810	21.432	23.835
Target Compounds							
12)	B 4,4'-DDE	7.632	8.560	301083	565173	0.623m	0.535
17)	MA 4,4'-DDT	8.478	9.421	335051	1297805	0.690m	1.371 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 02:35
Operator : AR\AJ
Sample : M3398-02
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
2021-08-10-FD-01


Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:35:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

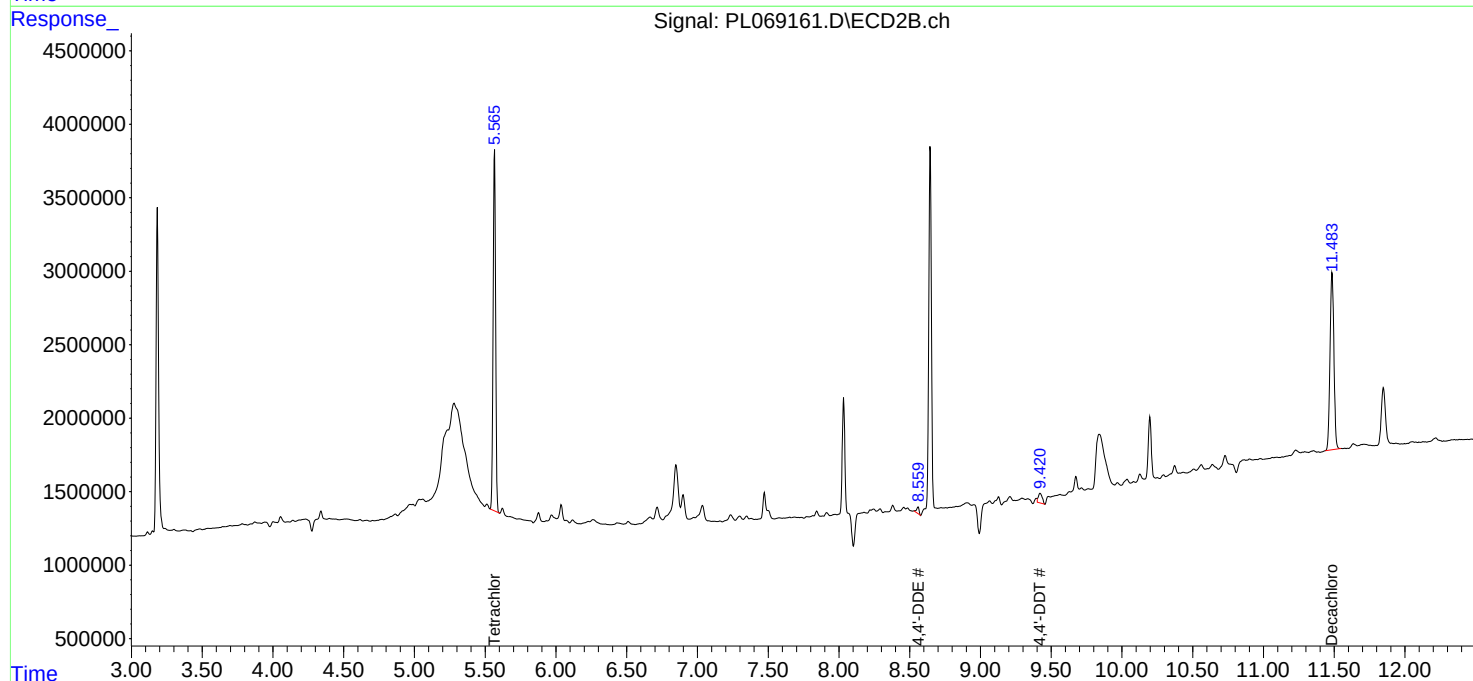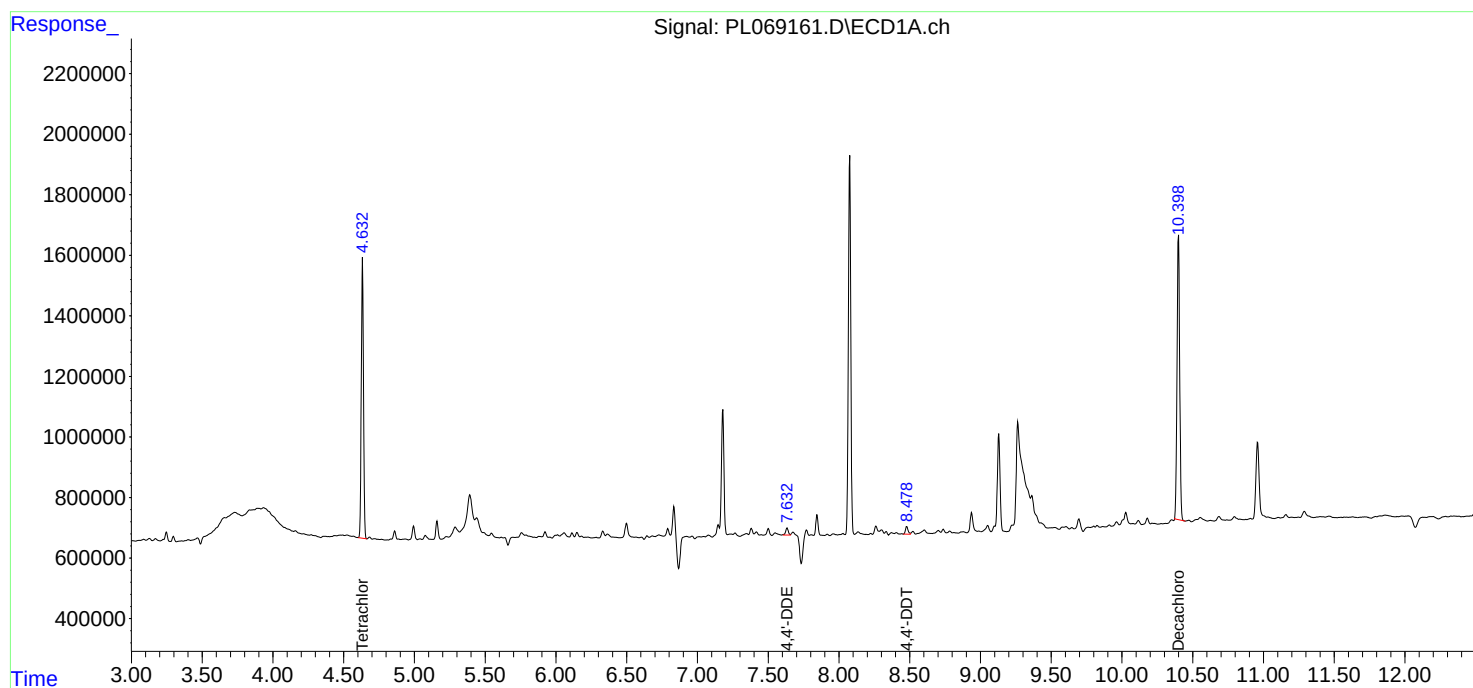

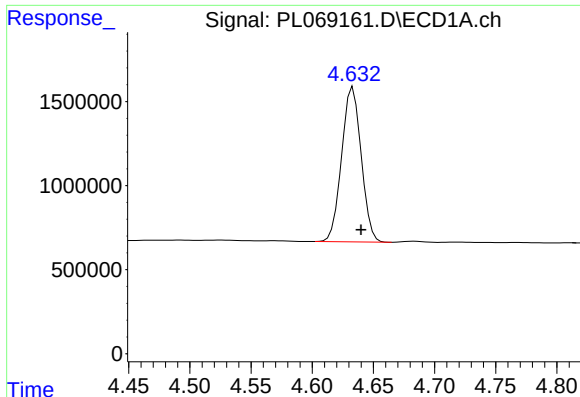


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: -0.007 min
Response: 10225440
Conc: 24.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
2021-08-10-FD-01


Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:22 PM

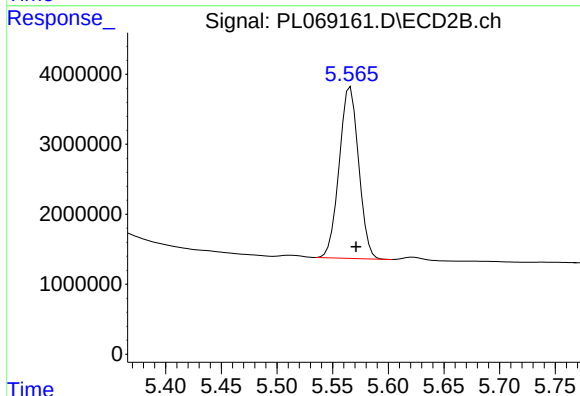


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 29808725
Conc: 29.36 ng/ml

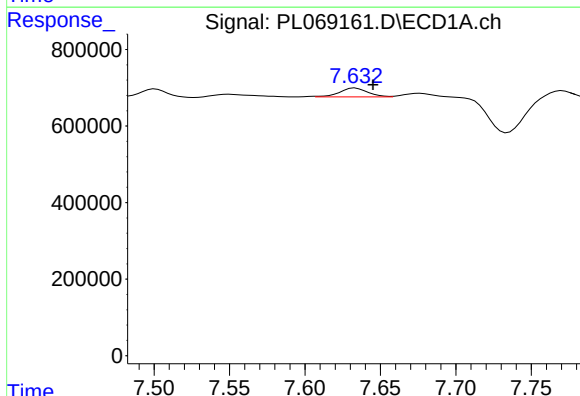


#12 4,4'-DDE

R.T.: 7.632 min
Delta R.T.: -0.013 min
Response: 301083
Conc: 0.62 ng/ml m

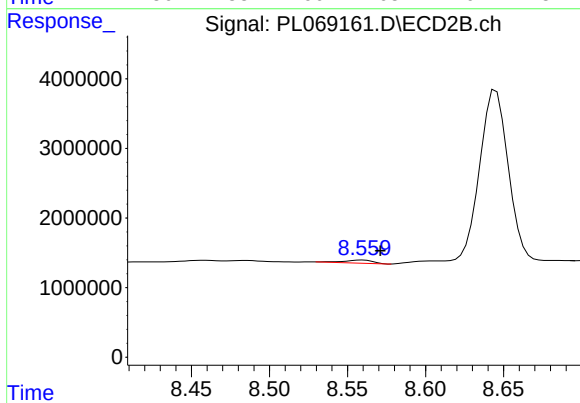

#12 4,4'-DDE

R.T.: 8.560 min
Delta R.T.: -0.011 min
Response: 565173
Conc: 0.53 ng/ml

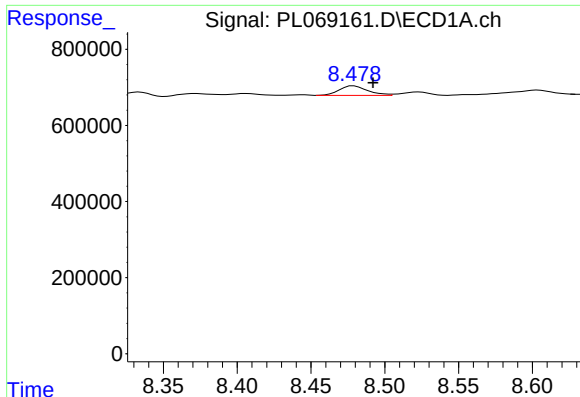


#17 4,4'-DDT

R.T.: 8.478 min
Delta R.T.: -0.015 min
Response: 335051
Conc: 0.69 ng/ml m

Instrument :
ECD_L
ClientSampleId :
2021-08-10-FD-01


Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:22 PM

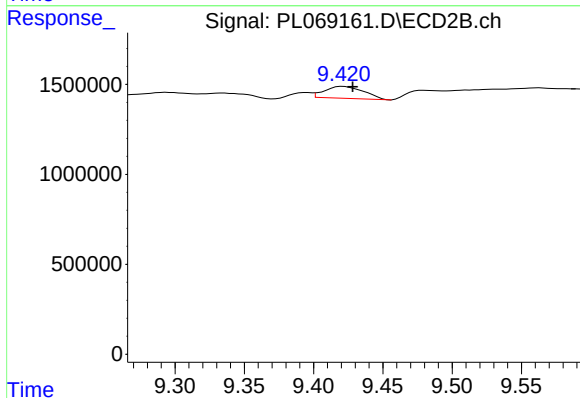


#17 4,4'-DDT

R.T.: 9.421 min
Delta R.T.: -0.007 min
Response: 1297805
Conc: 1.37 ng/ml

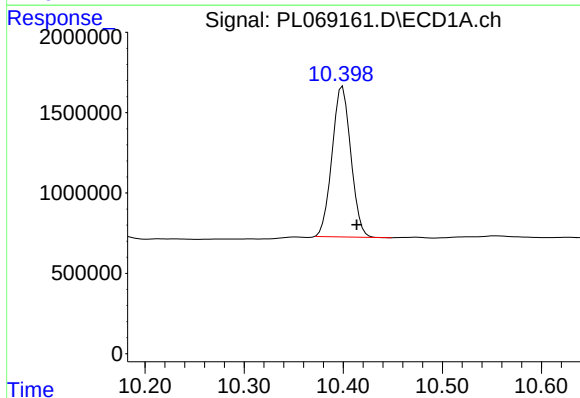

#28 Decachlorobiphenyl

R.T.: 10.399 min
Delta R.T.: -0.014 min
Response: 12317056
Conc: 21.43 ng/ml

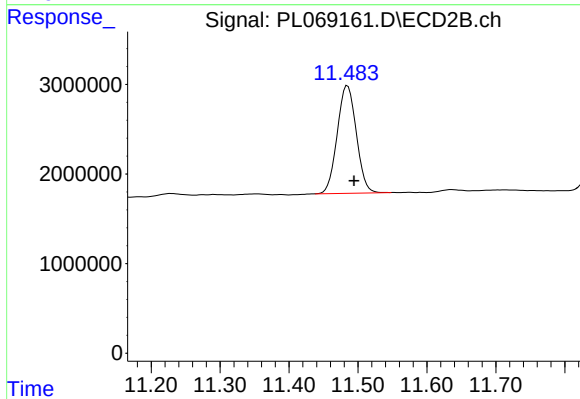

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.010 min
Response: 23125810
Conc: 23.84 ng/ml