

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
 Data File : PL069166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 03:58
 Operator : AR\AJ
 Sample : M3398-17
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SWCS-04-0205

Manual Integrations
 APPROVED

mohammad
 8/18/2021 4:17:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 07:37:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.566	6683421	18737317	16.158	18.454
28)	SA Decachlor...	10.400	11.485	7220155	13797155	12.563	14.220
Target Compounds							
17)	MA 4,4'-DDT	8.478	9.422	290557	538714	0.598m	0.569

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081721\
Data File : PL069166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 03:58
Operator : AR\AJ
Sample : M3398-17
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SWCS-04-0205


Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 07:37:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

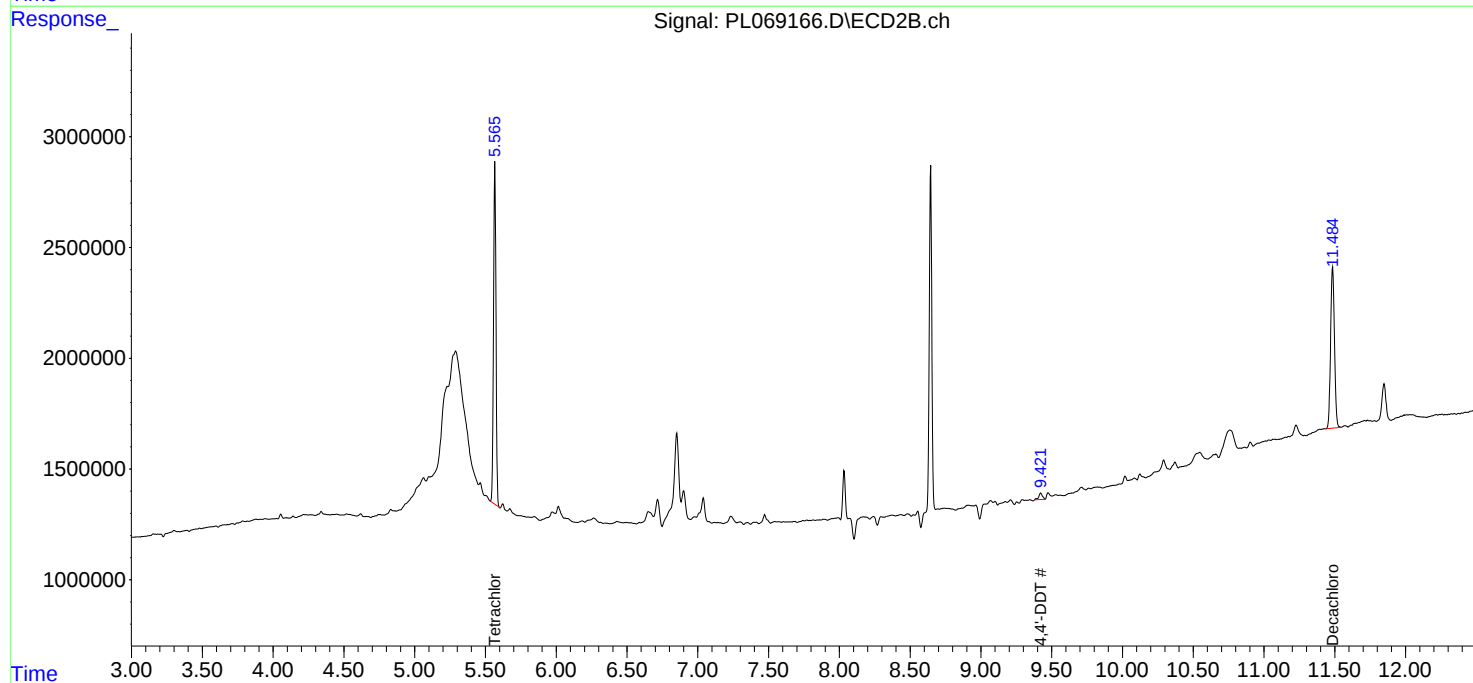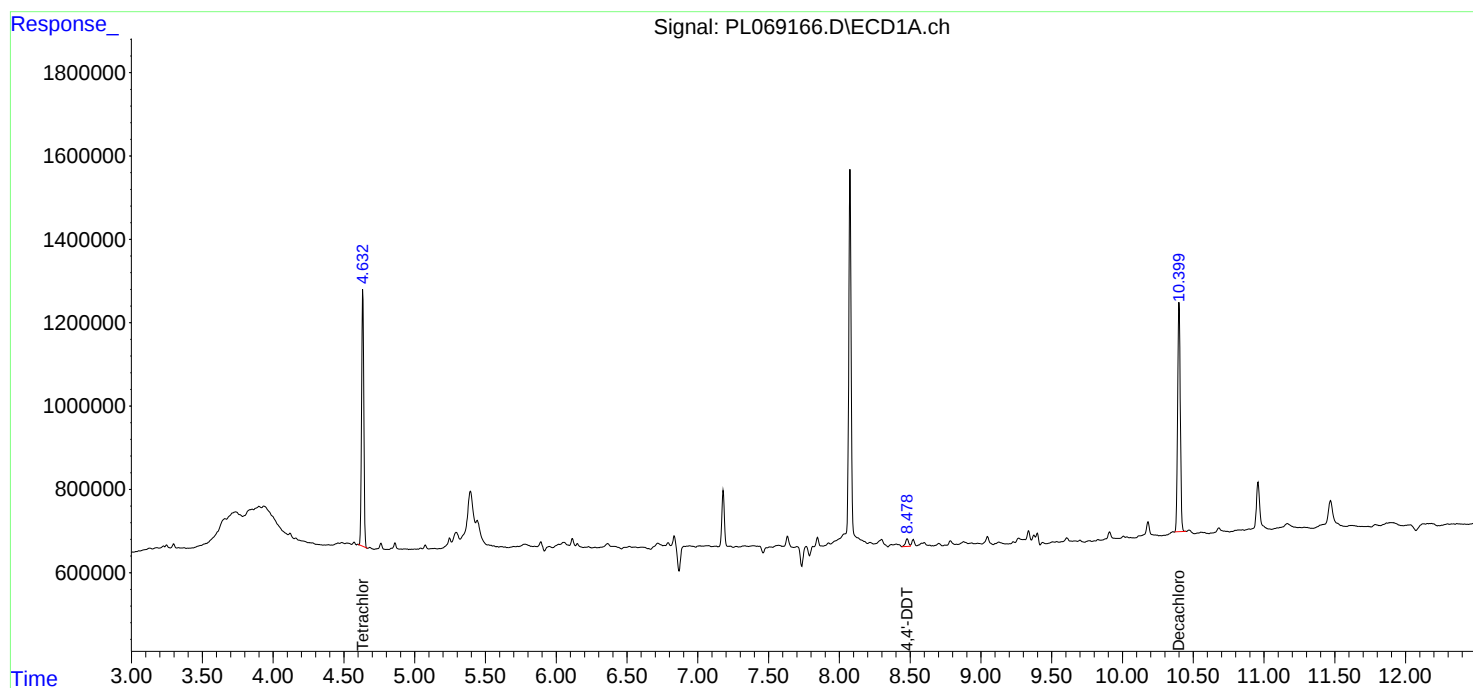

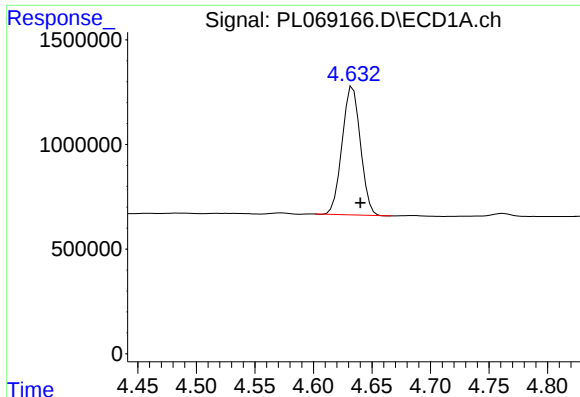


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 6683421
Conc: 16.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-04-0205


Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:38 PM

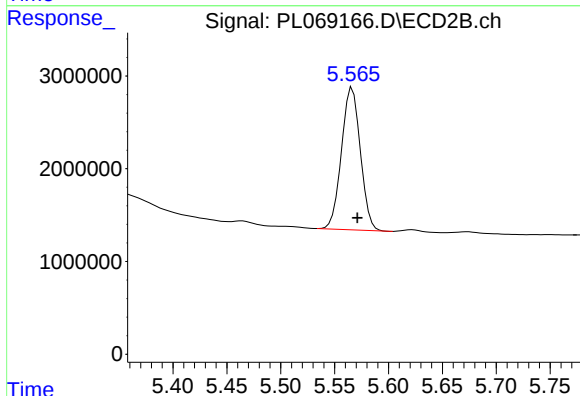


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 18737317
Conc: 18.45 ng/ml

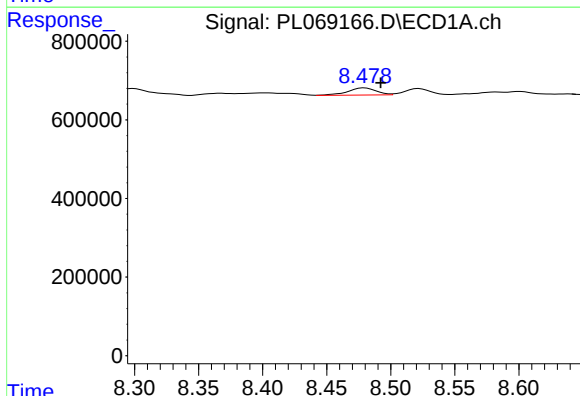


#17 4,4'-DDT

R.T.: 8.478 min
Delta R.T.: -0.014 min
Response: 290557
Conc: 0.60 ng/ml m

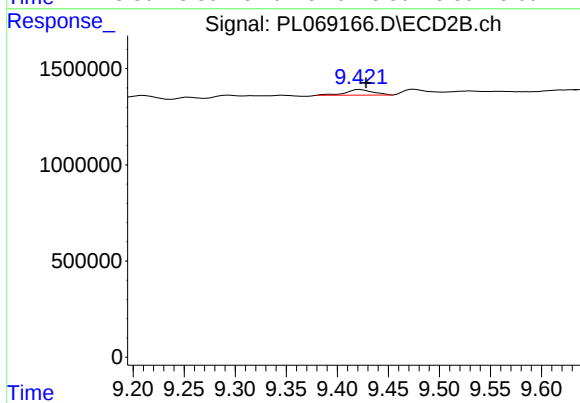

#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.006 min
Response: 538714
Conc: 0.57 ng/ml

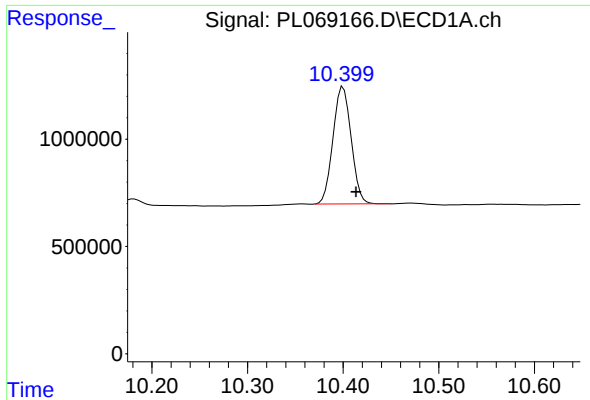


#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.014 min
Response: 7220155
Conc: 12.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SWCS-04-0205

Manual Integrations
APPROVED

mohammad
8/18/2021 4:17:38 PM

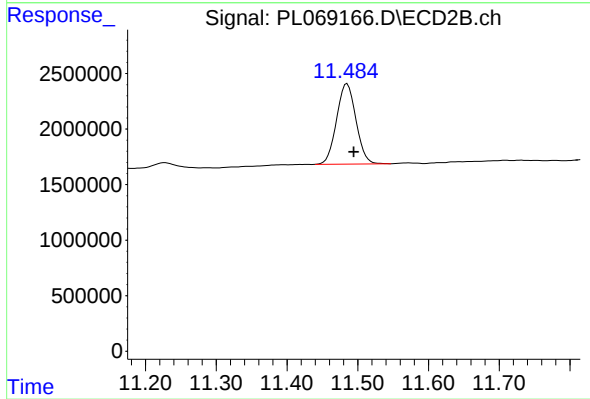

#28 Decachlorobiphenyl

R.T.: 11.485 min
Delta R.T.: -0.010 min
Response: 13797155
Conc: 14.22 ng/ml