

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081723\
 Data File : PL084807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2023 12:43
 Operator : AR\AJ
 Sample : 03937-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MANHOLE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/17/2023
 Supervised By :Ankita Jodhani 08/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 22:22:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.483	2.685	27524512	21132871	11.846	19.434m#
28)	SA Decachlor...	9.033	7.867	25680760	20542653	15.783	16.476m
Target Compounds							
14)	MA Endrin	6.514	5.554	28077671	19397064	12.874	15.858

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081723\
Data File : PL084807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2023 12:43
Operator : AR\AJ
Sample : 03937-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/17/2023
Supervised By : Ankita Jodhani 08/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 22:22:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

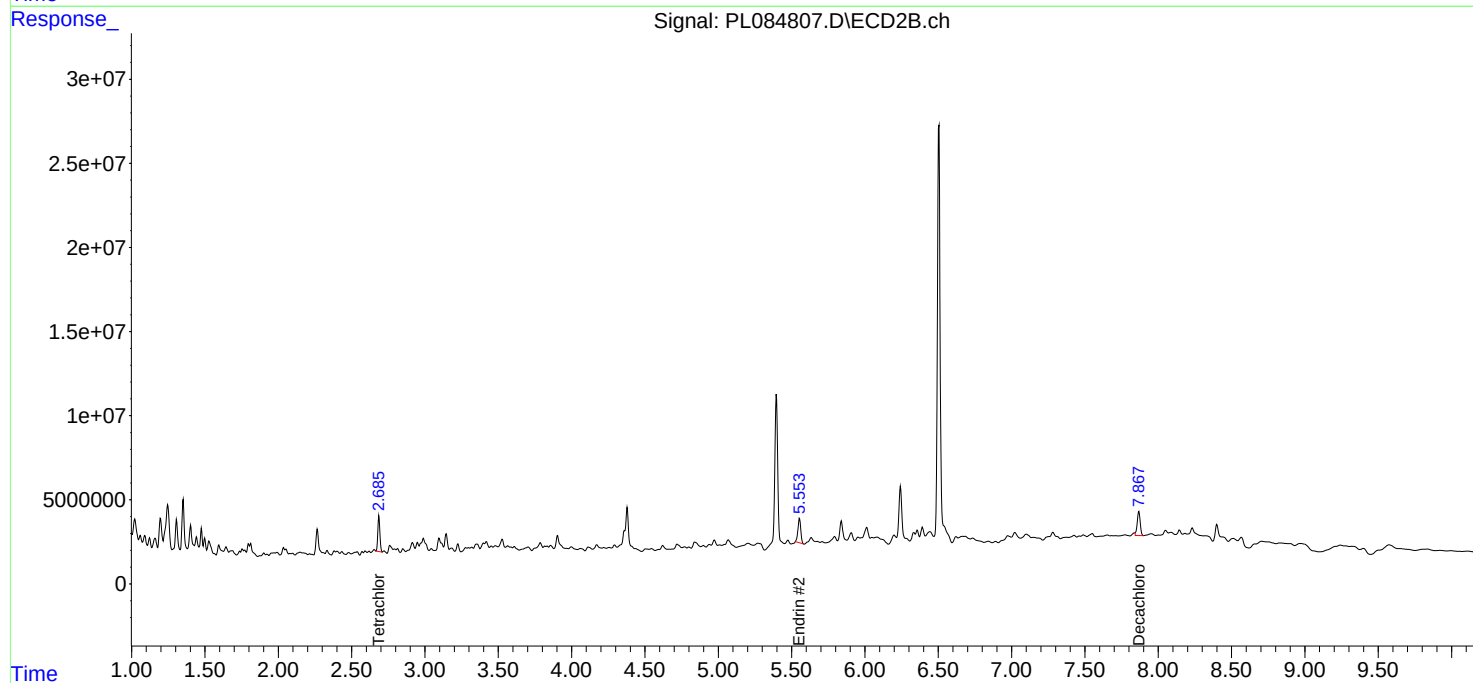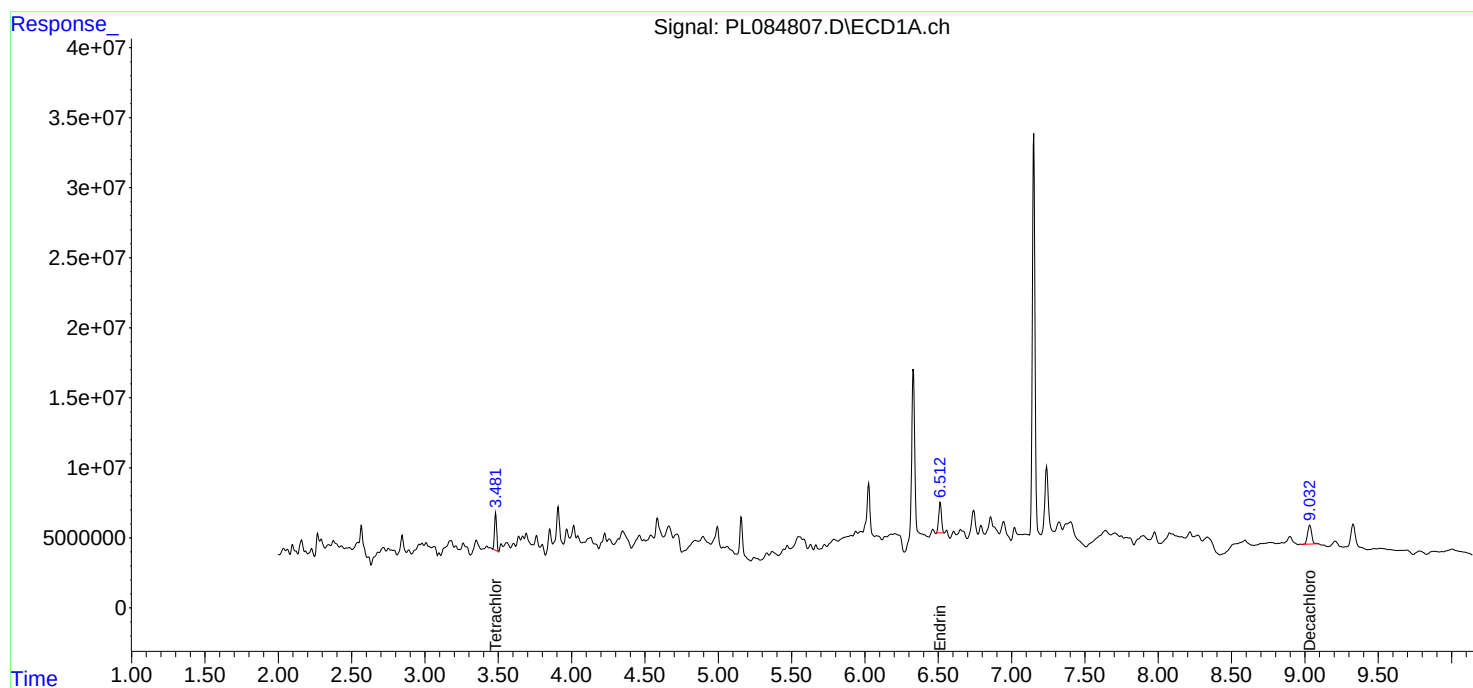

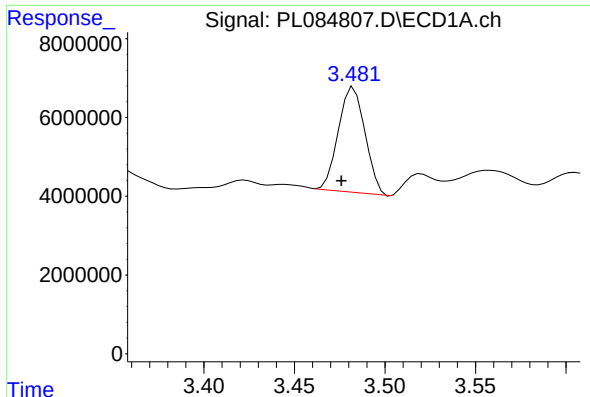


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: 0.007 min
Response: 27524512
Conc: 11.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/17/2023
Supervised By :Ankita Jodhani 08/17/2023

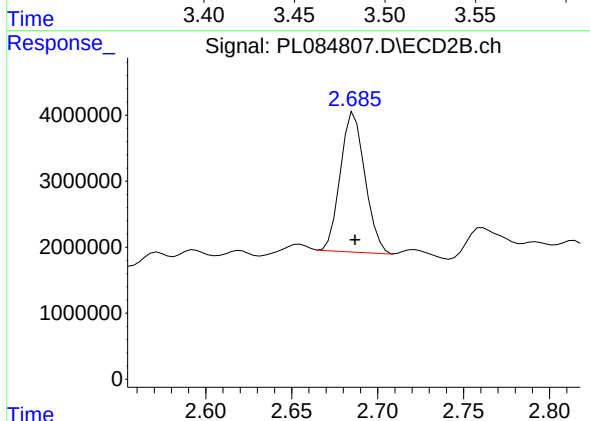


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.002 min
Response: 21132871
Conc: 19.43 ng/ml m

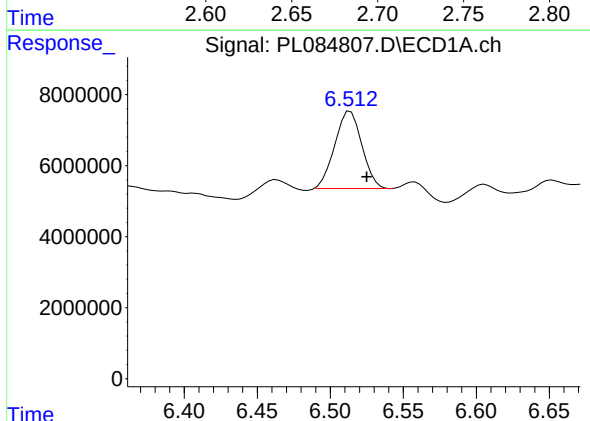


#14 Endrin

R.T.: 6.514 min
Delta R.T.: -0.011 min
Response: 28077671
Conc: 12.87 ng/ml

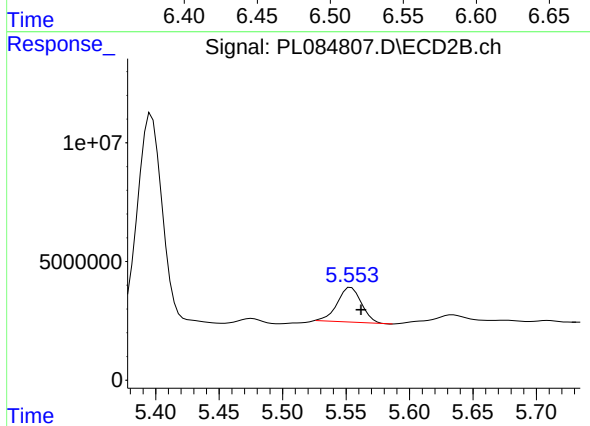

#14 Endrin

R.T.: 5.554 min
Delta R.T.: -0.008 min
Response: 19397064
Conc: 15.86 ng/ml

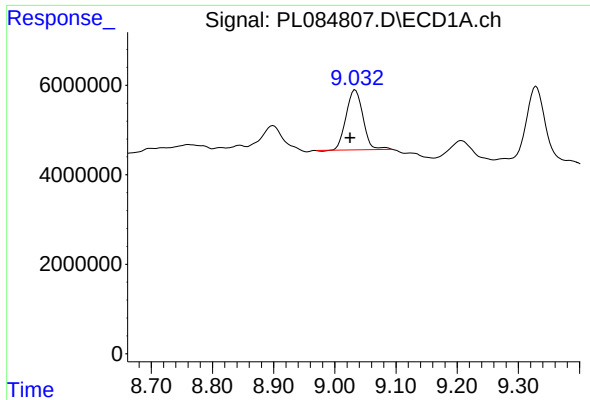


#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.009 min
Response: 25680760
Conc: 15.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
MANHOLE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/17/2023
Supervised By :Ankita Jodhani 08/17/2023

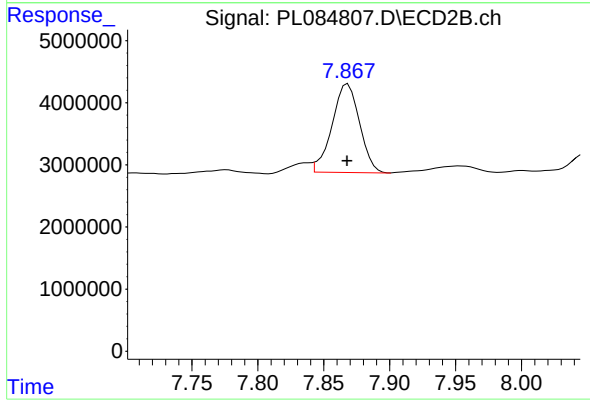

#28 Decachlorobiphenyl

R.T.: 7.867 min
Delta R.T.: 0.000 min
Response: 20542653
Conc: 16.48 ng/ml m