

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081820\
 Data File : PL060789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 13:20
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:16:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 02:13:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	4.010	96413182	142.2E6	50.000	50.000
28)	SA Decachlor...	8.218	9.099	74514137	104.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.331	5.006	23717298	53302411	500.000	500.000
24)	Chlordane-2	4.833	5.475	27477650	53849158	500.000	500.000
25)	Chlordane-3	5.403	6.124	69853317	201.6E6	500.000	500.000
26)	Chlordane-4	5.460	6.199	57255137	246.4E6	500.000	500.000
27)	Chlordane-5	6.296	7.005	24921111	38260530	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081820\
Data File : PL060789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 13:20
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:16:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 02:13:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

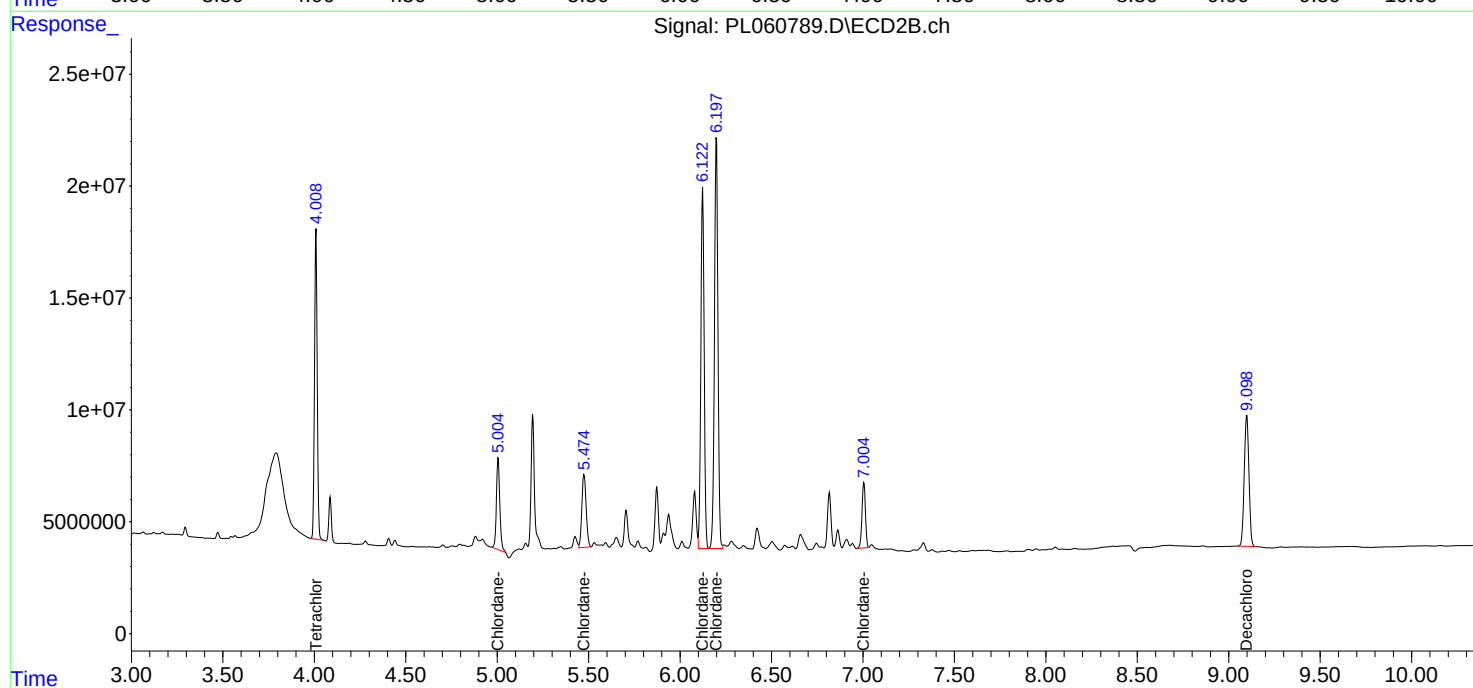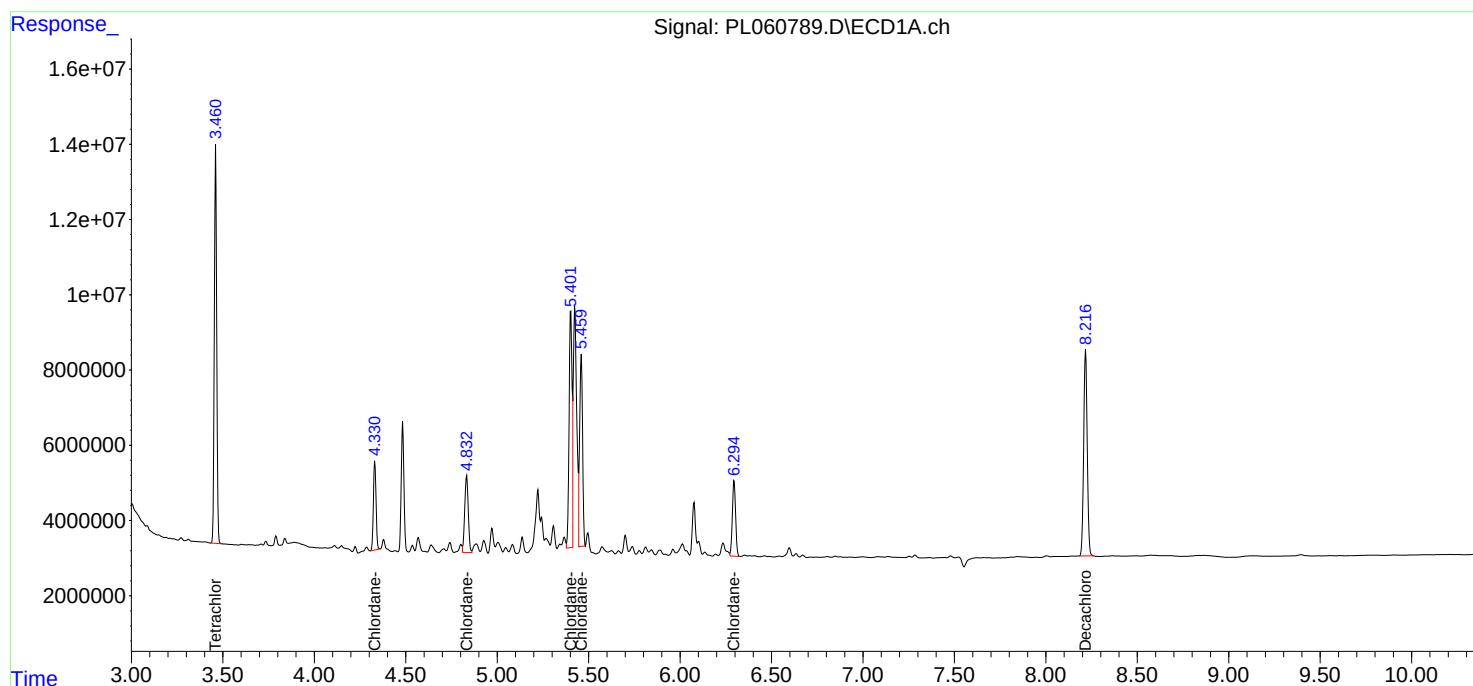


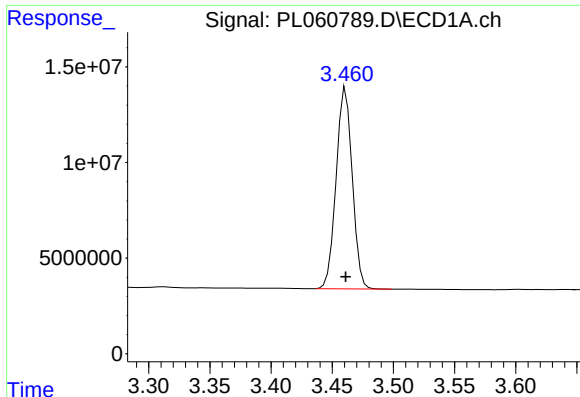

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 96413182
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

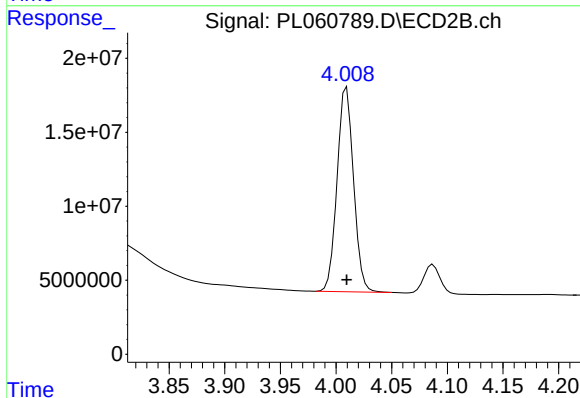


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 142232198
Conc: 50.00 ng/ml

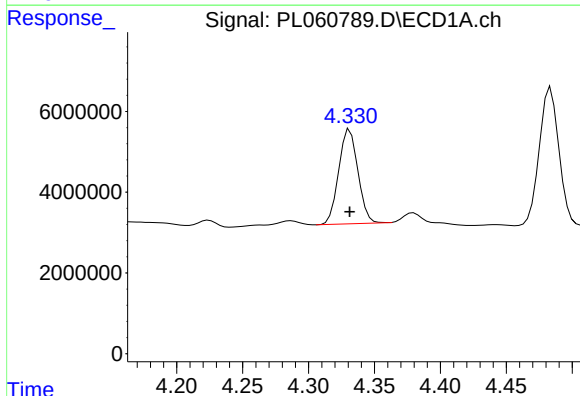


#23 Chlordane-1

R.T.: 4.331 min
Delta R.T.: 0.000 min
Response: 23717298
Conc: 500.00 ng/ml

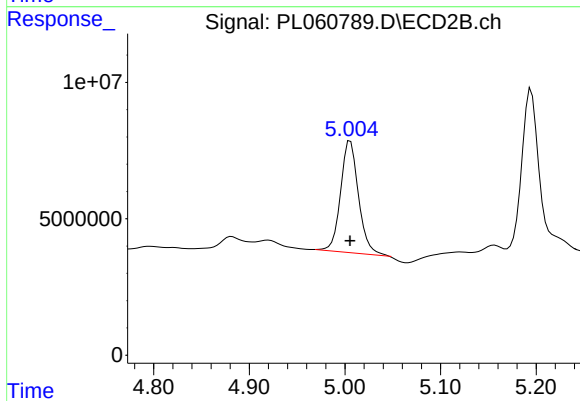

#23 Chlordane-1


R.T.: 5.006 min
Delta R.T.: 0.000 min
Response: 53302411
Conc: 500.00 ng/ml

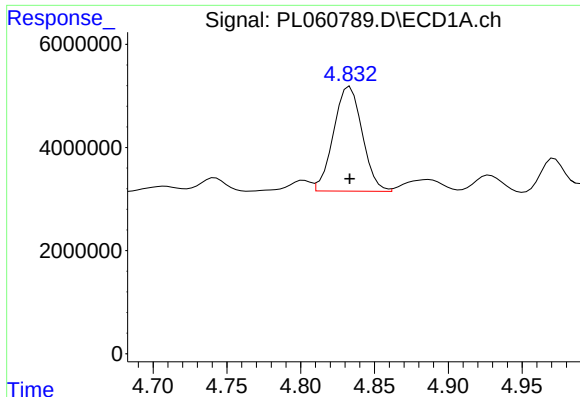

#24 Chlordane-2


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 27477650
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

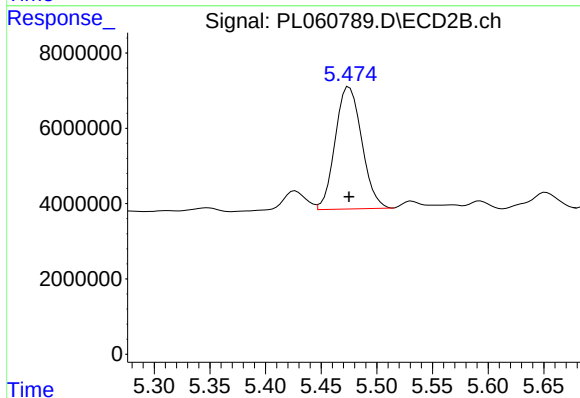


#24 Chlordane-2

R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 53849158
Conc: 500.00 ng/ml

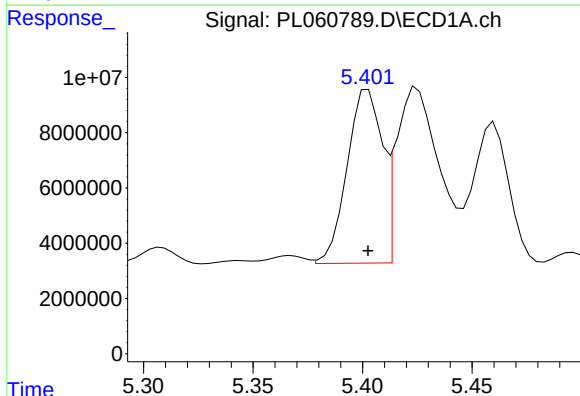


#25 Chlordane-3

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 69853317
Conc: 500.00 ng/ml

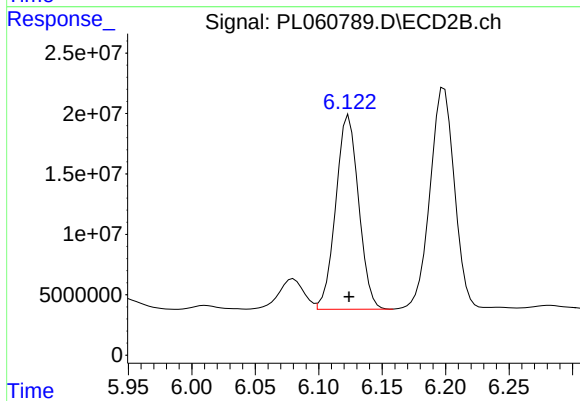

#25 Chlordane-3


R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 201626199
Conc: 500.00 ng/ml

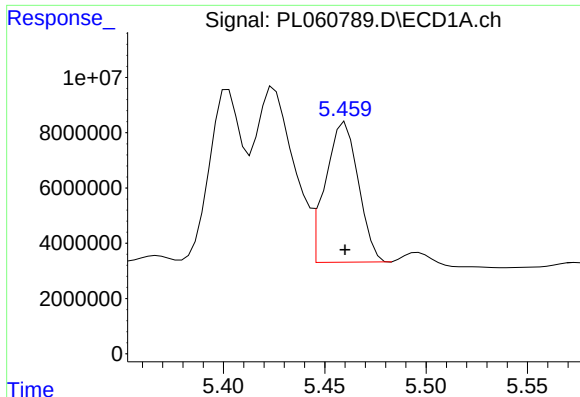

#26 Chlordane-4


R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 57255137
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

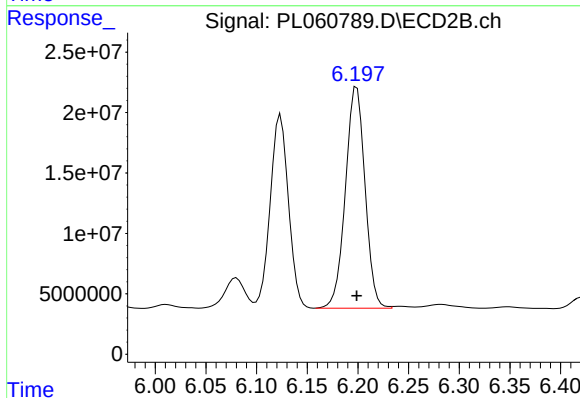


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 246405308
Conc: 500.00 ng/ml

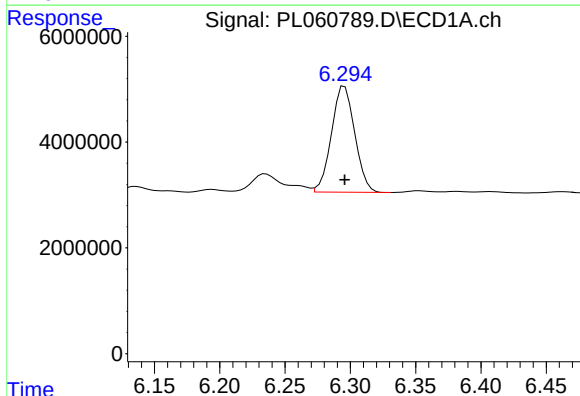


#27 Chlordane-5

R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 24921111
Conc: 500.00 ng/ml

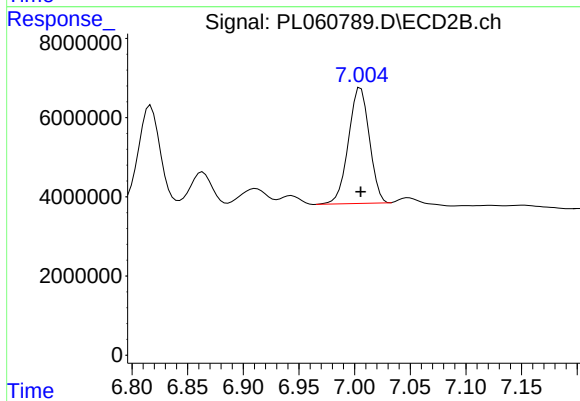

#27 Chlordane-5


R.T.: 7.005 min
Delta R.T.: 0.000 min
Response: 38260530
Conc: 500.00 ng/ml

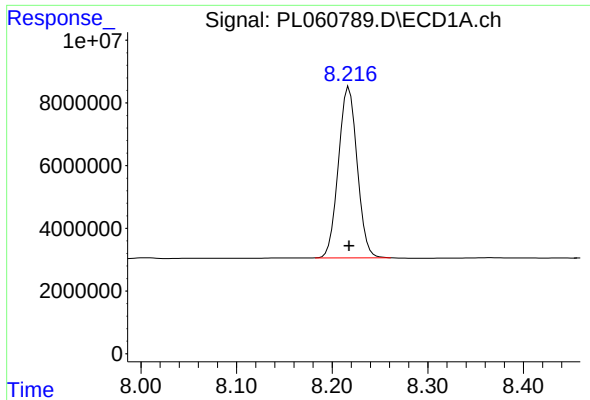

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: 0.000 min
Response: 74514137
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

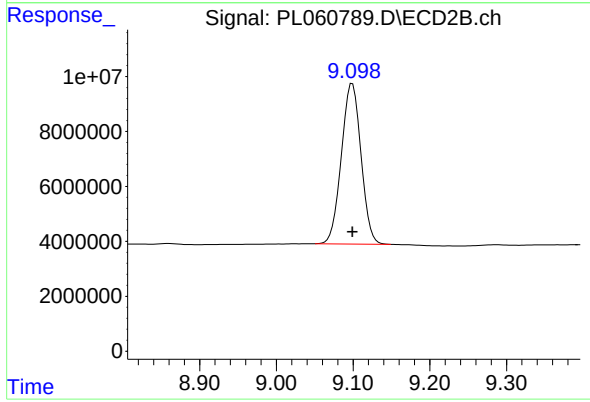

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 104325466
Conc: 50.00 ng/ml