

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081820\
 Data File : PL060806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2020 17:23
 Operator : DD\AJ
 Sample : L3719-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20200511-AMENDED-DISCRETE-00

Manual Integrations
 APPROVED

Ankita
 8/20/2020 1:07:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 02:40:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 02:25:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.484f	4.010	23327896	39850247	13.974m	14.326
28) SA Decachlor...	8.241f	9.099	12872617	19374361	9.012m	9.586
Target Compounds						
12) B 4,4'-DDE	5.648f	6.355	1258734	2602920	0.816m	0.860

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081820\
Data File : PL060806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2020 17:23
Operator : DD\AJ
Sample : L3719-05
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20200511-AMENDED-DISCRETE-00


Manual Integrations
APPROVED

Ankita
8/20/2020 1:07:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 02:40:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 02:25:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

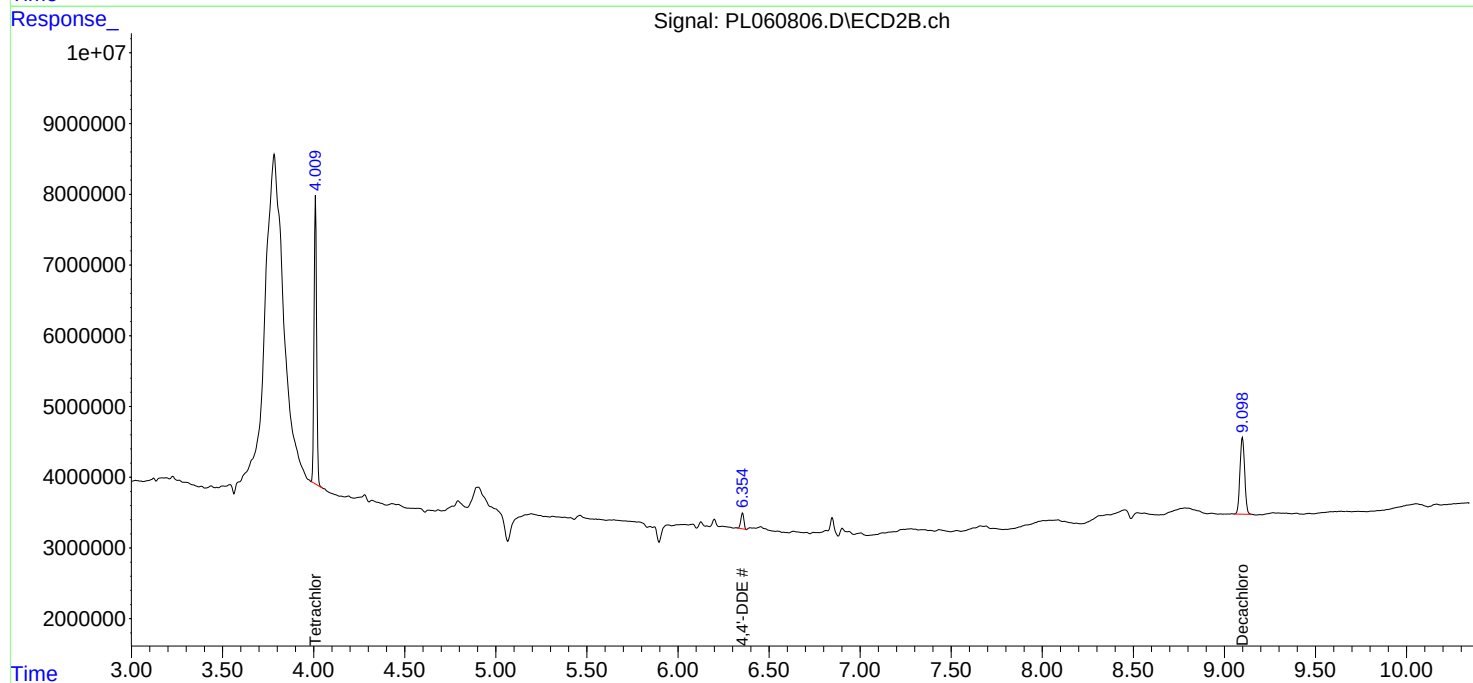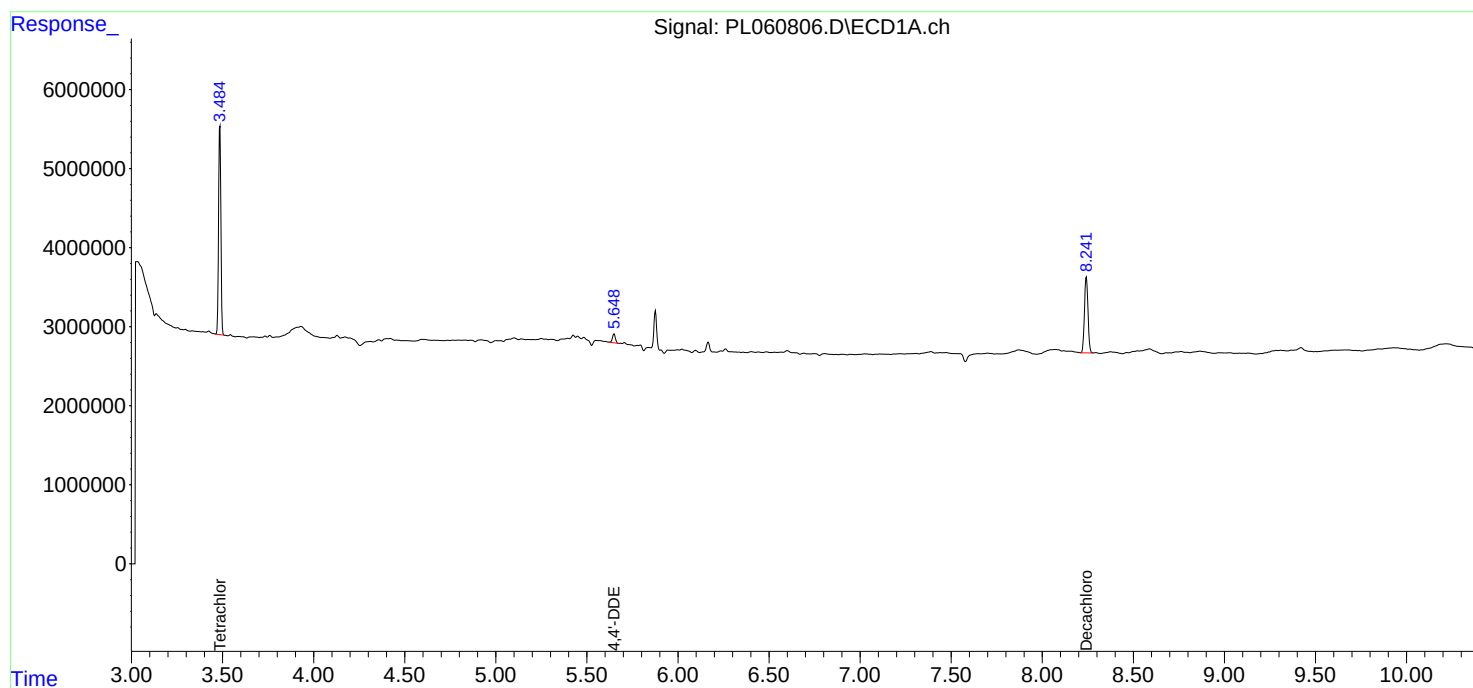

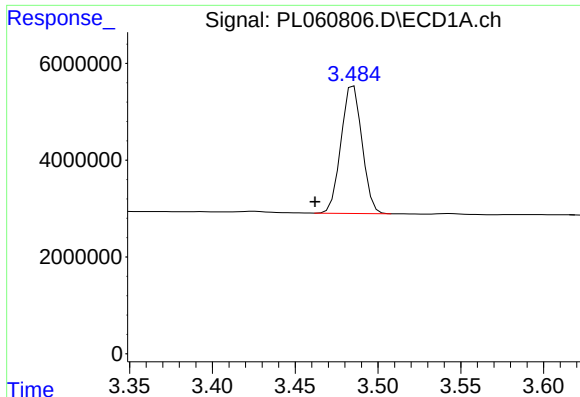


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: 0.022 min
Response: 23327896
Conc: 13.97 ng/ml m

Instrument :
ECD_L
ClientSampleId :
20200511-AMENDED-DISCRETE-00


Manual Integrations
APPROVED

Ankita
8/20/2020 1:07:29 PM

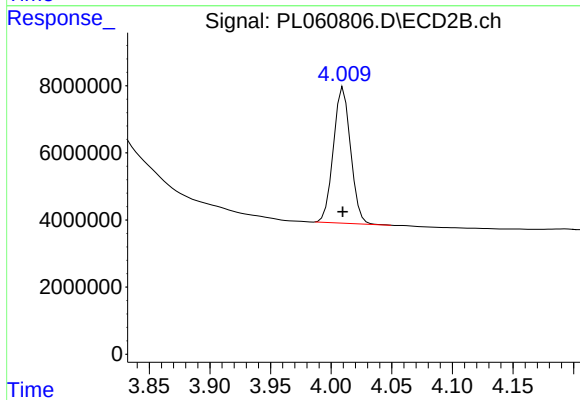


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 39850247
Conc: 14.33 ng/ml

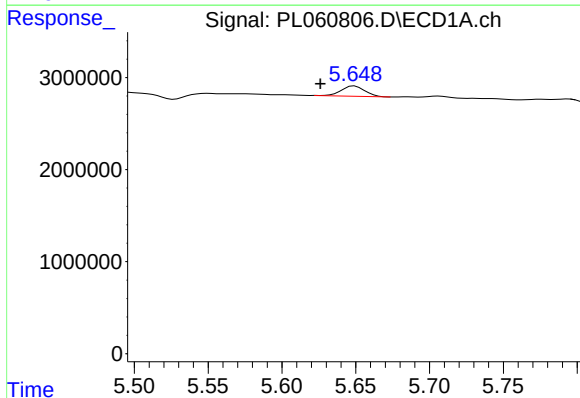


#12 4,4'-DDE

R.T.: 5.648 min
Delta R.T.: 0.022 min
Response: 1258734
Conc: 0.82 ng/ml m

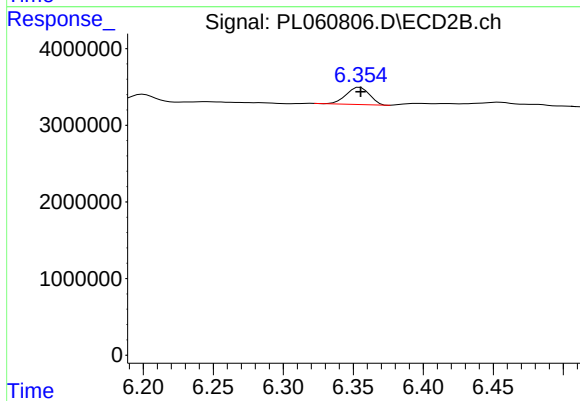

#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 2602920
Conc: 0.86 ng/ml

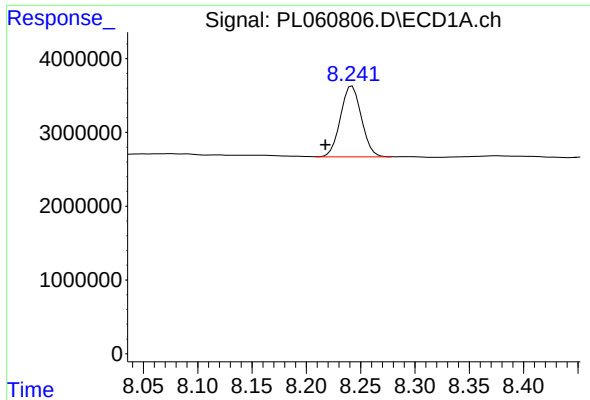


#28 Decachlorobiphenyl

R.T.: 8.241 min
Delta R.T.: 0.023 min
Response: 12872617
Conc: 9.01 ng/ml m

Instrument :
ECD_L
ClientSampleId :
20200511-AMENDED-DISCRETE-00

Manual Integrations
APPROVED

Ankita
8/20/2020 1:07:29 PM

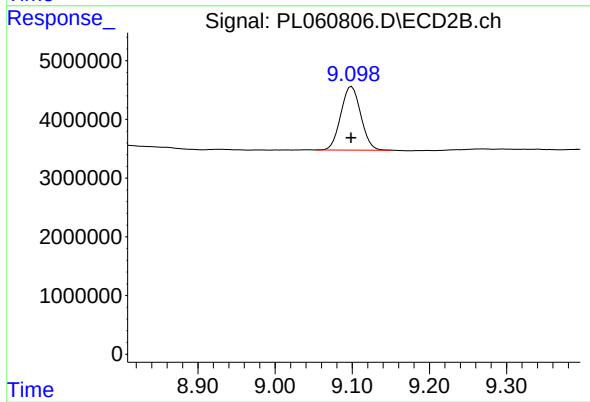

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.000 min
Response: 19374361
Conc: 9.59 ng/ml