

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
 Data File : PL069188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 16:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:52:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.569	8296193	24049032	20.057	23.686
28)	SA Decachlor...	10.405	11.492	11699564	21664327	20.358	22.329
Target Compounds							
8)	B Heptachlo...	0.000	8.037	0	276935	N.D.	0.240 #
10)	B gamma-Chl...	0.000	8.312	0	19071	N.D.	0.017 #
11)	B alpha-Chl...	0.000	8.409f	0	45747	N.D.	0.040 #
14)	MA Endrin	8.079f	0.000	541155	0	1.123	N.D. #
15)	B Endosulfa...	0.000	9.216	0	245793	N.D.	0.268 #
17)	MA 4,4'-DDT	0.000	9.440	0	113880	N.D.	0.120 #
22)	Mirex	0.000	10.560f	0	83501	N.D.	0.106 #
25)	Chlordane-3	0.000	8.312	0	19071	N.D.	0.117 #
26)	Chlordane-4	0.000	8.409f	0	45747	N.D.	0.231 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
Data File : PL069188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 16:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:52:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

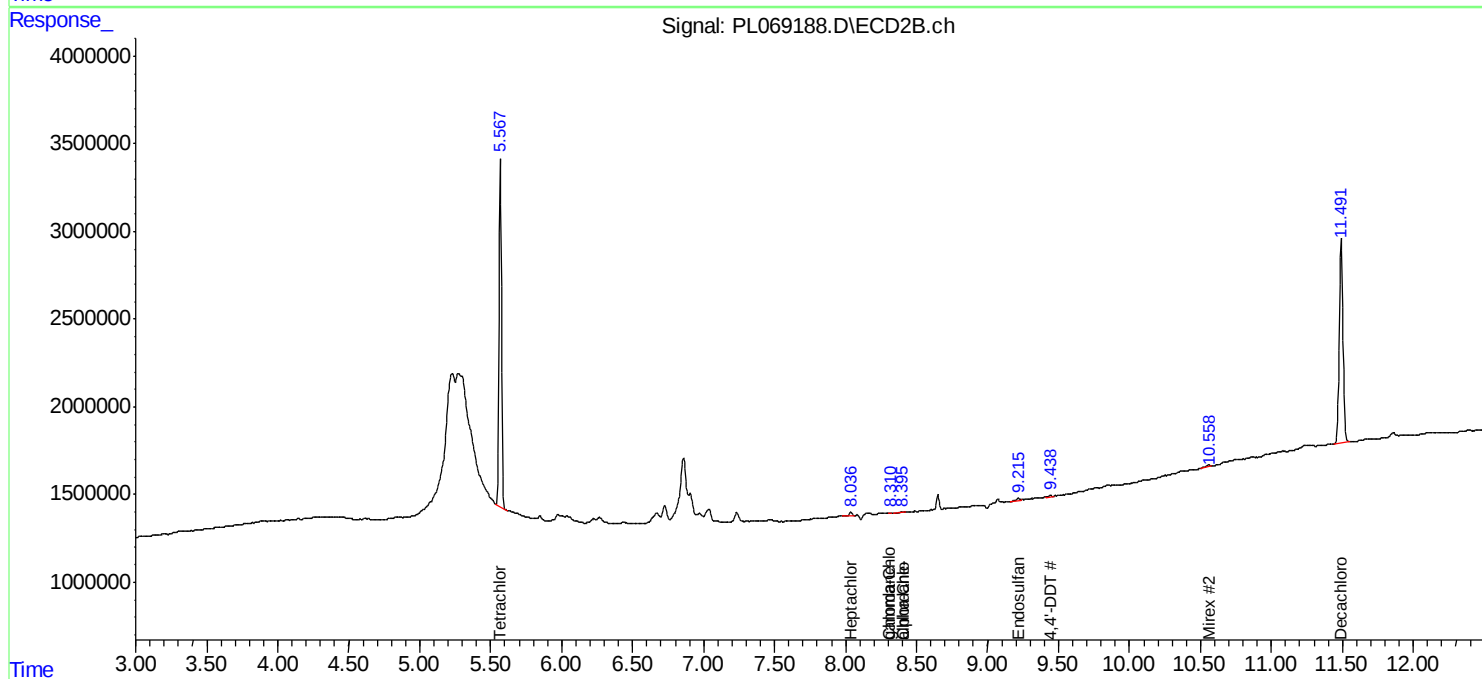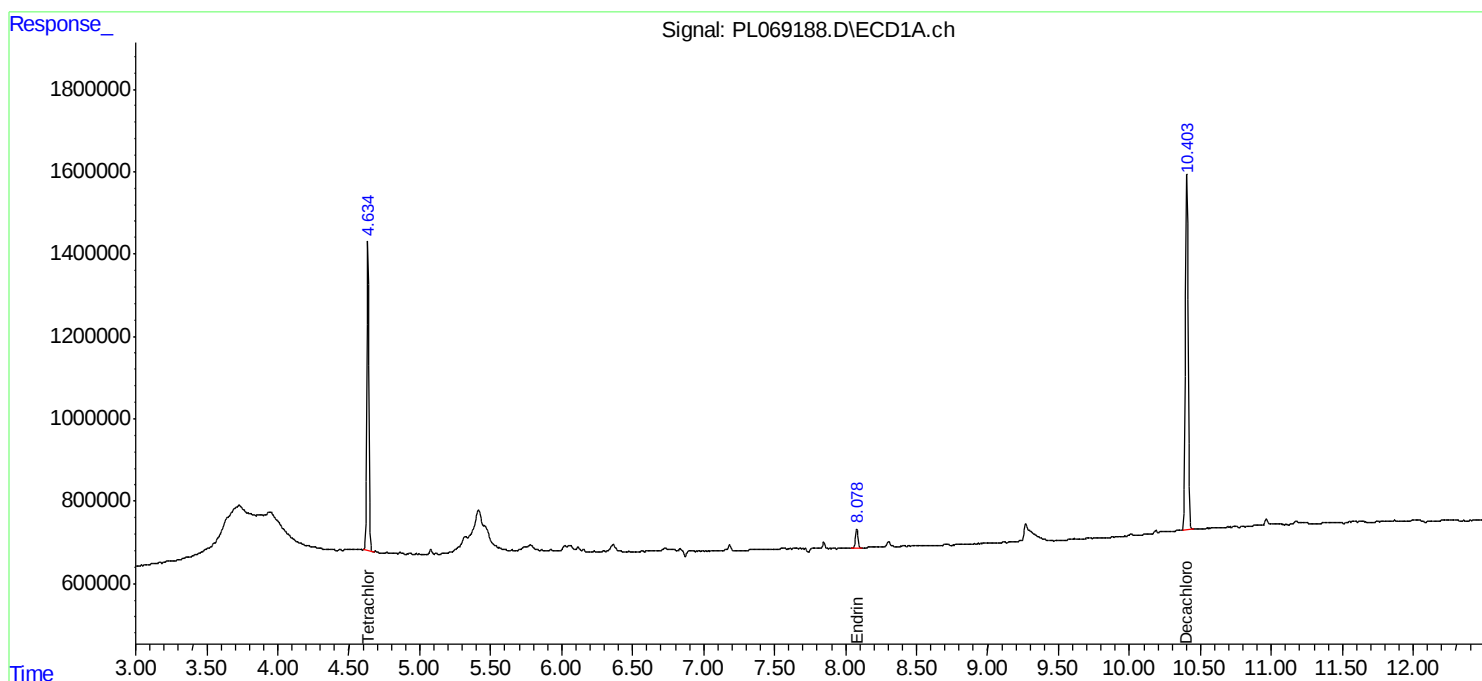


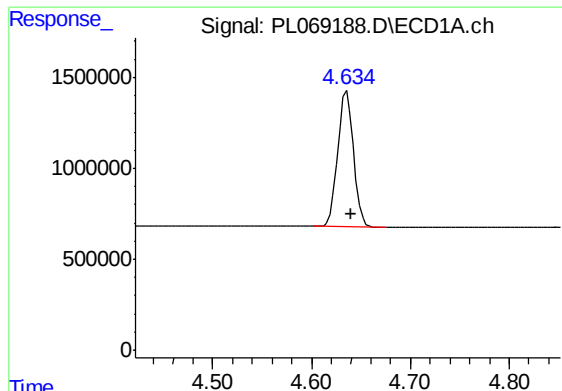

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8296193
Conc: 20.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

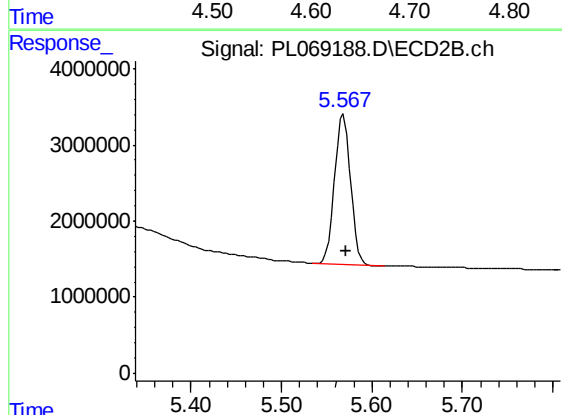


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 24049032
Conc: 23.69 ng/ml

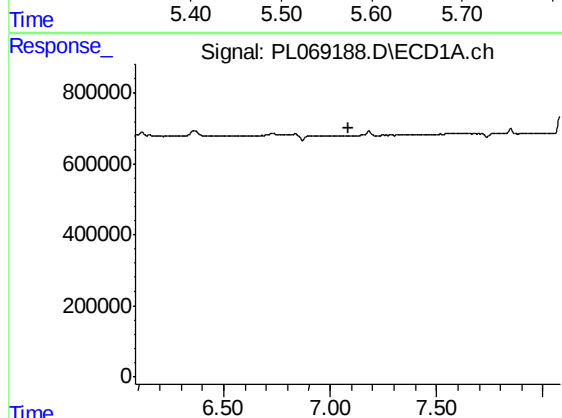


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

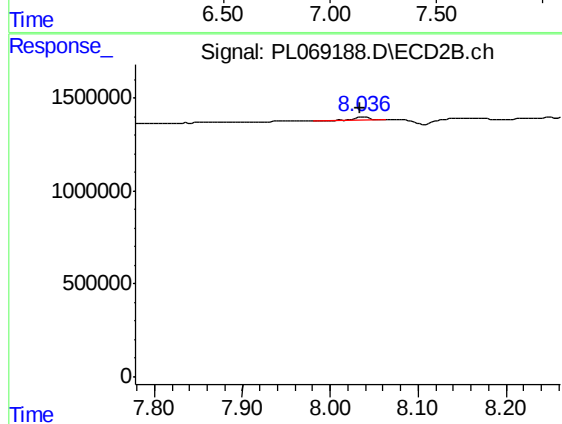

#8 Heptachlor epoxide


R.T.: 8.037 min
Delta R.T.: 0.003 min
Response: 276935
Conc: 0.24 ng/ml

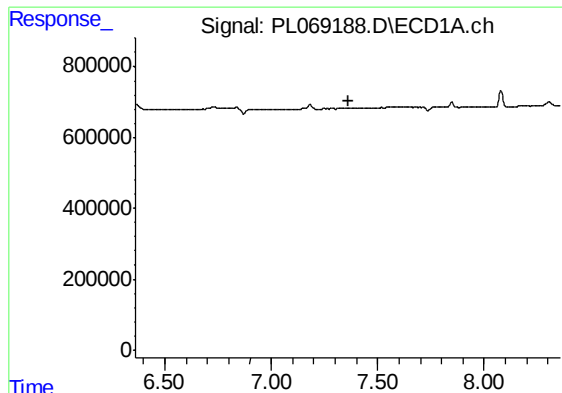

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

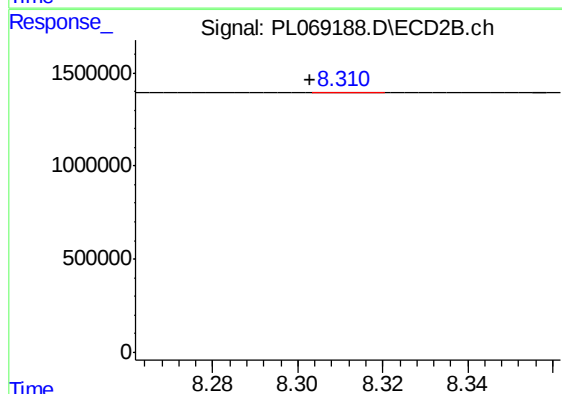


#10 gamma-Chlordane

R.T.: 8.312 min
Delta R.T.: 0.009 min
Response: 19071
Conc: 0.02 ng/ml

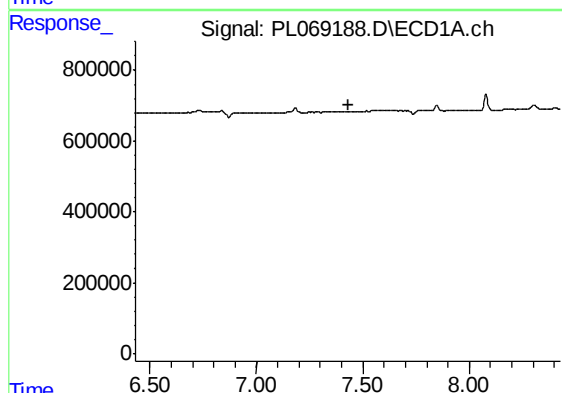


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

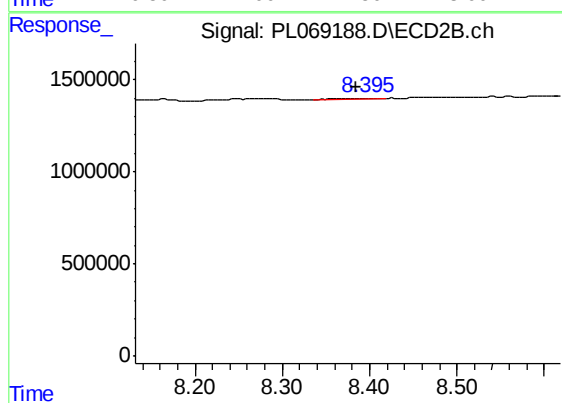

#11 alpha-Chlordane


R.T.: 8.409 min
Delta R.T.: 0.025 min
Response: 45747
Conc: 0.04 ng/ml

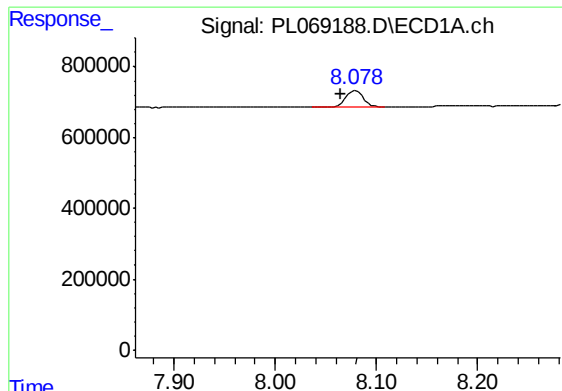

#14 Endrin


R.T.: 8.079 min
Delta R.T.: 0.015 min
Response: 541155
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

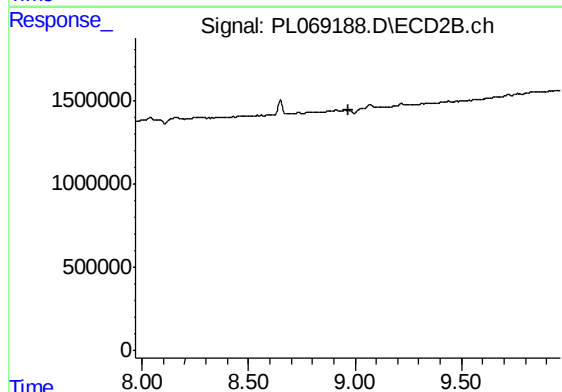


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

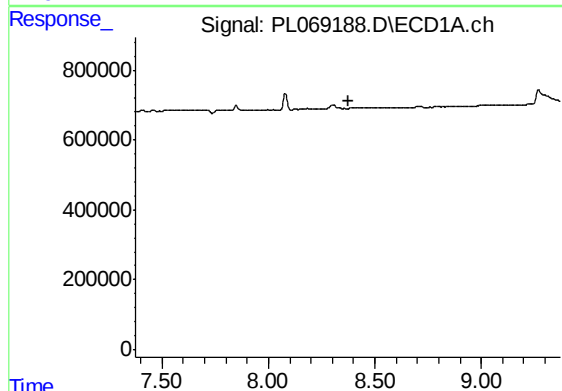


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

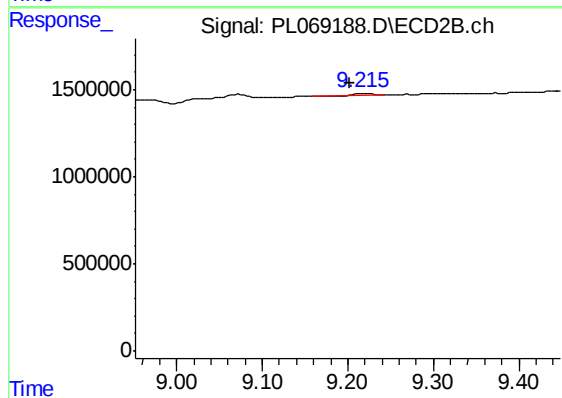

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.015 min
Response: 245793
Conc: 0.27 ng/ml

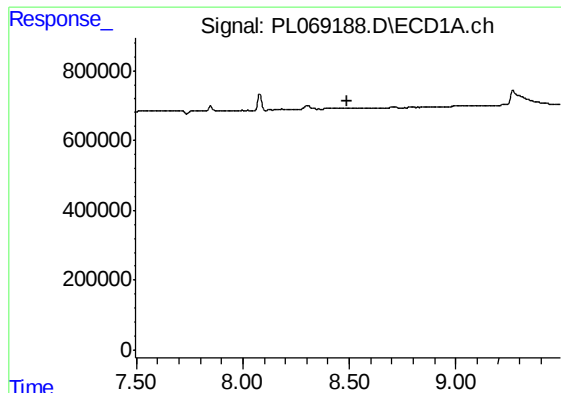

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

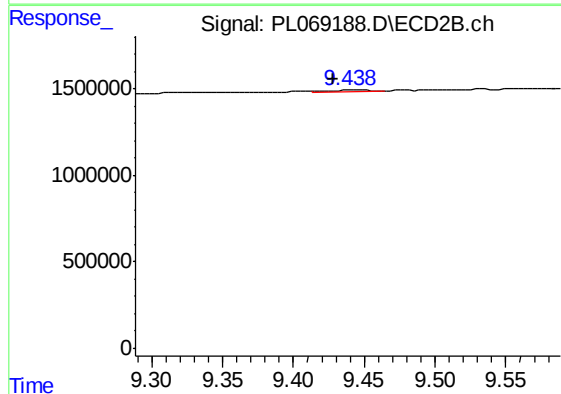


#17 4,4'-DDT

R.T.: 9.440 min
Delta R.T.: 0.011 min
Response: 113880
Conc: 0.12 ng/ml

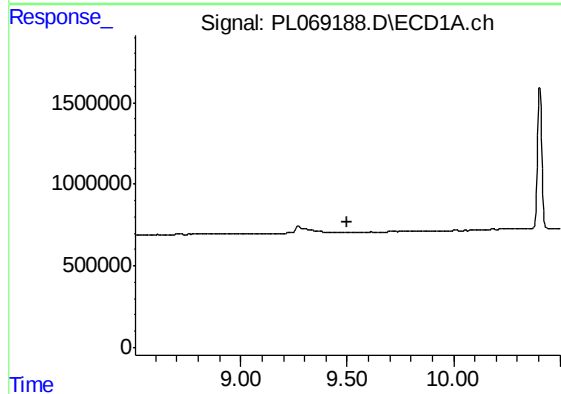


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

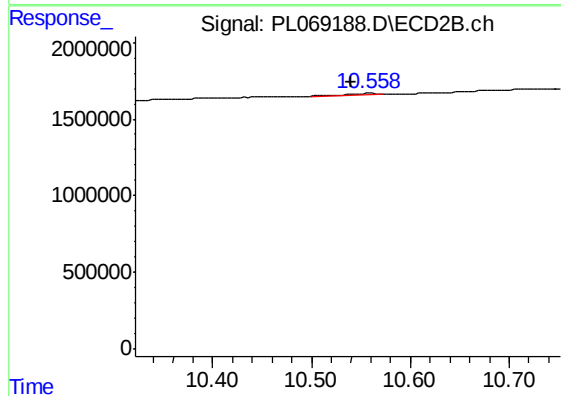

#22 Mirex


R.T.: 10.560 min
Delta R.T.: 0.020 min
Response: 83501
Conc: 0.11 ng/ml

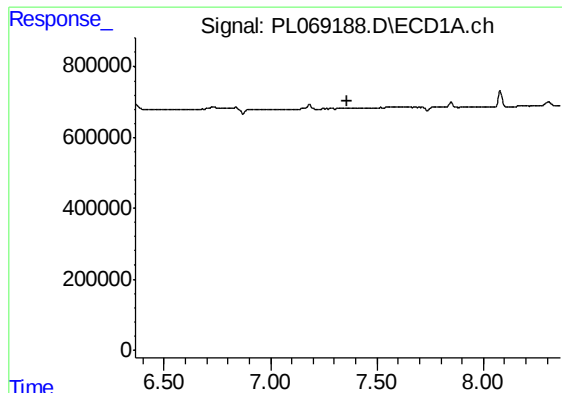

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

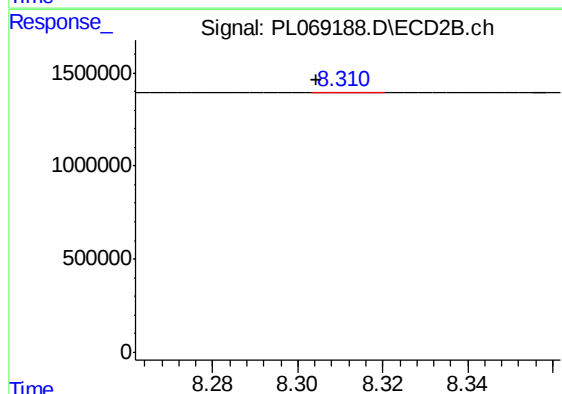


#25 Chlordane-3

R.T.: 8.312 min
Delta R.T.: 0.007 min
Response: 19071
Conc: 0.12 ng/ml

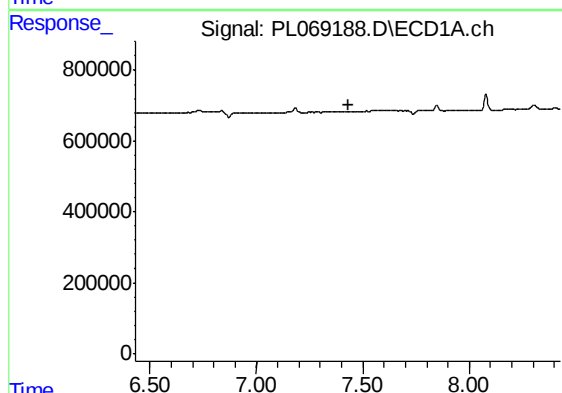


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

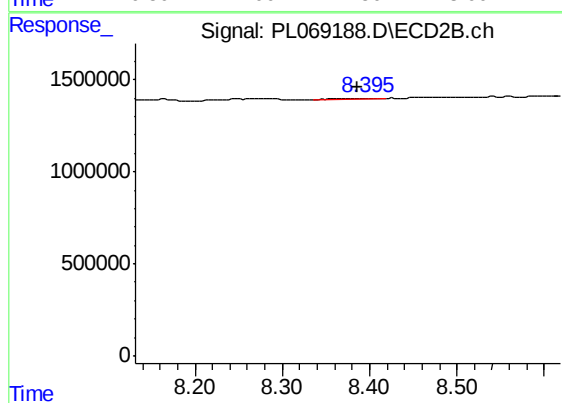

#26 Chlordane-4


R.T.: 8.409 min
Delta R.T.: 0.022 min
Response: 45747
Conc: 0.23 ng/ml

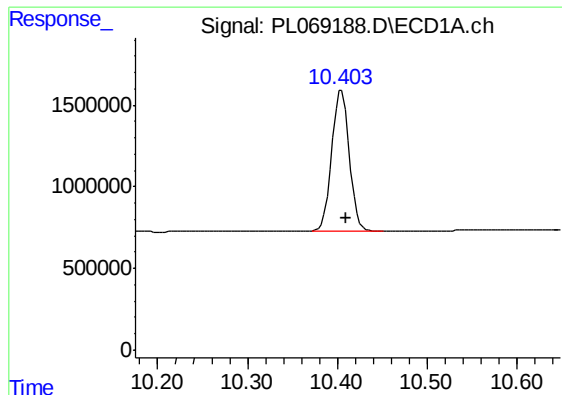

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.005 min
Response: 11699564
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

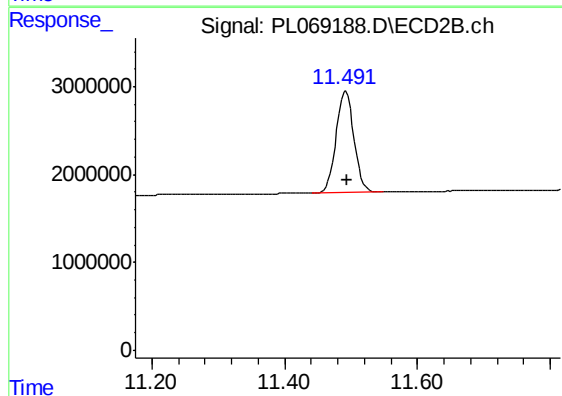

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: -0.003 min
Response: 21664327
Conc: 22.33 ng/ml