

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
 Data File : PL069198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2021 20:57
 Operator : AR\AJ
 Sample : M3435-35
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2021-08-12-EB-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 01:56:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.566	8212487	24953267	19.854	24.576
28)	SA Decachlor...	10.400	11.484	8244637	15477860	14.346	15.953
Target Compounds							
9)	A Endosulfan I	0.000	8.420f	0	310130	N.D.	0.294 #
10)	B gamma-Chl...	0.000	8.291	0	471344	N.D.	0.412 #
15)	B Endosulfa...	0.000	9.214	0	1504321	N.D.	1.640 #
22)	Mirex	0.000	10.563f	0	202548	N.D.	0.256 #
23)	Chlordane-1	0.000	6.975f	0	267522	N.D.	6.344 #
25)	Chlordane-3	0.000	8.291	0	471344	N.D.	2.885 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
Data File : PL069198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2021 20:57
Operator : AR\AJ
Sample : M3435-35
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2021-08-12-EB-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 01:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

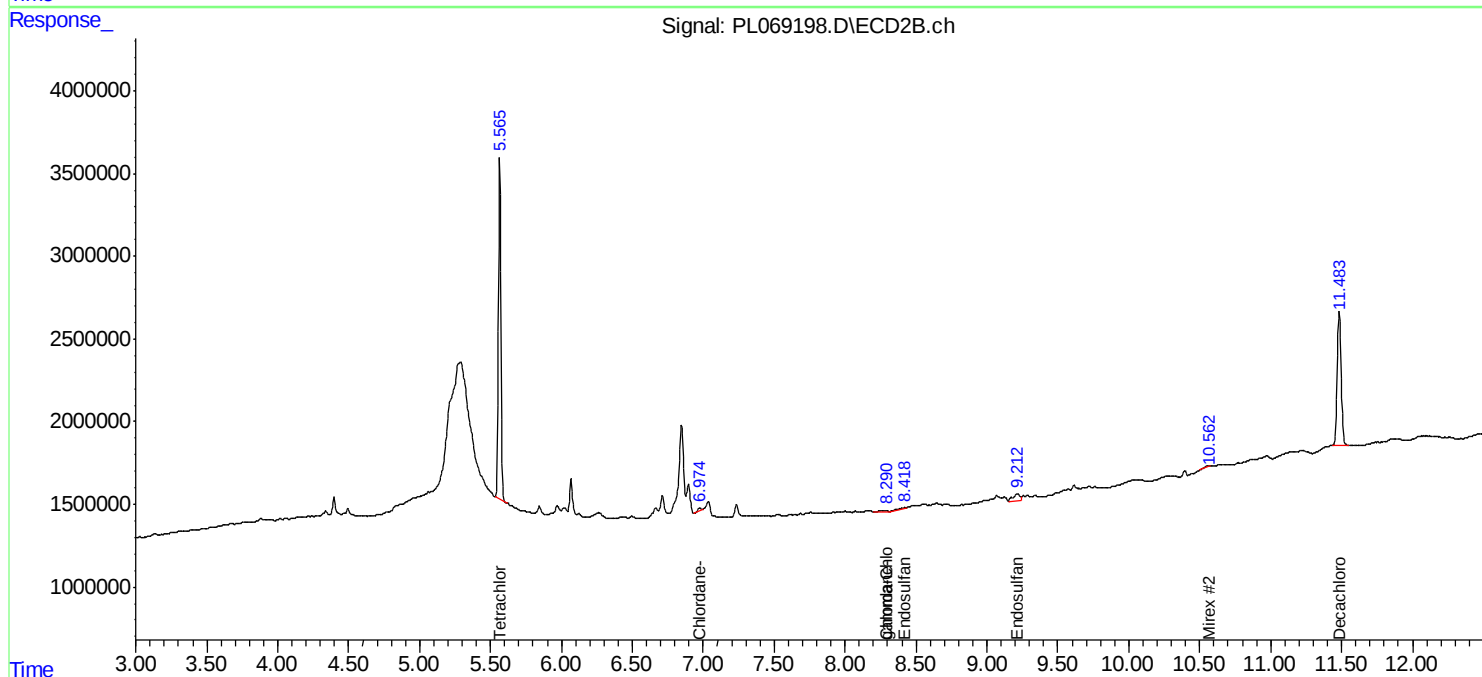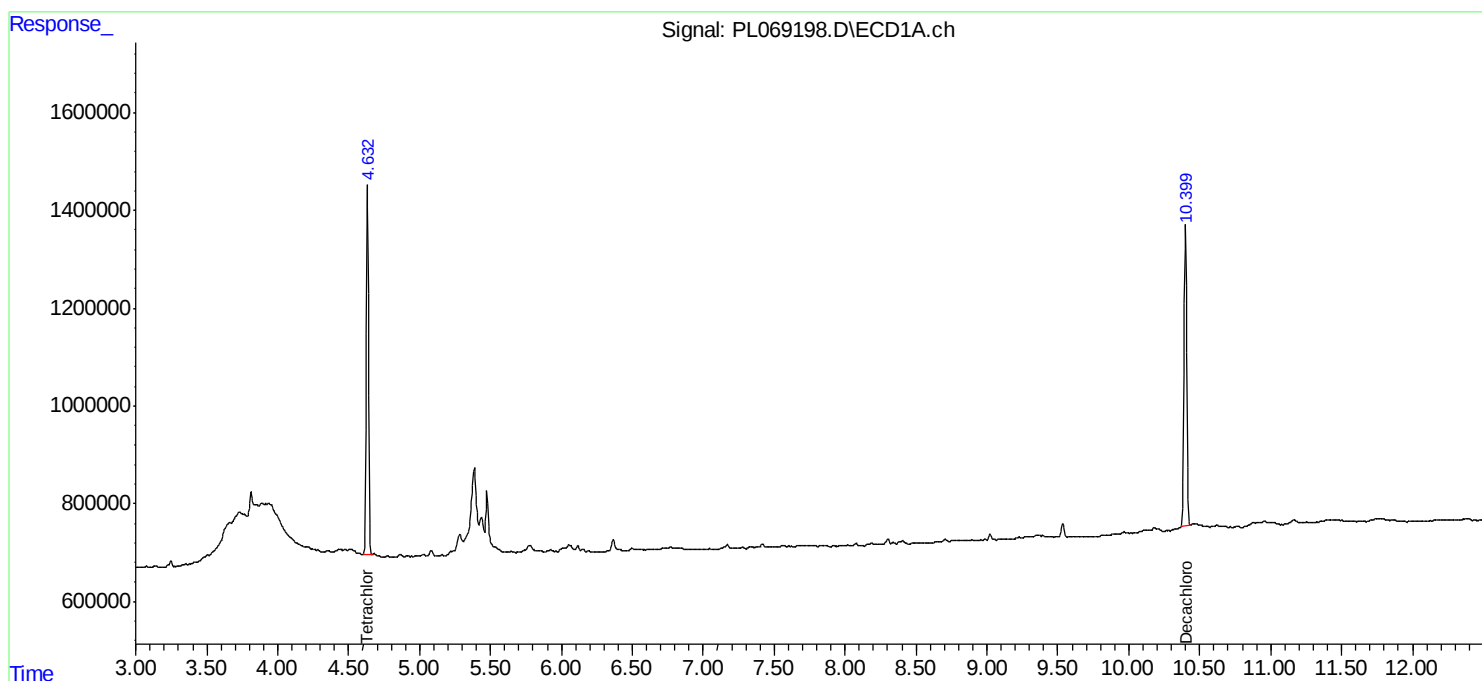


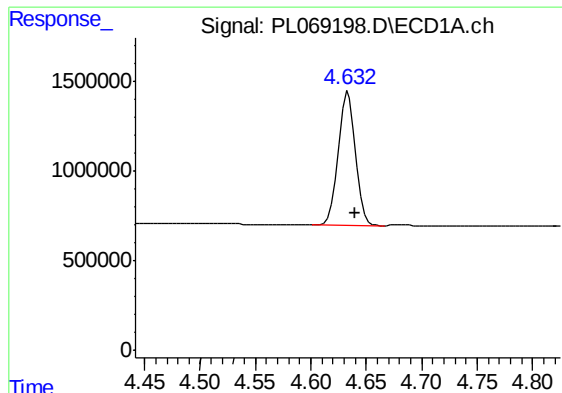

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 8212487
Conc: 19.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
2021-08-12-EB-03

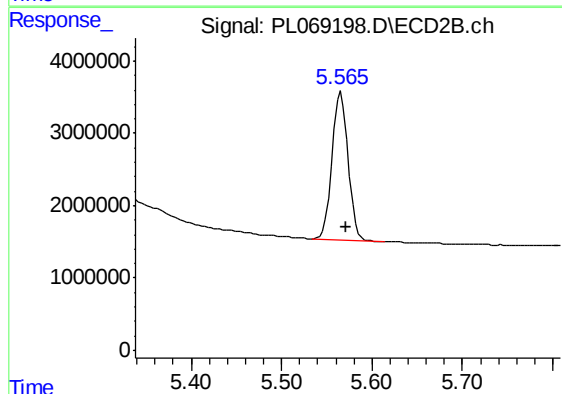


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 24953267
Conc: 24.58 ng/ml

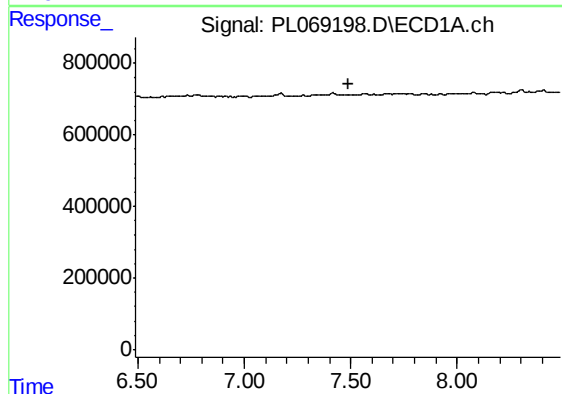


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

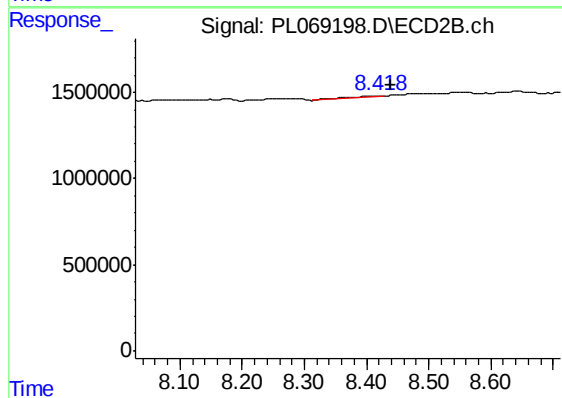

#9 Endosulfan I


R.T.: 8.420 min
Delta R.T.: -0.020 min
Response: 310130
Conc: 0.29 ng/ml

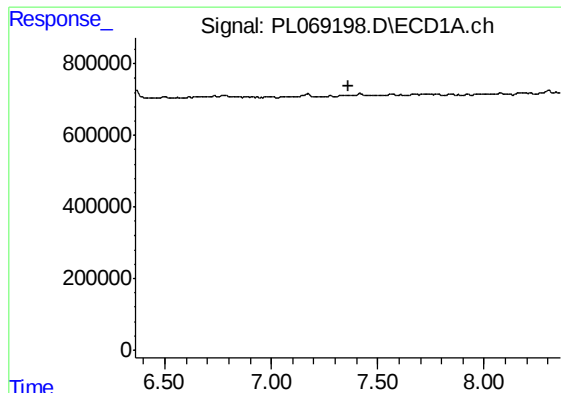

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2021-08-12-EB-03

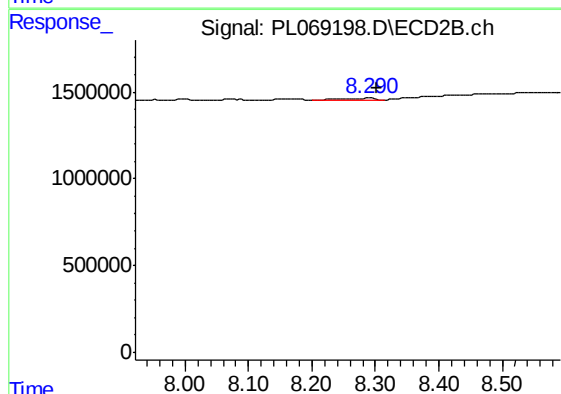


#10 gamma-Chlordane

R.T.: 8.291 min
Delta R.T.: -0.012 min
Response: 471344
Conc: 0.41 ng/ml

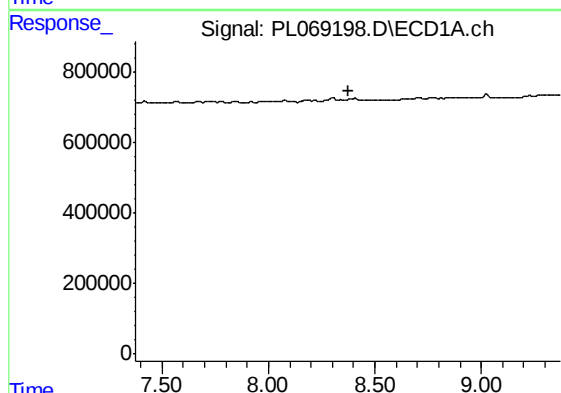


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

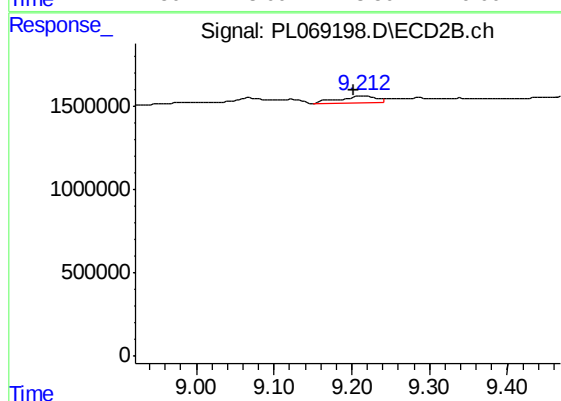

#15 Endosulfan II


R.T.: 9.214 min
Delta R.T.: 0.012 min
Response: 1504321
Conc: 1.64 ng/ml

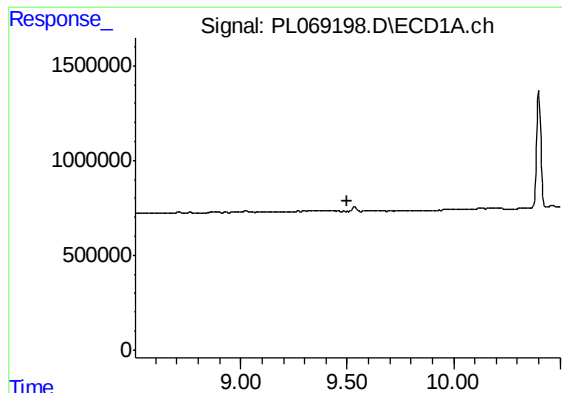

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2021-08-12-EB-03

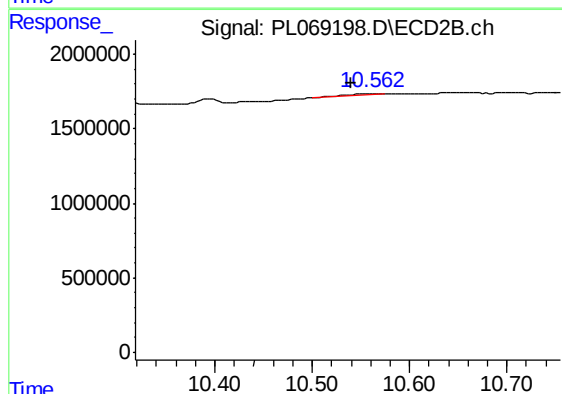


#22 Mirex

R.T.: 10.563 min
Delta R.T.: 0.023 min
Response: 202548
Conc: 0.26 ng/ml

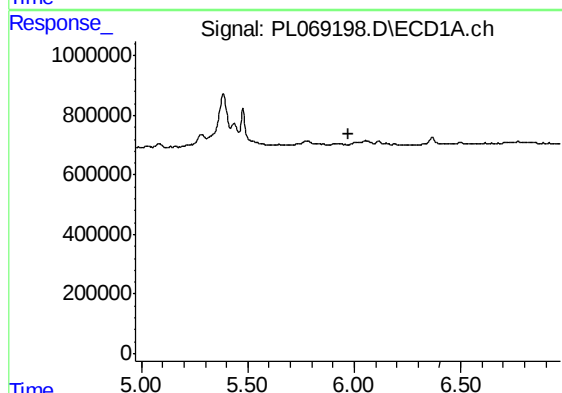


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

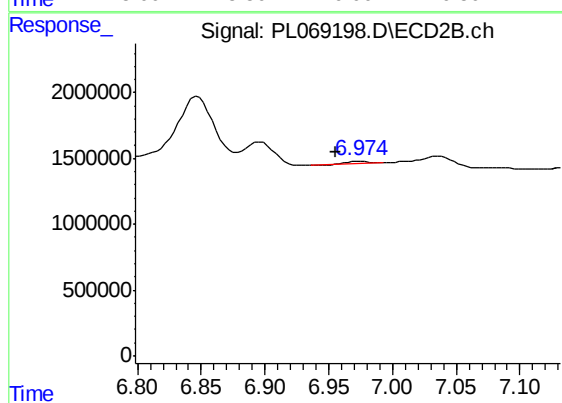

#23 Chlordane-1


R.T.: 6.975 min
Delta R.T.: 0.020 min
Response: 267522
Conc: 6.34 ng/ml

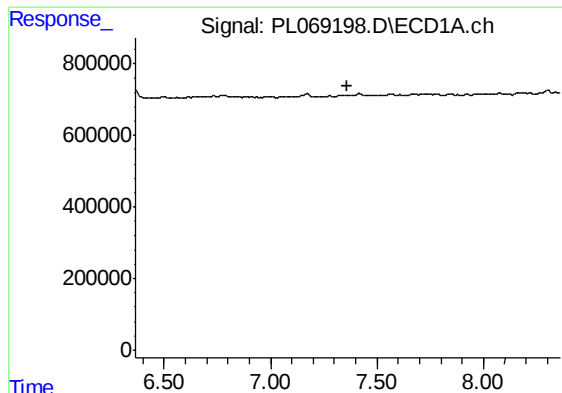

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2021-08-12-EB-03

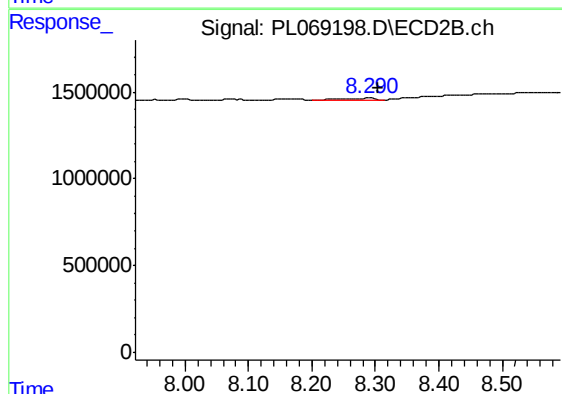


#25 Chlordane-3

R.T.: 8.291 min
Delta R.T.: -0.013 min
Response: 471344
Conc: 2.89 ng/ml

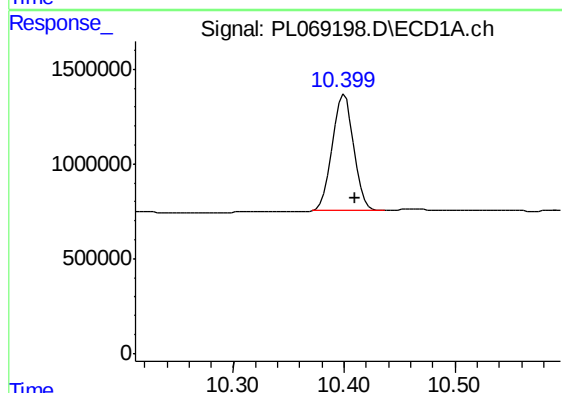

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.010 min
Response: 8244637
Conc: 14.35 ng/ml

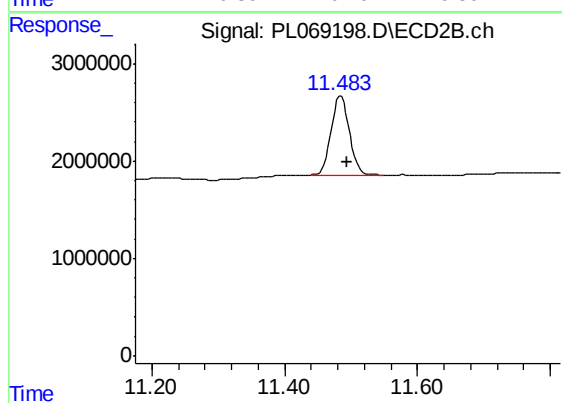

#28 Decachlorobiphenyl

R.T.: 11.484 min
Delta R.T.: -0.010 min
Response: 15477860
Conc: 15.95 ng/ml