

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
 Data File : PL069214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 03:17
 Operator : AR\AJ
 Sample : PB138506BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138506BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 04:58:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.634	5.566	9024903	27533416	21.818	27.118
28)	SA Decachlor...	10.401	11.487	12573796	23117220	21.879	23.826
Target Compounds							
8)	B Heptachlo...	0.000	8.033	0	174470	N.D.	0.151 #
9)	A Endosulfan I	0.000	8.444	0	24762	N.D.	0.023 #
10)	B gamma-Chl...	0.000	8.300	0	200969	N.D.	0.175 #
11)	B alpha-Chl...	0.000	8.390	0	106912	N.D.	0.093 #
14)	MA Endrin	8.076	0.000	722397	0	1.499	N.D. #
15)	B Endosulfa...	0.000	9.214	0	320502	N.D.	0.349 #
22)	Mirex	0.000	10.567f	0	240091	N.D.	0.304 #
23)	Chlordane-1	0.000	6.975f	0	129790	N.D.	3.078 #
25)	Chlordane-3	0.000	8.300	0	200969	N.D.	1.230 #
26)	Chlordane-4	0.000	8.390	0	106912	N.D.	0.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081821\
Data File : PL069214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 03:17
Operator : AR\AJ
Sample : PB138506BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB138506BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 04:58:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

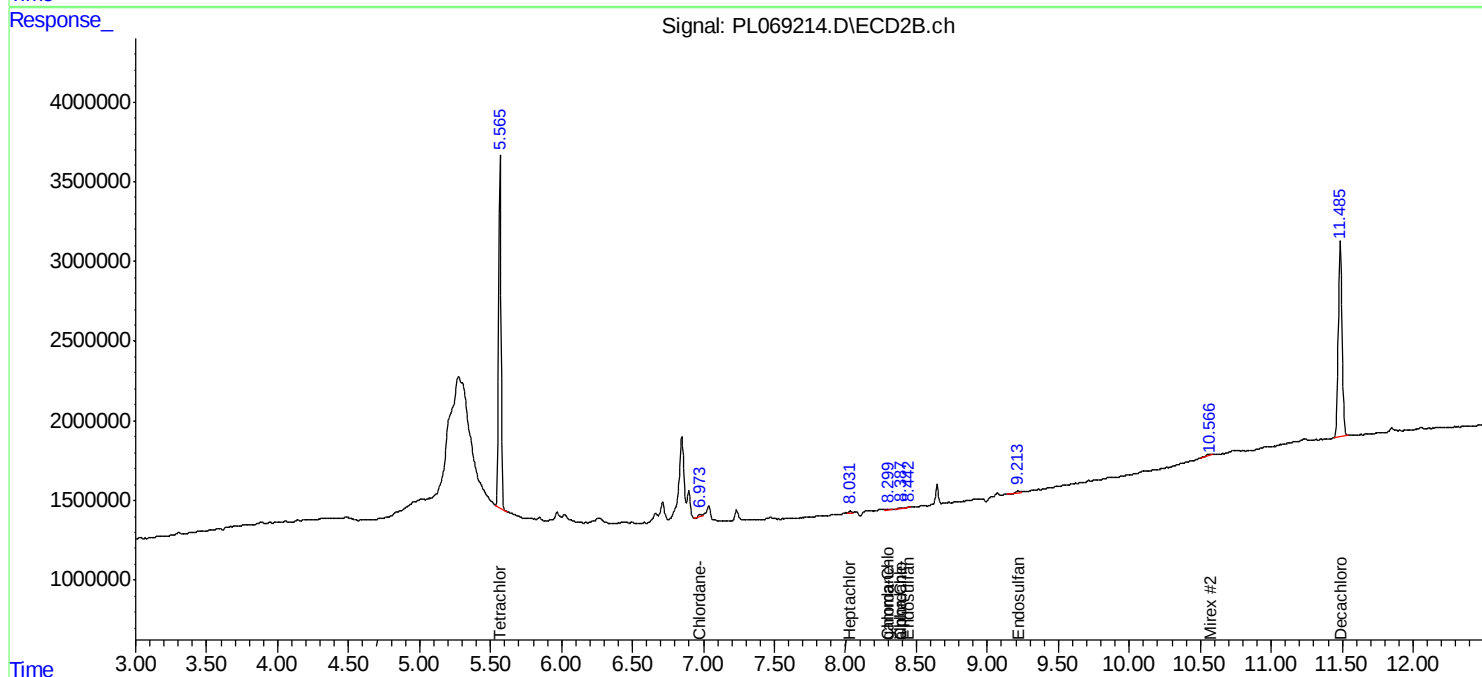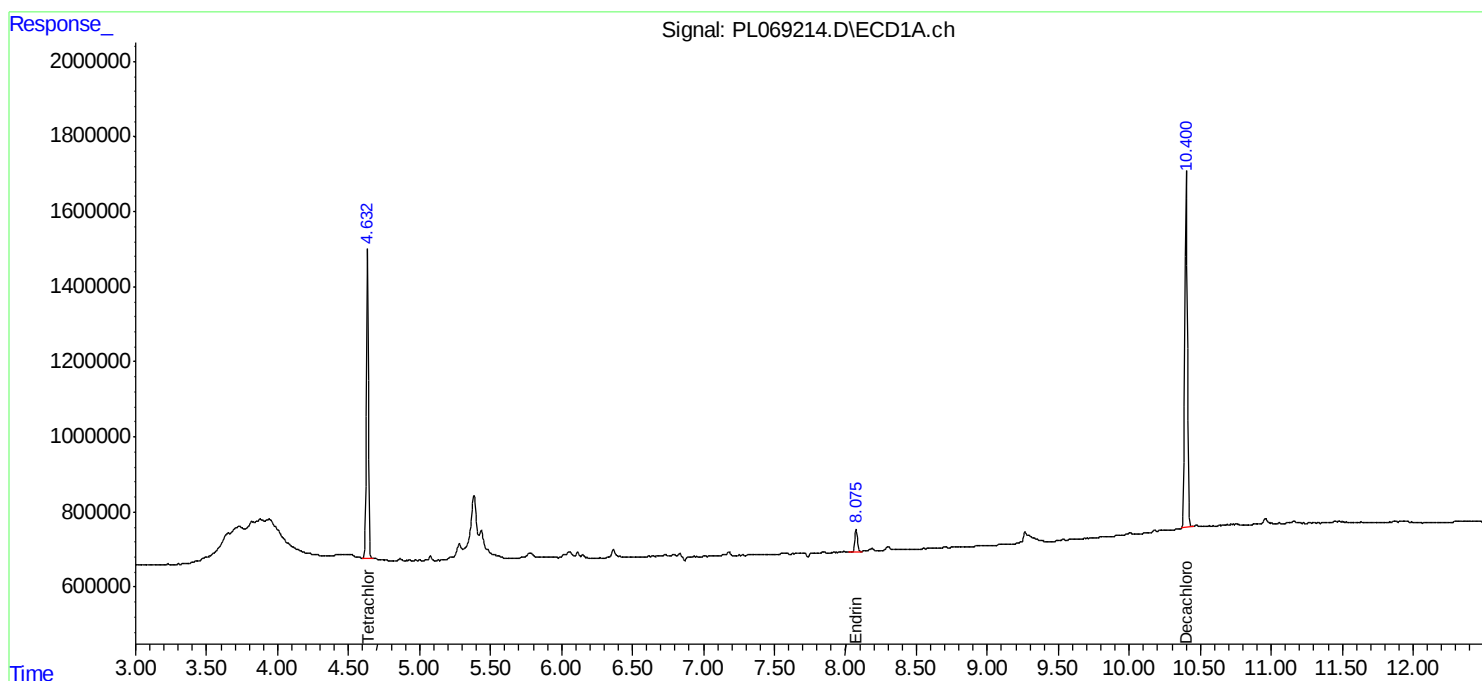


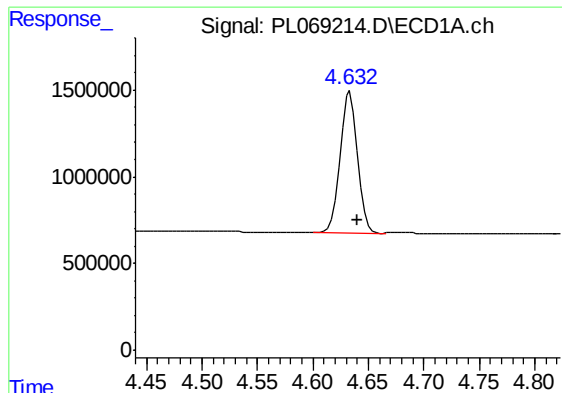

#1 Tetrachloro-m-xylene


R.T.: 4.634 min
Delta R.T.: -0.006 min
Response: 9024903
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138506BL

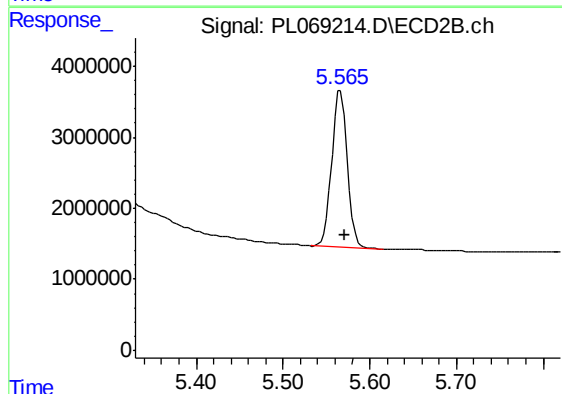


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 27533416
Conc: 27.12 ng/ml

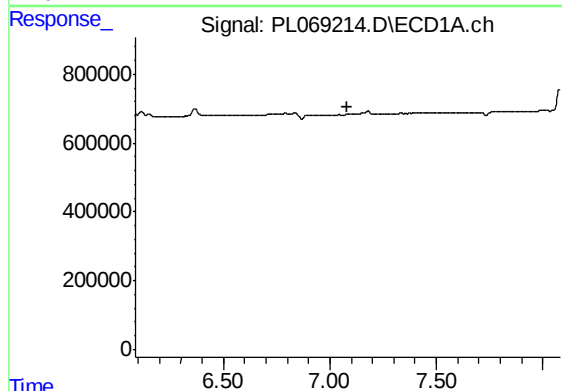


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

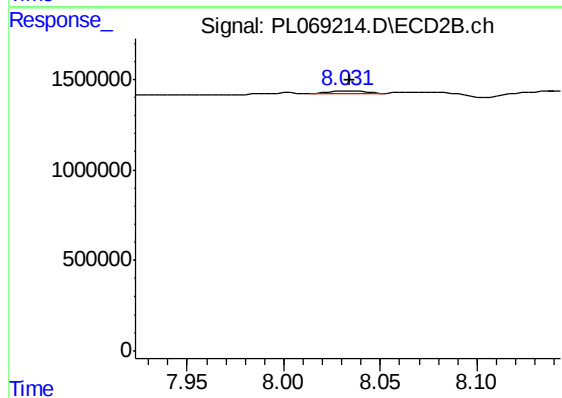

#8 Heptachlor epoxide


R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 174470
Conc: 0.15 ng/ml

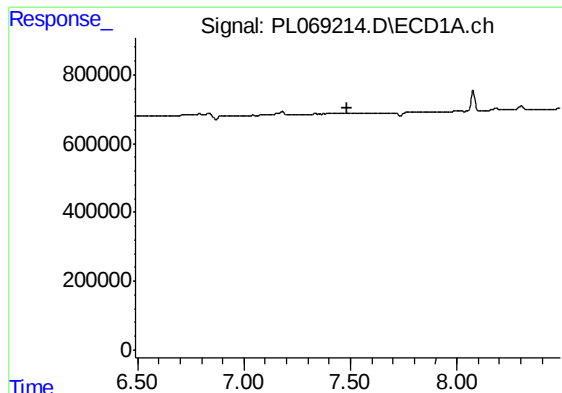

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138506BL

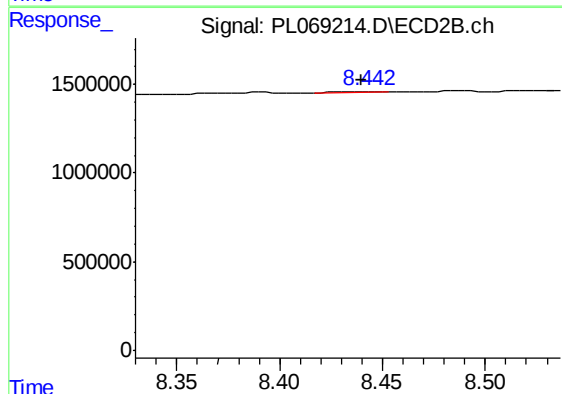


#9 Endosulfan I

R.T.: 8.444 min
Delta R.T.: 0.004 min
Response: 24762
Conc: 0.02 ng/ml

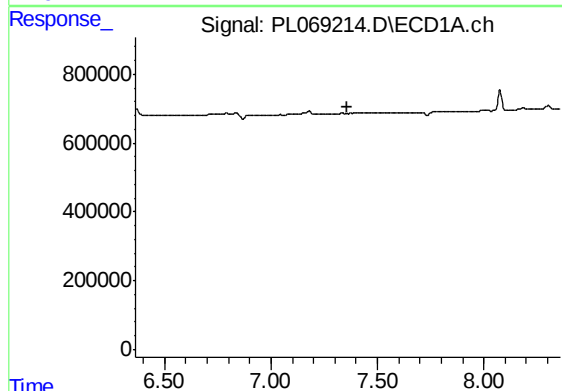


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

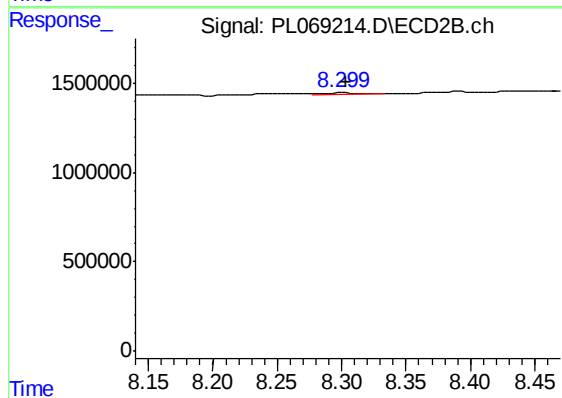

#10 gamma-Chlordane


R.T.: 8.300 min
Delta R.T.: -0.002 min
Response: 200969
Conc: 0.18 ng/ml

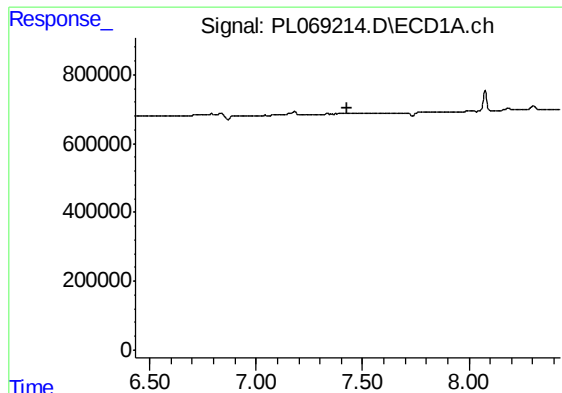

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138506BL

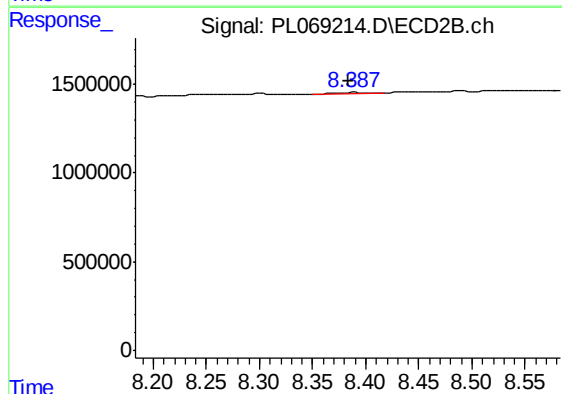


#11 alpha-Chlordane

R.T.: 8.390 min
Delta R.T.: 0.005 min
Response: 106912
Conc: 0.09 ng/ml

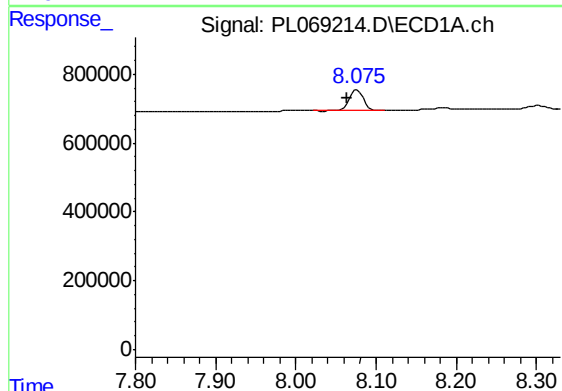


#14 Endrin

R.T.: 8.076 min
Delta R.T.: 0.012 min
Response: 722397
Conc: 1.50 ng/ml

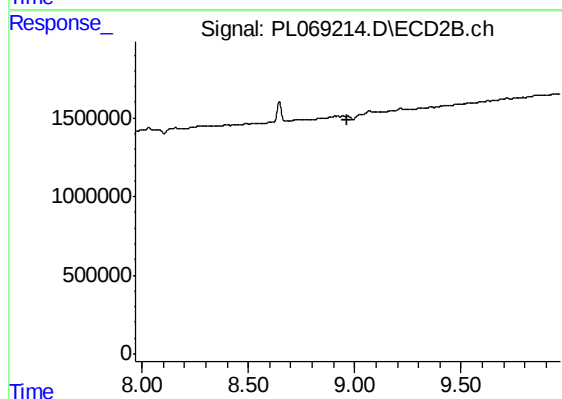

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

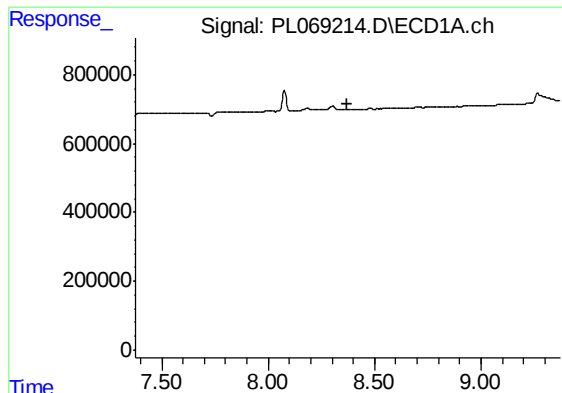

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138506BL

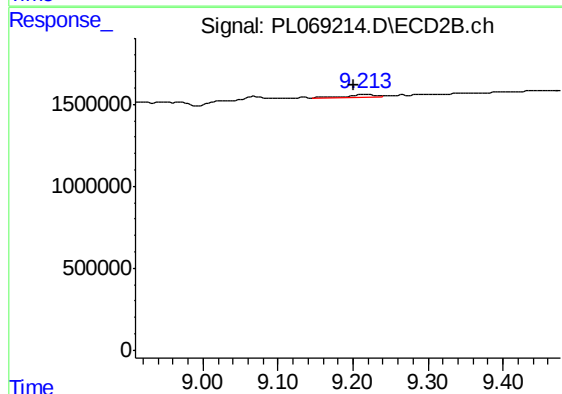


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.013 min
Response: 320502
Conc: 0.35 ng/ml

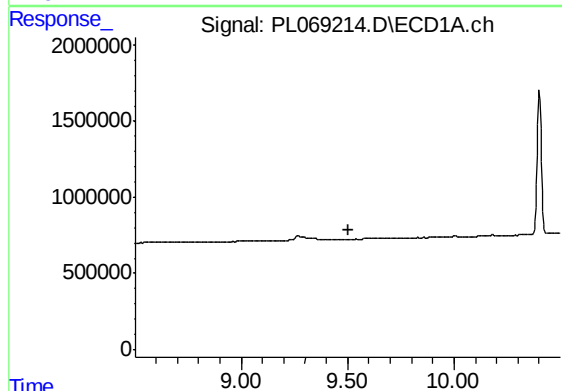


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

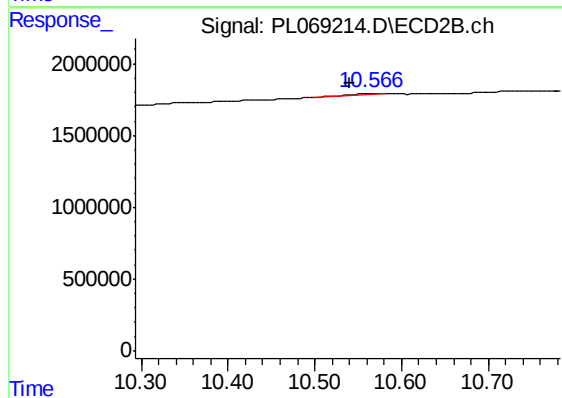

#22 Mirex


R.T.: 10.567 min
Delta R.T.: 0.027 min
Response: 240091
Conc: 0.30 ng/ml

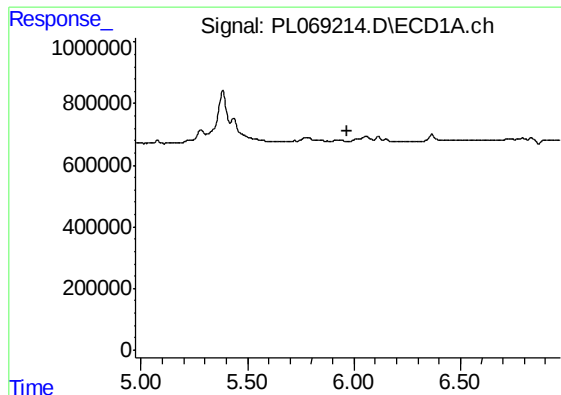

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138506BL

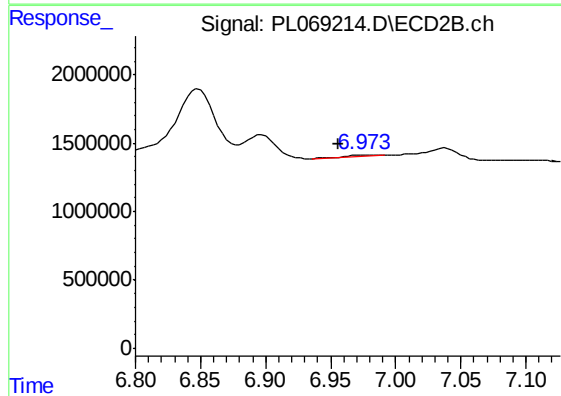


#23 Chlordane-1

R.T.: 6.975 min
Delta R.T.: 0.020 min
Response: 129790
Conc: 3.08 ng/ml

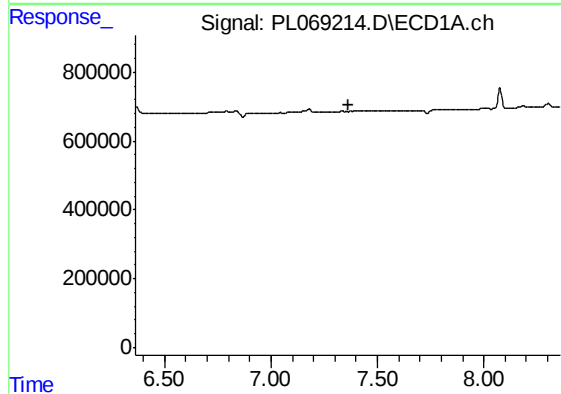


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

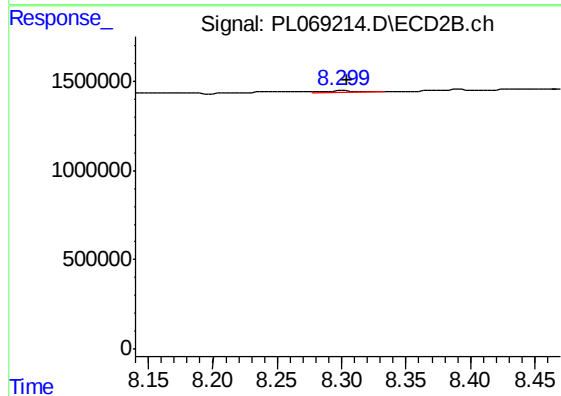

#25 Chlordane-3


R.T.: 8.300 min
Delta R.T.: -0.004 min
Response: 200969
Conc: 1.23 ng/ml

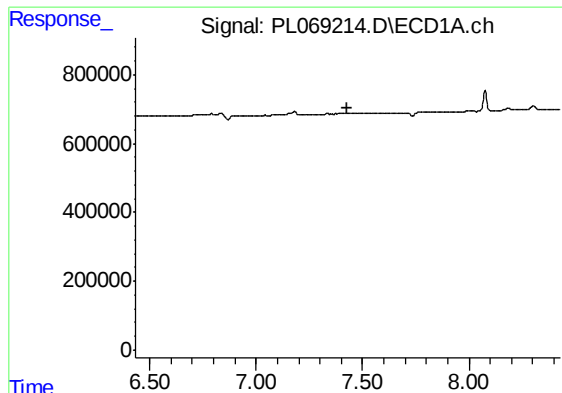

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138506BL

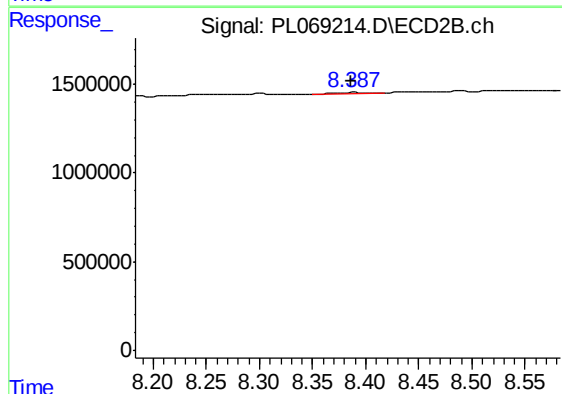


#26 Chlordane-4

R.T.: 8.390 min
Delta R.T.: 0.003 min
Response: 106912
Conc: 0.54 ng/ml

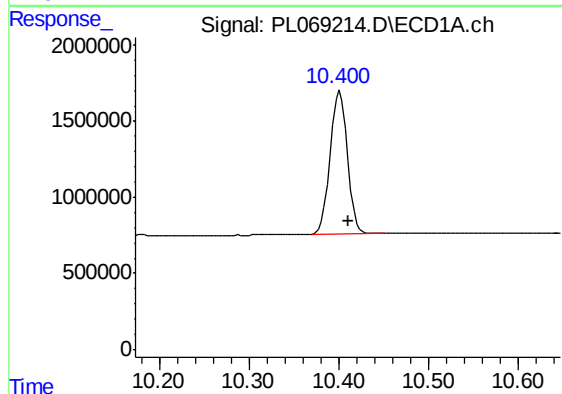

#28 Decachlorobiphenyl

R.T.: 10.401 min
Delta R.T.: -0.009 min
Response: 12573796
Conc: 21.88 ng/ml

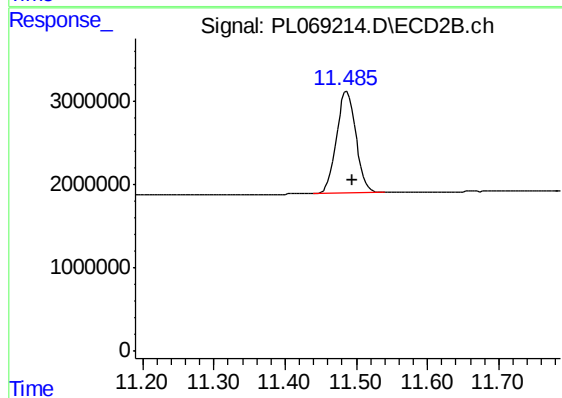

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 23117220
Conc: 23.83 ng/ml