

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081823\
 Data File : PL084839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2023 15:16
 Operator : AR\AJ
 Sample : 04047-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NEVINS-SB05-Z60-61-Q

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/18/2023
 Supervised By :Ankita Jodhani 08/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 21:45:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 16:21:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.685	18264959	8129357	7.861m	7.476
28) SA Decachlor...	9.026	7.865	15202553	10808365	9.343m	8.669

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081823\
Data File : PL084839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2023 15:16
Operator : AR\AJ
Sample : 04047-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NEVINS-SB05-Z60-61-Q


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/18/2023
Supervised By :Ankita Jodhani 08/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 21:45:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 16:21:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

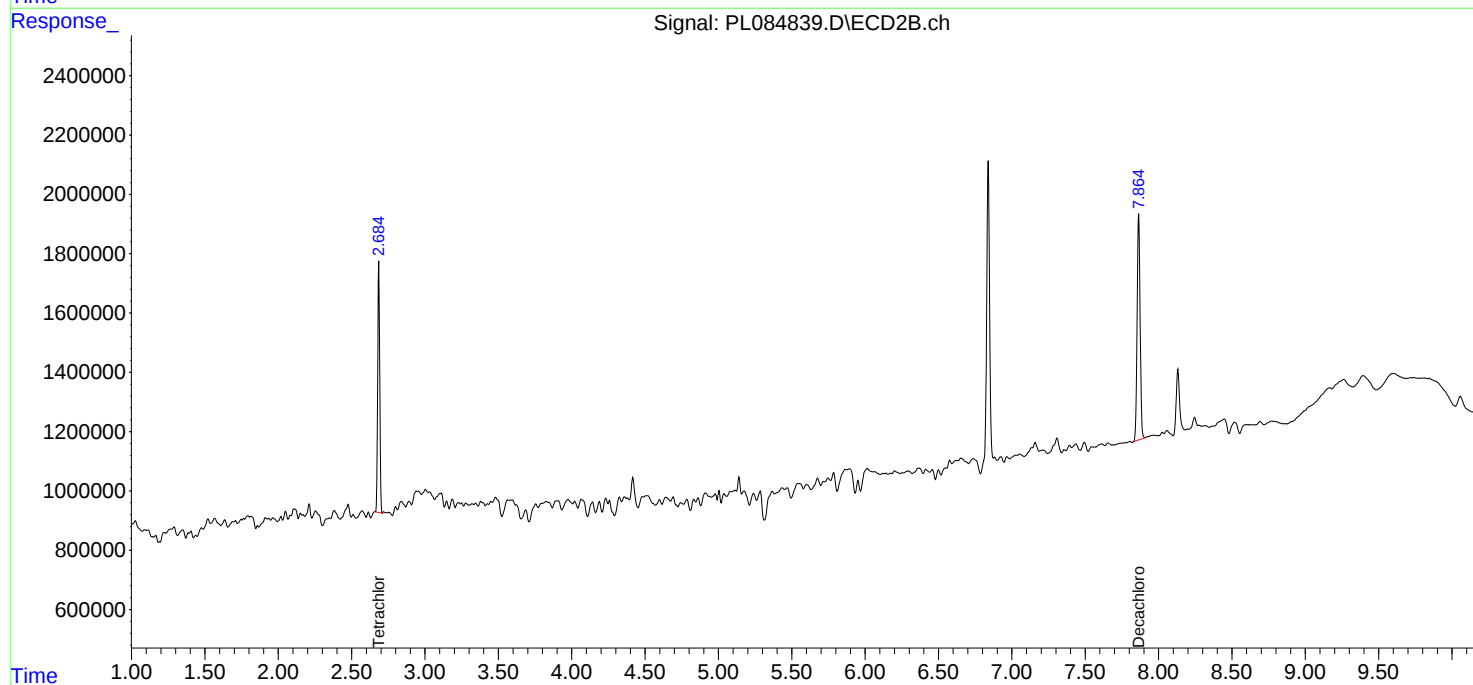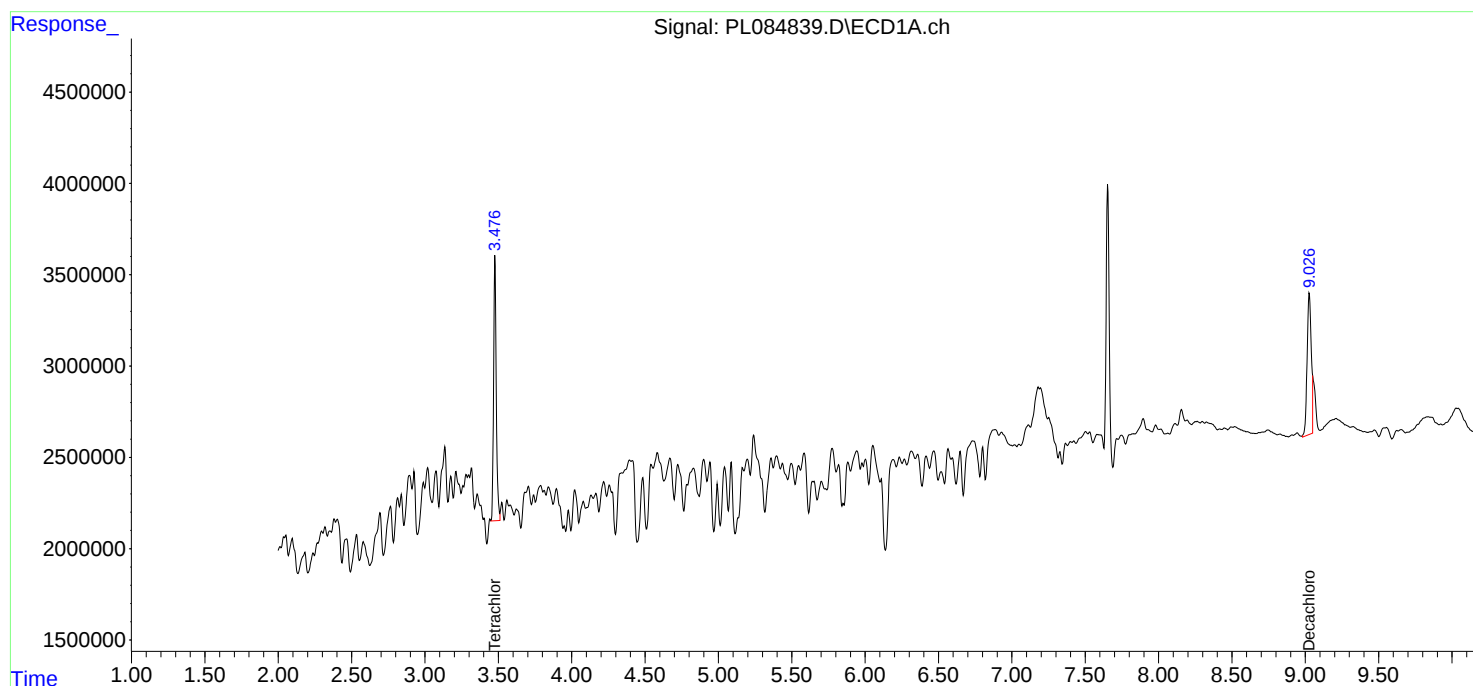

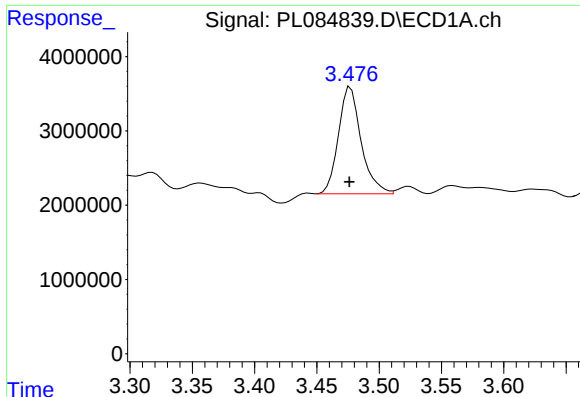


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.000 min
Response: 18264959
Conc: 7.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
NEVINS-SB05-Z60-61-Q


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/18/2023
Supervised By :Ankita Jodhani 08/18/2023

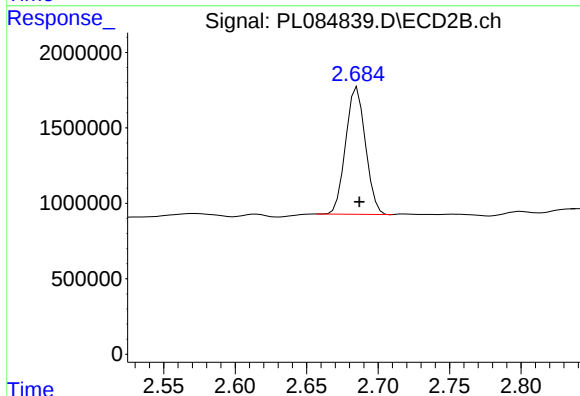


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.001 min
Response: 8129357
Conc: 7.48 ng/ml

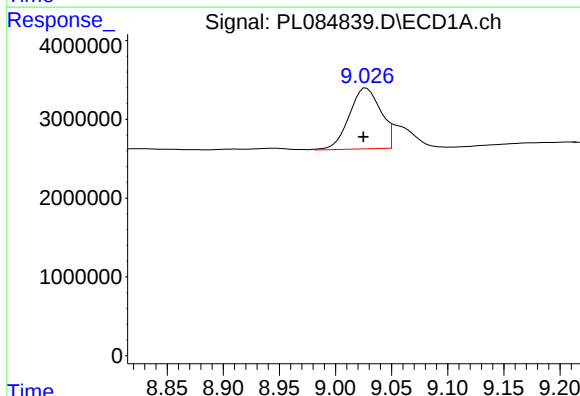

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.001 min
Response: 15202553
Conc: 9.34 ng/ml m

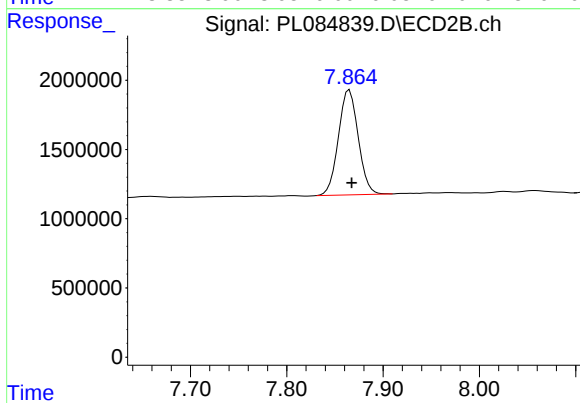

#28 Decachlorobiphenyl

R.T.: 7.865 min
Delta R.T.: -0.002 min
Response: 10808365
Conc: 8.67 ng/ml