

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081825\
 Data File : PL096855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Aug 2025 16:30
 Operator : AR\AJ
 Sample : Q2815-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TW-705R-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 06:00:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 08 15:43:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.823	73980277	68001961	23.259	14.233 #
28)	SA Decachlor...	9.007	7.987	24573818	40225957	10.305	9.272
Target Compounds							
4)	MA Heptachlor	4.924f	0.000	31607524	0	7.606	N.D. #
10)	B gamma-Chl...	0.000	5.050	0	45455635	N.D.	7.730 #
12)	B 4,4'-DDE	6.161	5.299	173.6E6	251.1E6	54.062	45.534
13)	MA Dieldrin	0.000	5.461f	0	225.6E6	N.D.	38.197 #
14)	MA Endrin	0.000	5.713	0	6216594	N.D.	1.150 #
16)	A 4,4'-DDD	6.669	5.852	405.9E6	635.7E6	160.537	135.109
17)	MA 4,4'-DDT	7.003	6.088f	7040332	10916286	2.455	2.158
18)	B Endrin al...	0.000	6.177	0	10043705	N.D.	2.763 #
19)	B Endosulfa...	7.124	0.000	7455655	0	2.594	N.D. #
25)	Chlordane-3	0.000	5.050	0	45455635	N.D.	65.375 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081825\
Data File : PL096855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Aug 2025 16:30
Operator : AR\AJ
Sample : Q2815-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 06:00:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Fri Aug 08 15:43:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

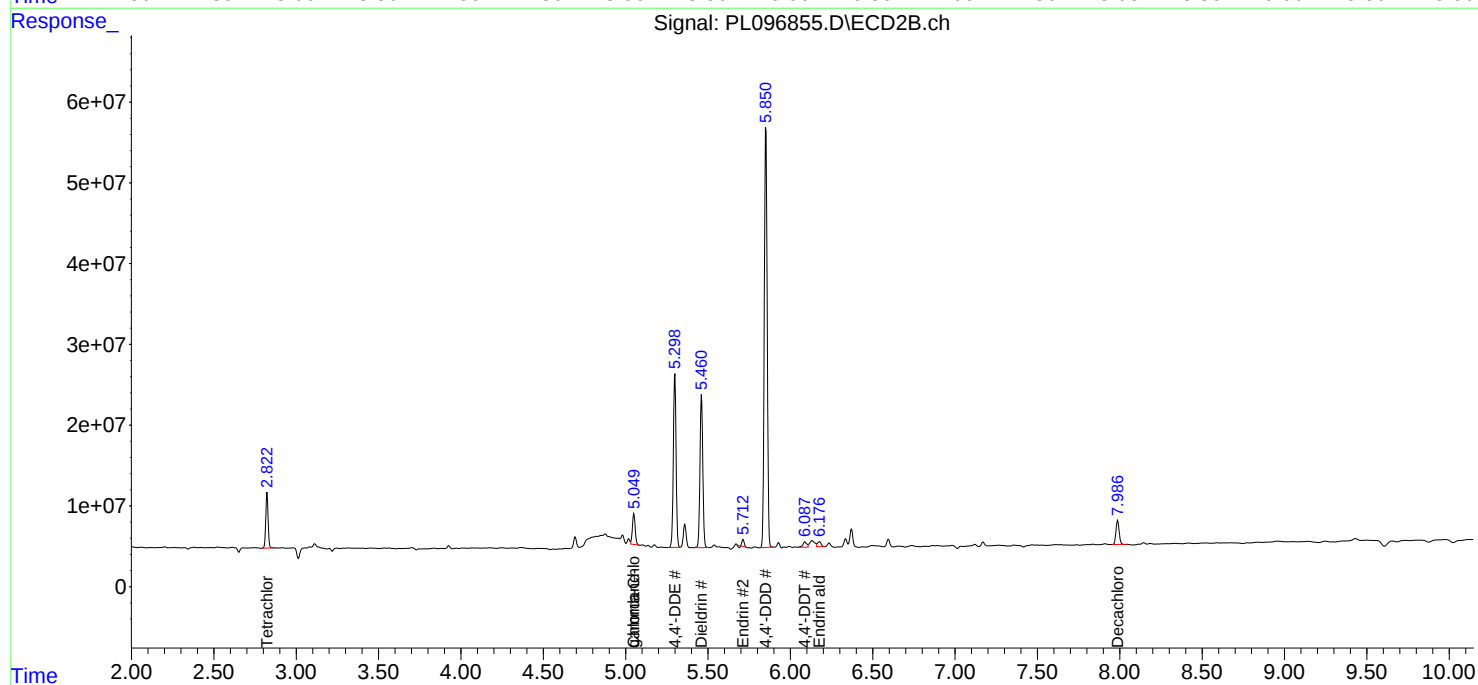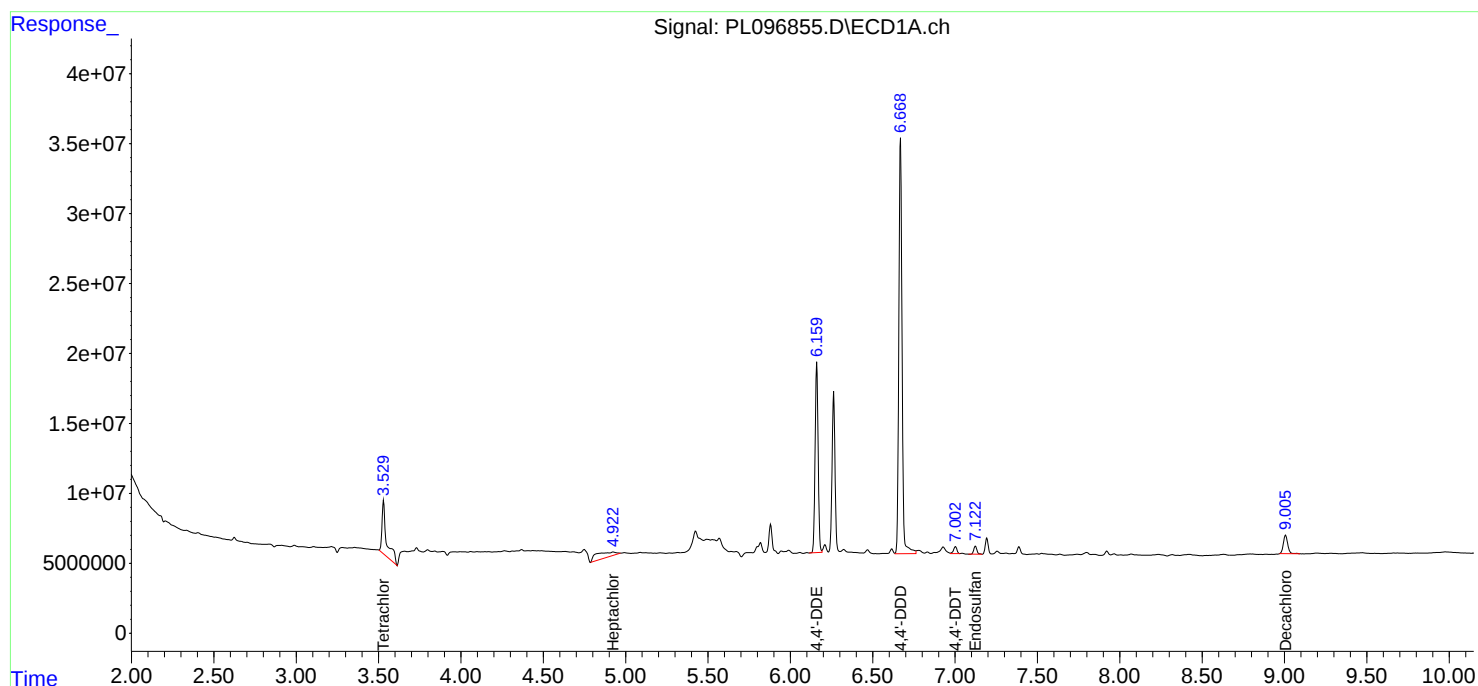


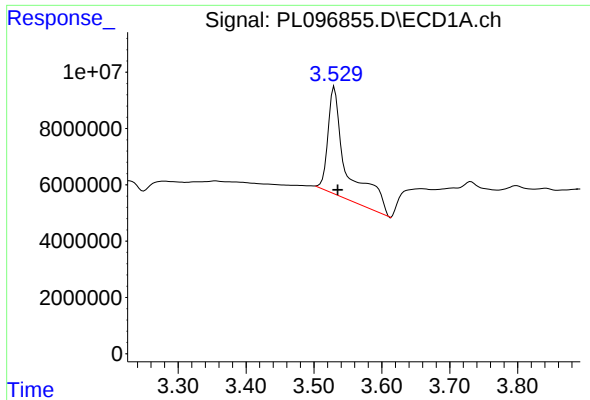

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: -0.005 min
Response: 73980277
Conc: 23.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

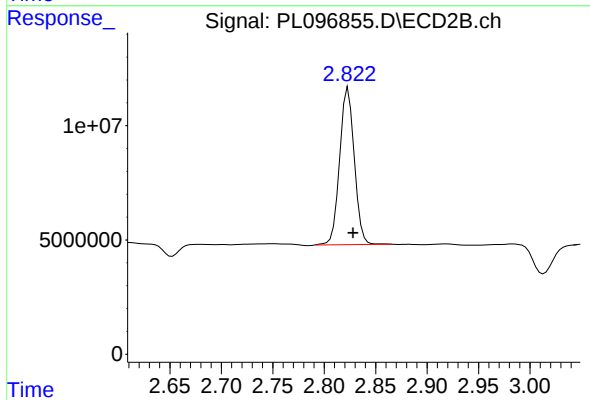


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: -0.005 min
Response: 68001961
Conc: 14.23 ng/ml

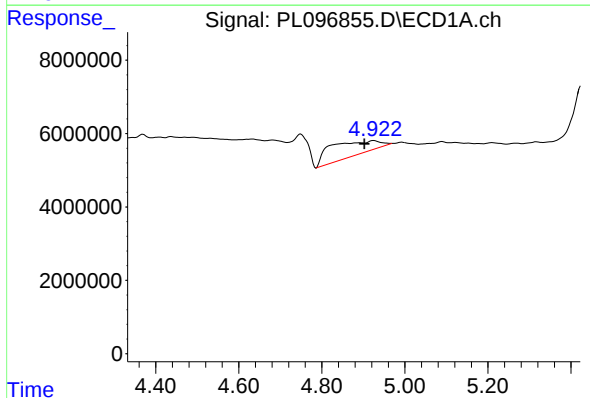


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.022 min
Response: 31607524
Conc: 7.61 ng/ml

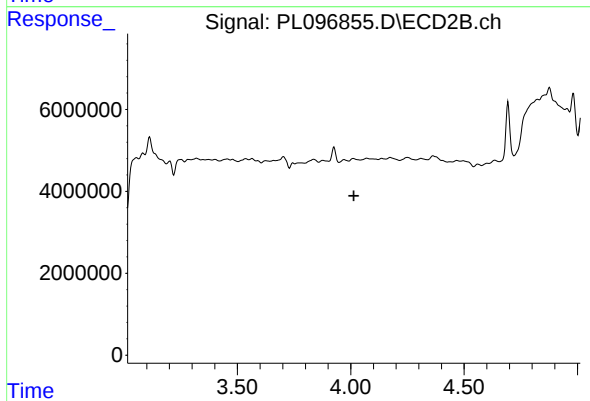

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.014 min
Response: 0
Conc: N.D.

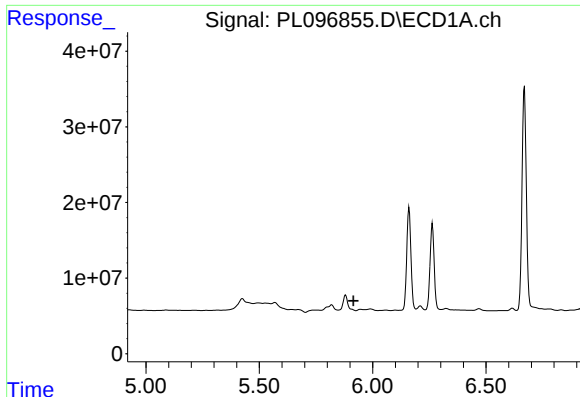

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

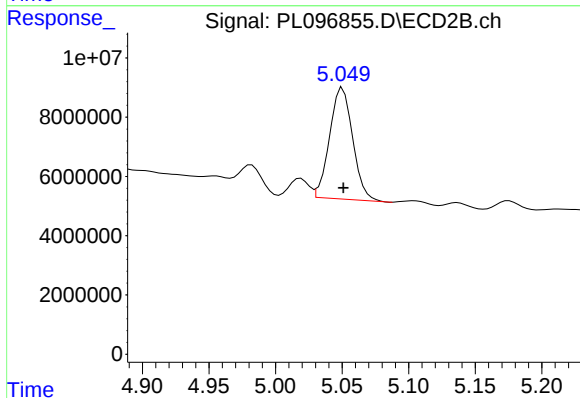


#10 gamma-Chlordane

R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 45455635
Conc: 7.73 ng/ml

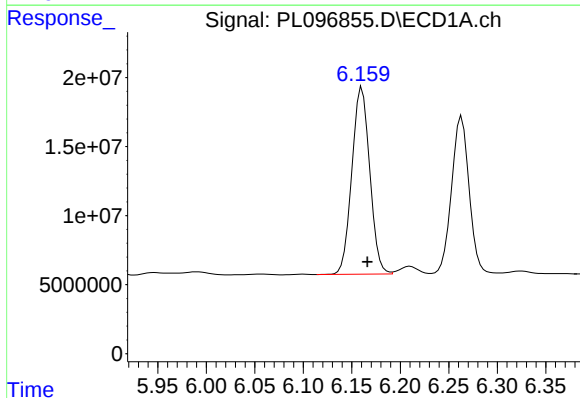


#12 4,4'-DDE

R.T.: 6.161 min
Delta R.T.: -0.006 min
Response: 173606744
Conc: 54.06 ng/ml

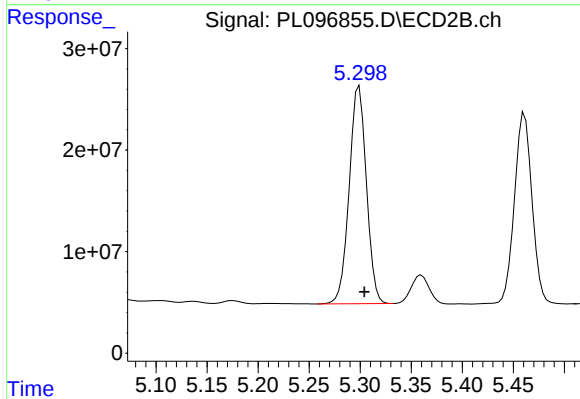

#12 4,4'-DDE


R.T.: 5.299 min
Delta R.T.: -0.005 min
Response: 251094235
Conc: 45.53 ng/ml

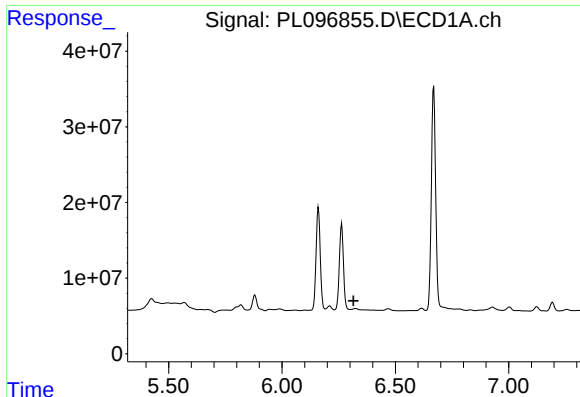

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

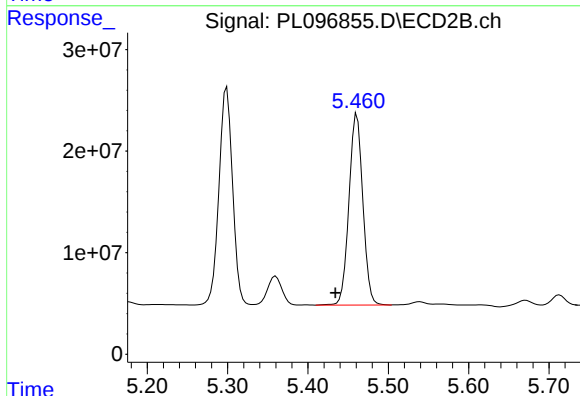


#13 Dieldrin

R.T.: 5.461 min
Delta R.T.: 0.027 min
Response: 225612345
Conc: 38.20 ng/ml

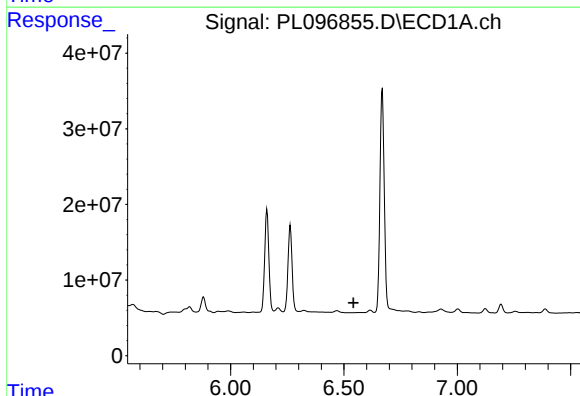


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

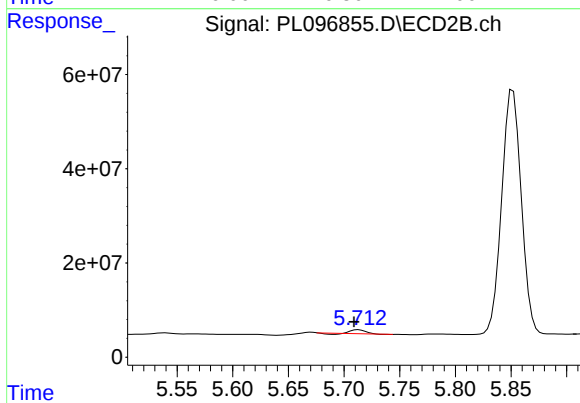

#14 Endrin


R.T.: 5.713 min
Delta R.T.: 0.004 min
Response: 6216594
Conc: 1.15 ng/ml

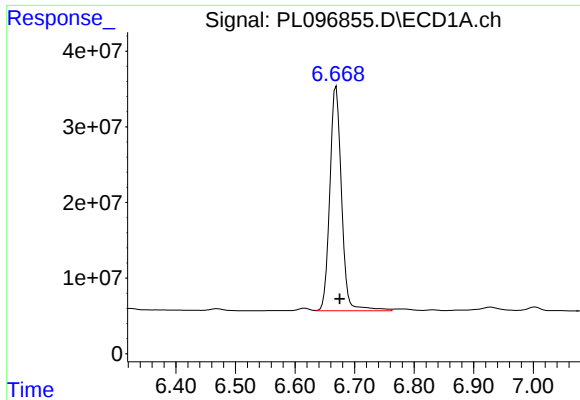

#16 4,4'-DDD


R.T.: 6.669 min
Delta R.T.: -0.006 min
Response: 405896514
Conc: 160.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

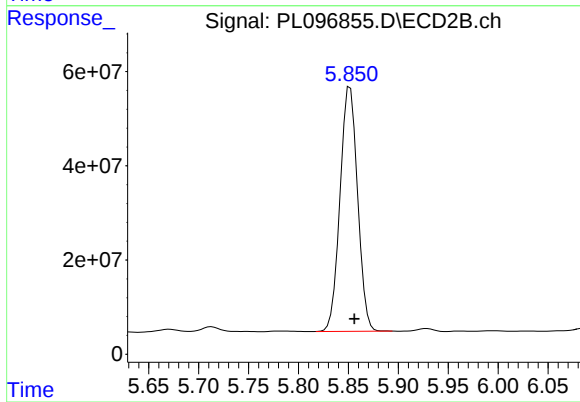


#16 4,4'-DDD

R.T.: 5.852 min
Delta R.T.: -0.004 min
Response: 635727139
Conc: 135.11 ng/ml

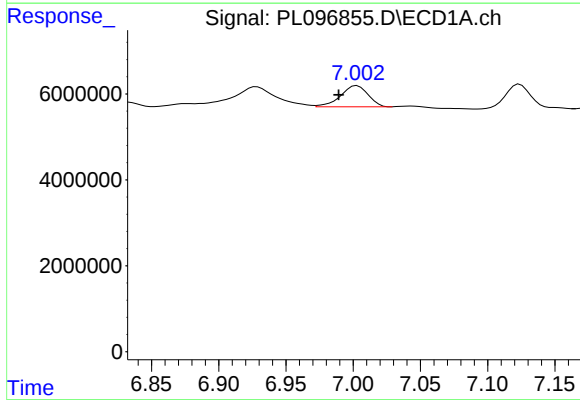


#17 4,4'-DDT

R.T.: 7.003 min
Delta R.T.: 0.014 min
Response: 7040332
Conc: 2.46 ng/ml

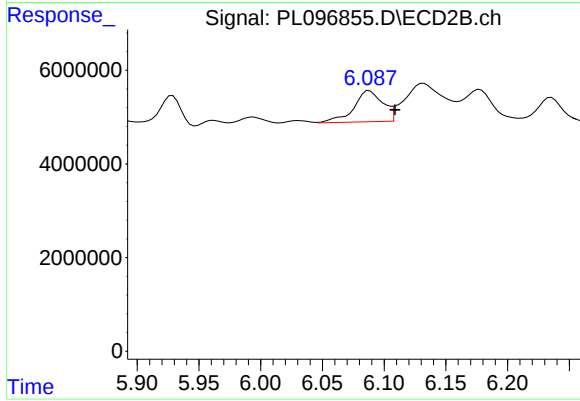

#17 4,4'-DDT


R.T.: 6.088 min
Delta R.T.: -0.021 min
Response: 10916286
Conc: 2.16 ng/ml

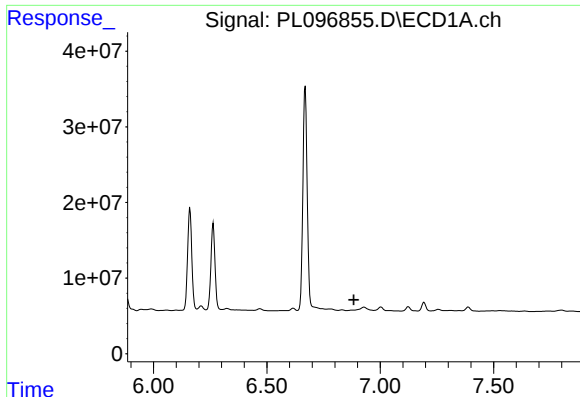

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.884 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

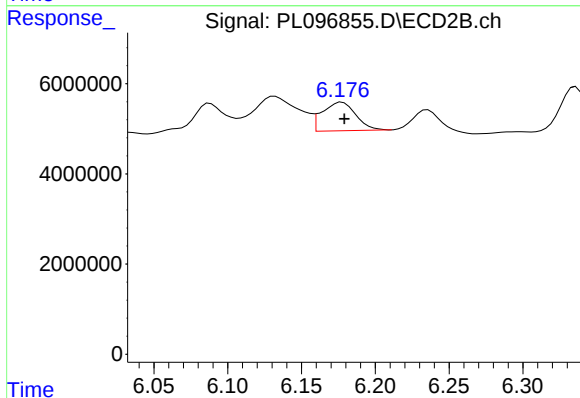


#18 Endrin aldehyde

R.T.: 6.177 min
Delta R.T.: -0.002 min
Response: 10043705
Conc: 2.76 ng/ml

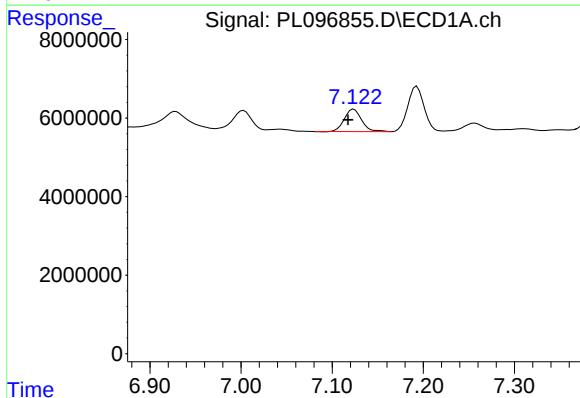


#19 Endosulfan Sulfate

R.T.: 7.124 min
Delta R.T.: 0.006 min
Response: 7455655
Conc: 2.59 ng/ml

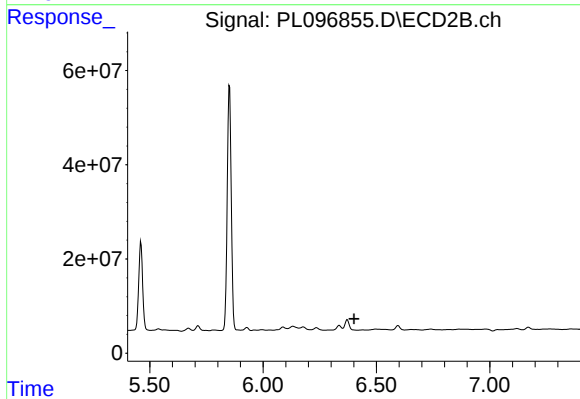

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.402 min
Response: 0
Conc: N.D.

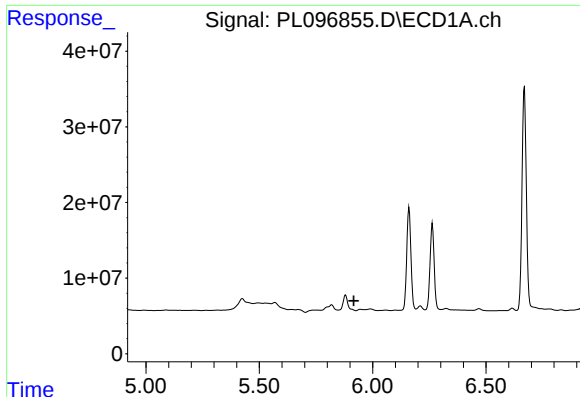

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.916 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TW-705R-S

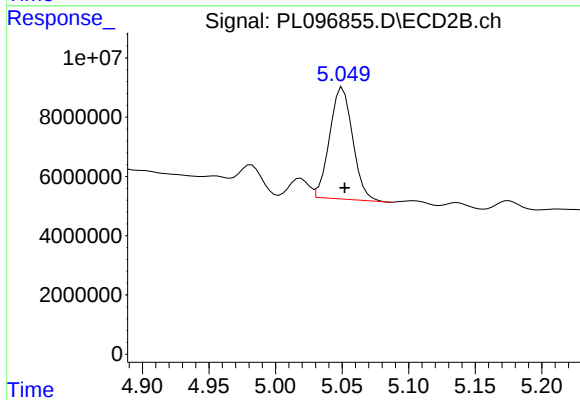


#25 Chlordane-3

R.T.: 5.050 min
Delta R.T.: -0.002 min
Response: 45455635
Conc: 65.38 ng/ml

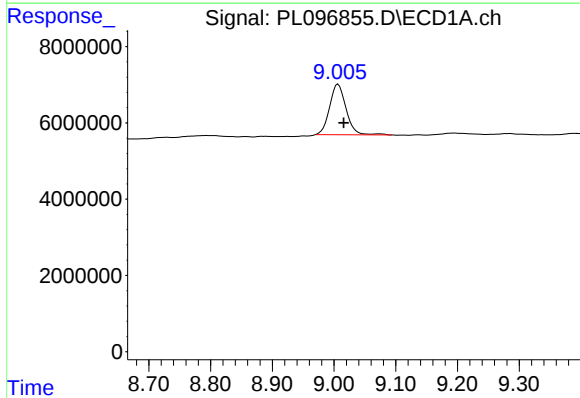

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.009 min
Response: 24573818
Conc: 10.30 ng/ml

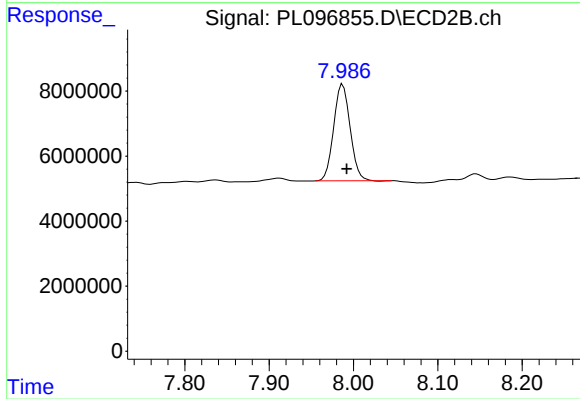

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.005 min
Response: 40225957
Conc: 9.27 ng/ml