

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081920\
 Data File : PL060833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2020 12:41
 Operator : DD\AJ
 Sample : L3499-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-081820

Manual Integrations
 APPROVED

Ankita
 8/20/2020 2:25:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:18:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.008	21350576	25035182	12.789m	9.000m#
28)	SA Decachlor...	8.219	9.097	20374244	31801810	14.263	15.734m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081920\
Data File : PL060833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2020 12:41
Operator : DD\AJ
Sample : L3499-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-01-081820


Manual Integrations
APPROVED

Ankita
8/20/2020 2:25:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:18:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

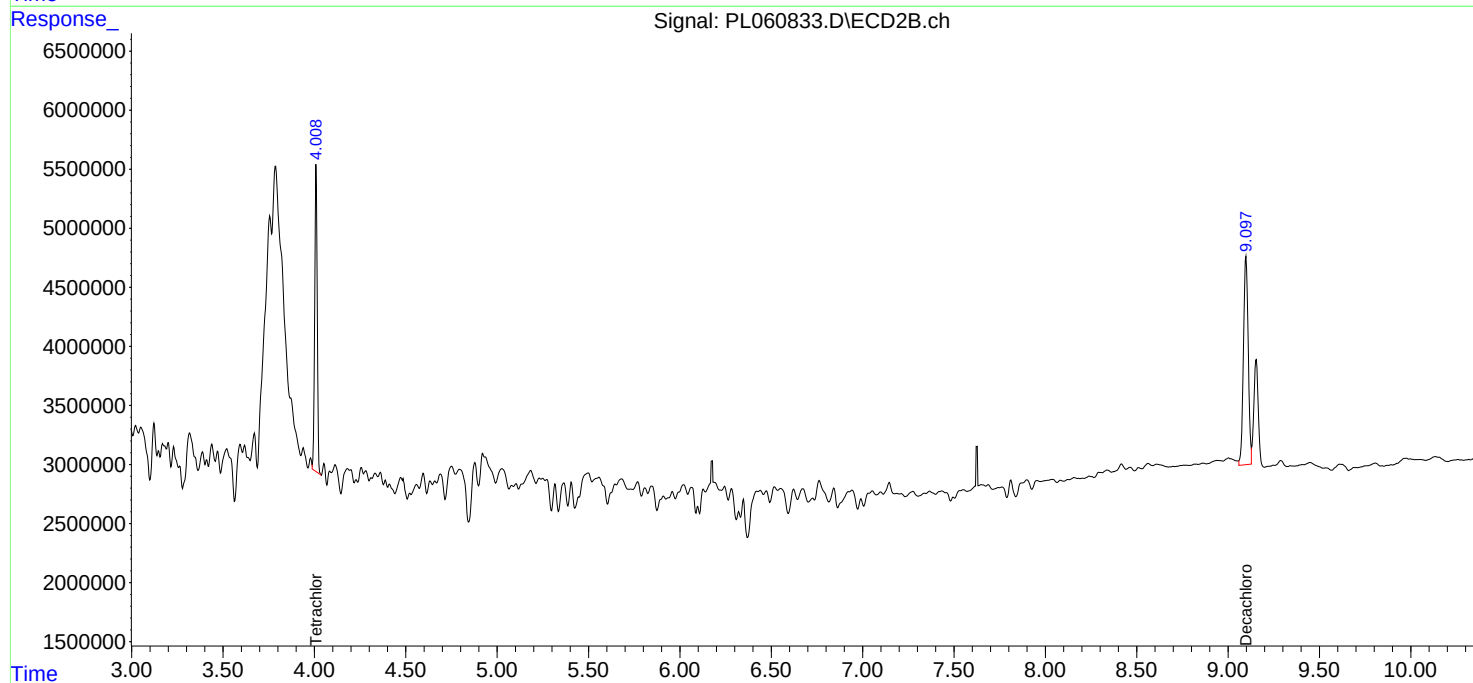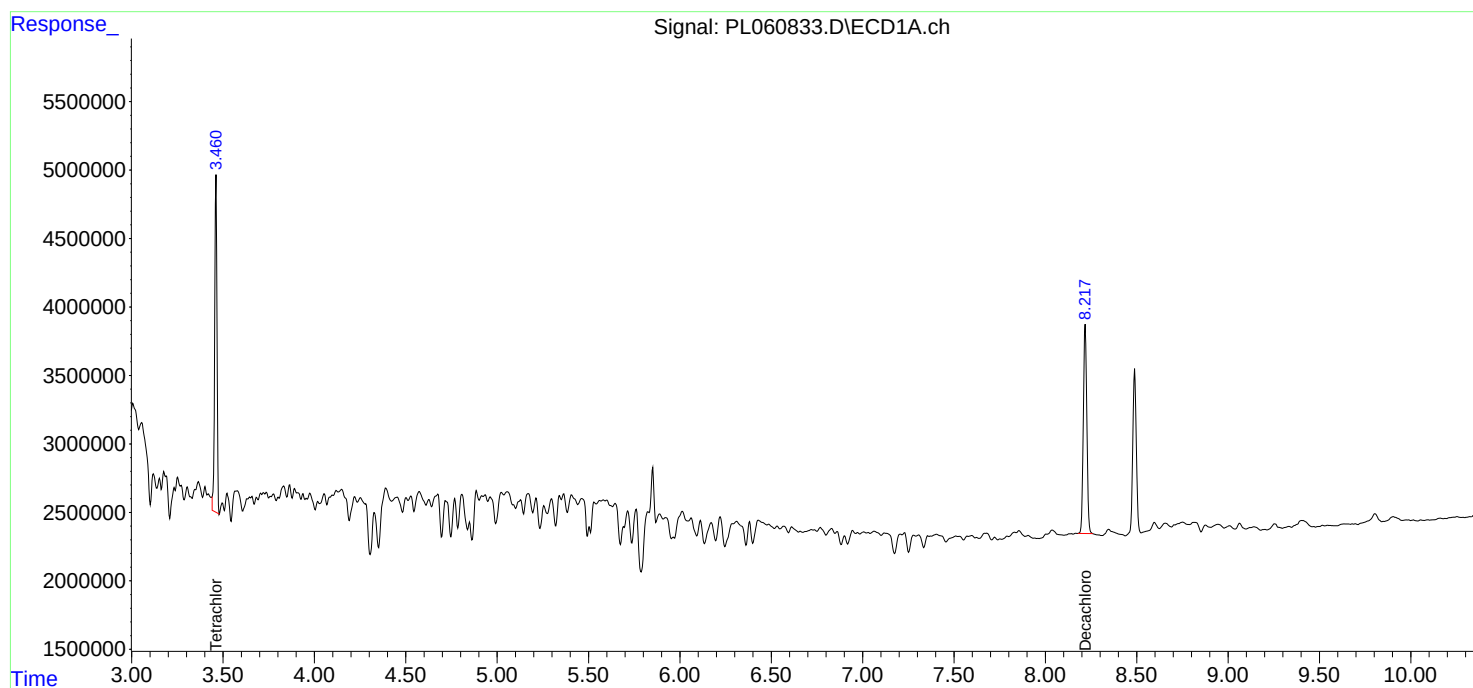

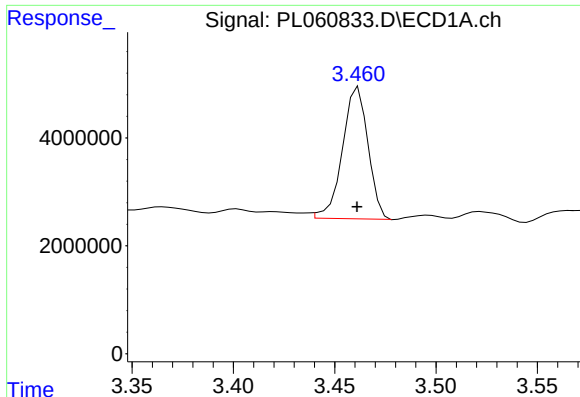


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 21350576
Conc: 12.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HD-01-081820


Manual Integrations
APPROVED

Ankita
8/20/2020 2:25:51 PM

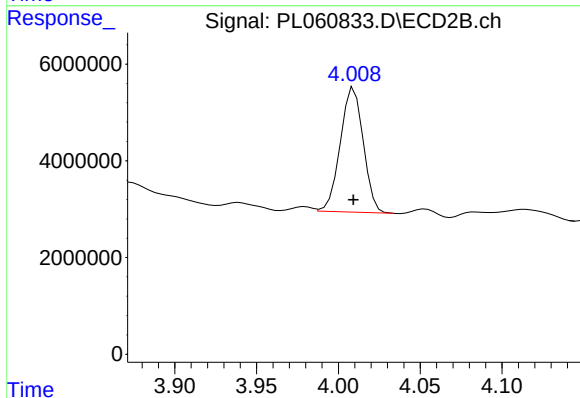


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: -0.001 min
Response: 25035182
Conc: 9.00 ng/ml m

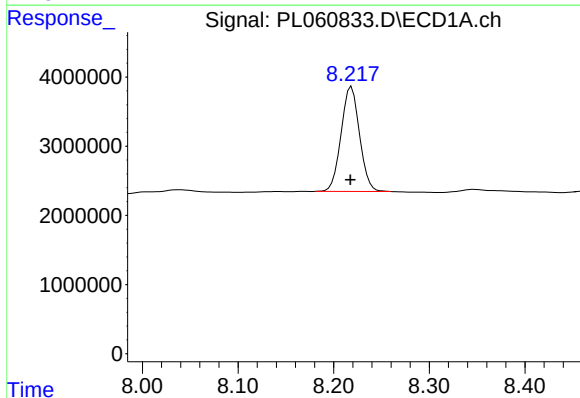

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.001 min
Response: 20374244
Conc: 14.26 ng/ml

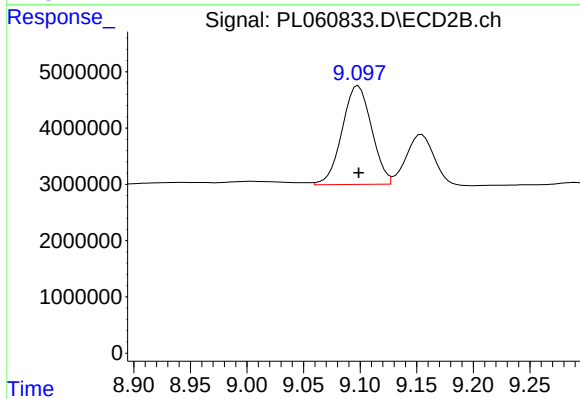

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 31801810
Conc: 15.73 ng/ml m