

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081920\
 Data File : PL060848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2020 17:09
 Operator : DD\AJ
 Sample : L3719-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-AMENDED-DISCRETE-005

Manual Integrations
 APPROVED

Ankita
 8/20/2020 2:25:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 18:51:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 19 06:13:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.009	29249162	42695128	17.521	15.349
28)	SA Decachlor...	8.217	9.097	21460754	27978846	15.024	13.843m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081920\
Data File : PL060848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2020 17:09
Operator : DD\AJ
Sample : L3719-09
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SPLP-AMENDED-DISCRETE-005


Manual Integrations
APPROVED

Ankita
8/20/2020 2:25:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 18:51:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081820.M
Quant Title : GC Extractables
QLast Update : Wed Aug 19 06:13:38 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

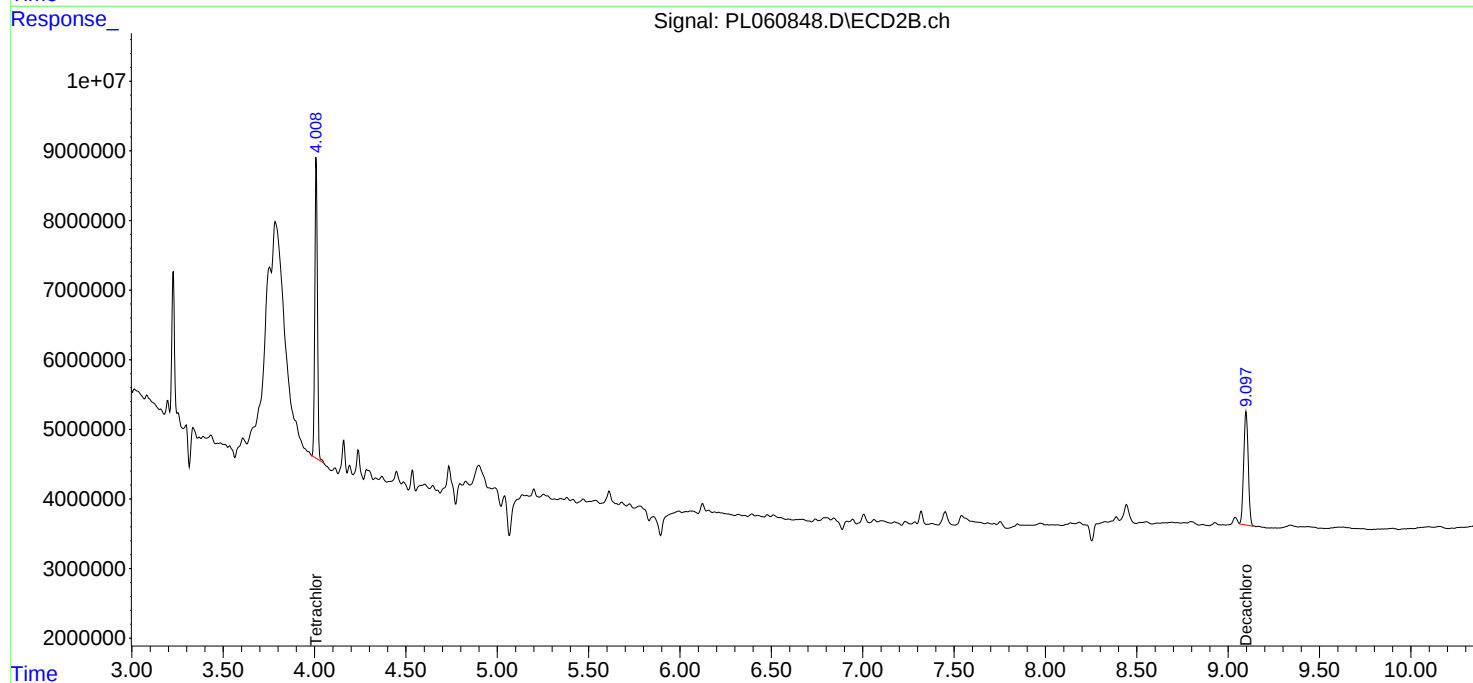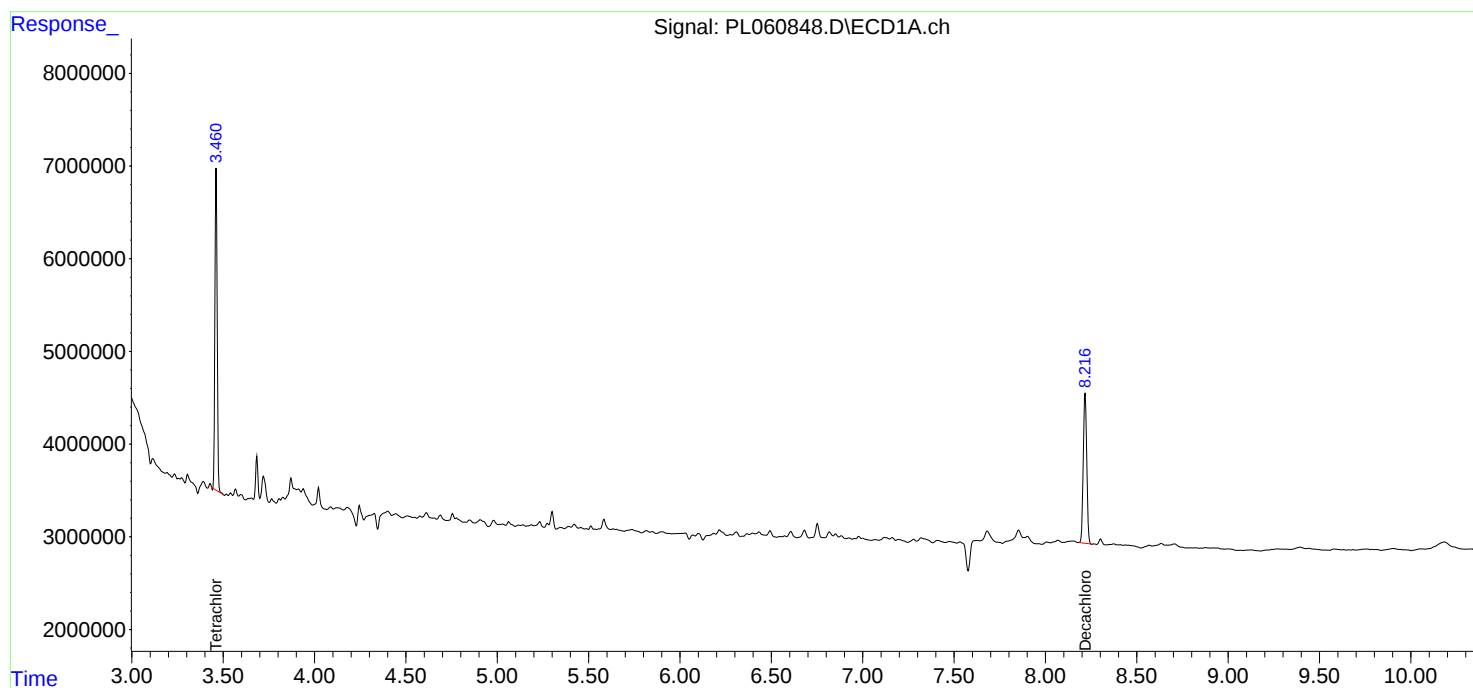

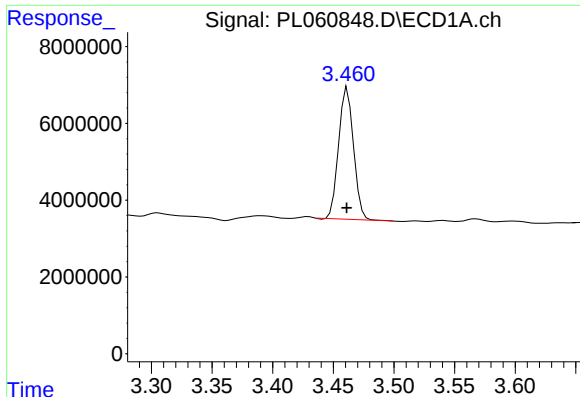


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: 0.000 min
Response: 29249162
Conc: 17.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-AMENDED-DISCRETE-005


Manual Integrations
APPROVED

Ankita
8/20/2020 2:25:59 PM

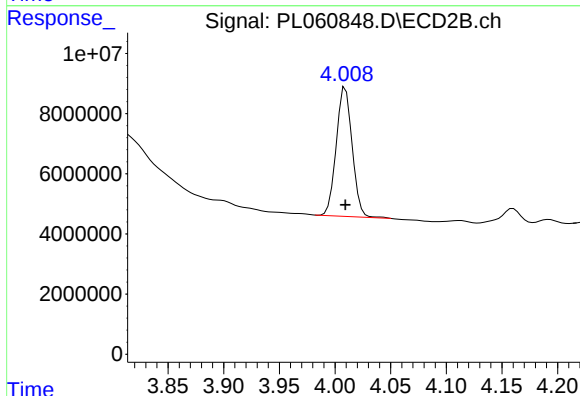


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.000 min
Response: 42695128
Conc: 15.35 ng/ml

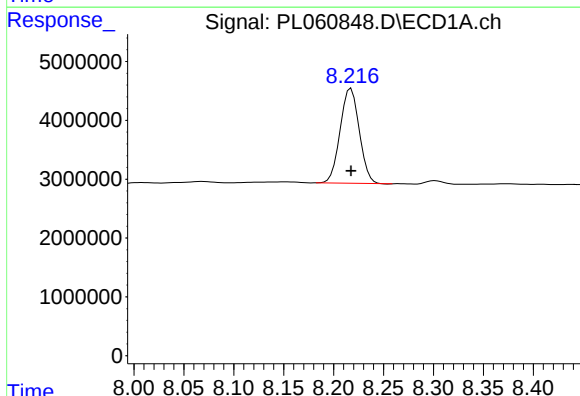

#28 Decachlorobiphenyl

R.T.: 8.217 min
Delta R.T.: 0.000 min
Response: 21460754
Conc: 15.02 ng/ml

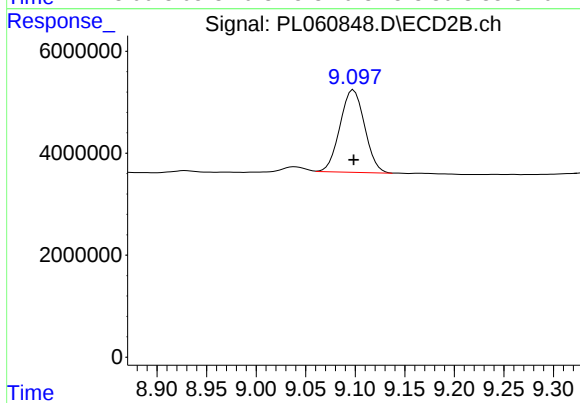

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.002 min
Response: 27978846
Conc: 13.84 ng/ml m