

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
 Data File : PL069222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 09:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 14:50:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.572	8523165	26593446	20.605	26.192 #
28)	SA Decachlor...	10.407	11.497	12526662	24018105	21.797	24.755
Target Compounds							
4)	MA Heptachlor	6.154f	0.000	1748156	0	2.976	N.D. #
6)	B beta-BHC	6.154	0.000	1748156	0	6.201	N.D. #
9)	A Endosulfan I	0.000	8.454	0	141711	N.D.	0.134 #
11)	B alpha-Chl...	0.000	8.385	0	245420	N.D.	0.214 #
15)	B Endosulfa...	0.000	9.219f	0	361233	N.D.	0.394 #
21)	B Endrin ke...	0.000	10.097f	0	305949	N.D.	0.300 #
23)	Chlordane-1	0.000	6.985f	0	33973	N.D.	0.806 #
26)	Chlordane-4	0.000	8.385	0	245420	N.D.	1.237 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
Data File : PL069222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 09:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 14:50:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

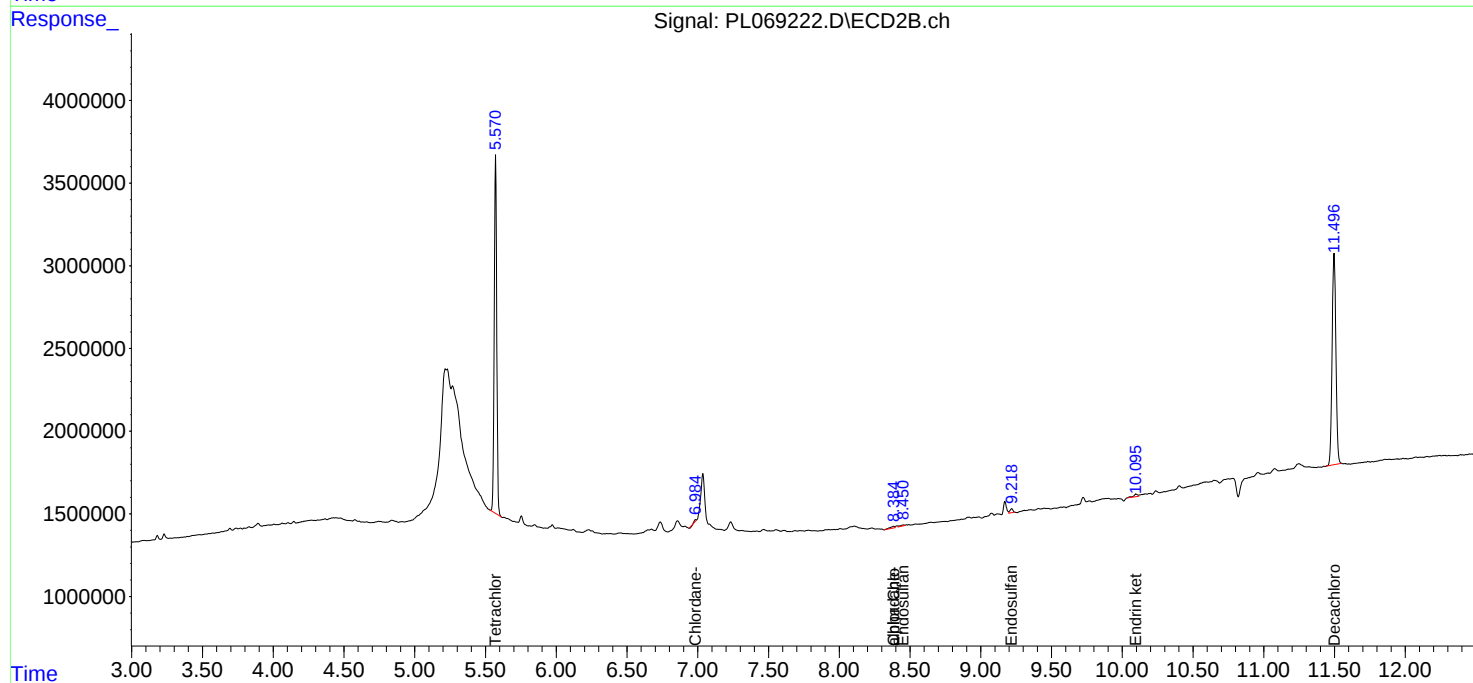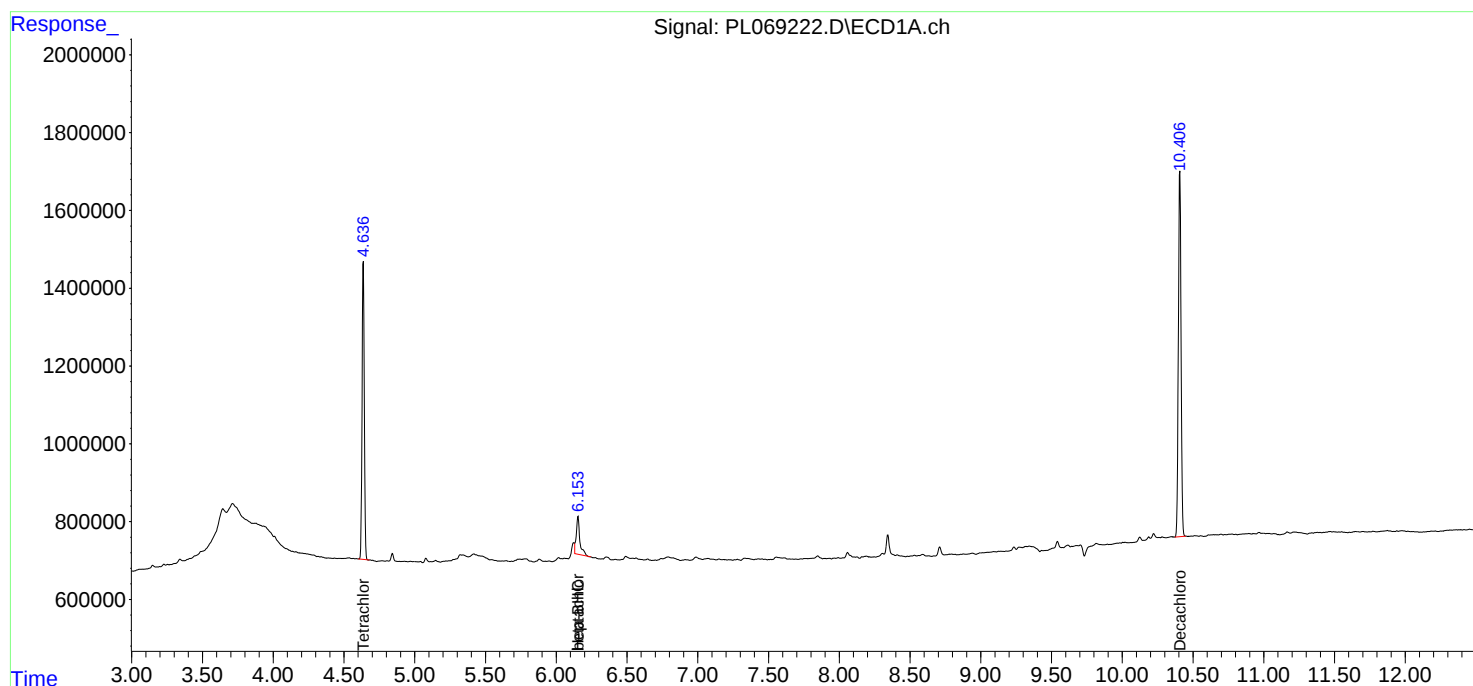


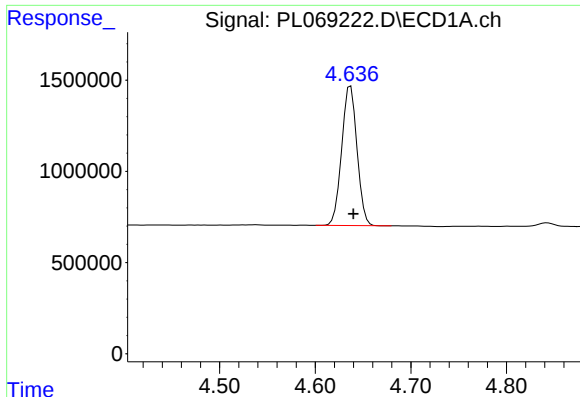

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 8523165
Conc: 20.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

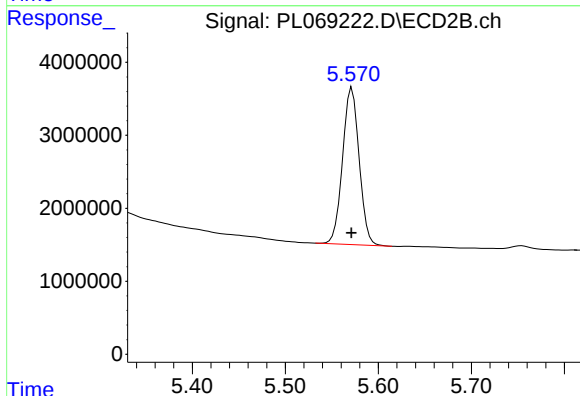


#1 Tetrachloro-m-xylene

R.T.: 5.572 min
Delta R.T.: 0.000 min
Response: 26593446
Conc: 26.19 ng/ml

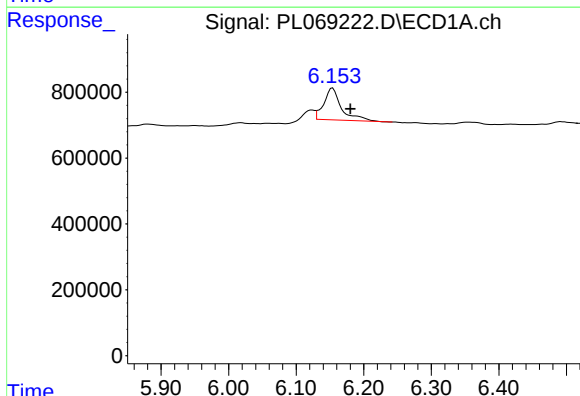


#4 Heptachlor

R.T.: 6.154 min
Delta R.T.: -0.027 min
Response: 1748156
Conc: 2.98 ng/ml

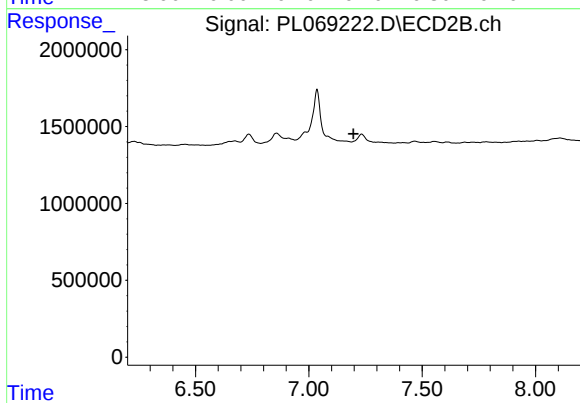

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.197 min
Response: 0
Conc: N.D.

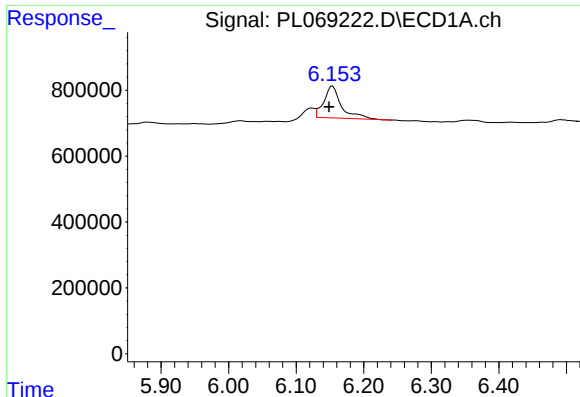

#6 beta-BHC


R.T.: 6.154 min
Delta R.T.: 0.005 min
Response: 1748156
Conc: 6.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

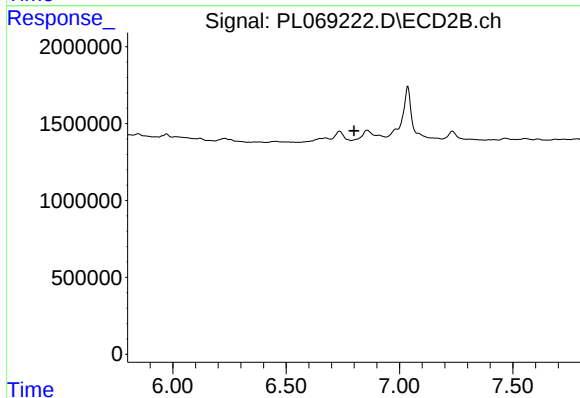


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

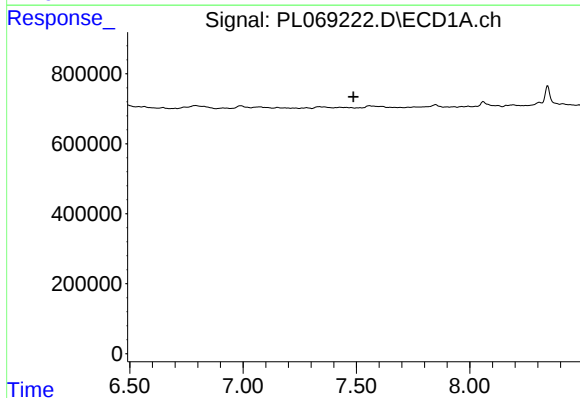


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

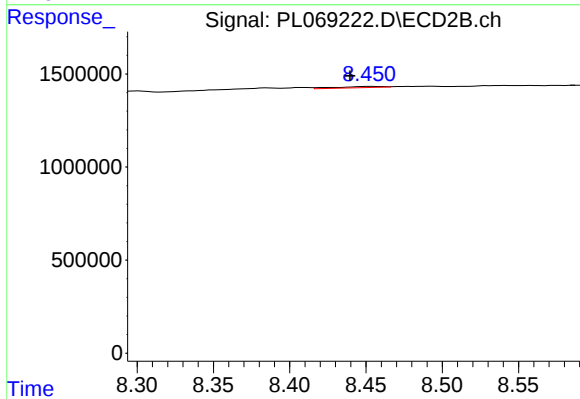

#9 Endosulfan I


R.T.: 8.454 min
Delta R.T.: 0.014 min
Response: 141711
Conc: 0.13 ng/ml

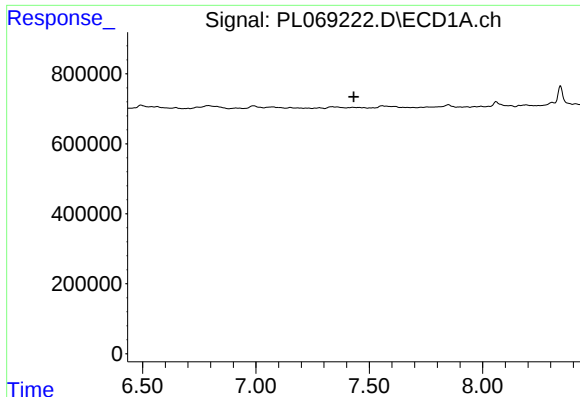

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

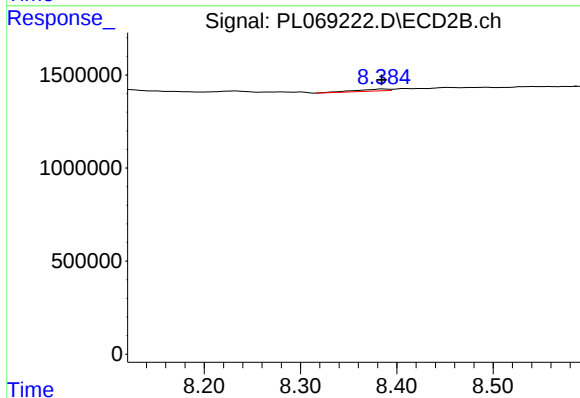


#11 alpha-Chlordane

R.T.: 8.385 min
Delta R.T.: 0.001 min
Response: 245420
Conc: 0.21 ng/ml

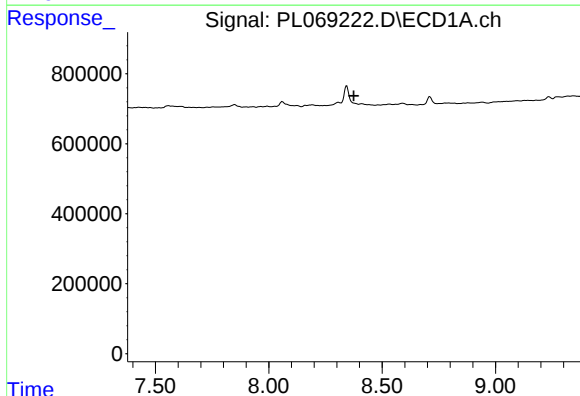


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

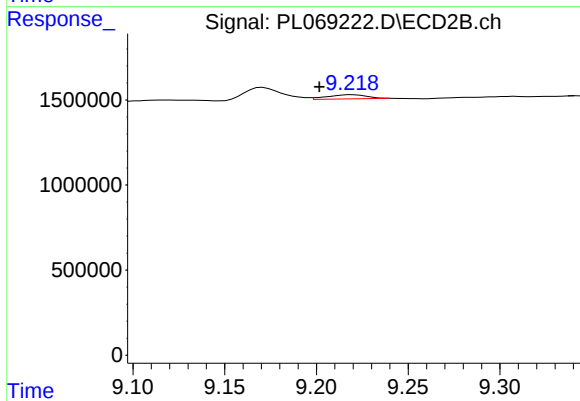

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.018 min
Response: 361233
Conc: 0.39 ng/ml

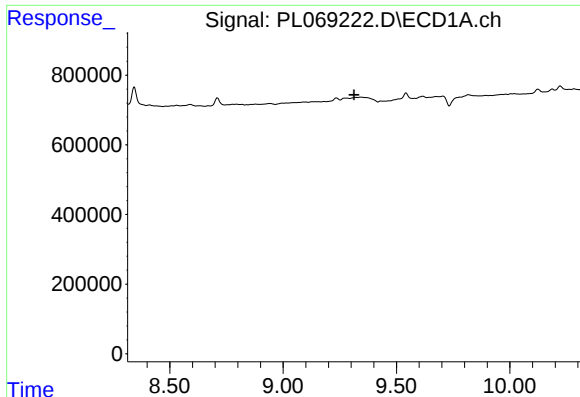

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

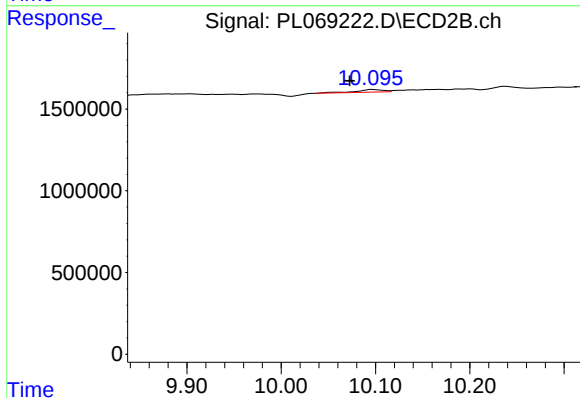


#21 Endrin ketone

R.T.: 10.097 min
Delta R.T.: 0.024 min
Response: 305949
Conc: 0.30 ng/ml

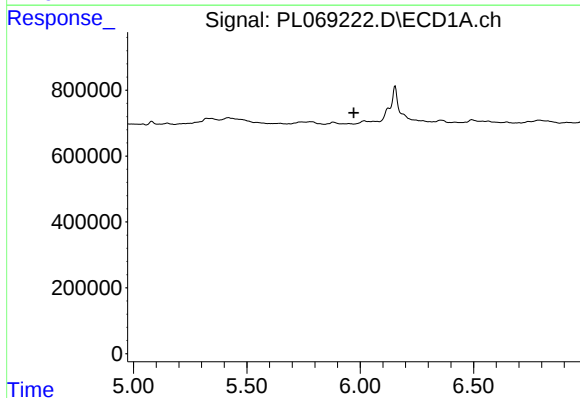


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

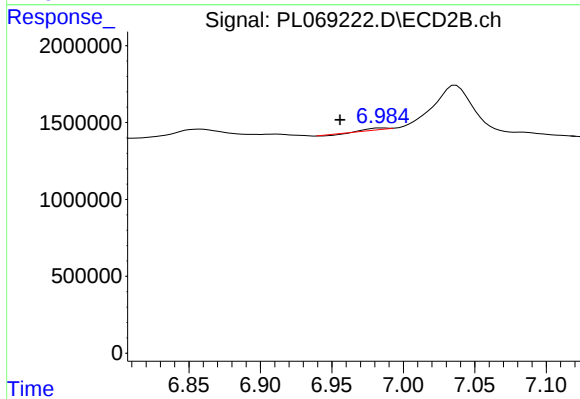

#23 Chlordane-1


R.T.: 6.985 min
Delta R.T.: 0.030 min
Response: 33973
Conc: 0.81 ng/ml

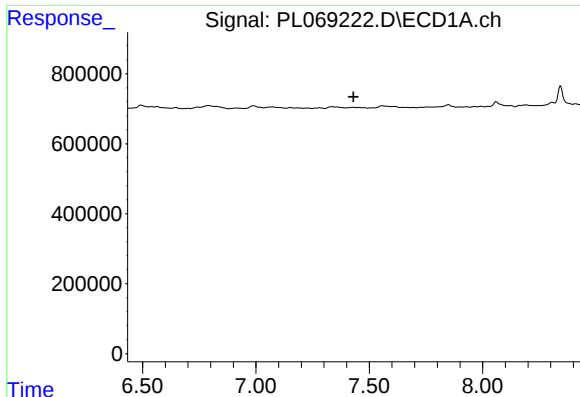

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

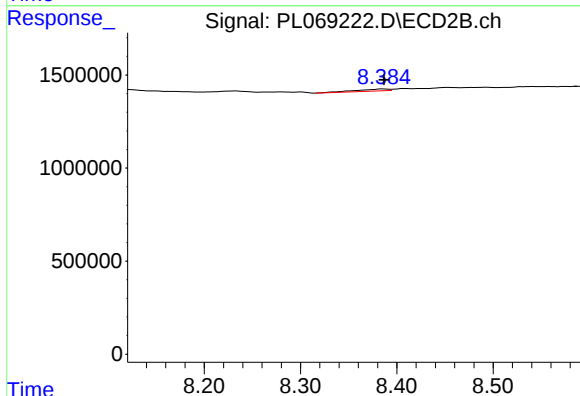


#26 Chlordane-4

R.T.: 8.385 min
Delta R.T.: -0.001 min
Response: 245420
Conc: 1.24 ng/ml

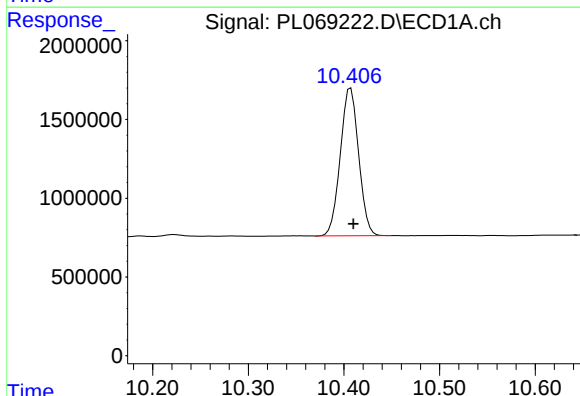

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.003 min
Response: 1252662
Conc: 21.80 ng/ml

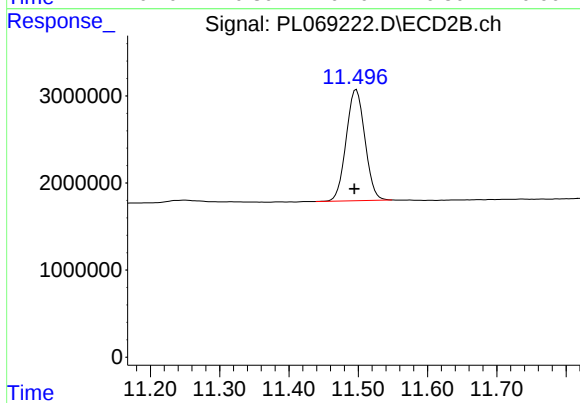

#28 Decachlorobiphenyl

R.T.: 11.497 min
Delta R.T.: 0.003 min
Response: 24018105
Conc: 24.75 ng/ml