

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
 Data File : PL069232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 14:12
 Operator : AR\AJ
 Sample : M3428-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 14:51:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.571	6337544	19911566	15.321	19.611 #
28)	SA Decachlor...	10.406	11.497	9555428	18607573	16.627	19.178
Target Compounds							
10)	B gamma-Chl...	0.000	8.303	0	222748	N.D.	0.194 #
11)	B alpha-Chl...	0.000	8.388	0	401257	N.D.	0.349 #
12)	B 4,4'-DDE	0.000	8.570	0	486099	N.D.	0.460 #
15)	B Endosulfa...	0.000	9.220f	0	259535	N.D.	0.283 #
17)	MA 4,4'-DDT	8.486	9.429	348587	711828	0.718	0.752
21)	B Endrin ke...	0.000	10.097f	0	50547	N.D.	0.050 #
25)	Chlordane-3	0.000	8.303	0	222748	N.D.	1.364 #
26)	Chlordane-4	0.000	8.388	0	401257	N.D.	2.023 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
Data File : PL069232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 14:12
Operator : AR\AJ
Sample : M3428-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 14:51:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

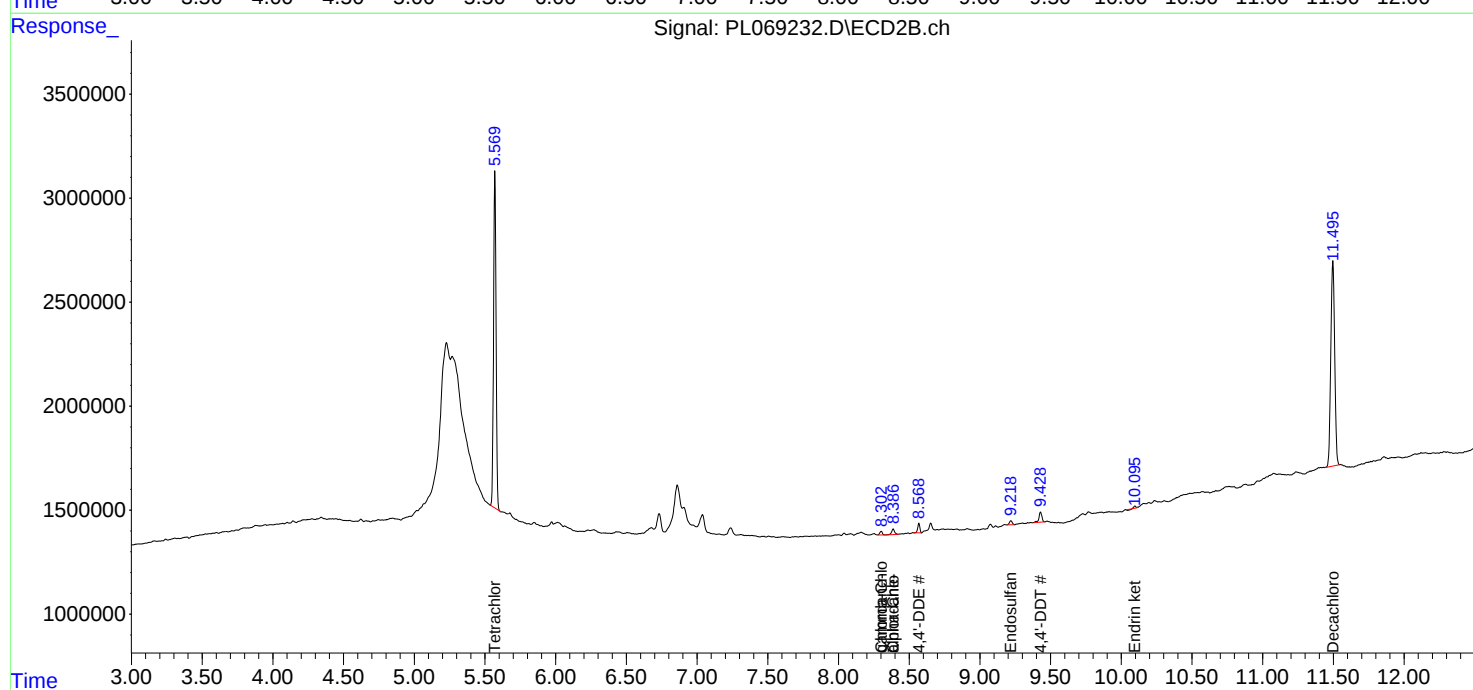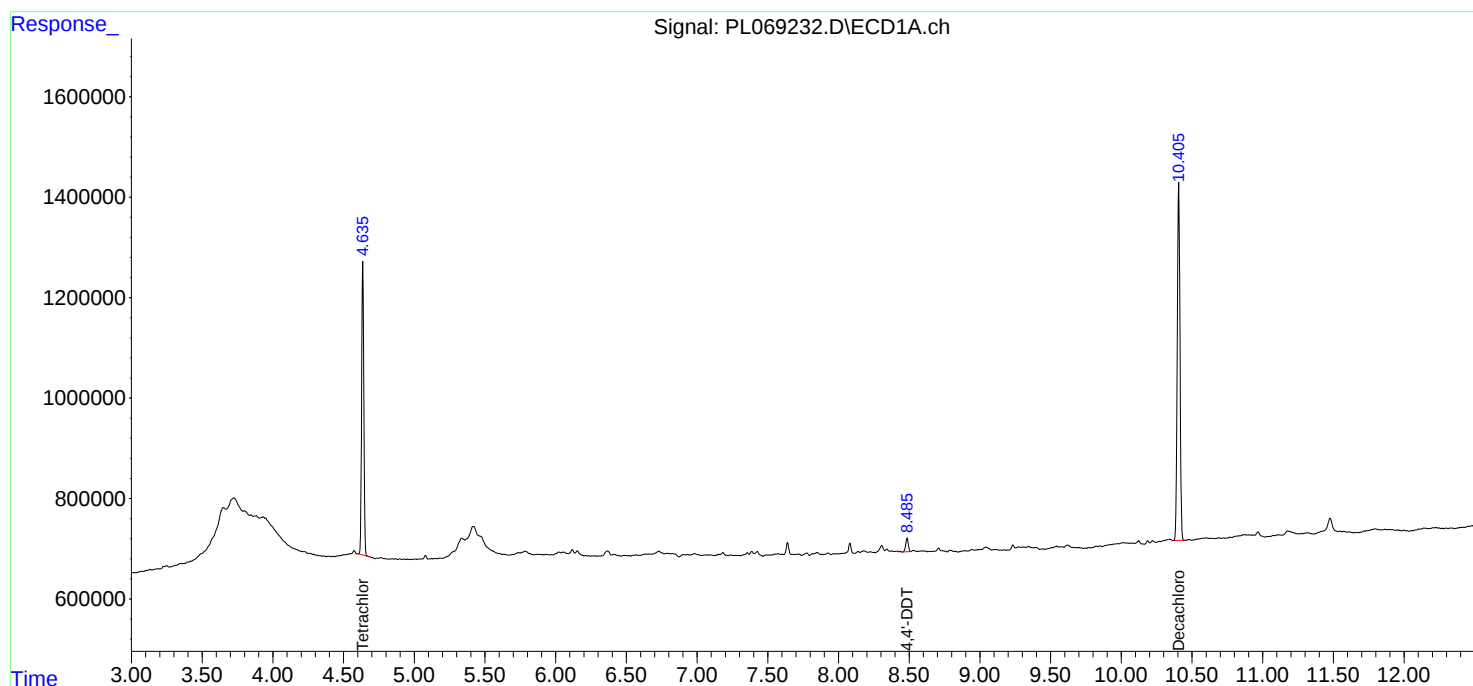


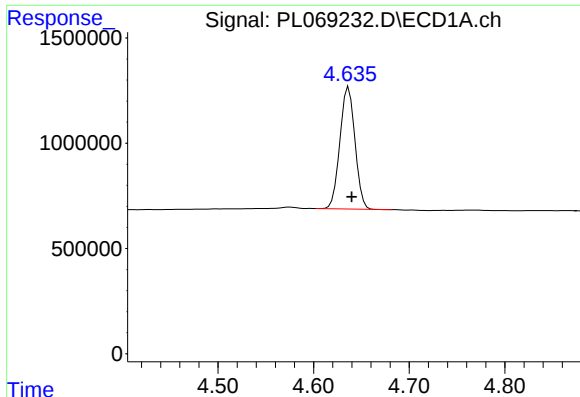

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 6337544
Conc: 15.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

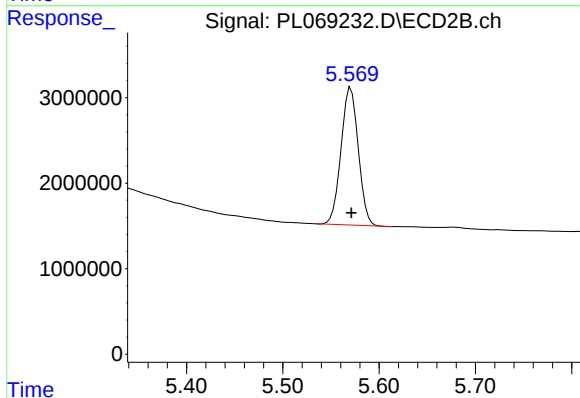


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 19911566
Conc: 19.61 ng/ml

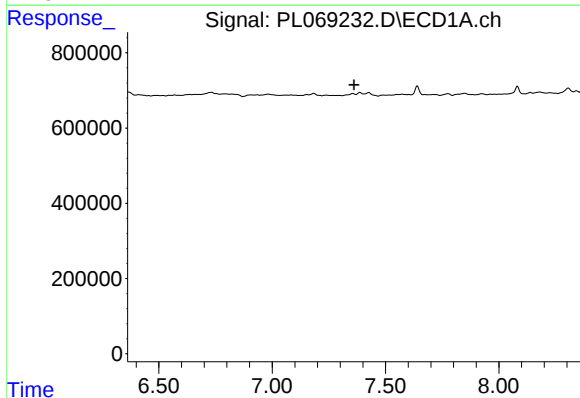


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

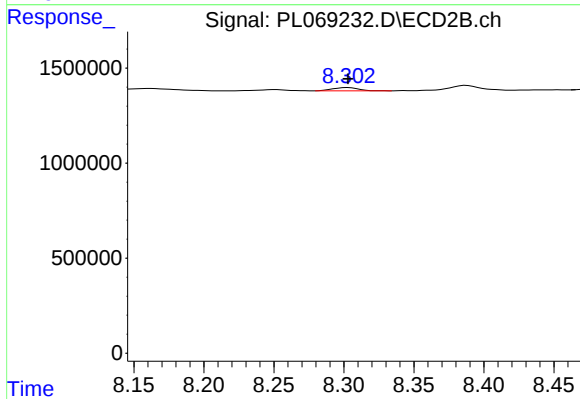

#10 gamma-Chlordane


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 222748
Conc: 0.19 ng/ml

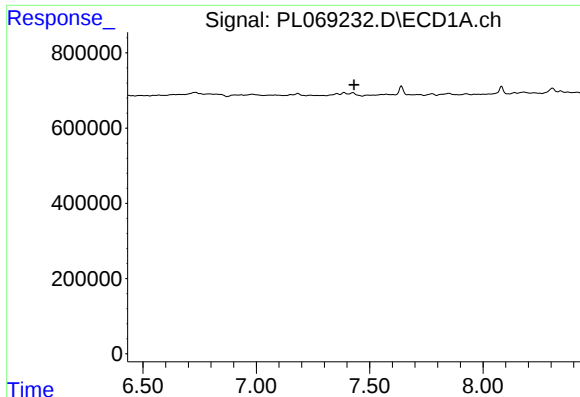

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

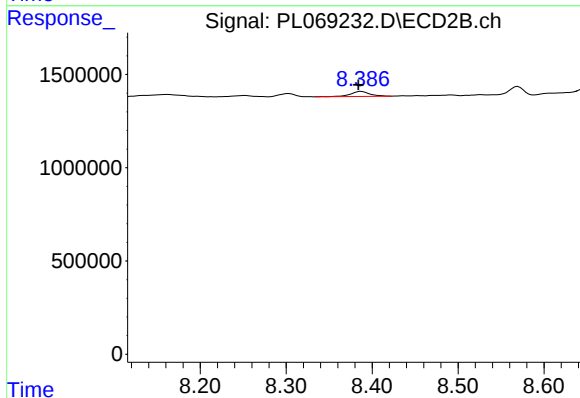


#11 alpha-Chlordane

R.T.: 8.388 min
Delta R.T.: 0.003 min
Response: 401257
Conc: 0.35 ng/ml

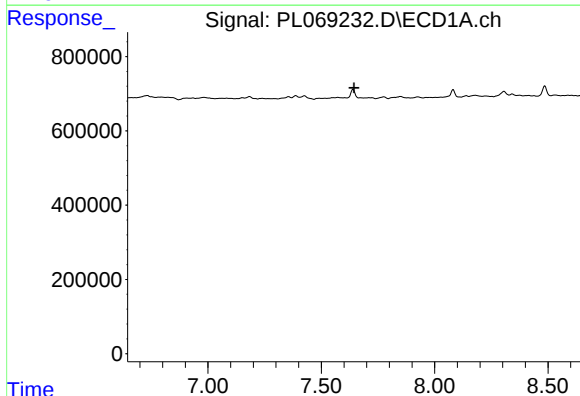


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.645 min
Response: 0
Conc: N.D.

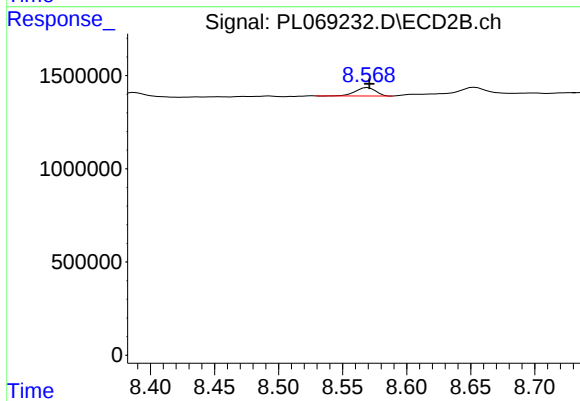

#12 4,4'-DDE


R.T.: 8.570 min
Delta R.T.: -0.001 min
Response: 486099
Conc: 0.46 ng/ml

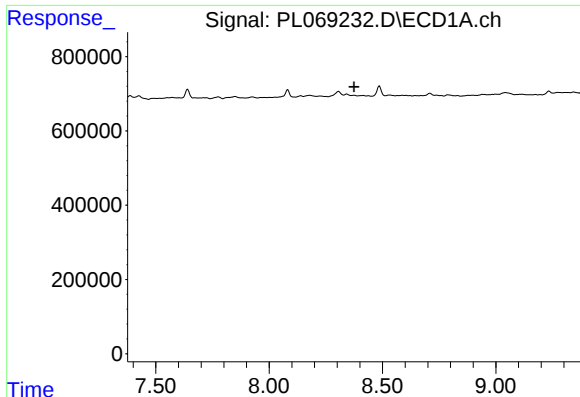

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

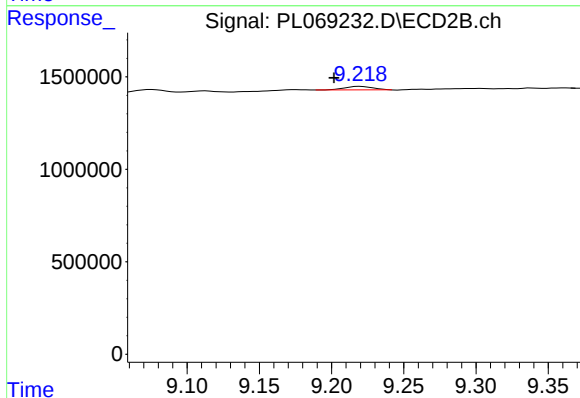


#15 Endosulfan II

R.T.: 9.220 min
Delta R.T.: 0.018 min
Response: 259535
Conc: 0.28 ng/ml

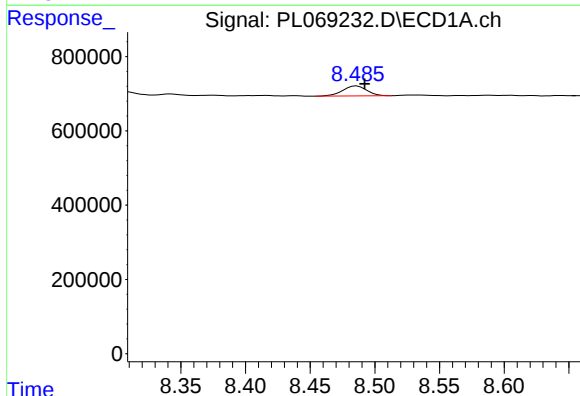


#17 4,4'-DDT

R.T.: 8.486 min
Delta R.T.: -0.006 min
Response: 348587
Conc: 0.72 ng/ml

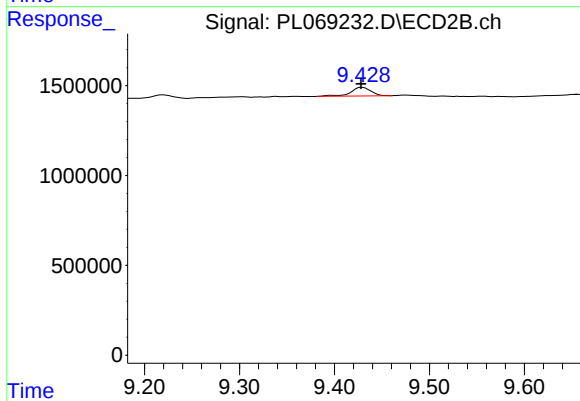

#17 4,4'-DDT


R.T.: 9.429 min
Delta R.T.: 0.001 min
Response: 711828
Conc: 0.75 ng/ml

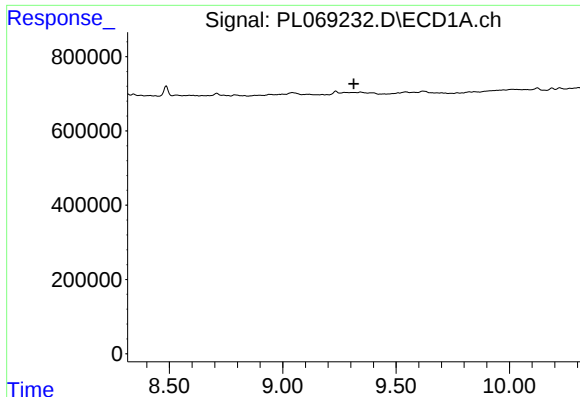

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

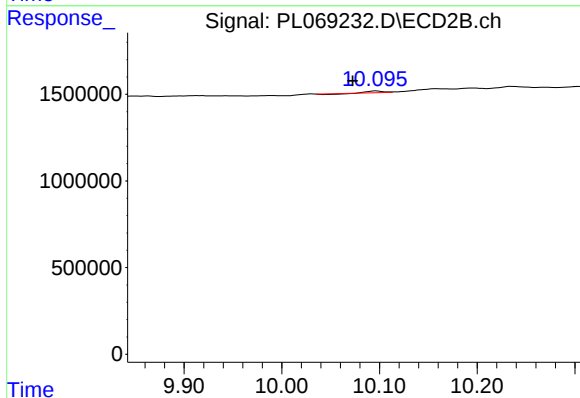


#21 Endrin ketone

R.T.: 10.097 min
Delta R.T.: 0.024 min
Response: 50547
Conc: 0.05 ng/ml

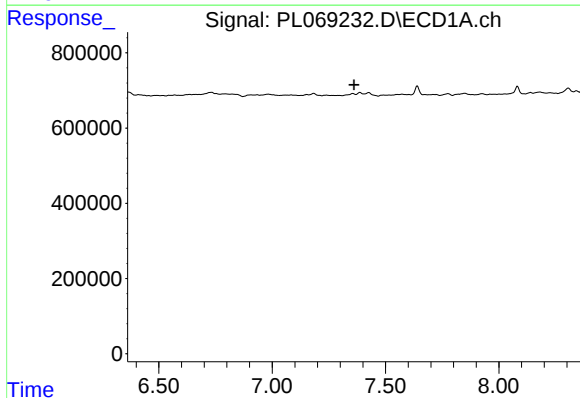


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

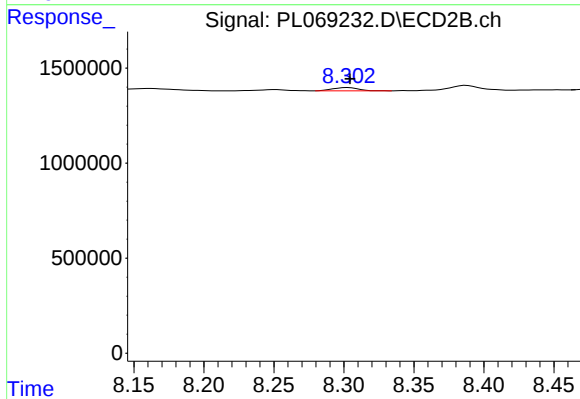

#25 Chlordane-3


R.T.: 8.303 min
Delta R.T.: -0.001 min
Response: 222748
Conc: 1.36 ng/ml

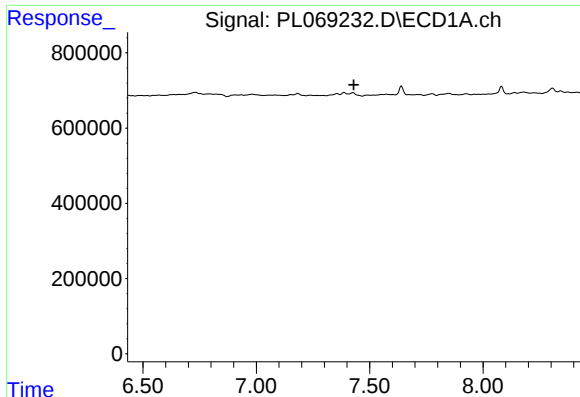

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

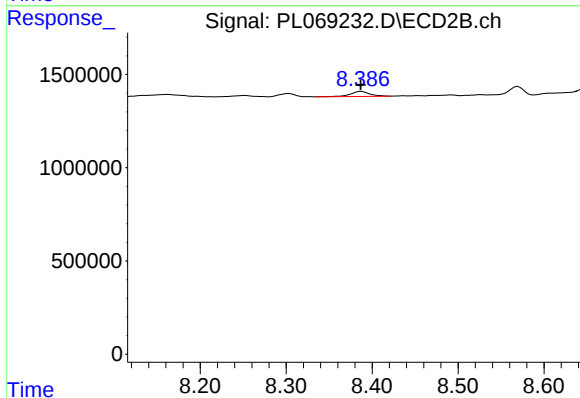


#26 Chlordane-4

R.T.: 8.388 min
Delta R.T.: 0.000 min
Response: 401257
Conc: 2.02 ng/ml

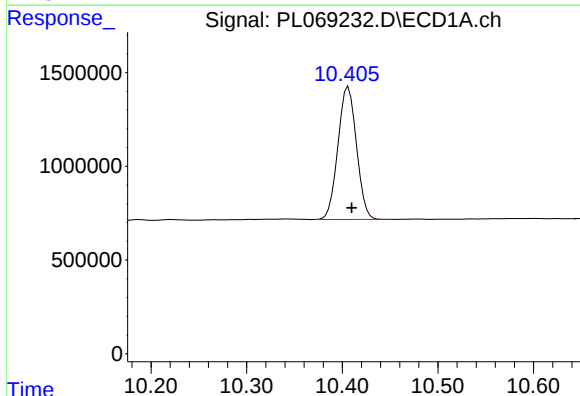

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.004 min
Response: 9555428
Conc: 16.63 ng/ml

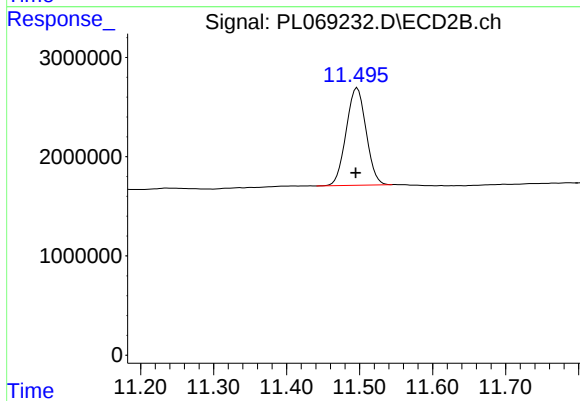

#28 Decachlorobiphenyl

R.T.: 11.497 min
Delta R.T.: 0.002 min
Response: 18607573
Conc: 19.18 ng/ml