

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
 Data File : PL069235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Aug 2021 15:02
 Operator : AR\AJ
 Sample : M3428-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 19 15:47:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.571	9312496	30189996	22.514	29.734 #
28)	SA Decachlor...	10.407	11.497	12402604	24406999	21.581	25.156
Target Compounds							
3)	MA gamma-BHC...	0.000	6.566f	0	174421	N.D.	0.134 #
11)	B alpha-Chl...	0.000	8.389	0	197430	N.D.	0.172 #
12)	B 4,4'-DDE	7.640	8.572	422180	1263991	0.874	1.196 #
13)	MA Dieldrin	0.000	8.729	0	244266	N.D.	0.225 #
15)	B Endosulfa...	0.000	9.220f	0	428906	N.D.	0.468 #
17)	MA 4,4'-DDT	8.486	9.430	519398	1176072	1.069	1.243
21)	B Endrin ke...	0.000	10.097f	0	246683	N.D.	0.242 #
26)	Chlordane-4	0.000	8.389	0	197430	N.D.	0.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081921\
Data File : PL069235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Aug 2021 15:02
Operator : AR\AJ
Sample : M3428-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 19 15:47:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

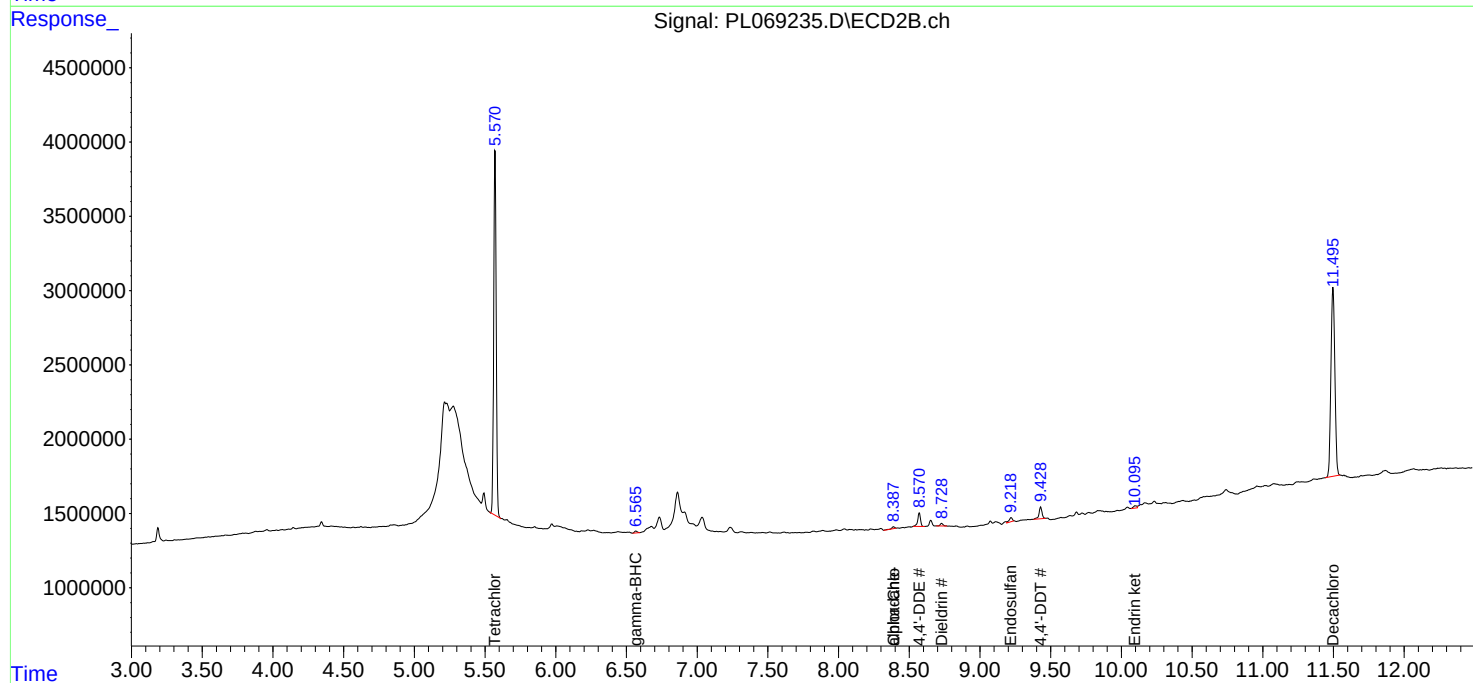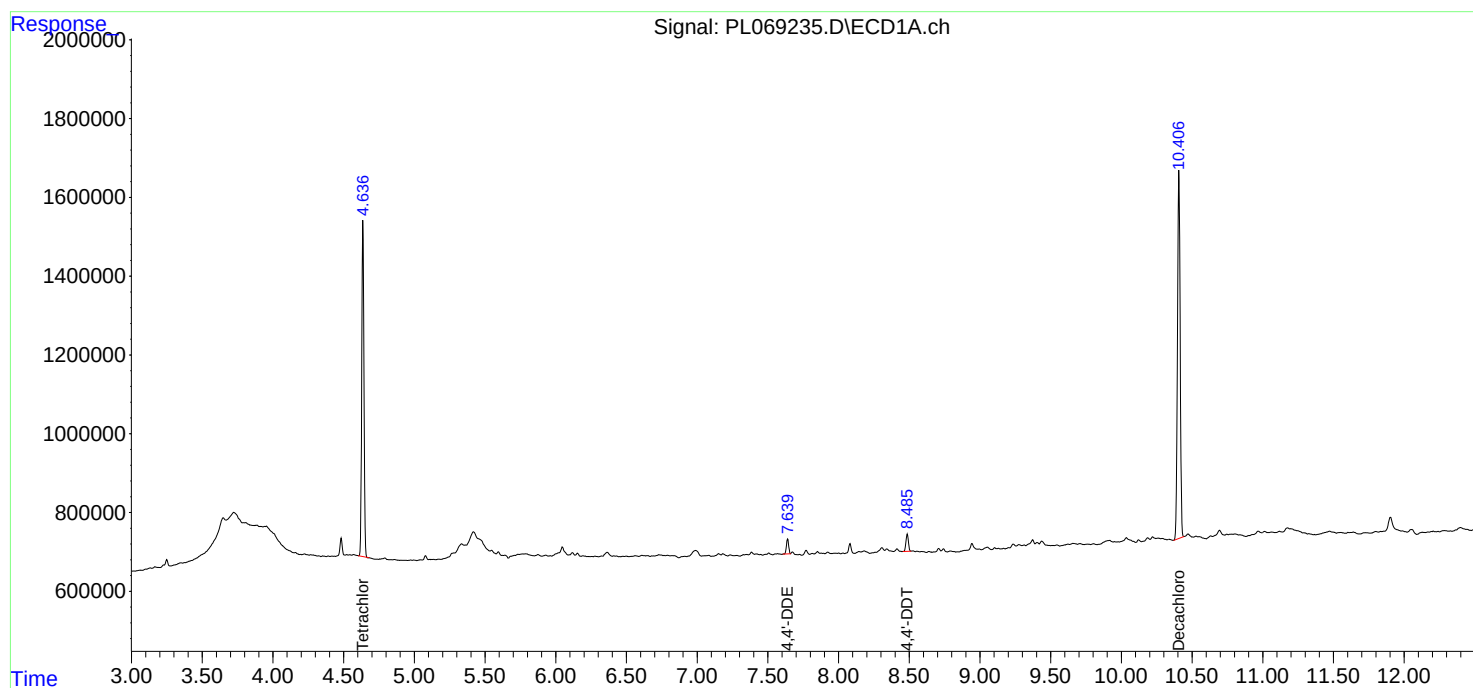


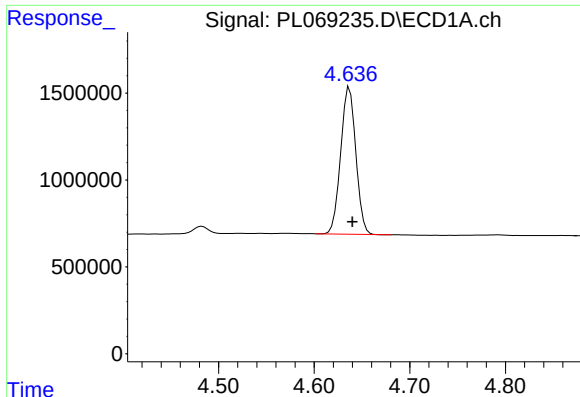

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 9312496
Conc: 22.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

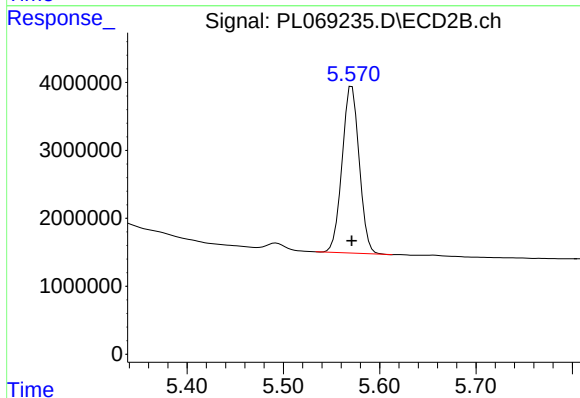


#1 Tetrachloro-m-xylene

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 30189996
Conc: 29.73 ng/ml

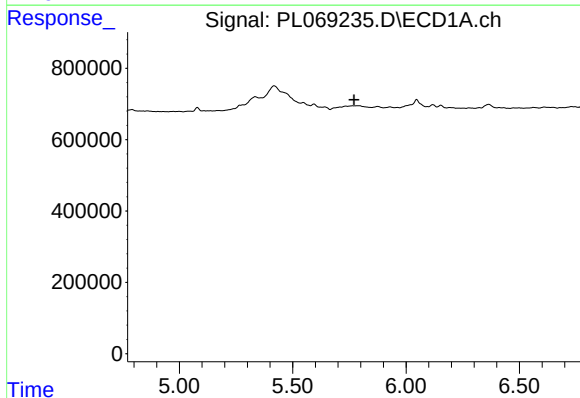


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.770 min
Response: 0
Conc: N.D.

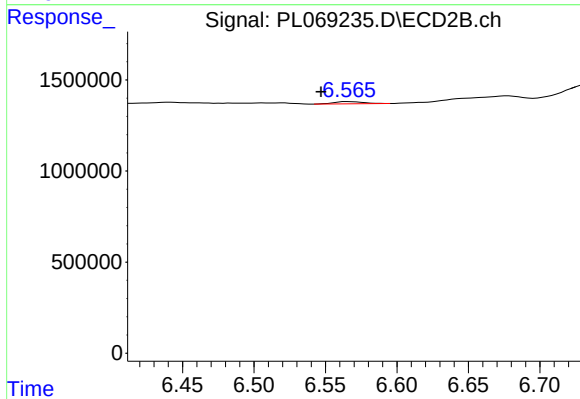

#3 gamma-BHC (Lindane)


R.T.: 6.566 min
Delta R.T.: 0.019 min
Response: 174421
Conc: 0.13 ng/ml

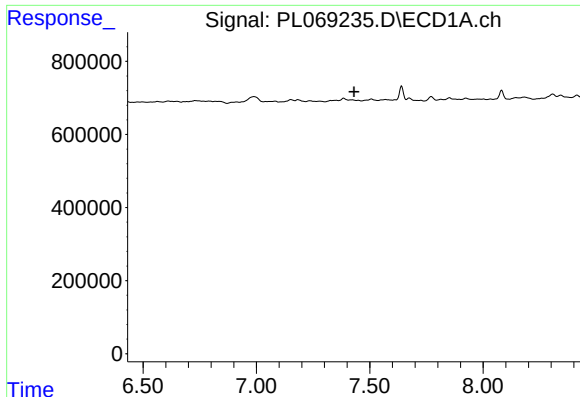

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.432 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

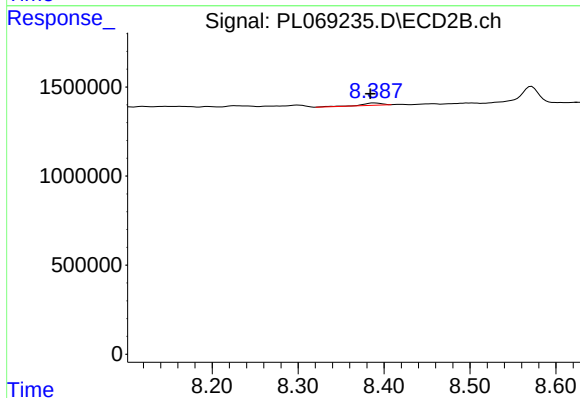


#11 alpha-Chlordane

R.T.: 8.389 min
Delta R.T.: 0.005 min
Response: 197430
Conc: 0.17 ng/ml

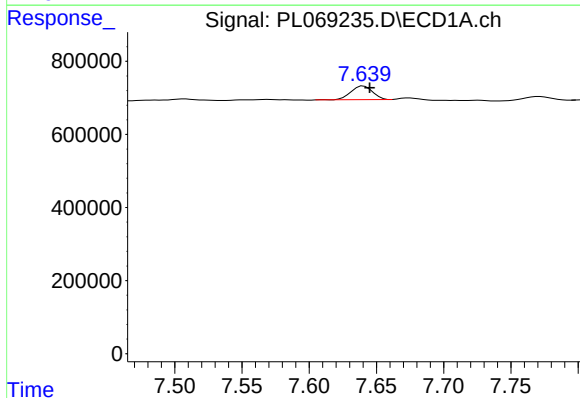


#12 4,4'-DDE

R.T.: 7.640 min
Delta R.T.: -0.005 min
Response: 422180
Conc: 0.87 ng/ml

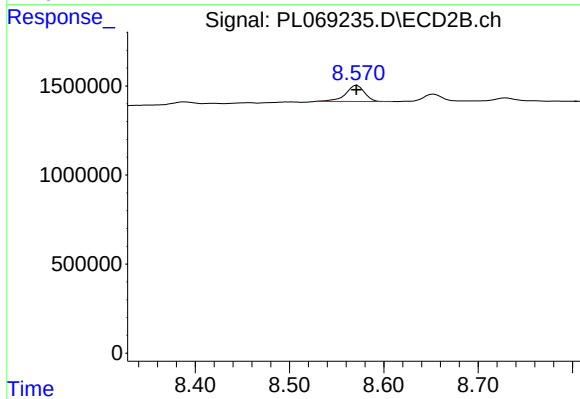

#12 4,4'-DDE


R.T.: 8.572 min
Delta R.T.: 0.000 min
Response: 1263991
Conc: 1.20 ng/ml

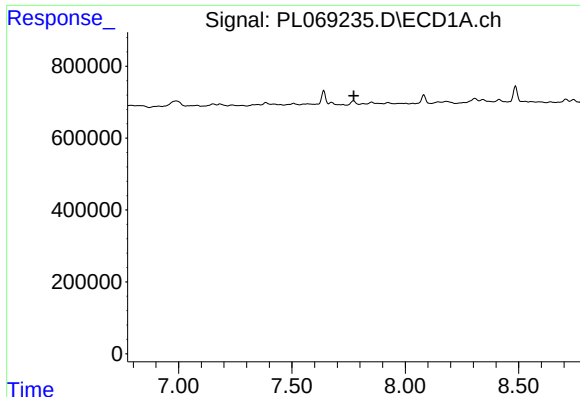

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

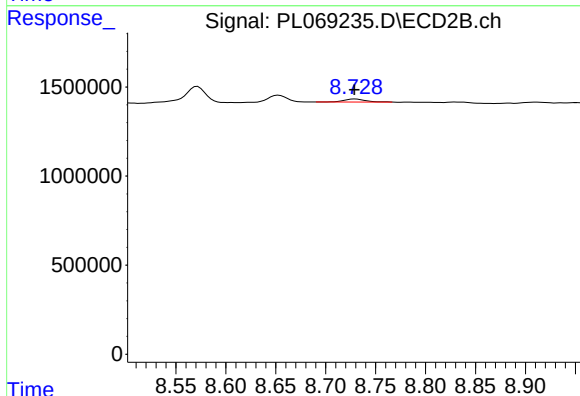


#13 Dieldrin

R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 244266
Conc: 0.23 ng/ml

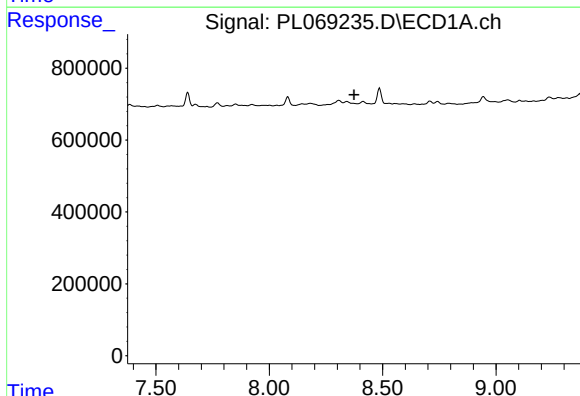


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

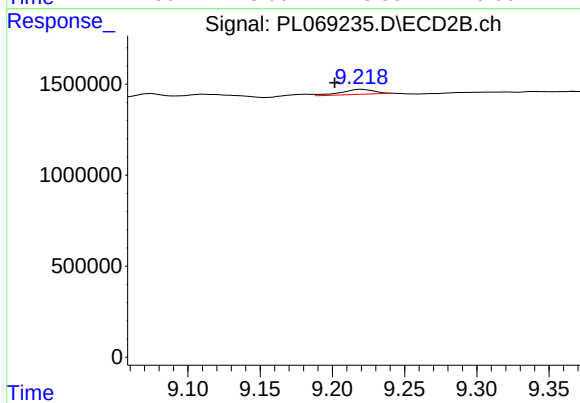

#15 Endosulfan II


R.T.: 9.220 min
Delta R.T.: 0.019 min
Response: 428906
Conc: 0.47 ng/ml

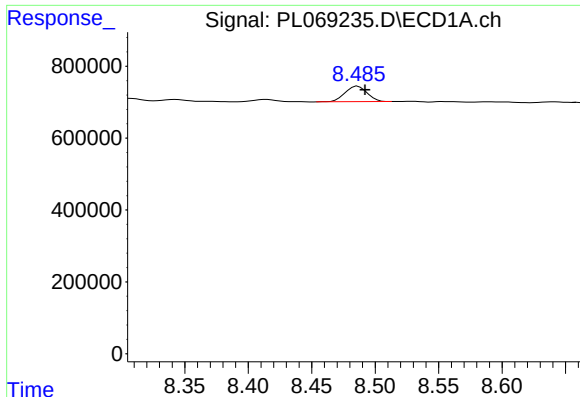

#17 4,4'-DDT


R.T.: 8.486 min
Delta R.T.: -0.006 min
Response: 519398
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

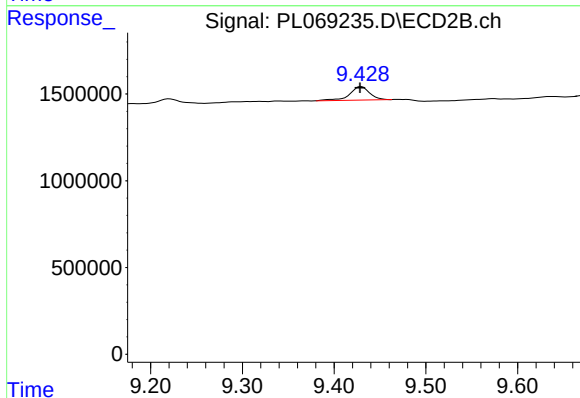


#17 4,4'-DDT

R.T.: 9.430 min
Delta R.T.: 0.002 min
Response: 1176072
Conc: 1.24 ng/ml

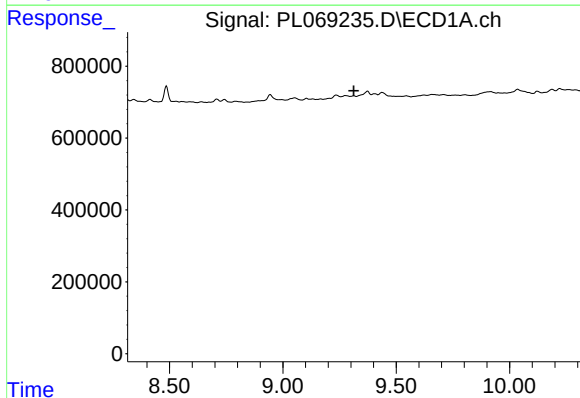


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

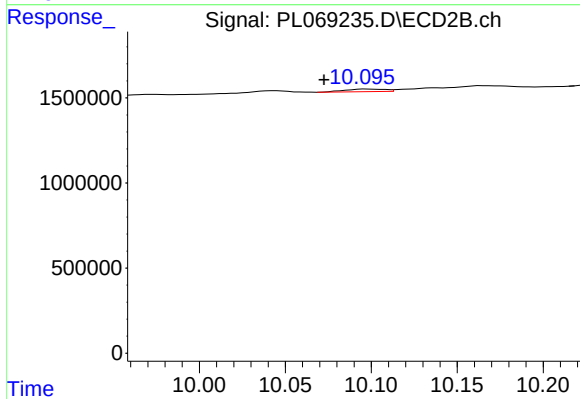

#21 Endrin ketone


R.T.: 10.097 min
Delta R.T.: 0.024 min
Response: 246683
Conc: 0.24 ng/ml

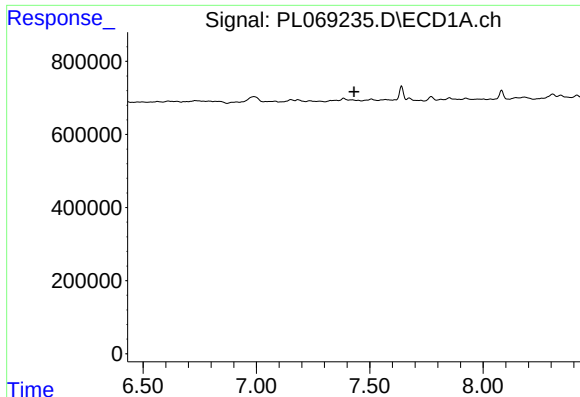

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

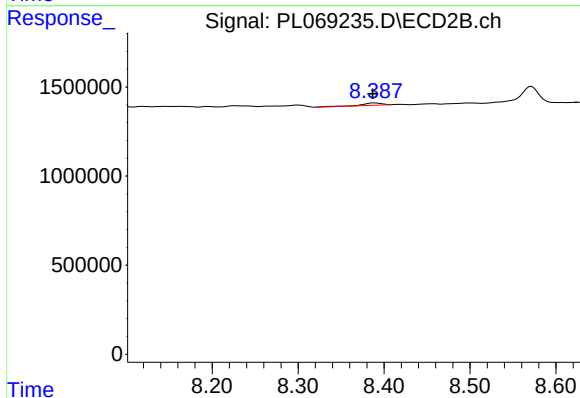


#26 Chlordane-4

R.T.: 8.389 min
Delta R.T.: 0.002 min
Response: 197430
Conc: 1.00 ng/ml

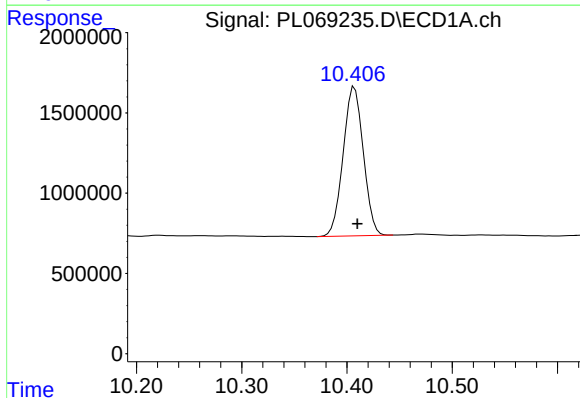

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.003 min
Response: 12402604
Conc: 21.58 ng/ml

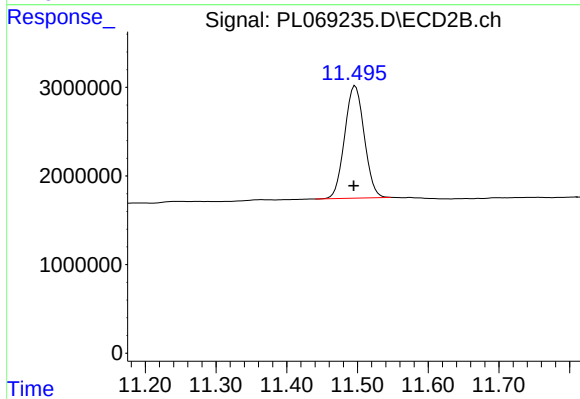

#28 Decachlorobiphenyl

R.T.: 11.497 min
Delta R.T.: 0.002 min
Response: 24406999
Conc: 25.16 ng/ml